

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
 Data File : VX021488.D
 Acq On : 25 Mar 2021 16:01
 Operator : JC/MD
 Sample : M1758-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	76	87	91	rBV5	3073	7672	1.93%	0.351%
2	2.429	220	228	234	rBV	2586	4945	1.24%	0.226%
3	2.587	248	255	263	rBV2	3309	6073	1.53%	0.278%
4	5.470	732	745	758	rBV2	47546	135806	34.15%	6.217%
5	5.635	761	773	784	rBV	72451	198259	49.86%	9.076%
6	6.035	827	841	857	rBV	52643	140324	35.29%	6.424%
7	6.829	963	976	987	rBV	118491	282434	71.03%	12.929%
8	8.694	1285	1293	1312	rBV	248411	397624	100.00%	18.202%
9	10.094	1525	1531	1549	rVB	271093	376139	94.60%	17.218%
10	11.118	1700	1705	1716	rVB	219650	293138	73.72%	13.419%
11	12.059	1860	1865	1874	rVB	273918	342117	86.04%	15.661%




Sum of corrected areas: 2184531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021488.D
Acq On : 25 Mar 2021 16:01
Operator : JC/MD
Sample : M1758-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

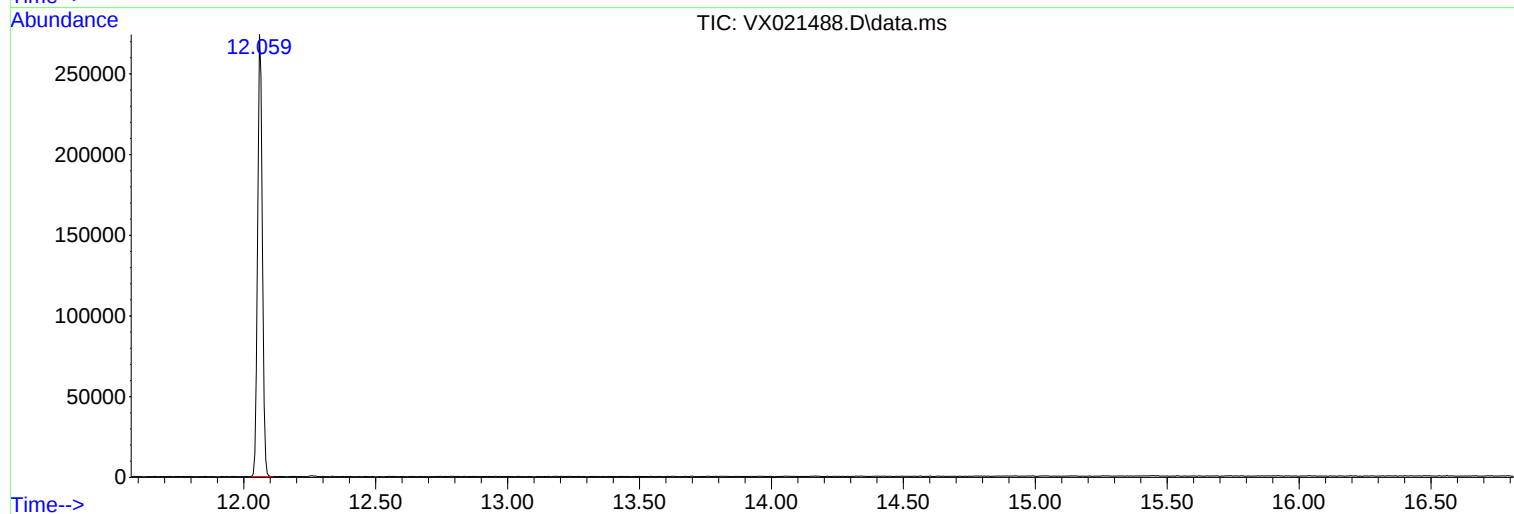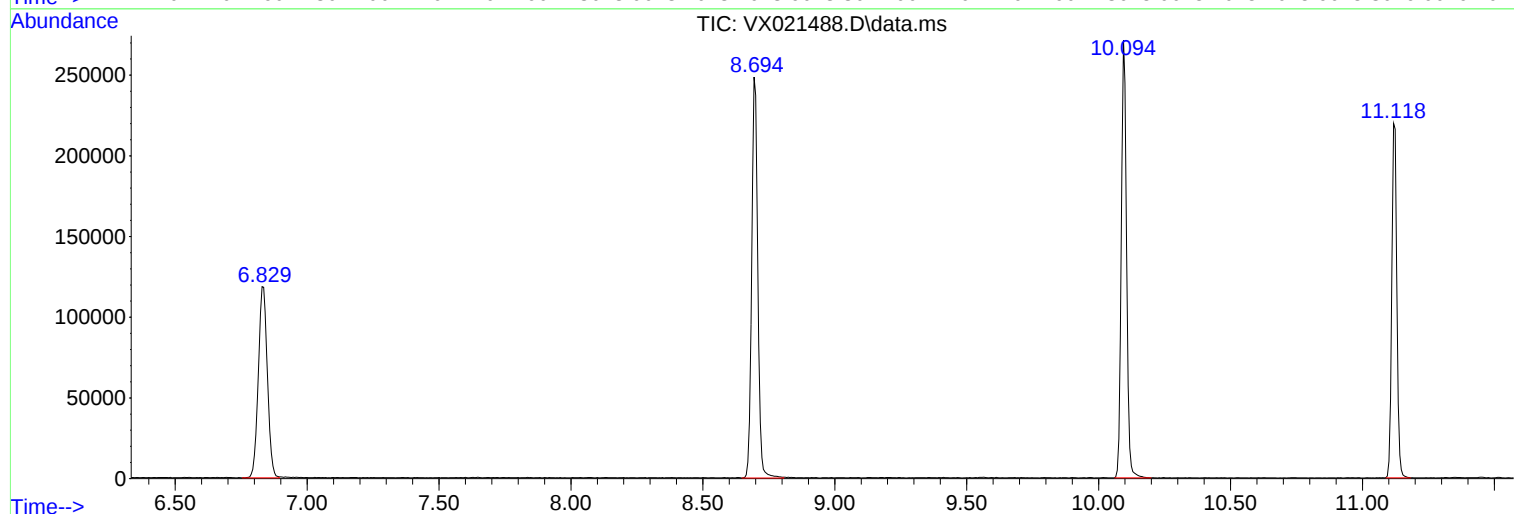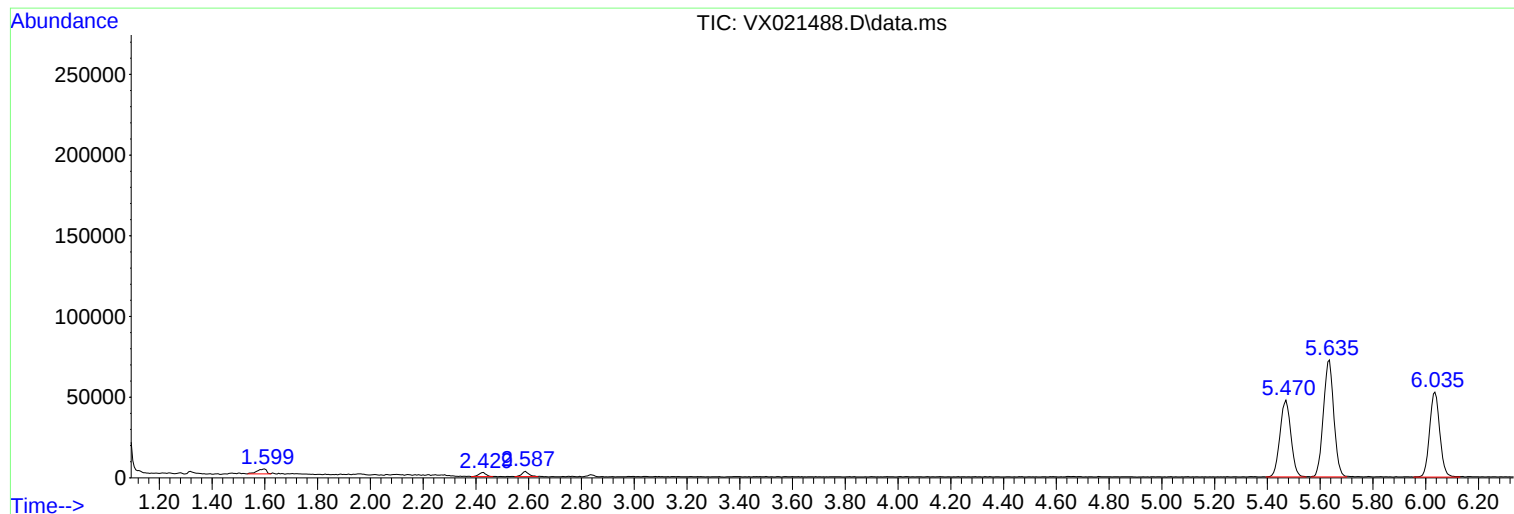

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021488.D
Acq On : 25 Mar 2021 16:01
Operator : JC/MD
Sample : M1758-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021488.D
Acq On : 25 Mar 2021 16:01
Operator : JC/MD
Sample : M1758-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
