

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
 Data File : VX021497.D
 Acq On : 25 Mar 2021 19:26
 Operator : JC/MD
 Sample : M1787-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE-122D3-20210319

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	77	87	94	rBV5	3604	7867	1.96%	0.353%
2	2.587	248	255	264	rBV3	2747	5954	1.48%	0.267%
3	5.464	733	744	756	rVV	48655	137015	34.16%	6.154%
4	5.623	760	771	788	rBV	71103	199115	49.64%	8.943%
5	6.029	830	840	852	rBV	54232	140163	34.94%	6.295%
6	6.829	966	976	988	rBV	121348	284614	70.96%	12.783%
7	7.188	1030	1037	1043	rBV3	5293	10760	2.68%	0.483%
8	8.694	1286	1293	1309	rBV	260435	401110	100.00%	18.016%
9	10.094	1525	1531	1546	rBV	280123	384016	95.74%	17.248%
10	11.118	1700	1705	1718	rVB	233701	299689	74.71%	13.460%
11	12.059	1859	1865	1875	rBV	291495	356163	88.79%	15.997%




Sum of corrected areas: 2226466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021497.D
Acq On : 25 Mar 2021 19:26
Operator : JC/MD
Sample : M1787-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-122D3-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

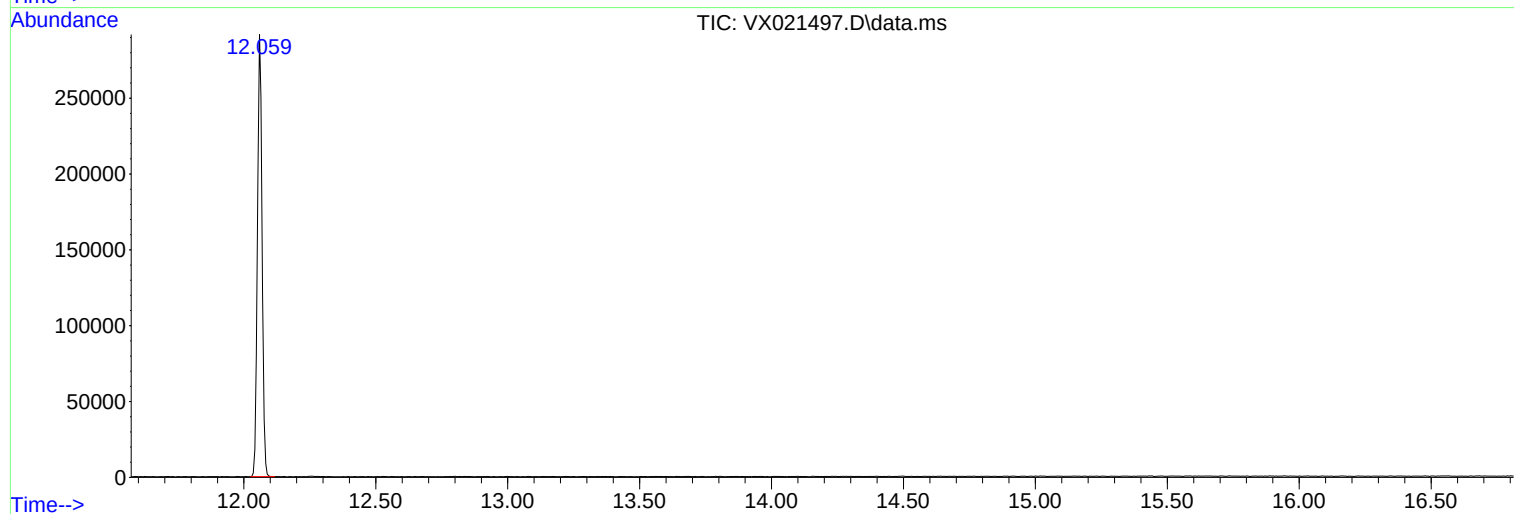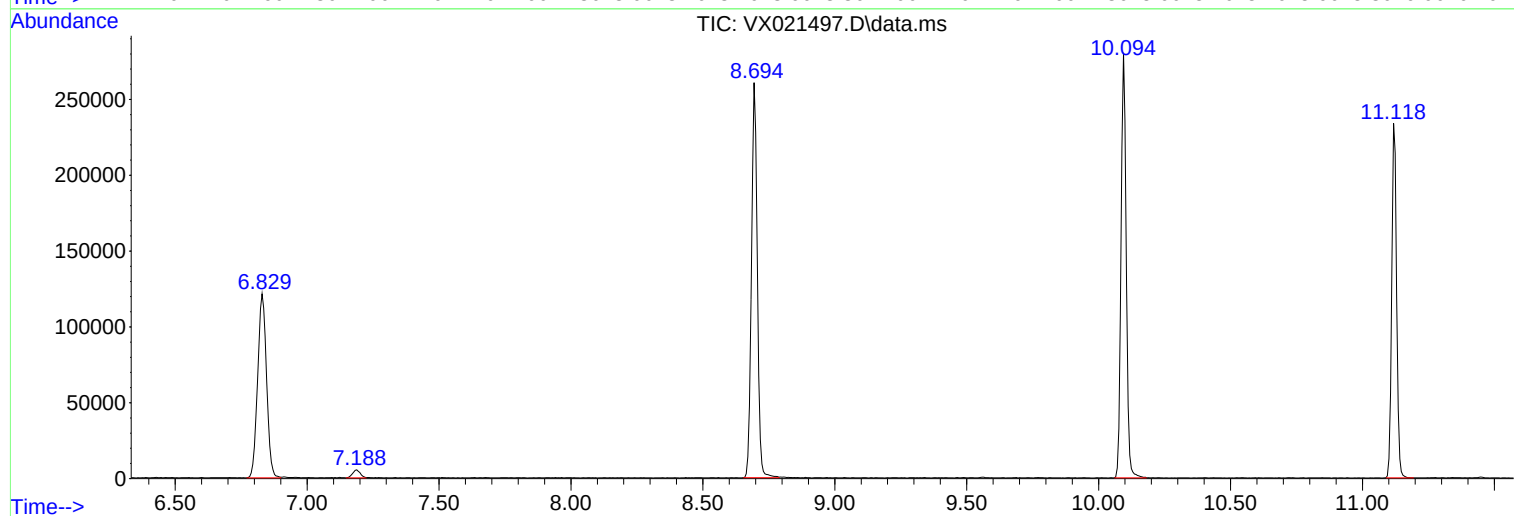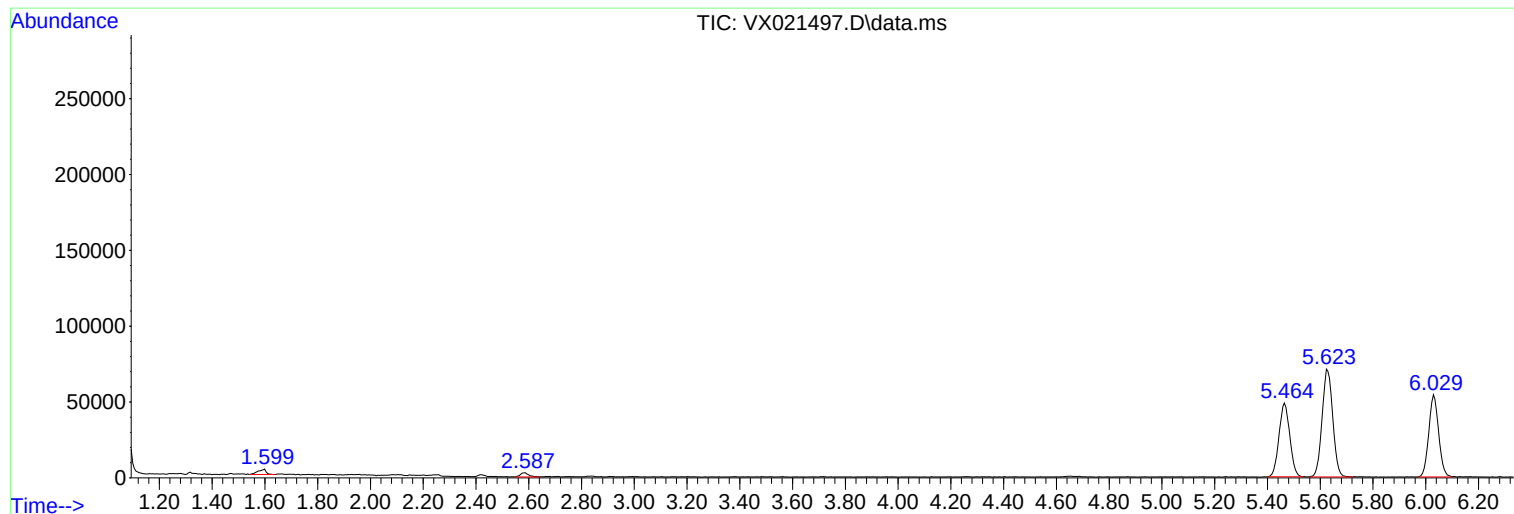

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021497.D
Acq On : 25 Mar 2021 19:26
Operator : JC/MD
Sample : M1787-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-122D3-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021497.D
Acq On : 25 Mar 2021 19:26
Operator : JC/MD
Sample : M1787-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-122D3-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------