

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
 Data File : VX021511.D
 Acq On : 26 Mar 2021 01:41
 Operator : JC/MD
 Sample : M1770-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-102S

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260

Signal : TIC: VX021511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	79	86	89	rVB5	3315	6601	1.61%	0.289%
2	2.581	245	254	265	rBV	11556	23476	5.74%	1.029%
3	5.182	686	696	704	rVB4	1862	5482	1.34%	0.240%
4	5.464	732	744	757	rBV	49896	141936	34.68%	6.222%
5	5.629	760	772	787	rVV	73371	204049	49.85%	8.945%
6	6.029	830	840	853	rBV	55591	145937	35.66%	6.398%
7	6.829	966	976	987	rBV	125946	294393	71.93%	12.906%
8	8.694	1285	1293	1312	rBV	258851	409299	100.00%	17.943%
9	9.318	1390	1399	1407	rBV2	8436	13048	3.19%	0.572%
10	10.094	1525	1531	1548	rVB	282192	389432	95.15%	17.072%
11	11.124	1700	1706	1717	rVB	224969	299696	73.22%	13.138%
12	12.059	1860	1865	1873	rVB	280708	347761	84.97%	15.245%




Sum of corrected areas: 2281110

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021511.D
Acq On : 26 Mar 2021 01:41
Operator : JC/MD
Sample : M1770-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-102S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

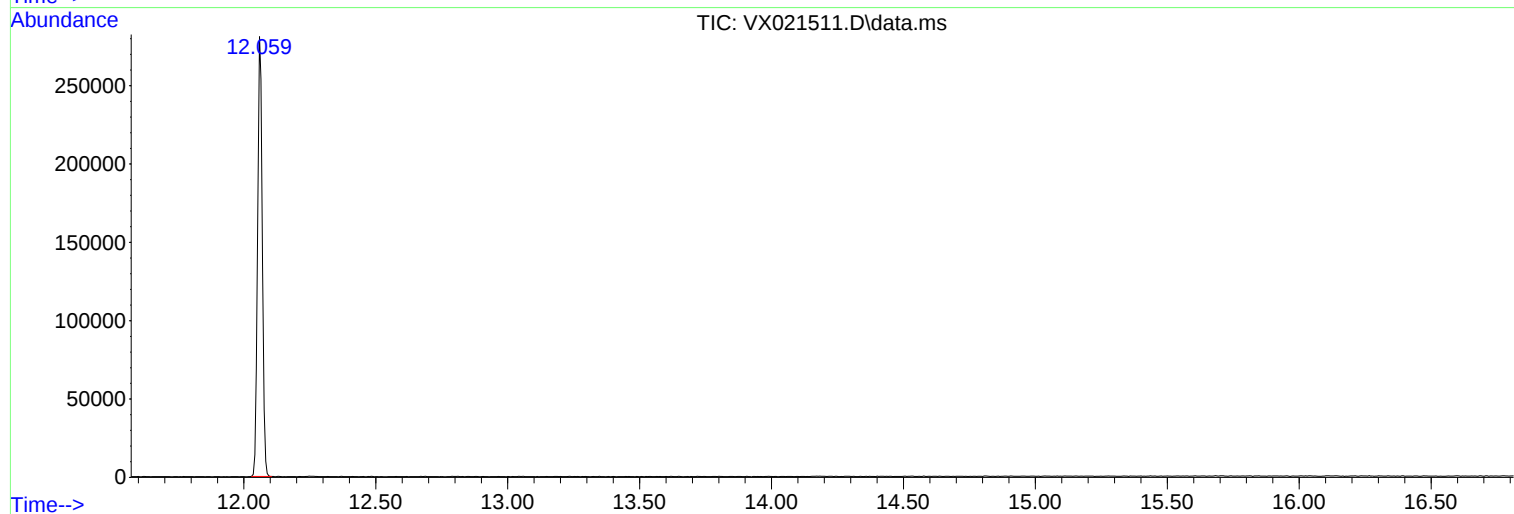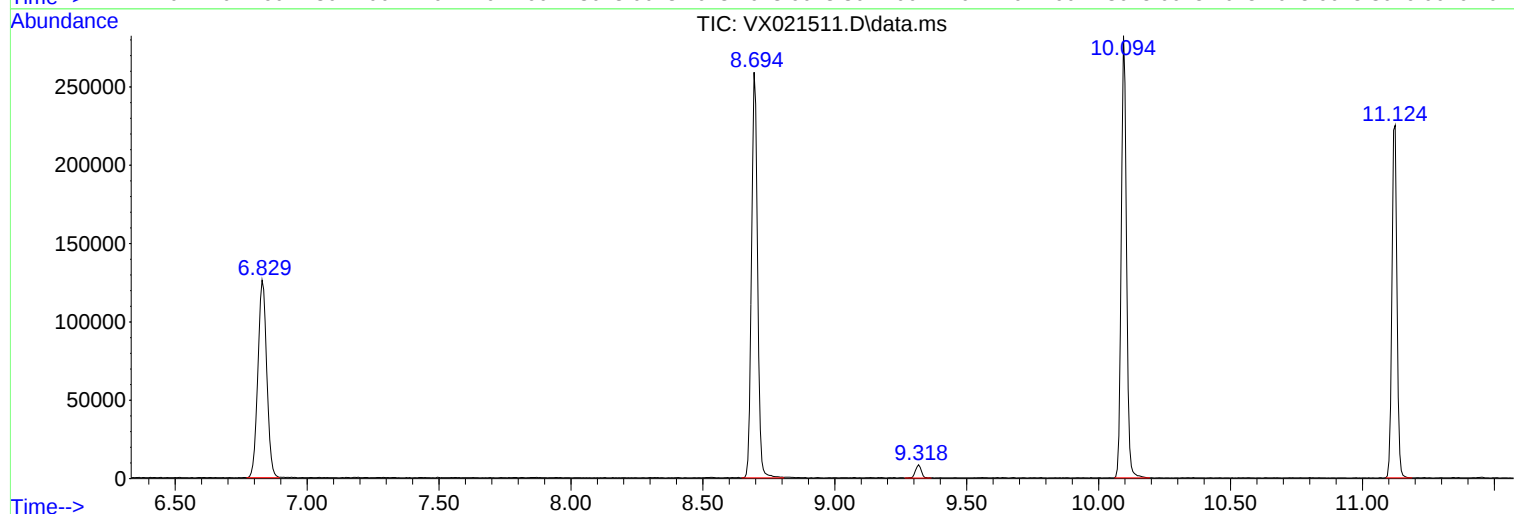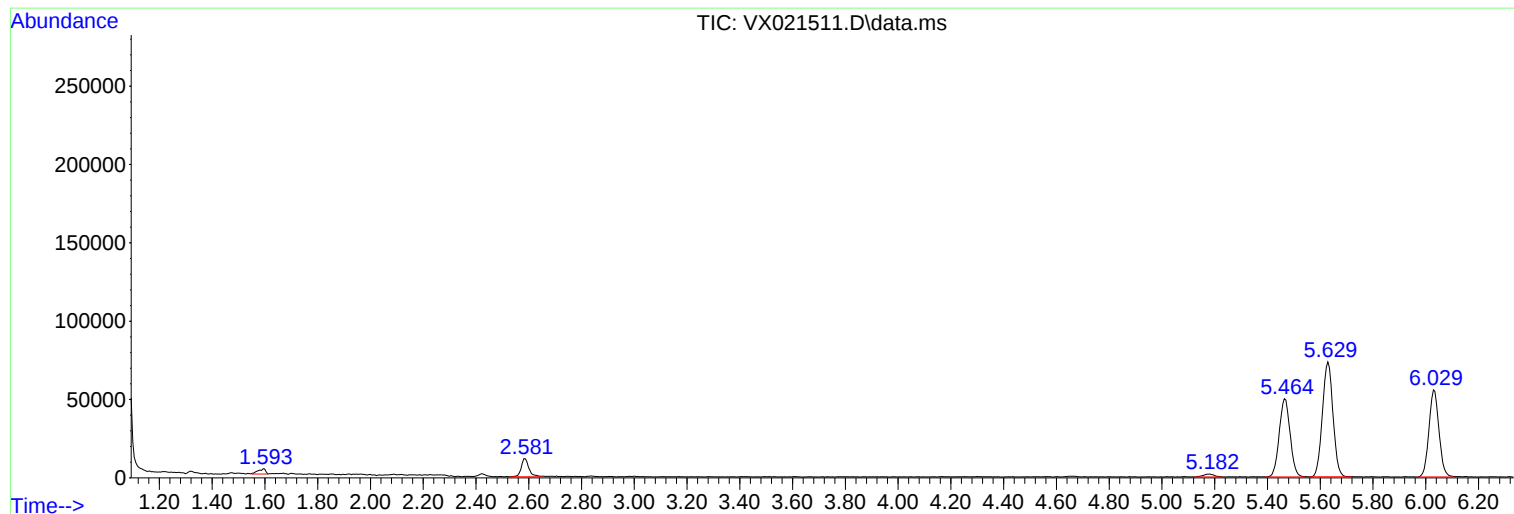

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021511.D
Acq On : 26 Mar 2021 01:41
Operator : JC/MD
Sample : M1770-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-102S










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.581	5.75 ug/l	23476	Pentafluorobenzene	5.629

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
2			4-Penten-2-ol	86	C5H10O	000625-31-0	9
3			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			Ethylamine	45	C2H7N	000075-04-7	5
5			Formamide	45	CH3NO	000075-12-7	4

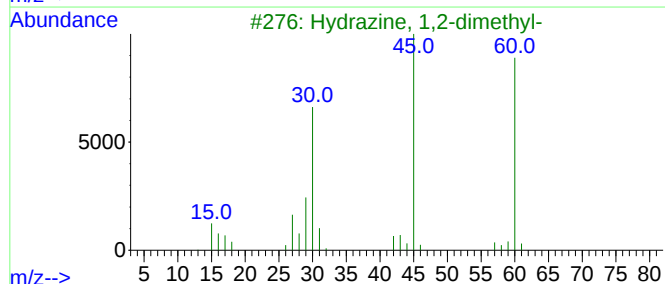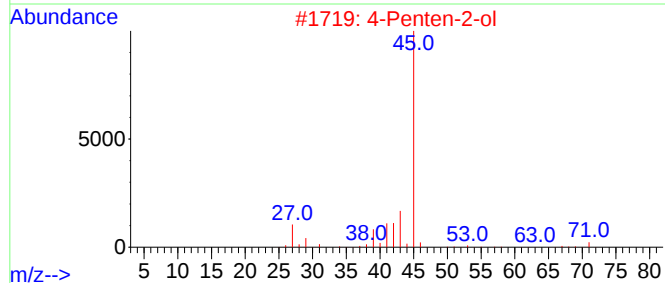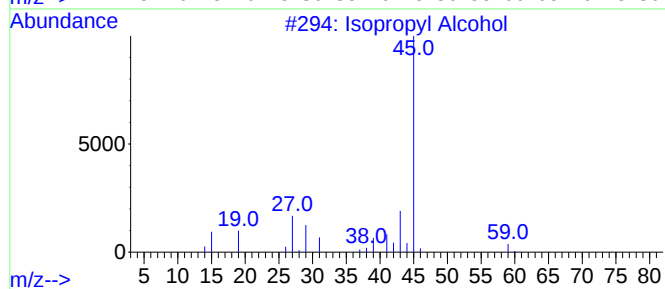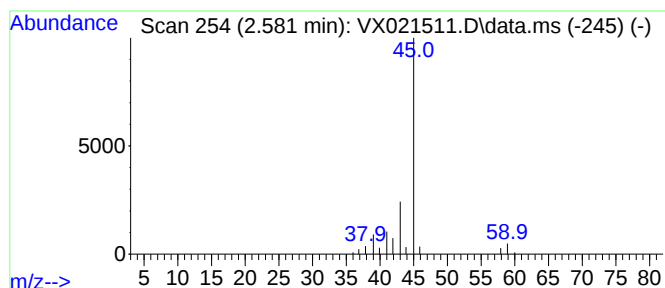

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021511.D
Acq On : 26 Mar 2021 01:41
Operator : JC/MD
Sample : M1770-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-102S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.581	5.8	ug/l	23476	1	5.629	204049	50.0