

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
 Data File : VX021519.D
 Acq On : 26 Mar 2021 04:49
 Operator : JC/MD
 Sample : M1777-06 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 238

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260

Signal : TIC: VX021519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	77	86	90	rVB4	3407	7464	1.87%	0.310%
2	1.770	112	116	123	rVB2	5910	8802	2.20%	0.366%
3	1.981	149	152	163	rVB3	3055	5534	1.38%	0.230%
4	2.099	167	172	178	rVB2	3258	5912	1.48%	0.246%
5	2.240	193	196	206	rVB7	2013	4847	1.21%	0.201%
6	2.423	222	227	235	rVB	4266	7241	1.81%	0.301%
7	5.464	734	744	759	rBV	48496	137857	34.47%	5.728%
8	5.629	761	772	784	rVV2	72748	199935	50.00%	8.307%
9	6.029	829	840	850	rBV	54127	141145	35.30%	5.864%
10	6.111	850	854	862	rVB3	1895	4509	1.13%	0.187%
11	6.829	965	976	990	rBV	121940	287471	71.89%	11.944%
12	8.694	1286	1293	1300	rBV	256298	399883	100.00%	16.615%
13	8.765	1300	1305	1311	rVB	15151	25494	6.38%	1.059%
14	10.094	1525	1531	1546	rBV	274188	376656	94.19%	15.650%
15	10.235	1549	1555	1560	rVB2	3181	4338	1.08%	0.180%
16	10.341	1567	1573	1579	rVB	16672	23377	5.85%	0.971%
17	10.682	1626	1631	1637	rVB	9467	12263	3.07%	0.510%
18	11.118	1700	1705	1717	rVB	215840	287221	71.83%	11.934%
19	11.418	1751	1756	1764	rVB	6767	12467	3.12%	0.518%
20	11.488	1764	1768	1775	rVB	3937	4614	1.15%	0.192%
21	11.653	1791	1796	1800	rVB	3840	4471	1.12%	0.186%
22	11.788	1814	1819	1824	rBV	15007	17777	4.45%	0.739%
23	12.059	1860	1865	1872	rBV	252725	321049	80.29%	13.339%
24	12.124	1872	1876	1883	rVB	7012	9118	2.28%	0.379%
25	12.283	1892	1903	1910	rVV2	9488	14556	3.64%	0.605%
26	12.353	1910	1915	1921	rVB3	3515	4892	1.22%	0.203%
27	12.759	1982	1984	1989	rVB3	3893	4474	1.12%	0.186%
28	13.000	2021	2025	2032	rVB	4356	5044	1.26%	0.210%
29	13.206	2056	2060	2064	rVB	4818	6181	1.55%	0.257%
30	13.330	2073	2081	2088	rBV2	12237	17648	4.41%	0.733%
31	13.459	2099	2103	2107	rBV2	10912	14118	3.53%	0.587%
32	13.895	2171	2177	2181	rVB4	3237	4344	1.09%	0.180%
33	14.271	2232	2241	2246	rBV	7936	13732	3.43%	0.571%
34	14.518	2278	2283	2288	rVB3	5836	7859	1.97%	0.327%
35	15.230	2399	2404	2411	rBV7	2250	4506	1.13%	0.187%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021519.D
Acq On : 26 Mar 2021 04:49
Operator : JC/MD
Sample : M1777-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
238

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Title : SW846 8260


Sum of corrected areas: 2406799

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021519.D
Acq On : 26 Mar 2021 04:49
Operator : JC/MD
Sample : M1777-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
238

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

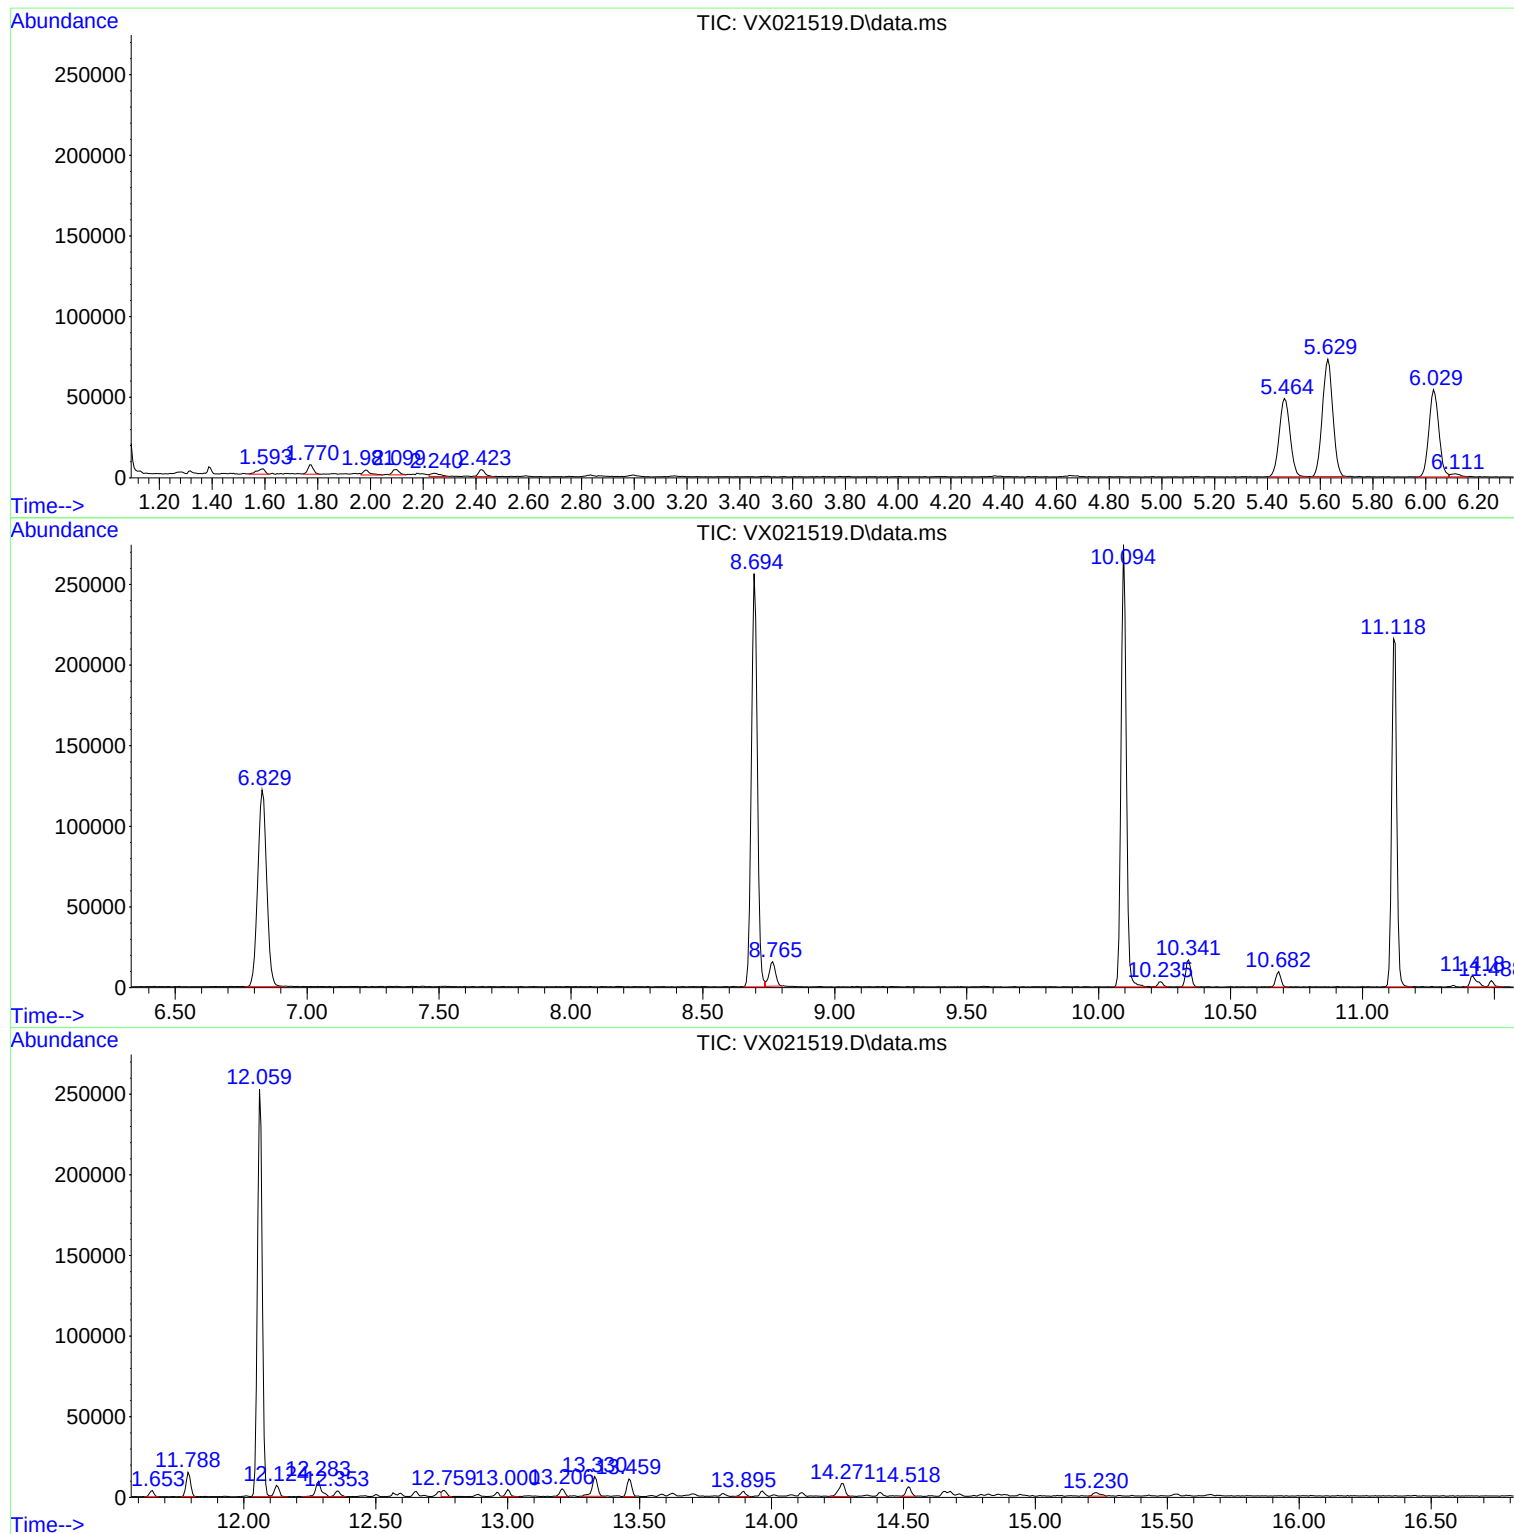

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021519.D
Acq On : 26 Mar 2021 04:49
Operator : JC/MD
Sample : M1777-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
238

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
Data File : VX021519.D
Acq On : 26 Mar 2021 04:49
Operator : JC/MD
Sample : M1777-06 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
238

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
