
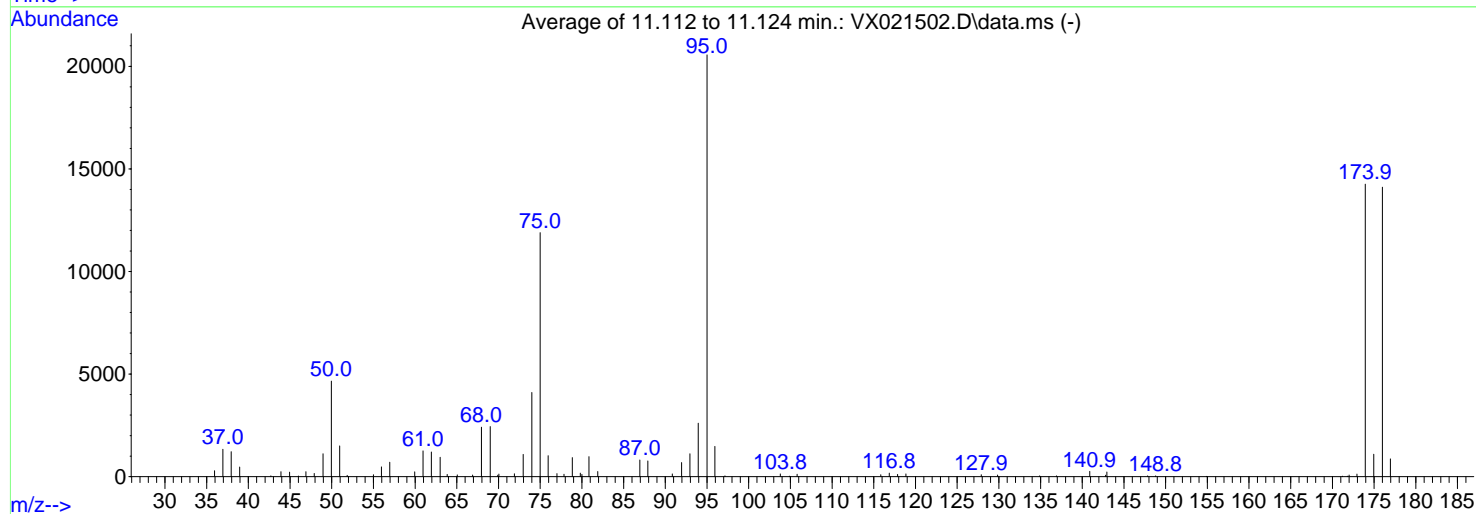


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032521\
 Data File : VX021502.D
 Acq On : 25 Mar 2021 21:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260
 Last Update : Wed Mar 24 12:25:26 2021

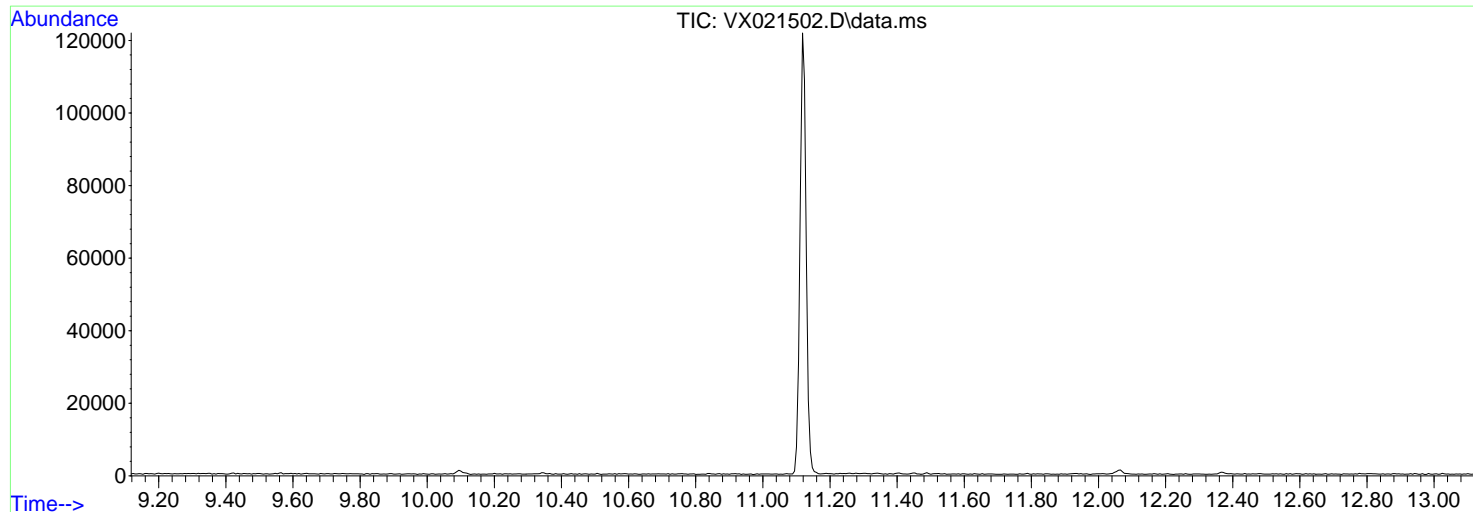

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	22.6	4655	PASS
75	95	30	60	57.9	11894	PASS
95	95	100	100	100.0	20560	PASS
96	95	5	9	7.2	1475	PASS
173	174	0.00	2	0.9	126	PASS
174	95	50	100	69.4	14260	PASS
175	174	5	9	7.7	1091	PASS
176	174	95	101	98.9	14106	PASS
177	176	5	9	6.2	868	PASS