

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032522\
 Data File : VX027696.D
 Acq On : 25 Mar 2022 12:31
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDICC005

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
 Title : SW846 8260

Signal : TIC: VX027696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.167	10	13	19	rVB	7204	6479	1.73%	0.178%
2	1.246	22	26	31	rVV	4106	7932	2.12%	0.218%
3	1.295	31	34	43	rVB	7646	9674	2.59%	0.266%
4	1.374	43	47	51	rBV	6791	6373	1.71%	0.175%
5	1.599	81	84	88	rVB2	6532	7224	1.93%	0.198%
6	1.679	94	97	102	rVB	3636	4557	1.22%	0.125%
7	1.886	126	131	138	rBV	8959	13137	3.51%	0.361%
8	2.136	166	172	180	rVB2	6882	10325	2.76%	0.284%
9	2.239	184	189	197	rVB	6004	8588	2.30%	0.236%
10	2.319	197	202	208	rBV2	17993	33710	9.02%	0.926%
11	2.386	208	213	219	rVB	11247	17708	4.74%	0.486%
12	2.447	219	223	228	rBV	2702	4052	1.08%	0.111%
13	2.508	228	233	240	rVB	7428	11502	3.08%	0.316%
14	2.666	251	259	263	rBV2	9976	18347	4.91%	0.504%
15	2.709	263	266	274	rVV2	4687	7848	2.10%	0.216%
16	2.788	274	279	286	rVB2	9744	16411	4.39%	0.451%
17	2.971	300	309	319	rBV2	3808	9068	2.43%	0.249%
18	3.075	319	326	341	rBV4	16459	74364	19.90%	2.042%
19	3.611	407	414	425	rBV	7374	14886	3.98%	0.409%
20	3.727	425	433	450	rBV2	27546	96680	25.87%	2.655%
21	4.489	548	558	565	rBV6	13800	41687	11.15%	1.145%
22	4.562	565	570	578	rVB	9094	21894	5.86%	0.601%
23	4.660	578	586	592	rBV3	5578	14312	3.83%	0.393%
24	4.733	592	598	600	rBV2	2512	5326	1.43%	0.146%
25	4.922	616	629	637	rBV6	8326	27935	7.47%	0.767%
26	5.019	637	645	652	rVV2	12783	39864	10.67%	1.095%
27	5.099	652	658	669	rVB2	7166	21623	5.79%	0.594%
28	5.391	695	706	712	rBV4	11296	32168	8.61%	0.884%
29	5.477	712	720	725	rVV4	10474	31524	8.43%	0.866%
30	5.556	725	733	747	rVV	76505	237719	63.60%	6.529%
31	5.690	749	755	766	rVB5	12969	40690	10.89%	1.118%
32	5.952	792	798	805	rBV3	5468	14569	3.90%	0.400%
33	6.044	805	813	820	rBV2	14342	39135	10.47%	1.075%
34	6.349	855	863	874	rBV4	7238	19765	5.29%	0.543%
35	6.763	921	931	944	rBV	121260	283540	75.86%	7.788%
36	7.129	984	991	999	rBV4	10935	23579	6.31%	0.648%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032522\
 Data File : VX027696.D
 Acq On : 25 Mar 2022 12:31
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDICC005

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
 Title : SW846 8260

37	7.385	1025	1033	1037	rBV2	15480	33484	8.96%	0.920%
38	7.434	1037	1041	1051	rVB2	11847	22626	6.05%	0.621%
39	7.586	1060	1066	1073	rVB3	7229	14135	3.78%	0.388%
40	7.696	1075	1084	1095	rVV4	9412	23286	6.23%	0.640%
41	7.812	1095	1103	1113	rVB2	12144	32253	8.63%	0.886%
42	8.116	1147	1153	1161	rBV2	2548	4566	1.22%	0.125%
43	8.245	1165	1174	1182	rBV2	40154	63630	17.02%	1.748%
44	8.373	1189	1195	1204	rVB3	10415	17926	4.80%	0.492%
45	8.580	1222	1229	1236	rBV	56578	92806	24.83%	2.549%
46	8.653	1236	1241	1247	rVV2	24347	37882	10.14%	1.040%
47	8.720	1247	1252	1261	rVB	29050	43053	11.52%	1.182%
48	8.982	1290	1295	1302	rVB2	10419	14822	3.97%	0.407%
49	9.122	1312	1318	1320	rBV	12189	18045	4.83%	0.496%
50	9.153	1320	1323	1331	rVB	15696	22543	6.03%	0.619%
51	9.275	1338	1343	1346	rBV	22568	33055	8.84%	0.908%
52	9.311	1346	1349	1356	rVB	14978	20836	5.57%	0.572%
53	9.433	1363	1369	1379	rBV	46533	63925	17.10%	1.756%
54	9.525	1379	1384	1389	rVV2	8886	12470	3.34%	0.342%
55	9.580	1389	1393	1396	rVV	14881	20533	5.49%	0.564%
56	9.610	1396	1398	1404	rVB	8168	10729	2.87%	0.295%
57	10.055	1465	1471	1483	rVB	248137	365353	97.75%	10.035%
58	10.165	1483	1489	1491	rBV	17589	24908	6.66%	0.684%
59	10.195	1491	1494	1501	rVB	34787	44230	11.83%	1.215%
60	10.305	1506	1512	1520	rBV	63975	88831	23.77%	2.440%
61	10.647	1562	1568	1578	rVB2	44464	82264	22.01%	2.259%
62	10.799	1589	1593	1597	rBV	6863	9083	2.43%	0.249%
63	10.842	1597	1600	1608	rVB	18090	22672	6.07%	0.623%
64	10.964	1614	1620	1625	rBV	36698	46832	12.53%	1.286%
65	11.018	1625	1629	1635	rVB	10213	12957	3.47%	0.356%
66	11.085	1635	1640	1644	rBV	18950	24959	6.68%	0.686%
67	11.201	1654	1659	1663	rBV2	25533	50922	13.62%	1.399%
68	11.244	1663	1666	1672	rVV3	19083	33899	9.07%	0.931%
69	11.305	1672	1676	1682	rVV	35327	43349	11.60%	1.191%
70	11.366	1682	1686	1692	rVV	30963	38925	10.41%	1.069%
71	11.451	1695	1700	1707	rBV	62572	82440	22.06%	2.264%
72	11.719	1737	1744	1747	rBV2	47739	66861	17.89%	1.836%
73	11.756	1747	1750	1755	rVB	34521	41787	11.18%	1.148%
74	11.890	1767	1772	1778	rVB	34763	43326	11.59%	1.190%
75	11.969	1781	1785	1788	rBV	28012	33429	8.94%	0.918%
76	12.024	1788	1794	1804	rVB2	255933	373746	100.00%	10.265%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032522\
 Data File : VX027696.D
 Acq On : 25 Mar 2022 12:31
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDICC005

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M

Title : SW846 8260

77	12.335	1840	1845	1853	rBV	58564	69581	18.62%	1.911%
78	12.543	1873	1879	1884	rBV	16618	21683	5.80%	0.596%
79	12.945	1941	1945	1951	rVB3	6241	8133	2.18%	0.223%
80	13.286	1996	2001	2006	rBV	30641	36930	9.88%	1.014%
81	13.591	2047	2051	2056	rVB	18783	23091	6.18%	0.634%
82	13.725	2069	2073	2077	rBV	16614	18183	4.87%	0.499%
83	13.780	2077	2082	2087	rVB	24806	31360	8.39%	0.861%
84	13.963	2107	2112	2117	rBV2	20024	24407	6.53%	0.670%




Sum of corrected areas: 3640941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032522\
Data File : VX027696.D
Acq On : 25 Mar 2022 12:31
Operator : JC/MD
Sample : VSTDIC005
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDIC005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

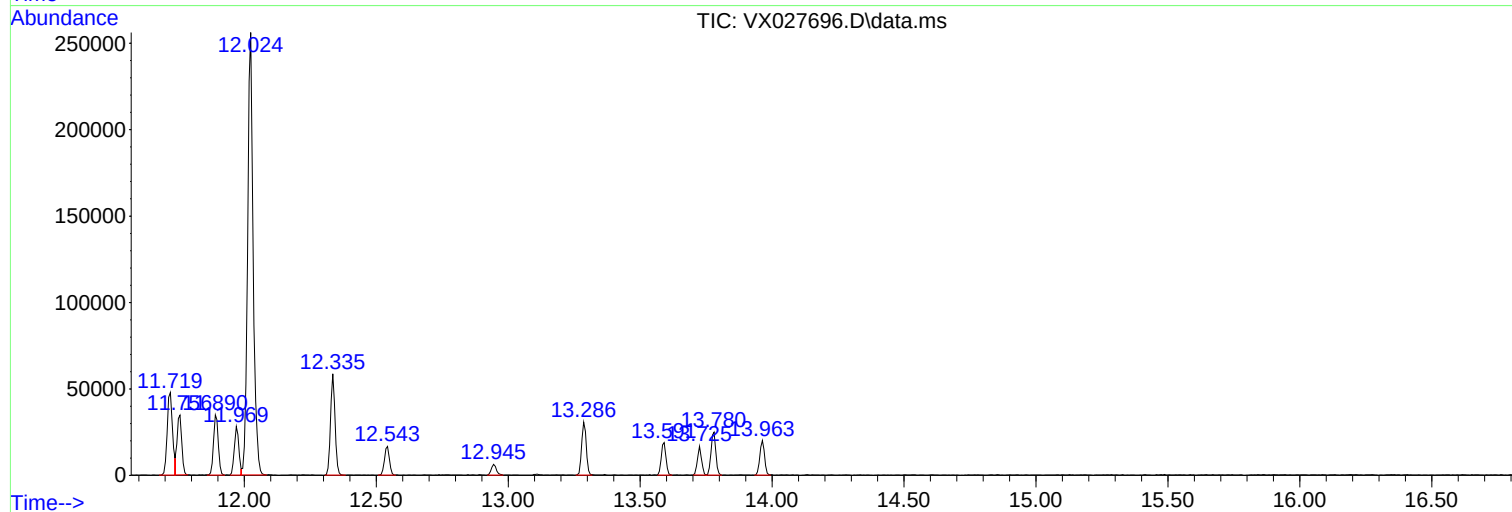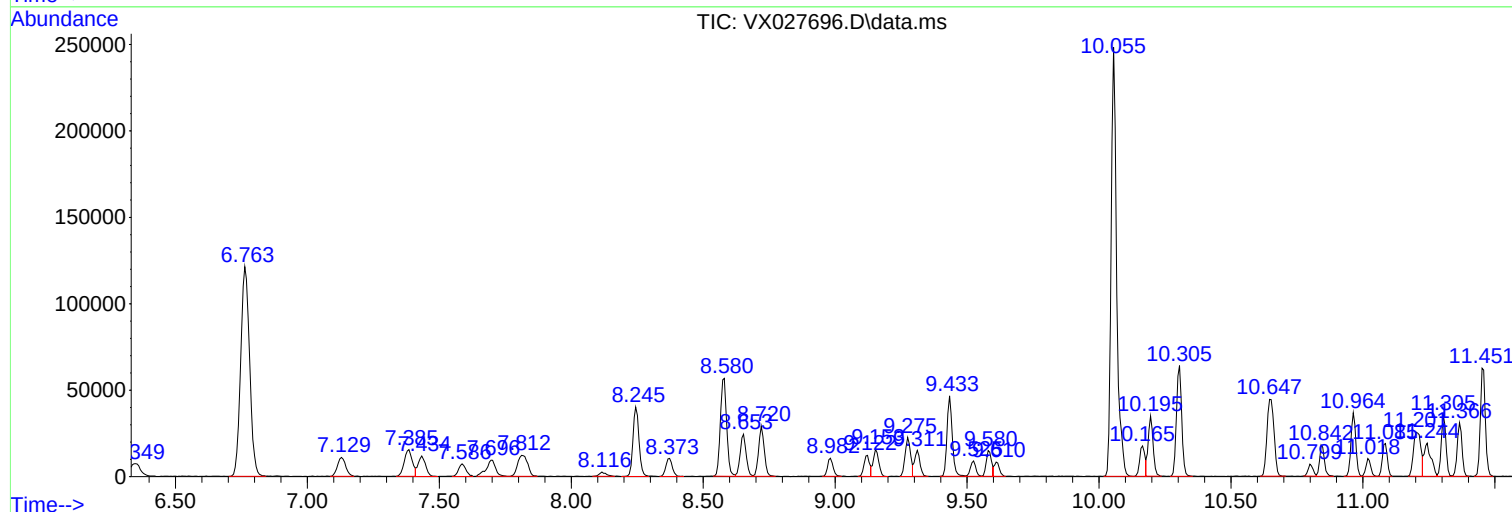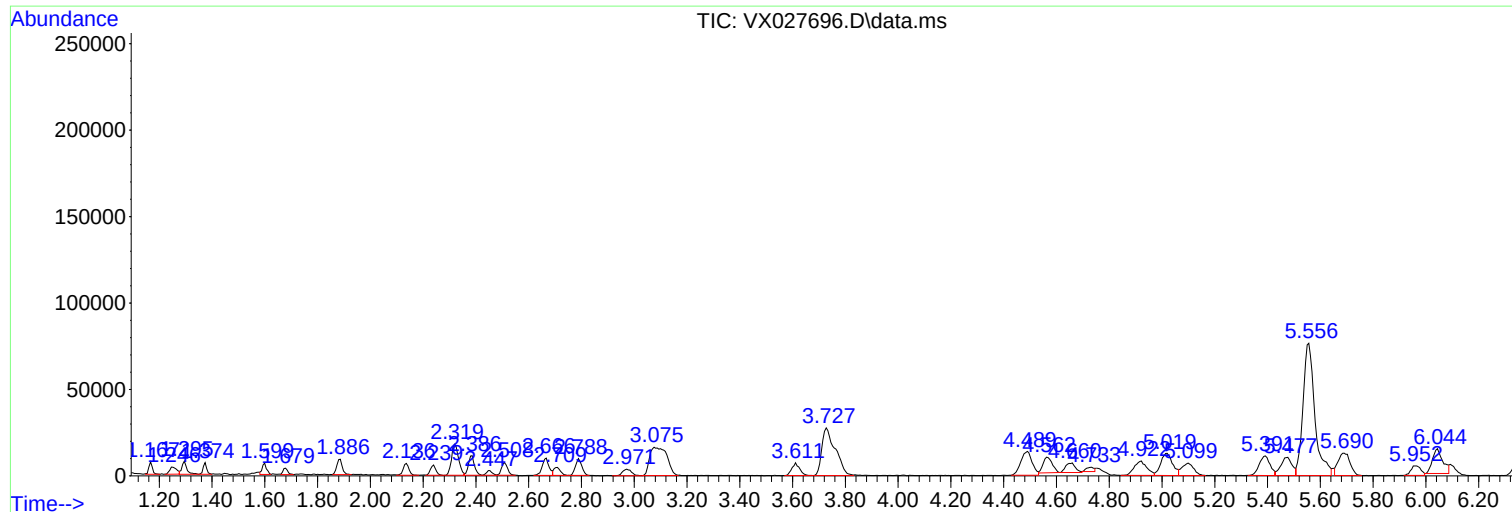

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032522\
Data File : VX027696.D
Acq On : 25 Mar 2022 12:31
Operator : JC/MD
Sample : VSTDICC005
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDICC005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032522\
Data File : VX027696.D
Acq On : 25 Mar 2022 12:31
Operator : JC/MD
Sample : VSTDICC005
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDICC005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------