

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032525\
 Data File : VX045449.D
 Acq On : 25 Mar 2025 18:41
 Operator : JC/MD
 Sample : Q1629-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RW09-MW01D3-20250320

Quant Time: Mar 26 01:43:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	71670	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	137481	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	129073	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	54362	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	60622	53.176	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	106.360%
35) Dibromofluoromethane	5.385	113	45171	49.136	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.280%
50) Toluene-d8	8.647	98	159922	47.985	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.960%
62) 4-Bromofluorobenzene	11.079	95	57139	51.738	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	103.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032525\
Data File : VX045449.D
Acq On : 25 Mar 2025 18:41
Operator : JC/MD
Sample : Q1629-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RW09-MW01D3-20250320

Quant Time: Mar 26 01:43:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




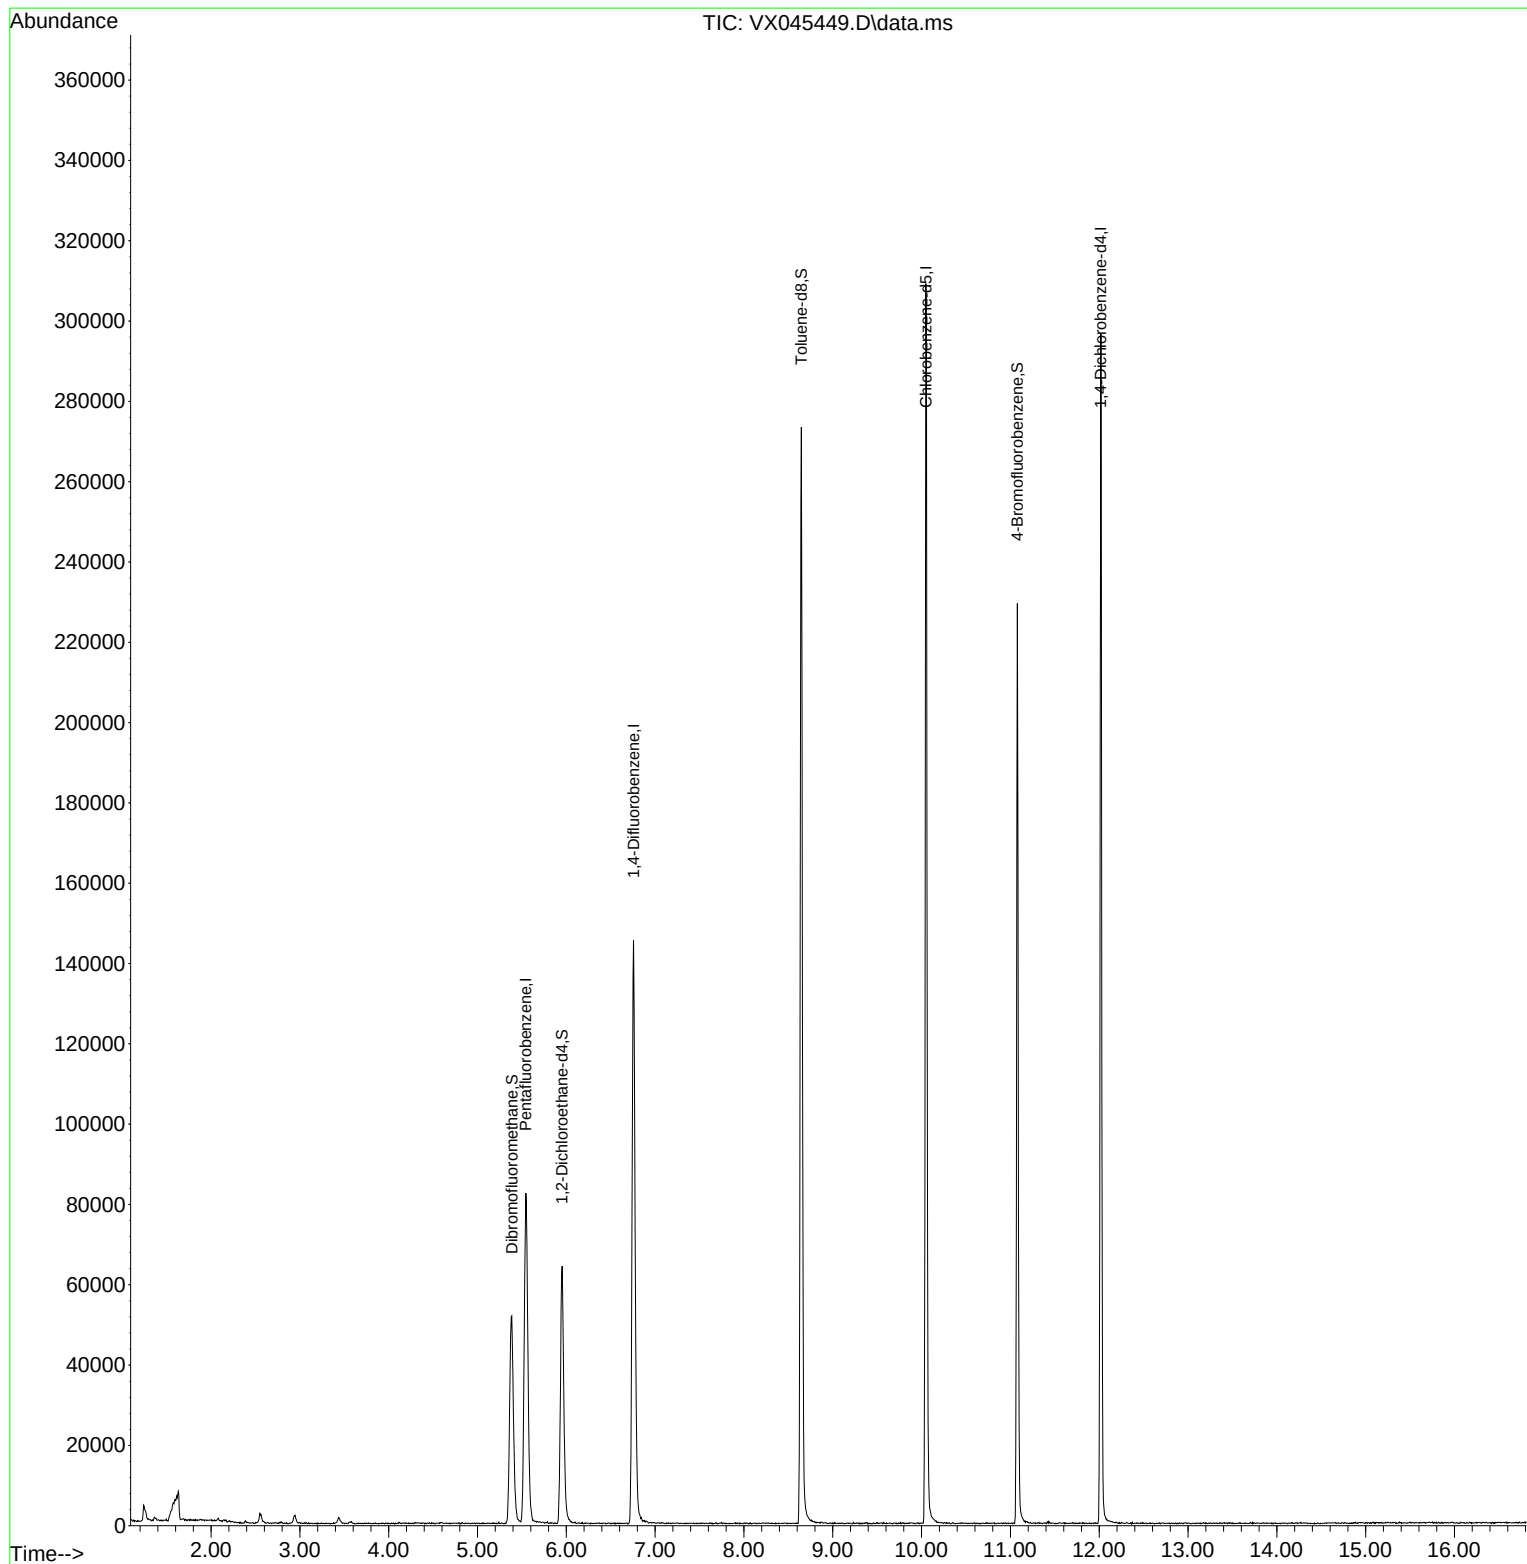


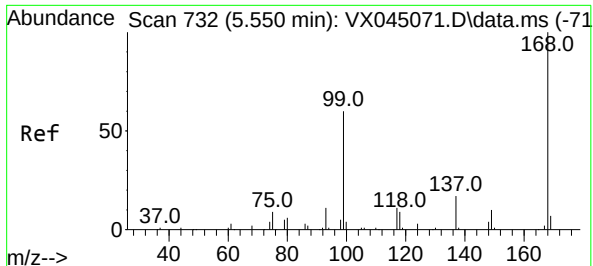

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.006 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41




Instrument :
MSVOA_X
ClientSampleId :
RW09-MW01D3-20250320


Tgt Ion:168 Resp: 71670
Ion Ratio Lower Upper
168 100
99 68.8 48.2 72.4

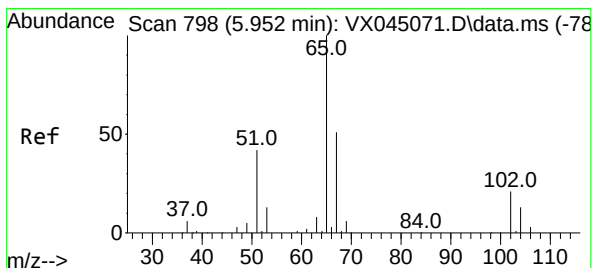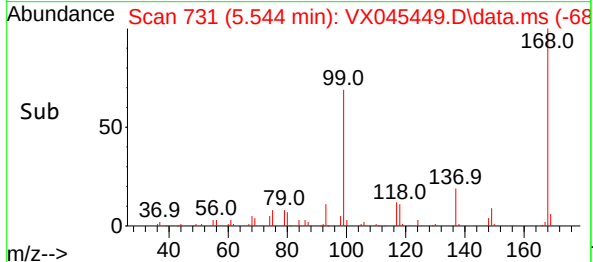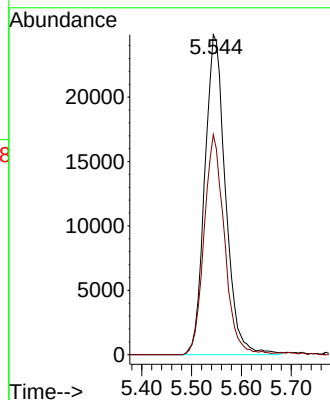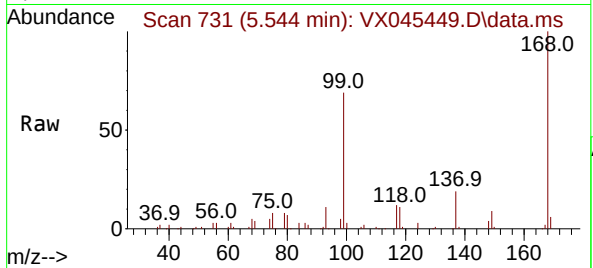

#33
1,2-Dichloroethane-d4
Concen: 53.176 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41

Tgt Ion: 65 Resp: 60622
Ion Ratio Lower Upper
65 100
67 50.7 0.0 106.2


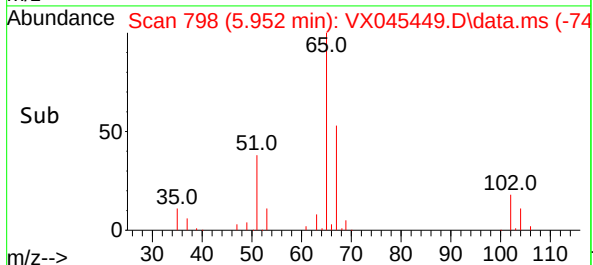
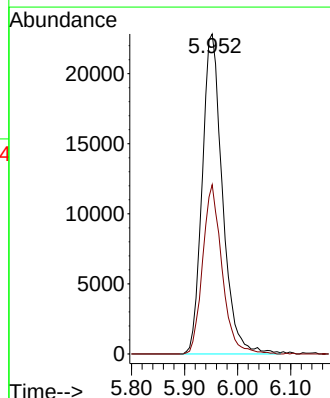
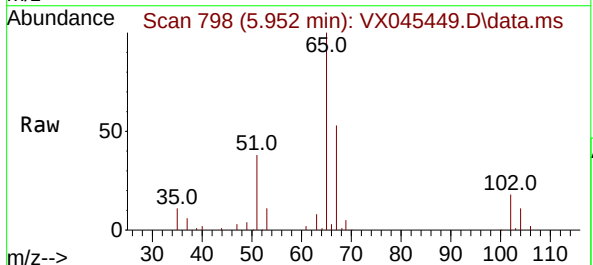


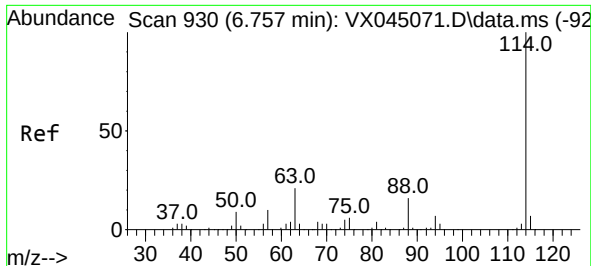

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41




Instrument :
MSVOA_X
ClientSampleId :
RW09-MW01D3-20250320


Tgt Ion:114 Resp: 137481
Ion Ratio Lower Upper
114 100
63 23.6 0.0 41.8
88 17.1 0.0 32.8

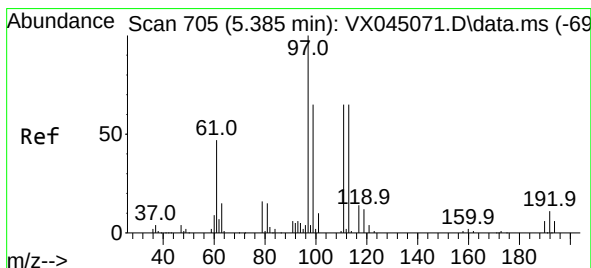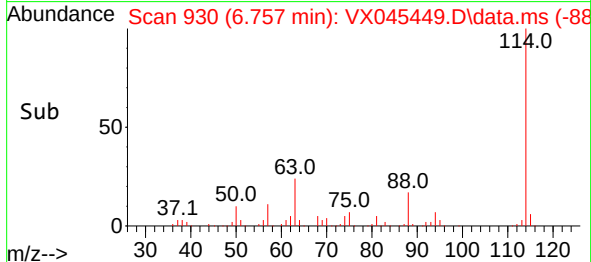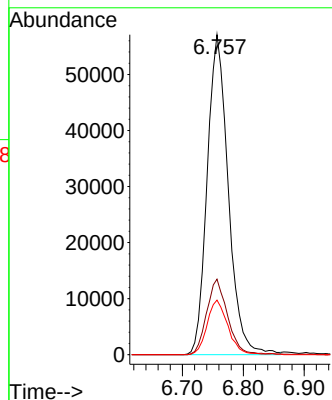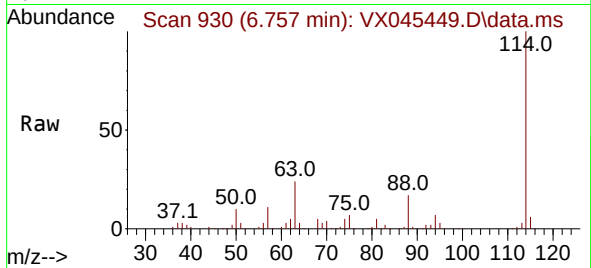

#35
Dibromofluoromethane
Concen: 49.136 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41

Tgt Ion:113 Resp: 45171
Ion Ratio Lower Upper
113 100
111 103.8 81.8 122.6
192 16.7 14.3 21.5


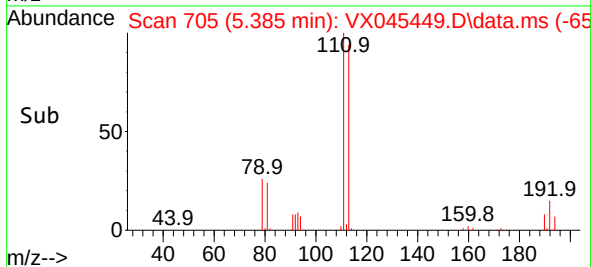
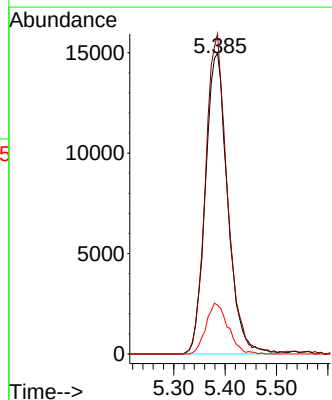
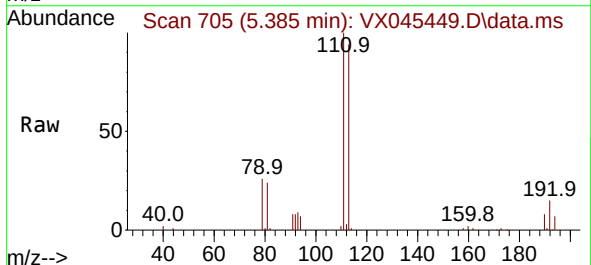


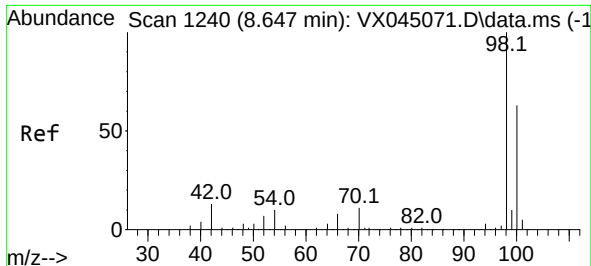

#50
Toluene-d8
Concen: 47.985 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41




Instrument :
MSVOA_X
ClientSampleId :
RW09-MW01D3-20250320


Tgt Ion: 98 Resp: 159922
Ion Ratio Lower Upper
98 100
100 64.4 52.0 78.0

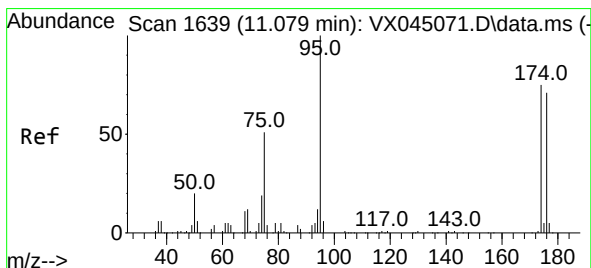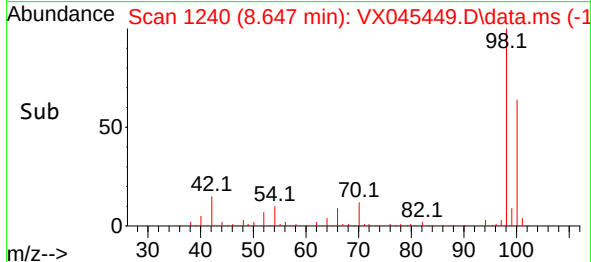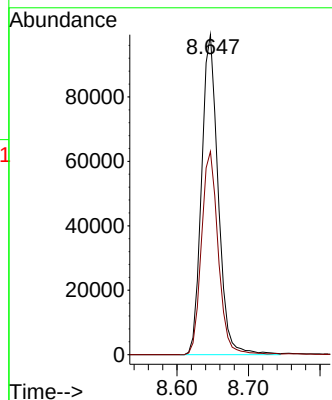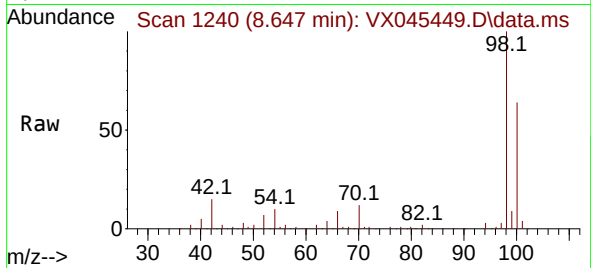

#62
4-Bromofluorobenzene
Concen: 51.738 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41

Tgt Ion: 95 Resp: 57139
Ion Ratio Lower Upper
95 100
174 69.8 0.0 148.2
176 69.2 0.0 141.4


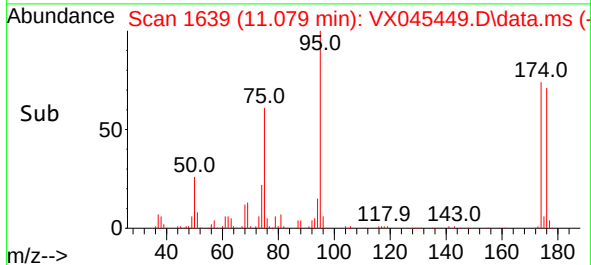
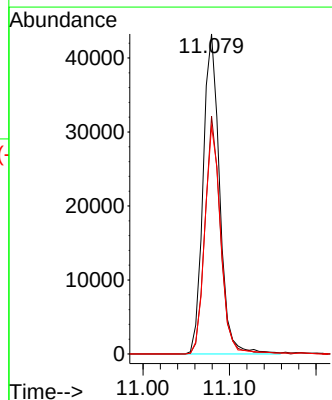
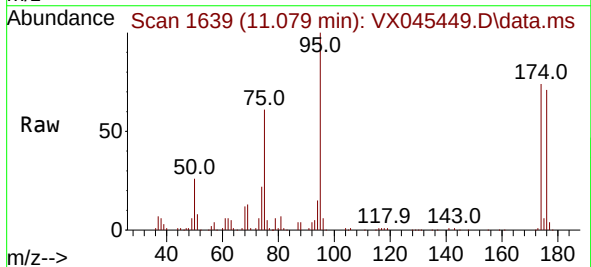


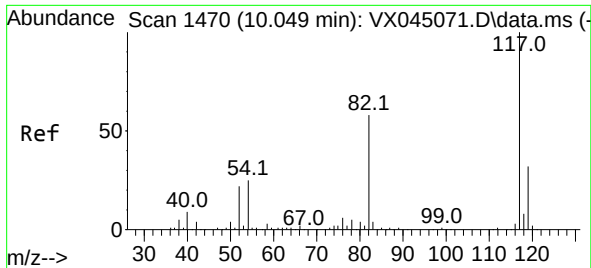

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41

Instrument :
MSVOA_X
ClientSampleId :
RW09-MW01D3-20250320

Tgt Ion:117 Resp: 129073
Ion Ratio Lower Upper
117 100
82 60.4 46.3 69.5
119 33.0 25.7 38.5

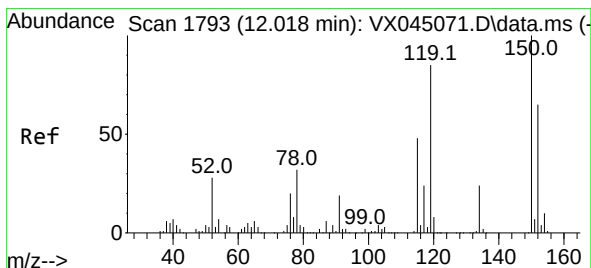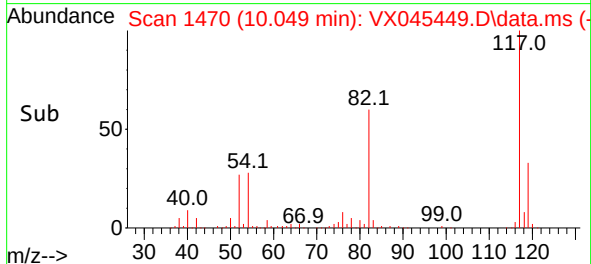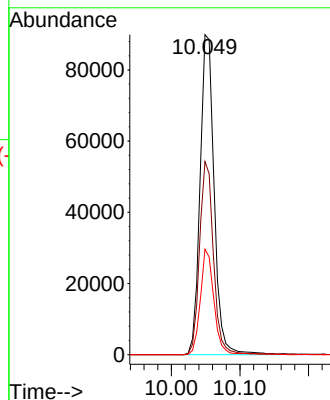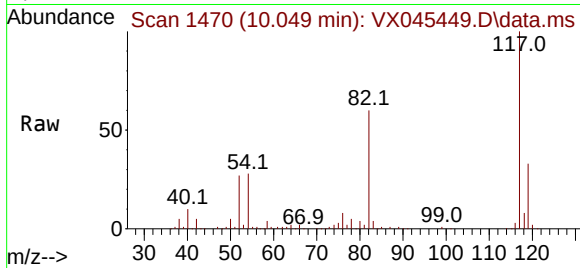

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045449.D
Acq: 25 Mar 2025 18:41

Tgt Ion:152 Resp: 54362
Ion Ratio Lower Upper
152 100
115 62.0 44.2 132.6
150 156.9 0.0 349.0

