

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032525\
Data File : VX045432.D
Acq On : 25 Mar 2025 11:59
Operator : JC/MD
Sample : VX0325MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0325MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M

Title : SW846 8260

Signal : TIC: VX045432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	69	80	81	rBV5	4886	12670	2.70%	0.520%
2	5.379	691	704	721	rBV2	53296	161809	34.44%	6.639%
3	5.544	721	731	748	rVB2	76726	222923	47.45%	9.146%
4	5.952	788	798	812	rBV	61504	168852	35.94%	6.928%
5	6.757	921	930	944	rBV	136943	331835	70.63%	13.615%
6	8.647	1233	1240	1257	rBV	289459	469836	100.00%	19.277%
7	10.049	1465	1470	1483	rBV	303542	418213	89.01%	17.159%
8	11.079	1634	1639	1652	rBV	231482	300425	63.94%	12.326%
9	12.018	1788	1793	1804	rBV	270060	345213	73.48%	14.164%
10	13.780	2077	2082	2087	rBV	3815	5482	1.17%	0.225%




Sum of corrected areas: 2437258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032525\
Data File : VX045432.D
Acq On : 25 Mar 2025 11:59
Operator : JC/MD
Sample : VX0325MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0325MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

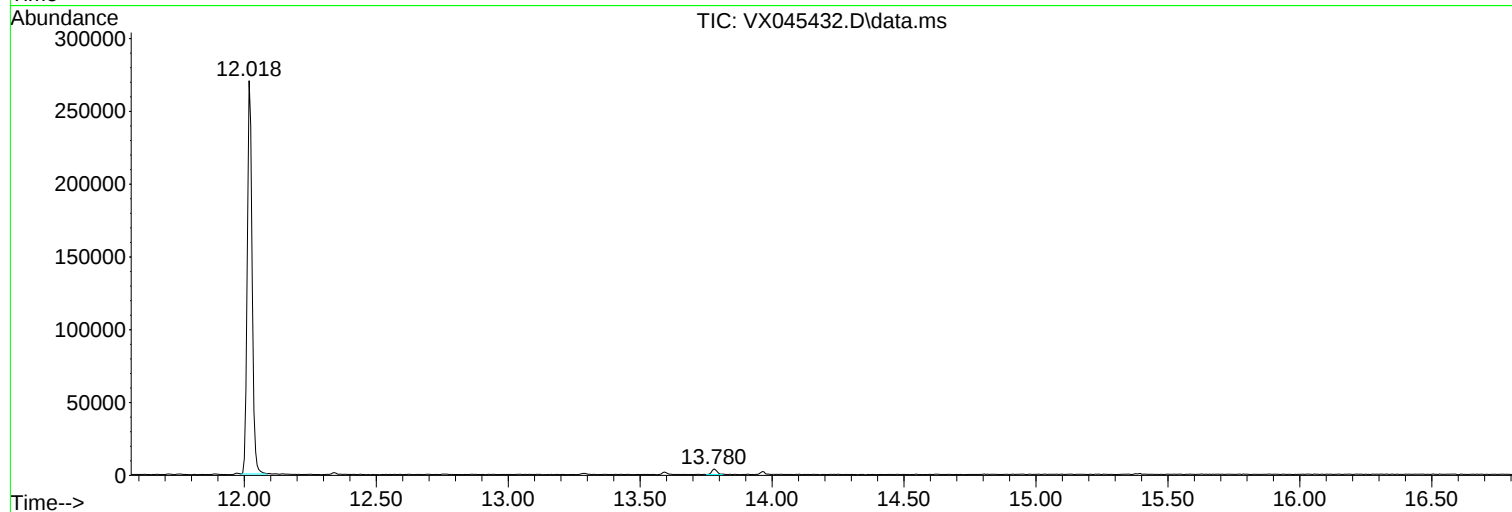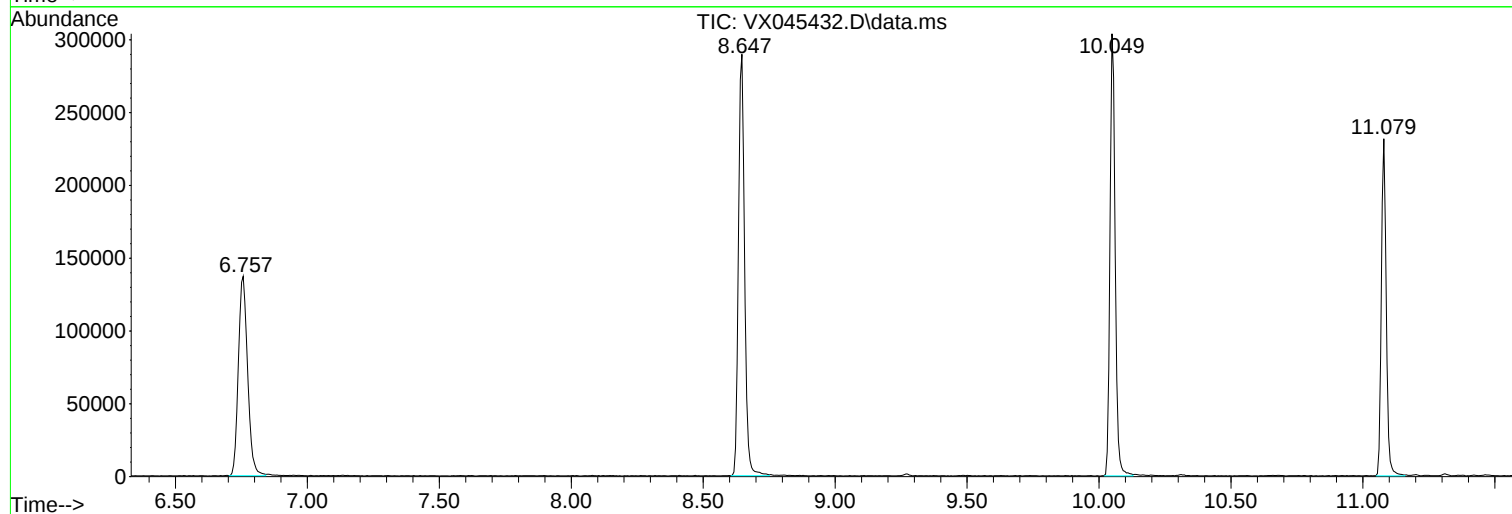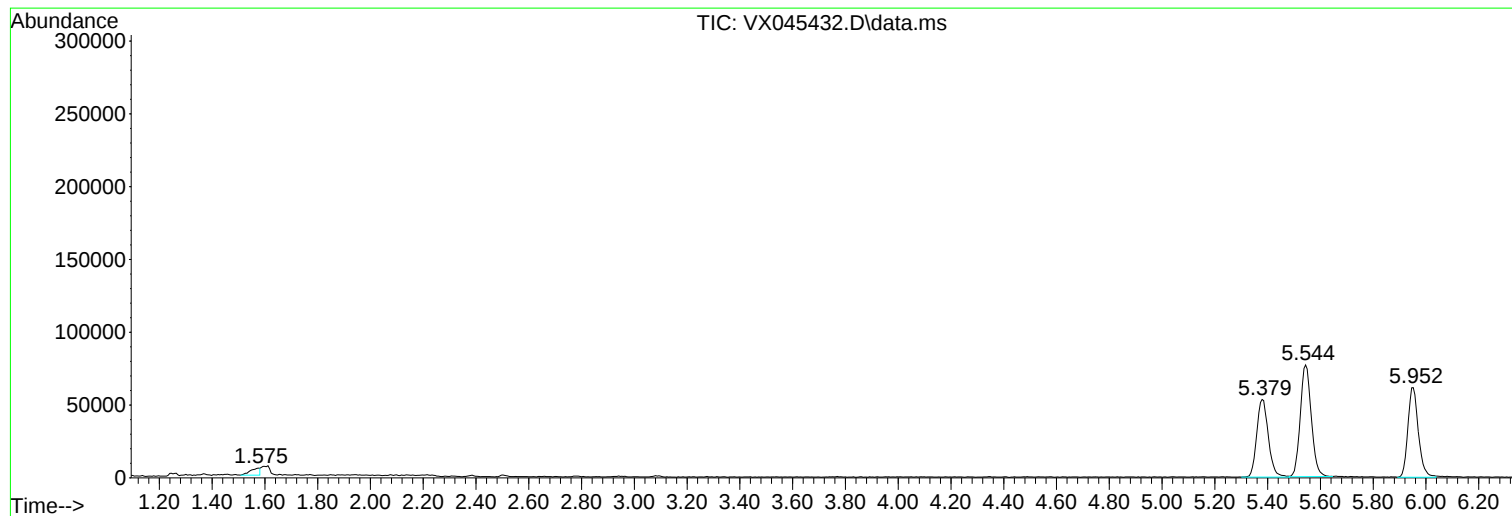

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032525\
Data File : VX045432.D
Acq On : 25 Mar 2025 11:59
Operator : JC/MD
Sample : VX0325MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0325MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032525\
Data File : VX045432.D
Acq On : 25 Mar 2025 11:59
Operator : JC/MD
Sample : VX0325MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0325MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc