

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032620\
 Data File : VX015359.D
 Acq On : 26 Mar 2020 15:29
 Operator : JC/SP
 Sample : L1981-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-1-1-4-COMP

Quant Time: Mar 31 04:45:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X032520W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu Mar 26 02:31:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	4.98	128	196774	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.84	114	1105446	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.10	117	983120	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.04	65	469164	30.51	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	101.70%
60) 4-Bromofluorobenzene	11.12	95	507947	30.19	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	100.63%
63) Toluene-d8	8.70	98	1287068	30.81	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	102.70%

Target Compounds


					Ovalue	
8) Diethyl Ether	2.17	74	7046	1.149	ug/l	71
15) Acetone	2.42	58	11660	6.832	ug/l	92
23) tert-Butyl Alcohol	3.01	59	39147	11.857	ug/l #	98
64) Chlorobenzene	10.12	112	114741	3.584	ug/l	97
83) 1,3-Dichlorobenzene	12.01	146	8851	0.329	ug/l	90
89) 1,2,4-Trichlorobenzene	13.63	180	18624	0.880	ug/l	99
90) Hexachlorobutadiene	13.76	225	7120	0.639	ug/l	96
91) Naphthalene	13.82	128	39720	0.648	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032620\
Data File : VX015359.D
Acq On : 26 Mar 2020 15:29
Operator : JC/SP
Sample : L1981-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-1-1-4-COMP

Quant Time: Mar 31 04:45:11 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X032520W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu Mar 26 02:31:53 2020
Response via : Initial Calibration

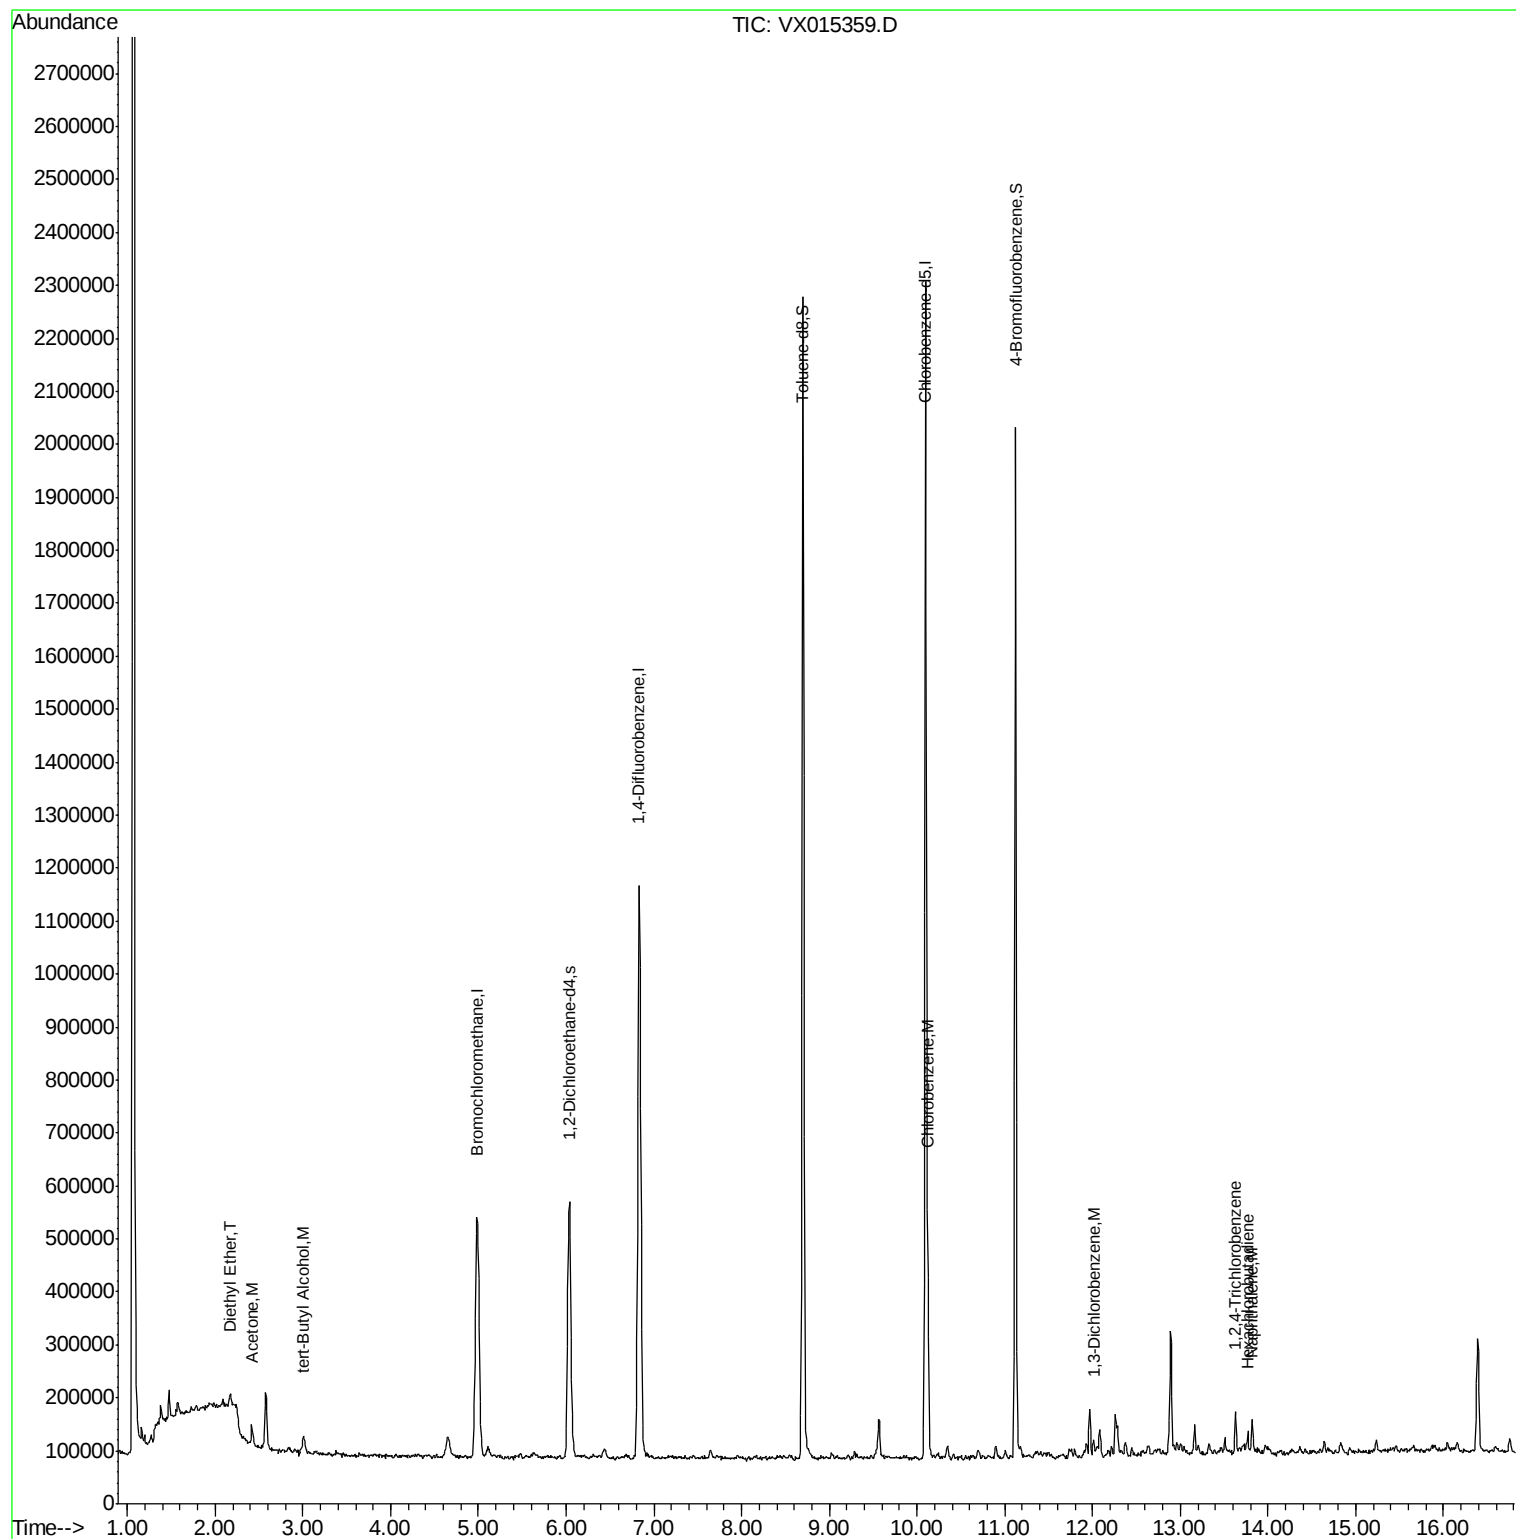



#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 4.98 min Scan# 672

Delta R.T. -0.01 min

Lab File: VX015359.D

Acq: 26 Mar 2020 15:29

Instrument :

MSVOA_X

ClientSampleId :

MH-1-1-4-COMP


Tot Ion:128 Resp: 196774

Ion Ratio Lower Upper

128 100

49 173.8 0.0 428.0

130 129.7 0.0 324.5

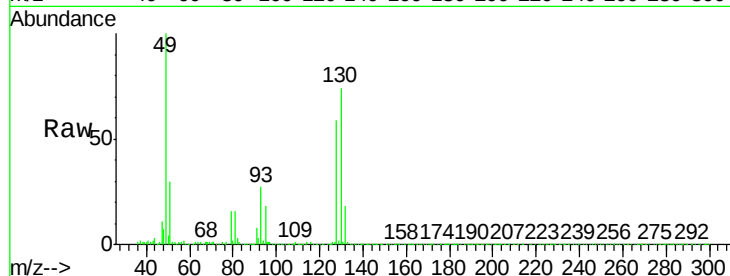

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

150000

100000

50000

0



4.98

4.90

5.00

5.10

Time-->



#8

Diethyl Ether

Concen: 1.149 ug/l

RT: 2.17 min Scan# 210

Delta R.T. -0.00 min

Lab File: VX015359.D


Acq: 26 Mar 2020 15:29

Tgt Ion: 74 Resp: 7046

Ion Ratio Lower Upper

74 100

45 139.5 21.8 196.4



Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

8000

6000

4000

2000


0


2.17

2.15

2.20

Time-->







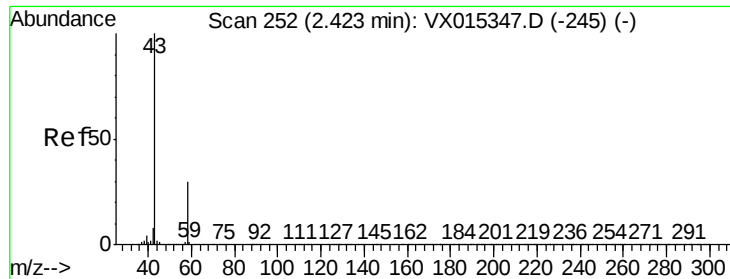

#15
Acetone
Concen: 6.832 ug/l
RT: 2.42 min Scan# 251
Delta R.T. -0.01 min
Lab File: VX015359.D
Acq: 26 Mar 2020 15:29




Instrument :
MSVOA_X
ClientSampleId :
MH-1-1-4-COMP


Tot Ion: 58 Resp: 11660
Ion Ratio Lower Upper
58 100
43 352.5 267.8 401.8

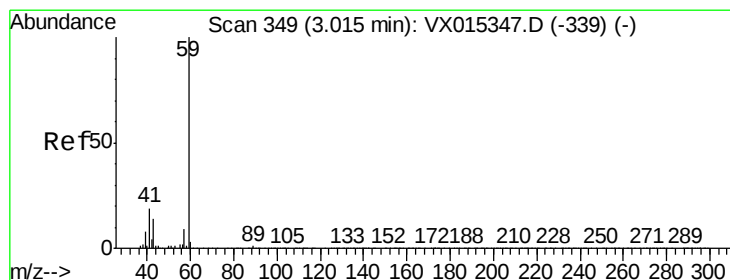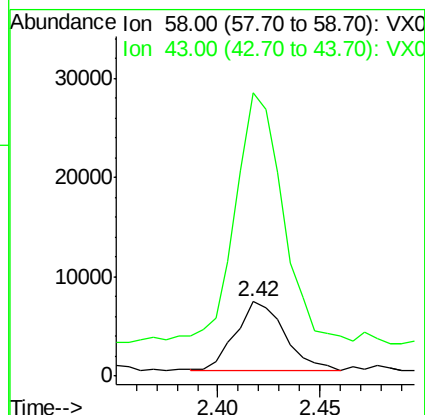

#23
tert-Butyl Alcohol
Concen: 11.857 ug/l
RT: 3.01 min Scan# 348
Delta R.T. -0.01 min
Lab File: VX015359.D
Acq: 26 Mar 2020 15:29

Tgt Ion: 59 Resp: 39147
Ion Ratio Lower Upper
59 100
52 2.3 0.2 0.2#



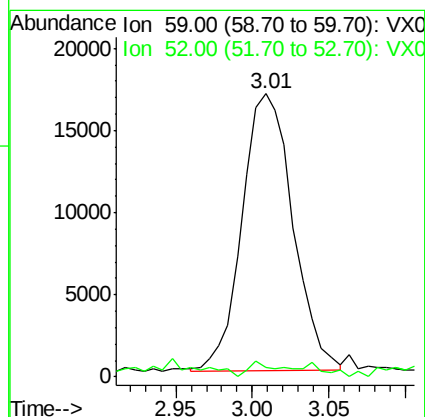





#27
 1,2-Dichloroethane-d4
 Concen: 30.512 ug/l
 RT: 6.04 min Scan# 845
 Delta R.T. 0.01 min
 Lab File: VX015359.D
 Acq: 26 Mar 2020 15:29




Instrument :
 MSVOA_X
 ClientSampleId :
 MH-1-1-4-COMP


Tot Ion: 65 Resp: 469164
 Ion Ratio Lower Upper
 65 100
 67 50.0 40.9 61.3

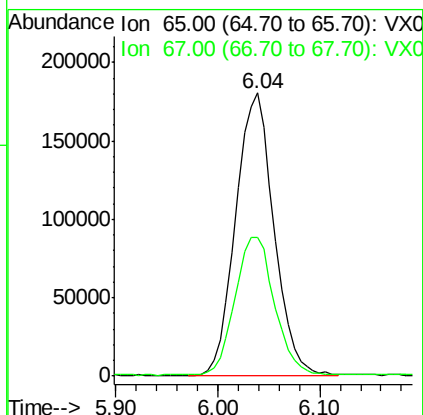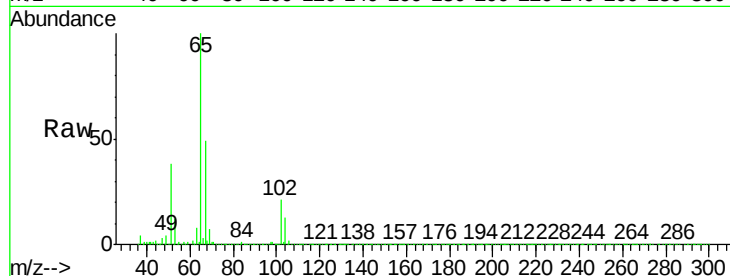

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.84 min Scan# 976
 Delta R.T. -0.00 min
 Lab File: VX015359.D
 Acq: 26 Mar 2020 15:29

Tgt Ion: 114 Resp: 1105446
 Ion Ratio Lower Upper
 114 100
 63 22.1 17.4 26.2
 88 16.4 12.9 19.3



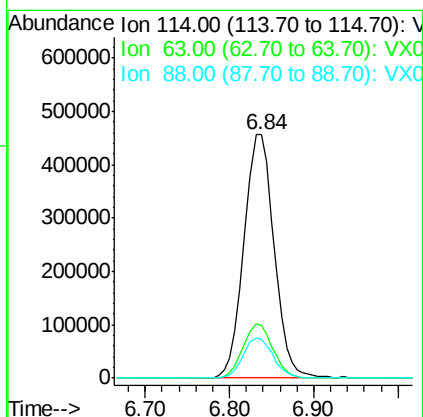



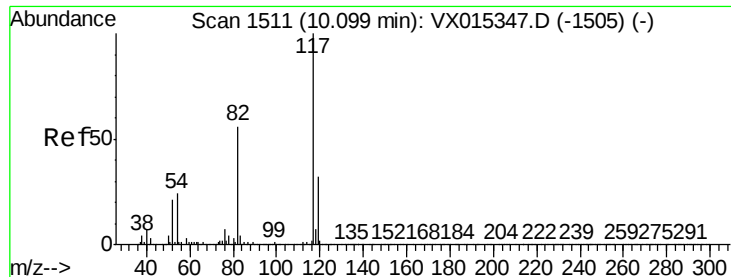

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.10 min Scan# 1511
Delta R.T. -0.00 min
Lab File: VX015359.D
Acq: 26 Mar 2020 15:29




Instrument :
MSVOA_X
ClientSampleId :
MH-1-1-4-COMP


Tot Ion	Ratio	Lower	Upper
117	100		
82	56.8	45.0	67.6
119	31.9	25.5	38.3

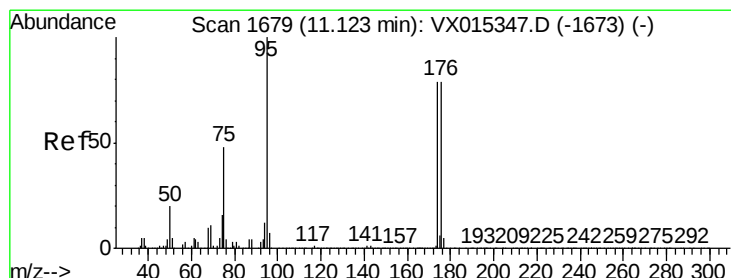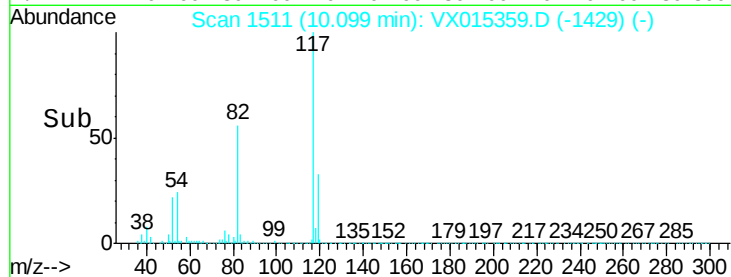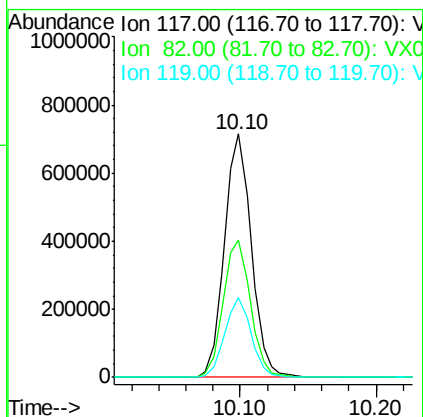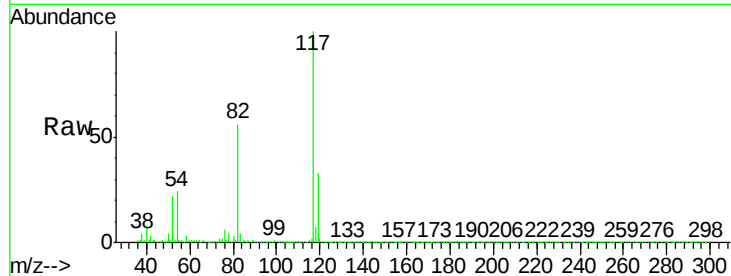

#60
4-Bromofluorobenzene
Concen: 30.190 ug/l
RT: 11.12 min Scan# 1679
Delta R.T. -0.00 min
Lab File: VX015359.D
Acq: 26 Mar 2020 15:29

Tgt Ion	Ratio	Lower	Upper
95	100		
174	82.8	66.4	99.6
176	80.6	64.1	96.1

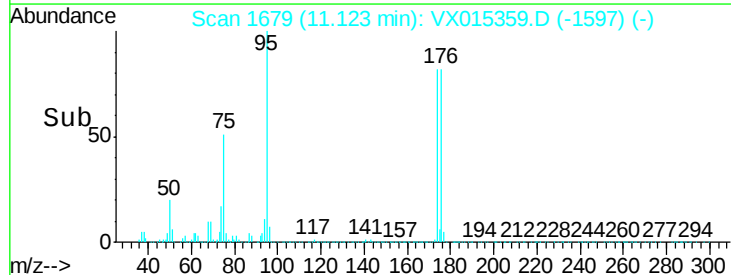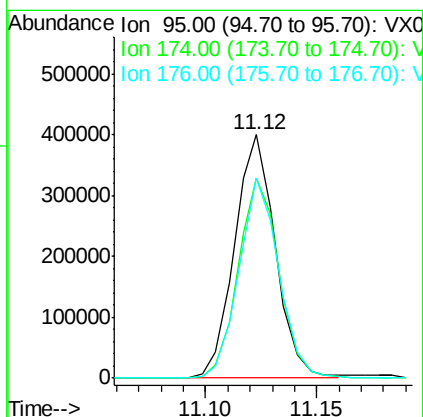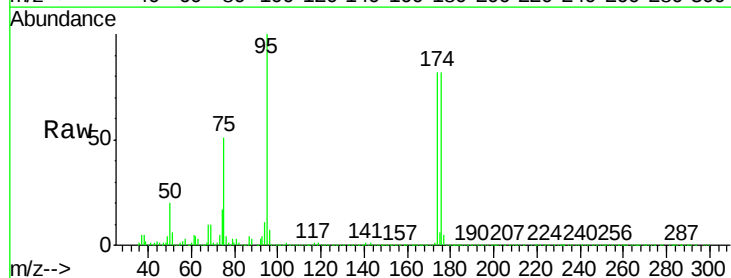



#63

Toluene-d8

Concen: 30.814 ug/l

RT: 8.70 min Scan# 1281

Delta R.T. -0.00 min

Lab File: VX015359.D

Acq: 26 Mar 2020 15:29

Instrument :

MSVOA_X

ClientSampleId :


MH-1-1-4-COMP

Tot Ion: 98 Resp: 1287068

Ion Ratio Lower Upper




98 100

100 66.4 52.2 78.2



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

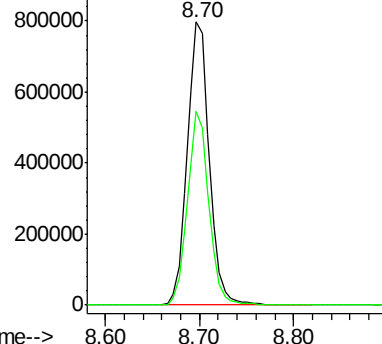

#64

Chlorobenzene

Concen: 3.584 ug/l

RT: 10.12 min Scan# 1515

Delta R.T. -0.00 min

Lab File: VX015359.D


Acq: 26 Mar 2020 15:29

Tgt Ion: 112 Resp: 114741

Ion Ratio Lower Upper



112 100


114 30.8 25.8 38.8



Abundance Ion 112.00 (111.70 to 112.70): V

Ion 114.00 (113.70 to 114.70): V




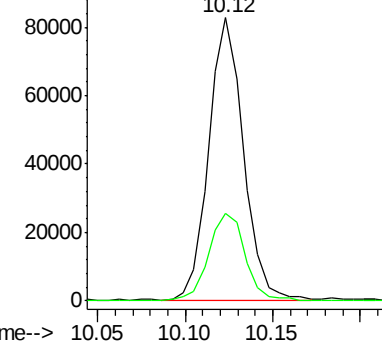


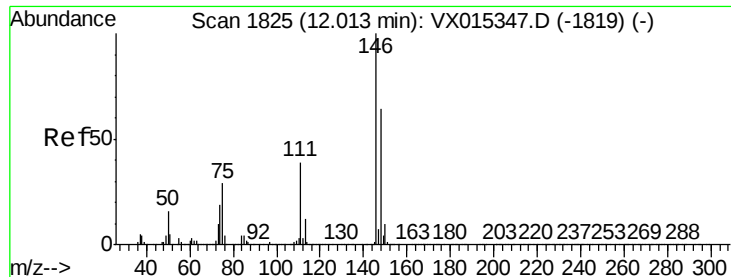

#83
 1,3-Dichlorobenzene
 Concen: 0.329 ug/l
 RT: 12.01 min Scan# 1825
 Delta R.T. -0.00 min
 Lab File: VX015359.D
 Acq: 26 Mar 2020 15:29




Instrument :
 MSVOA_X
 ClientSampleId :
 MH-1-1-4-COMP


Tot Ion:146 Resp: 8851
 Ion Ratio Lower Upper
 146 100
 111 44.2 20.1 60.2
 148 72.8 31.4 94.2

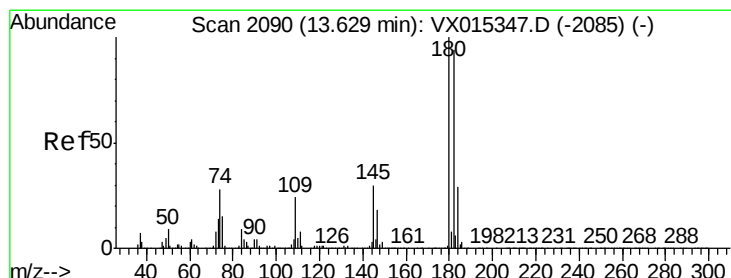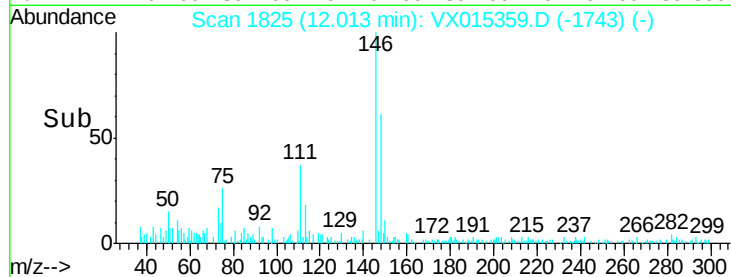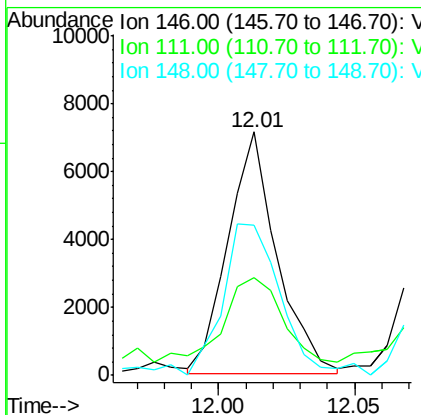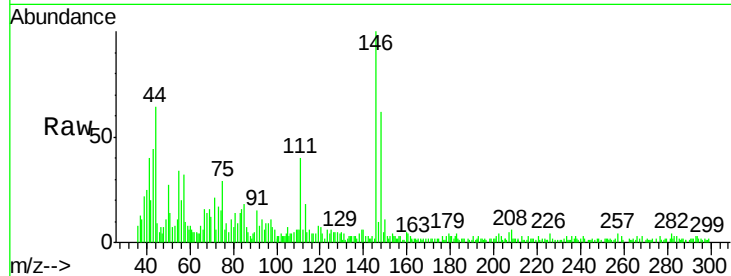

#89
 1,2,4-Trichlorobenzene
 Concen: 0.880 ug/l
 RT: 13.63 min Scan# 2090
 Delta R.T. -0.00 min
 Lab File: VX015359.D
 Acq: 26 Mar 2020 15:29

Tgt Ion:180 Resp: 18624
 Ion Ratio Lower Upper
 180 100
 182 96.1 76.9 115.3
 145 33.1 24.3 36.5

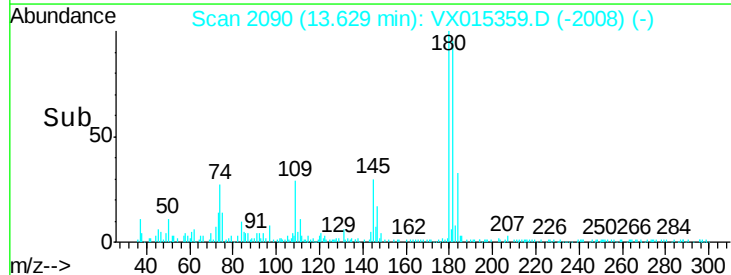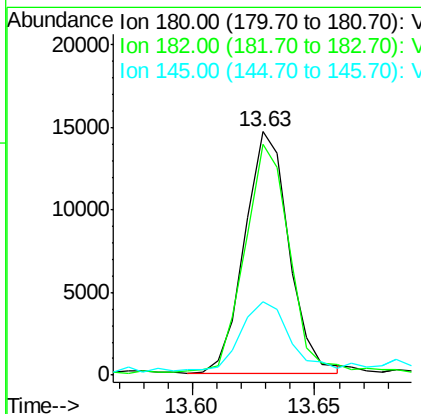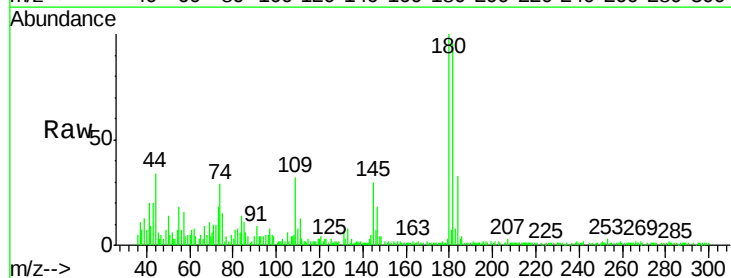



#90

Hexachlorobutadiene

Concen: 0.639 ug/l

RT: 13.76 min Scan# 2112

Delta R.T. -0.01 min

Lab File: VX015359.D

Acq: 26 Mar 2020 15:29

Instrument :

MSVOA_X

ClientSampleId :

MH-1-1-4-COMP


Tot Ion:225 Resp: 7120

Ion Ratio Lower Upper

225 100

223 63.1 0.0 127.0




227 68.6 0.0 126.8



Abundance Ion 225.00 (224.70 to 225.70): V

Ion 223.00 (222.70 to 223.70): V

Ion 227.00 (226.70 to 227.70): V

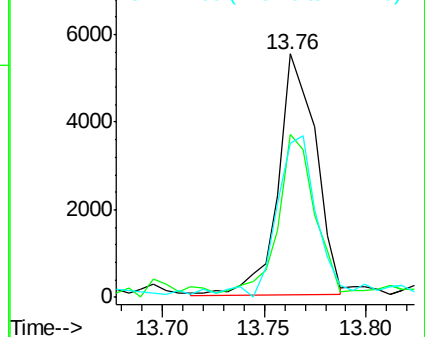

#91

Naphthalene

Concen: 0.648 ug/l

RT: 13.82 min Scan# 2121

Delta R.T. -0.00 min

Lab File: VX015359.D

Acq: 26 Mar 2020 15:29


Tgt Ion:128 Resp: 39720

Ion Ratio Lower Upper

128 100

127 15.9 10.3 15.5#

129 10.4 8.9 13.3



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

