


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032620\
 Data File : VX015352.D
 Acq On : 26 Mar 2020 09:57
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X032520W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Mar 26 02:31:53 2020

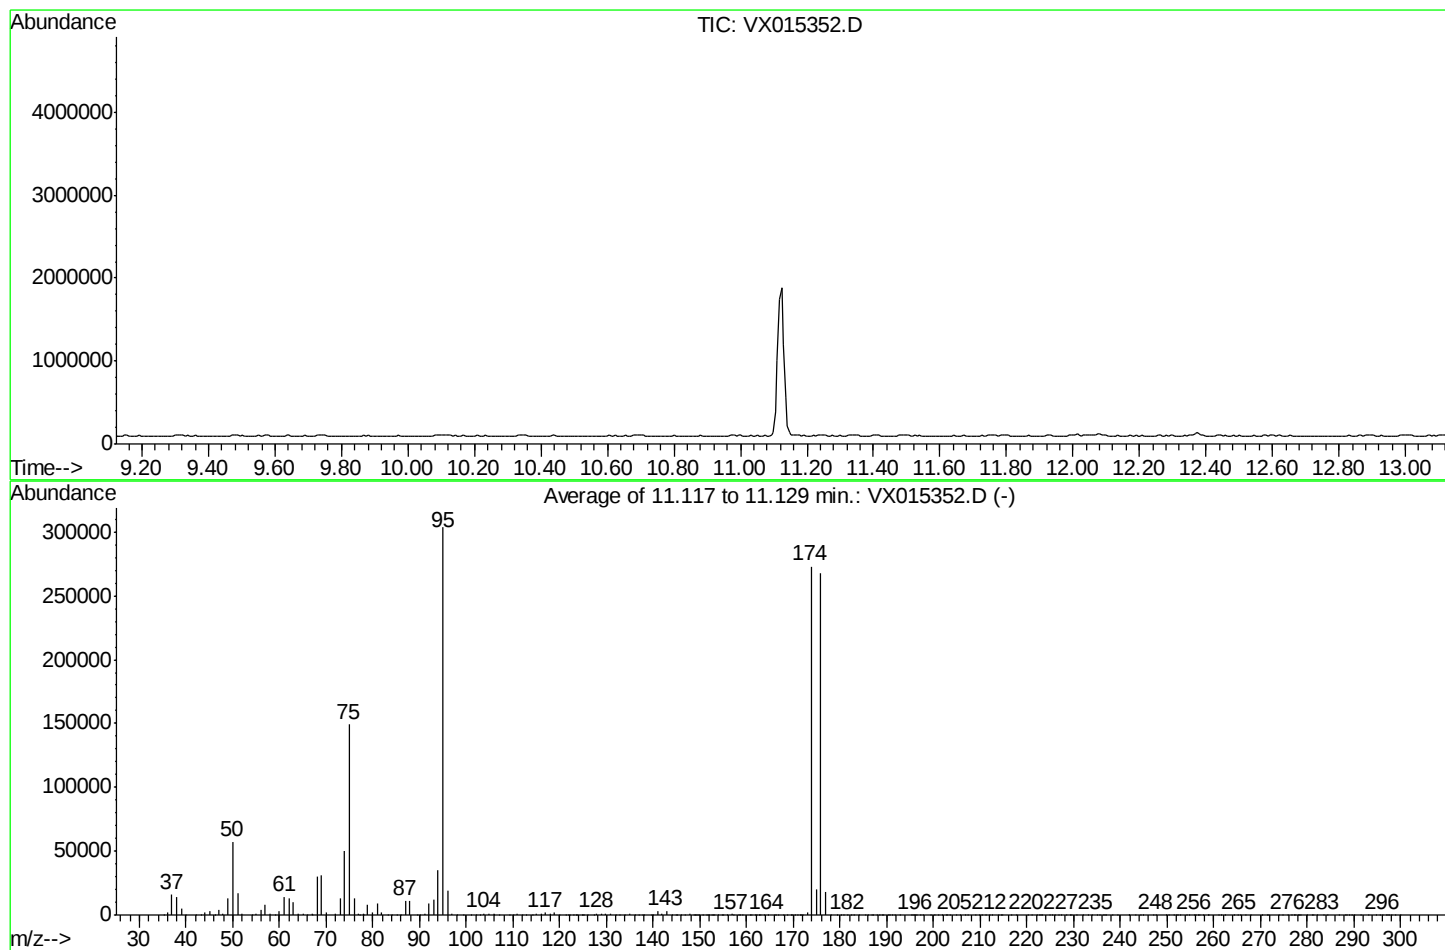

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	57480	PASS
75	95	30	60	49.2	149265	PASS
95	95	100	100	100.0	303636	PASS
96	95	5	9	6.3	19270	PASS
173	174	0.00	2	0.7	1850	PASS
174	95	50	100	90.0	273216	PASS
175	174	5	9	7.4	20188	PASS
176	174	95	101	98.0	267626	PASS
177	176	5	9	6.8	18145	PASS