

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032621\
 Data File : VX021553.D
 Acq On : 27 Mar 2021 01:09
 Operator : JC/MD
 Sample : M1787-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE-126D1-20210319

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	78	87	91	rVB6	3235	7000	1.71%	0.287%
2	5.464	733	744	760	rBV2	50036	142198	34.84%	5.827%
3	5.629	760	772	786	rVB	74119	205018	50.23%	8.402%
4	6.029	829	840	852	rBV	55678	144395	35.37%	5.918%
5	6.829	965	976	990	rBV	125620	293466	71.89%	12.027%
6	7.188	1027	1037	1048	rBV	94915	200009	49.00%	8.197%
7	8.694	1286	1293	1305	rBV	260972	408196	100.00%	16.728%
8	9.318	1394	1399	1403	rVB2	5574	7910	1.94%	0.324%
9	10.094	1525	1531	1547	rVB	286862	387865	95.02%	15.895%
10	11.118	1700	1705	1716	rVB	224861	298031	73.01%	12.214%
11	12.059	1860	1865	1871	rBV	277638	346044	84.77%	14.181%




Sum of corrected areas: 2440132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032621\
Data File : VX021553.D
Acq On : 27 Mar 2021 01:09
Operator : JC/MD
Sample : M1787-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-126D1-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

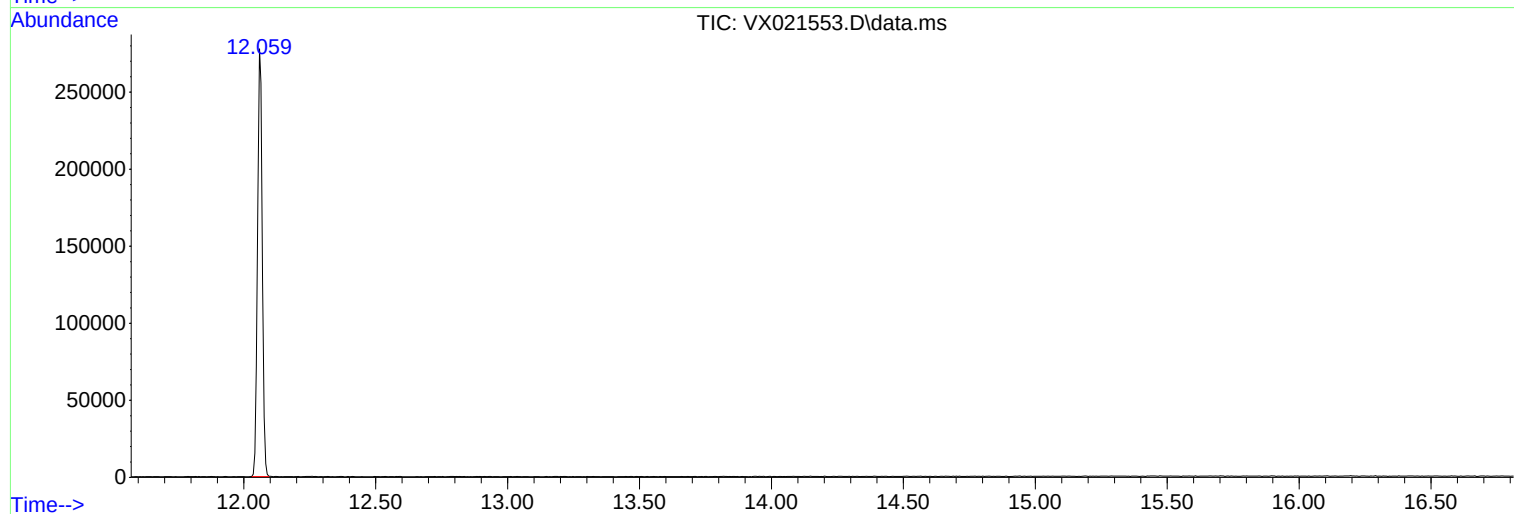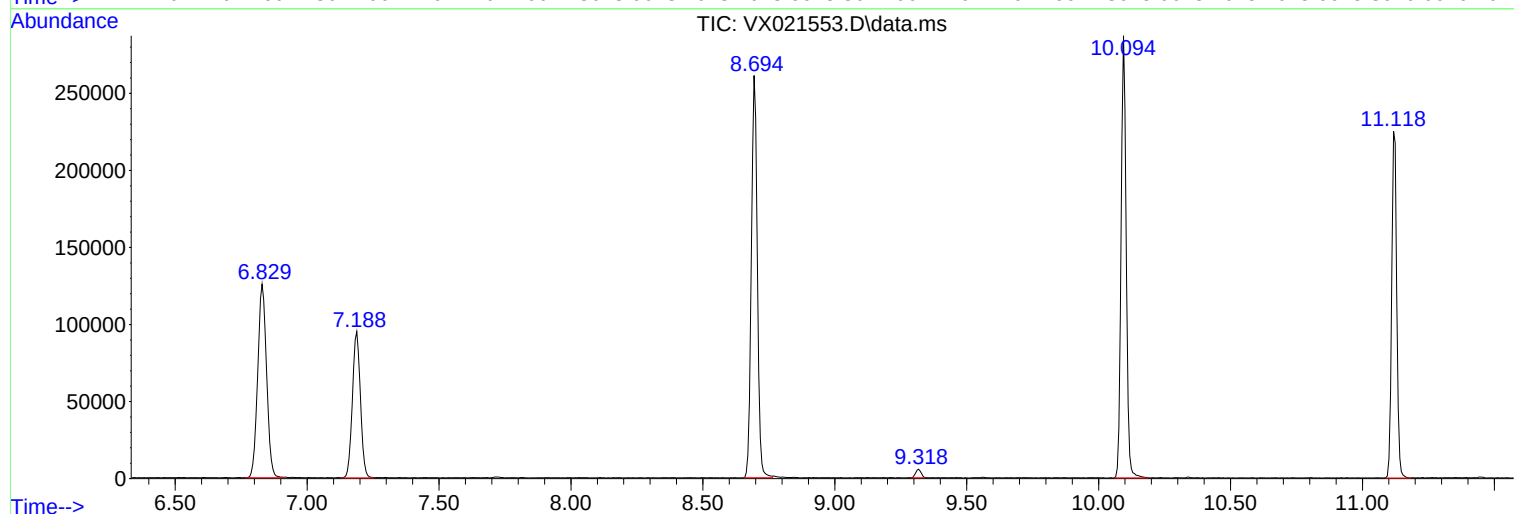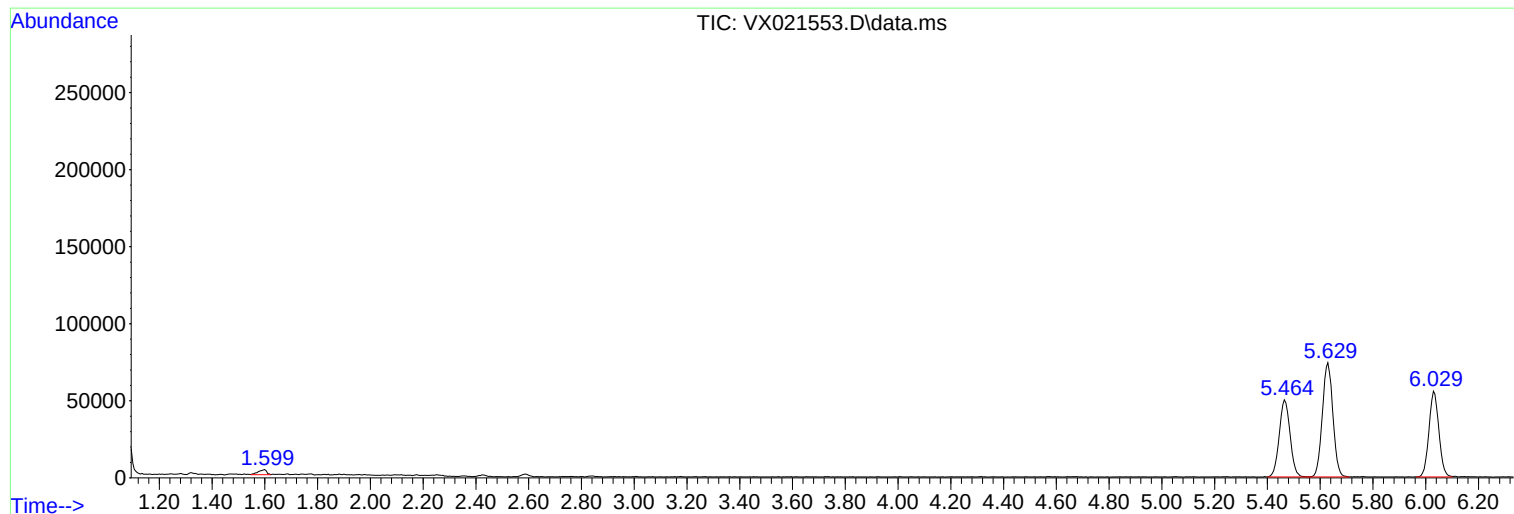

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032621\
Data File : VX021553.D
Acq On : 27 Mar 2021 01:09
Operator : JC/MD
Sample : M1787-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-126D1-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032621\
Data File : VX021553.D
Acq On : 27 Mar 2021 01:09
Operator : JC/MD
Sample : M1787-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE-126D1-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------