

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032621\  
 Data File : VX021559.D  
 Acq On : 27 Mar 2021 03:30  
 Operator : JC/MD  
 Sample : M1787-22  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 40 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW202D-20210320

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021559.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.593       | 76            | 86          | 91           | rBV6     | 3219           | 6573          | 1.73%           | 0.276%        |
| 2         | 1.917       | 137           | 141         | 145          | rBV      | 3365           | 4833          | 1.27%           | 0.203%        |
| 3         | 2.587       | 249           | 255         | 266          | rBV      | 3117           | 6629          | 1.74%           | 0.278%        |
| 4         | 3.670       | 427           | 439         | 449          | rBV2     | 5268           | 12568         | 3.30%           | 0.527%        |
| 5         | 4.564       | 582           | 591         | 601          | rBV3     | 9115           | 25672         | 6.74%           | 1.077%        |
| 6         | 5.464       | 732           | 744         | 757          | rBV2     | 47960          | 134340        | 35.28%          | 5.637%        |
| 7         | 5.629       | 761           | 772         | 782          | rBV2     | 66820          | 187797        | 49.32%          | 7.880%        |
| 8         | 6.029       | 830           | 840         | 853          | rBV      | 51737          | 136027        | 35.72%          | 5.708%        |
| 9         | 6.158       | 856           | 862         | 870          | rVB4     | 2041           | 4890          | 1.28%           | 0.205%        |
| 10        | 6.829       | 966           | 976         | 989          | rBV2     | 115001         | 274316        | 72.04%          | 11.510%       |
| 11        | 7.188       | 1027          | 1037        | 1049         | rBV      | 79291          | 168091        | 44.14%          | 7.053%        |
| 12        | 8.694       | 1285          | 1293        | 1308         | rBV      | 243626         | 380785        | 100.00%         | 15.978%       |
| 13        | 9.318       | 1390          | 1399        | 1408         | rBV      | 38139          | 55675         | 14.62%          | 2.336%        |
| 14        | 10.094      | 1525          | 1531        | 1545         | rBV      | 272953         | 364414        | 95.70%          | 15.291%       |
| 15        | 11.124      | 1700          | 1706        | 1715         | rBV      | 215038         | 282299        | 74.14%          | 11.845%       |
| 16        | 12.059      | 1859          | 1865        | 1876         | rVB      | 269107         | 338339        | 88.85%          | 14.197%       |




Sum of corrected areas: 2383248

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032621\  
Data File : VX021559.D  
Acq On : 27 Mar 2021 03:30  
Operator : JC/MD  
Sample : M1787-22  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW202D-20210320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

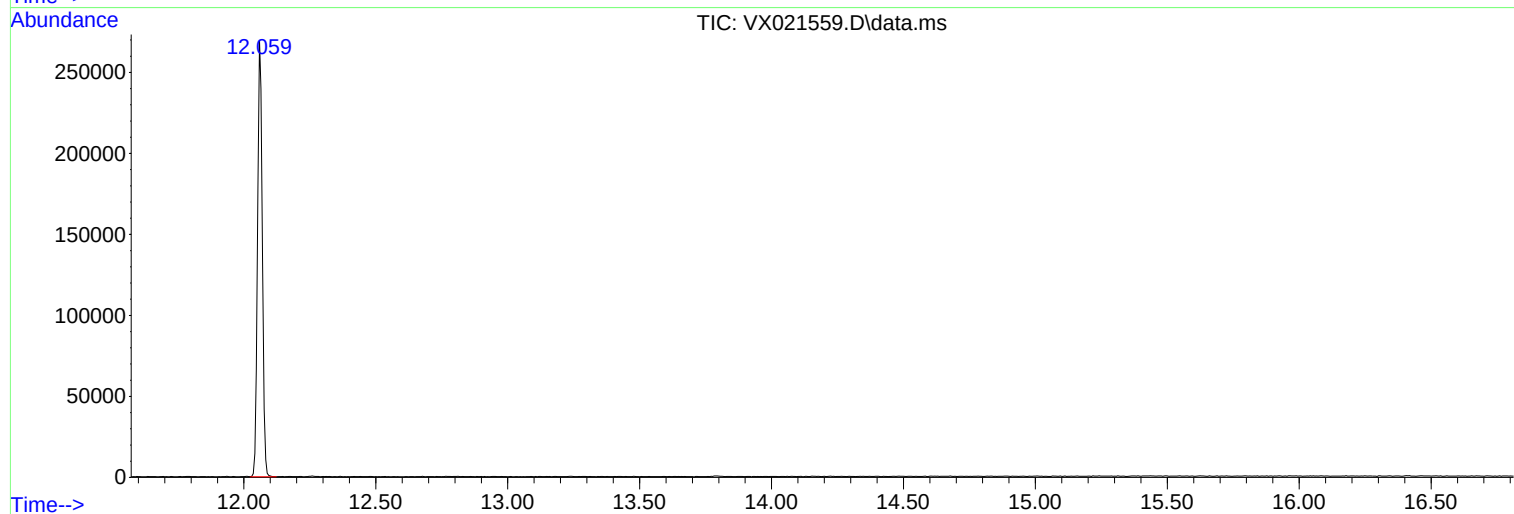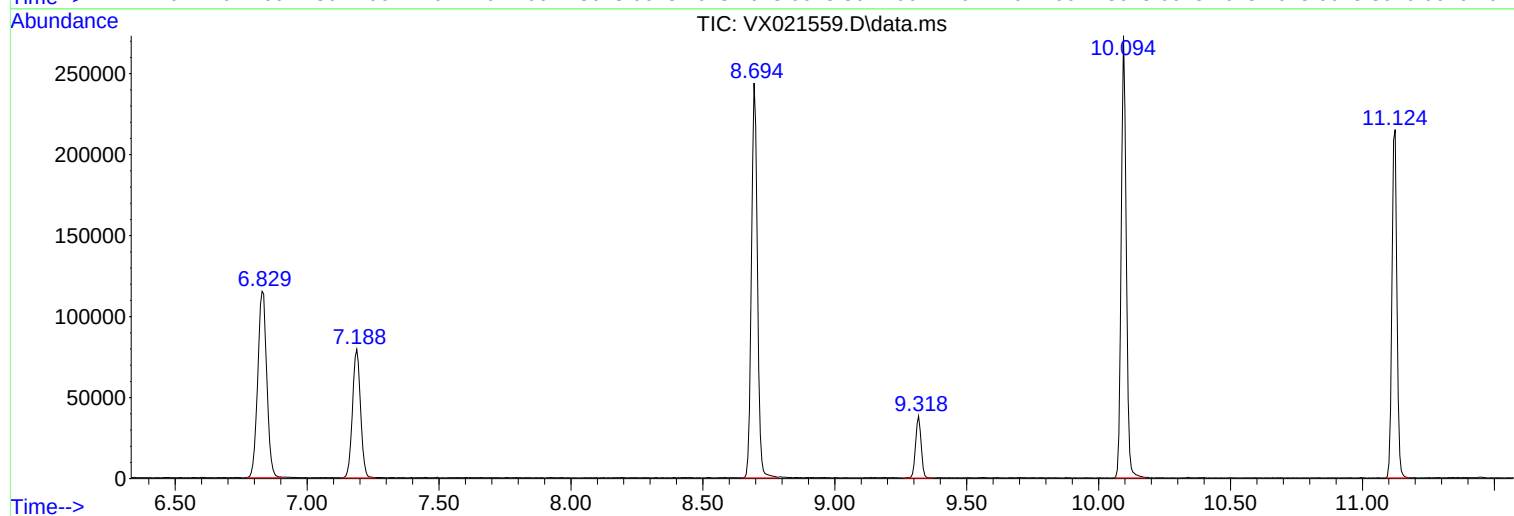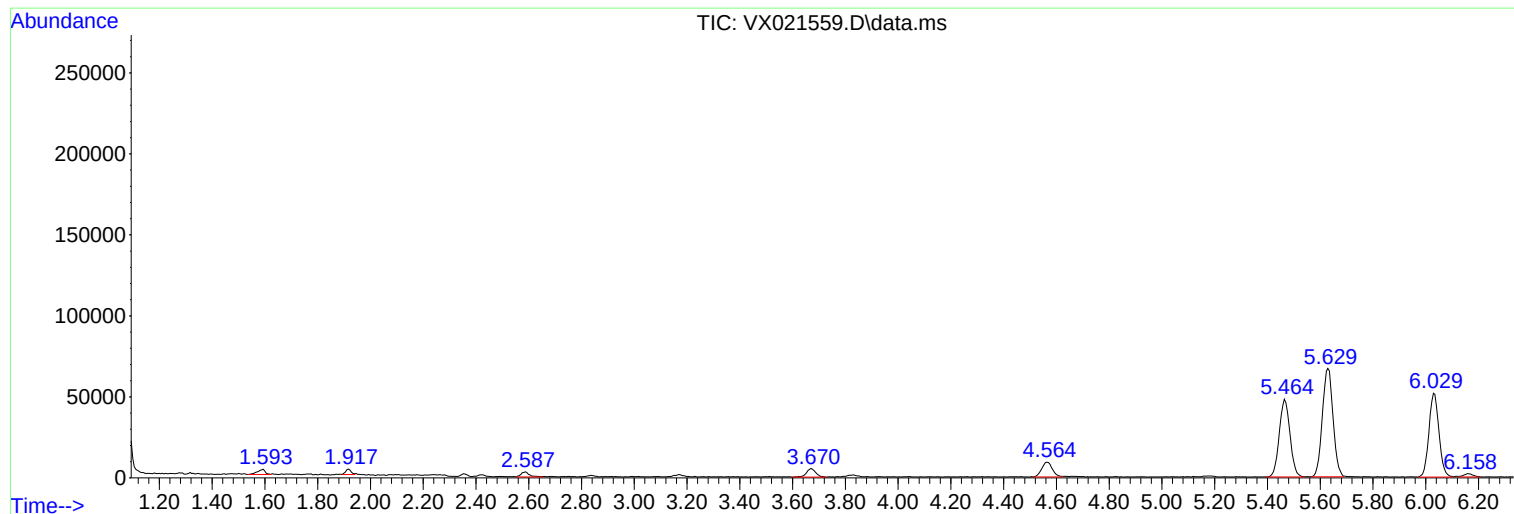

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032621\  
Data File : VX021559.D  
Acq On : 27 Mar 2021 03:30  
Operator : JC/MD  
Sample : M1787-22  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW202D-20210320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032621\  
Data File : VX021559.D  
Acq On : 27 Mar 2021 03:30  
Operator : JC/MD  
Sample : M1787-22  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW202D-20210320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----