
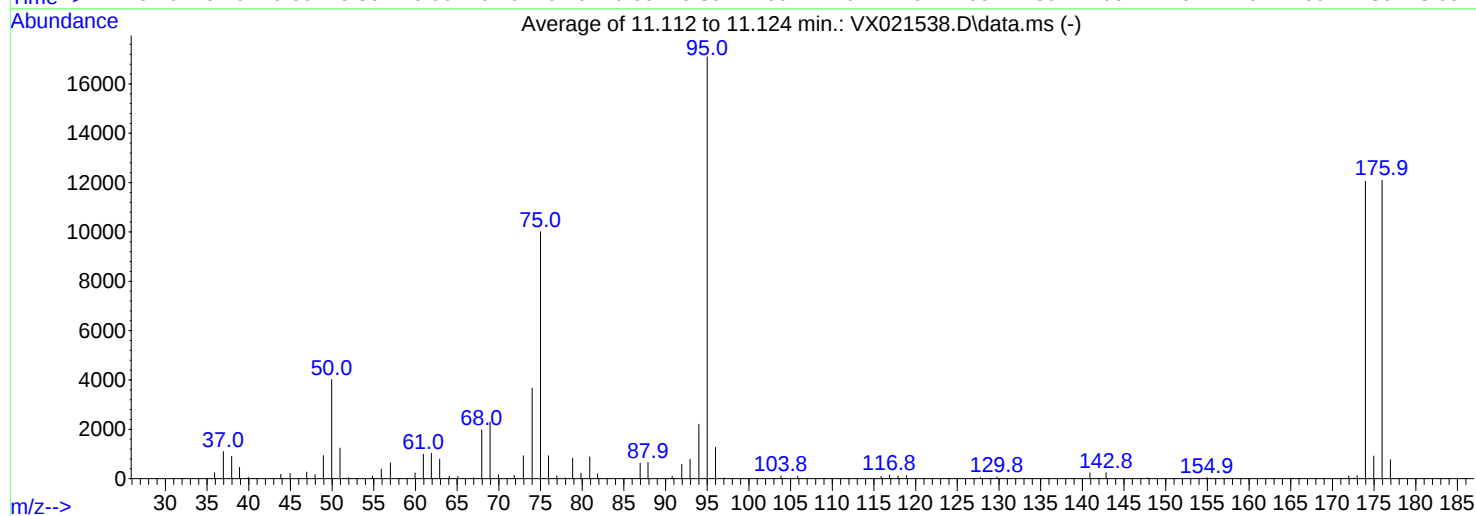


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032621\
 Data File : VX021538.D
 Acq On : 26 Mar 2021 18:32
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260
 Last Update : Sat Mar 27 04:47:38 2021

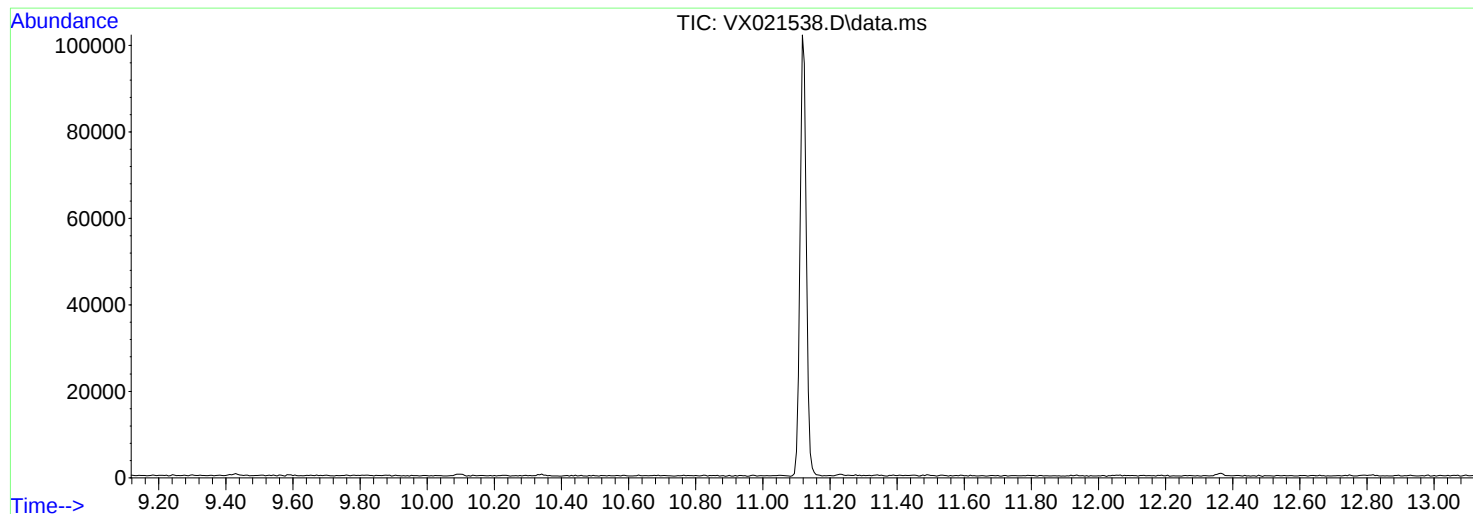

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1699

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	4014	PASS
75	95	30	60	58.6	10017	PASS
95	95	100	100	100.0	17097	PASS
96	95	5	9	7.4	1264	PASS
173	174	0.00	2	1.0	125	PASS
174	95	50	100	70.5	12051	PASS
175	174	5	9	7.6	912	PASS
176	174	95	101	100.4	12096	PASS
177	176	5	9	6.3	765	PASS