

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
 Data File : VX027731.D
 Acq On : 26 Mar 2022 16:50
 Operator : JC/MD
 Sample : N2076-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-20220322

Quant Time: Mar 28 05:18:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 25 16:26:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	62161	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	112067	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	101402	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	41541	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	51280	50.298	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 100.600%			
35) Dibromofluoromethane	5.391	113	37084	50.390	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 100.780%			
50) Toluene-d8	8.653	98	136623	48.024	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 96.040%			
62) 4-Bromofluorobenzene	11.079	95	52842	45.776	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 91.560%			
Target Compounds						
						Qvalue
5) Bromomethane	1.611	94	74	0.257	ug/l	# 3
6) Chloroethane	1.685	64	72	0.156	ug/l	# 43
10) Methyl Iodide	2.447	142	102	2.996	ug/l	# 41
11) Tert butyl alcohol	2.947	59	3282	17.290	ug/l	# 72
14) Allyl chloride	2.648	41	44	0.035	ug/l	# 25
16) Acetone	2.380	43	1136	2.635	ug/l	# 88
17) Carbon Disulfide	2.520	76	68	0.038	ug/l	# 75
18) Methyl Acetate	2.709	43	95	0.086	ug/l	# 46
19) Methyl tert-butyl Ether	2.934	73	23	0.009	ug/l	# 55
20) Methylene Chloride	2.800	84	185	0.240	ug/l	# 58
25) 2-Butanone	4.574	43	57	0.082	ug/l	# 44
26) 2,2-Dichloropropane	4.580	77	69	0.064	ug/l	# 52
31) Cyclohexane	5.550	56	1696	1.372	ug/l	# 22
36) 1,1-Dichloropropene	5.556	75	5767	4.961	ug/l	# 48
37) Ethyl Acetate	4.574	43	57	0.042	ug/l	# 65
38) Carbon Tetrachloride	5.556	117	7105	6.255	ug/l	# 15
42) 1,2-Dichloroethane	6.098	62	48	0.035	ug/l	# 73
51) 4-Methyl-2-Pentanone	8.653	43	609	0.434	ug/l	# 1
52) Toluene	8.726	92	75	0.037	ug/l	# 1
67) Ethyl Benzene	10.305	91	266	0.067	ug/l	# 44
68) m/p-Xylenes	10.293	106	83	0.058	ug/l	# 21
73) Isopropylbenzene	11.079	105	114	0.033	ug/l	# 48
76) 1,2,3-Trichloropropane	11.085	75	29348	25.374	ug/l	# 38
78) n-propylbenzene	11.317	91	47	0.012	ug/l	# 52
79) 2-Chlorotoluene	11.317	91	47	0.018	ug/l	# 40
80) 1,3,5-Trimethylbenzene	11.384	105	19	0.006	ug/l	# 28
81) trans-1,4-Dichloro-2-b...	11.085	75	29348	86.371	ug/l	# 15
82) 4-Chlorotoluene	11.317	91	47	0.016	ug/l	# 45
84) 1,2,4-Trimethylbenzene	11.756	105	130	0.044	ug/l	# 31
85) sec-Butylbenzene	11.756	105	130	0.037	ug/l	# 56
87) 1,3-Dichlorobenzene	12.042	146	20	0.014	ug/l	# 1
88) 1,4-Dichlorobenzene	12.042	146	20	0.014	ug/l	# 1
95) Naphthalene	13.774	128	43	0.015	ug/l	# 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Quant Time: Mar 28 05:18:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 25 16:26:59 2022
Response via : Initial Calibration








#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Instrument :
MSVOA_X
ClientSampleId :
TB-20220322



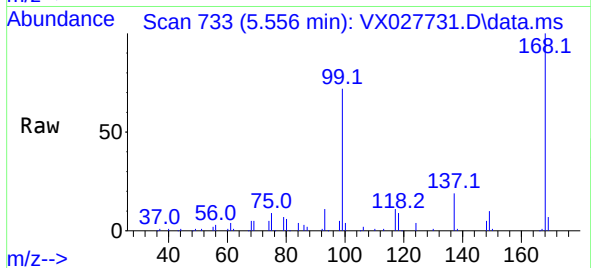


Tgt Ion:168 Resp: 62161
Ion Ratio Lower Upper
168 100
99 72.0 41.7 62.5#



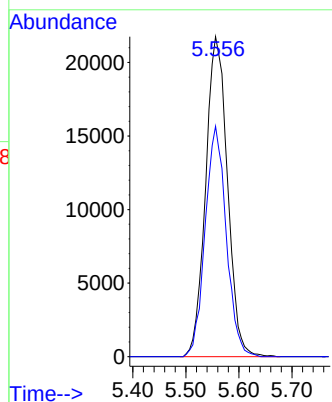


#5
Bromomethane
Concen: 0.257 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 94 Resp: 74
Ion Ratio Lower Upper
94 100
96 0.0 75.3 112.9#

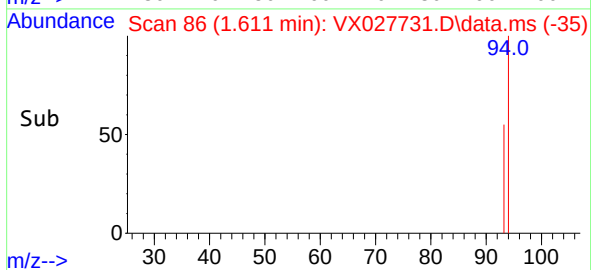





Abundance Scan 97 (1.678 min): VX027698.D\data.ms (-88)

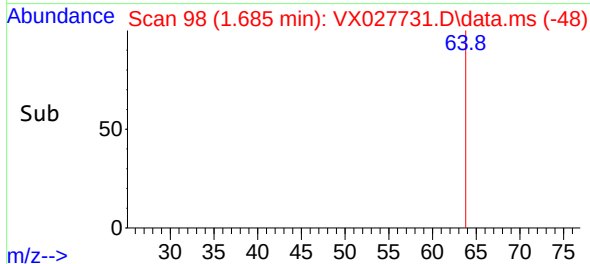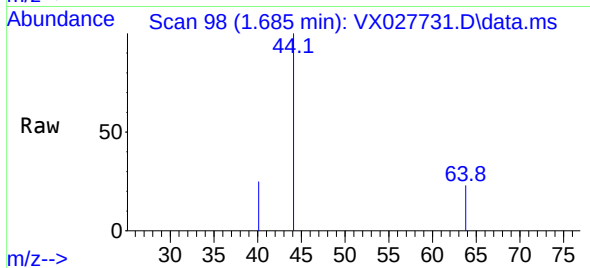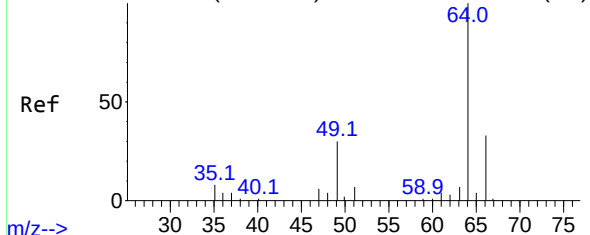

#6
Chloroethane
Concen: 0.156 ug/l
RT: 1.685 min Scan# 91
Delta R.T. 0.007 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50


Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion: 64 Resp: 72
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#

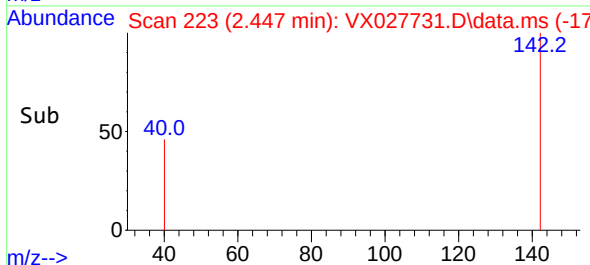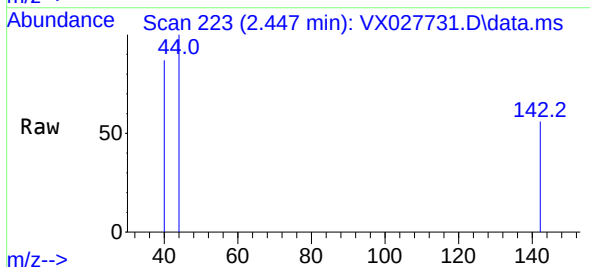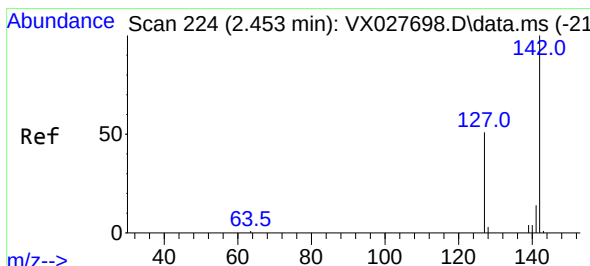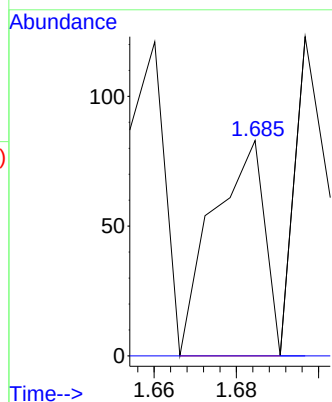

#10
Methyl Iodide
Concen: 2.996 ug/l
RT: 2.447 min Scan# 223
Delta R.T. -0.006 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 142 Resp: 102
Ion Ratio Lower Upper
142 100
127 0.0 33.9 50.9#
141 0.0 11.4 17.2#

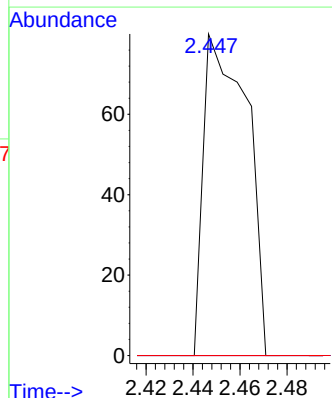



#11

Tert butyl alcohol

Concen: 17.290 ug/l

RT: 2.947 min Scan# 309

Delta R.T. -0.024 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :

MSVOA_X

ClientSampleId :





TB-20220322

Tgt Ion: 59 Resp: 3282

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

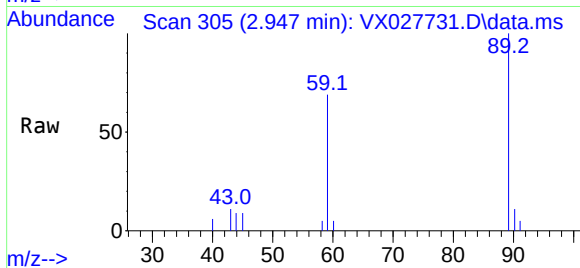

#14

Allyl chloride

Concen: 0.035 ug/l

RT: 2.648 min Scan# 256

Delta R.T. -0.018 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50




Tgt Ion: 41 Resp: 44


Ion Ratio Lower Upper

41 100

39 0.0 50.4 75.6#

76 0.0 32.7 49.1#


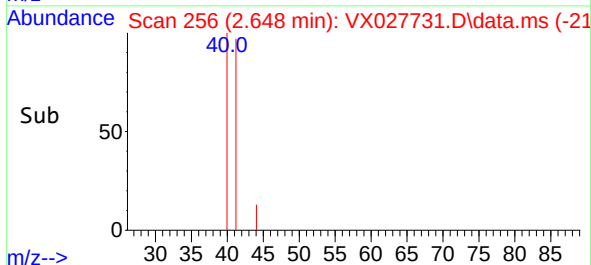
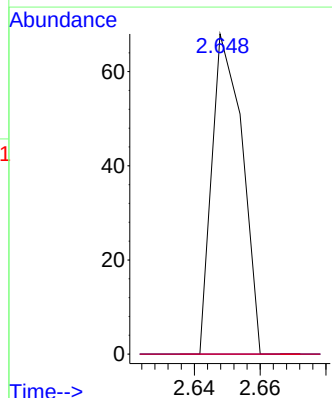
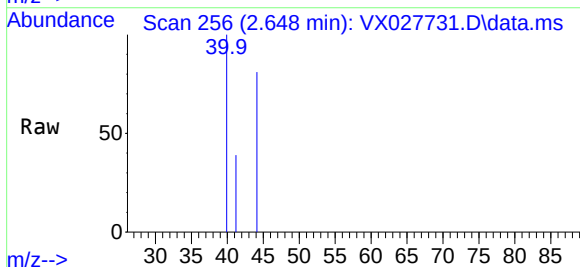




#16
Acetone
Concen: 2.635 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion: 43 Resp: 1136
Ion Ratio Lower Upper
43 100
58 29.1 28.8 43.2

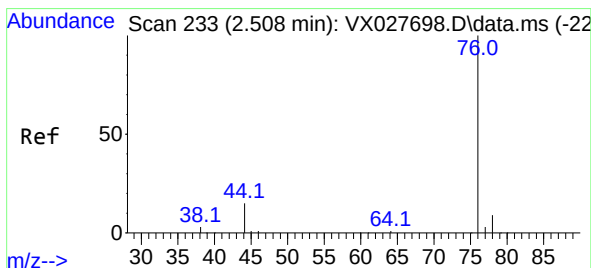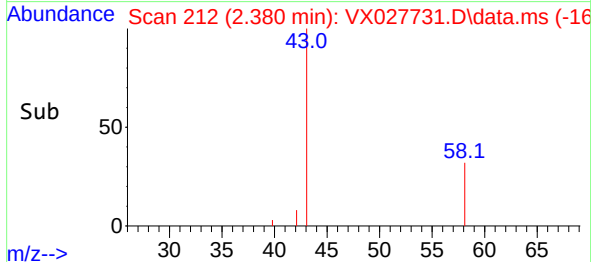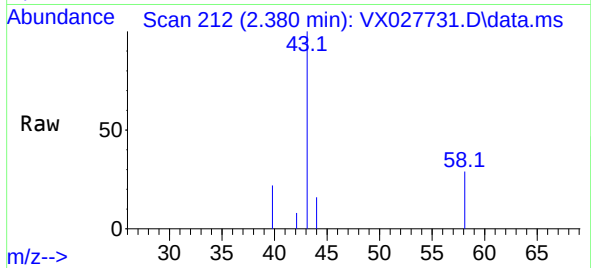

#17
Carbon Disulfide
Concen: 0.038 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.012 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 76 Resp: 68
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

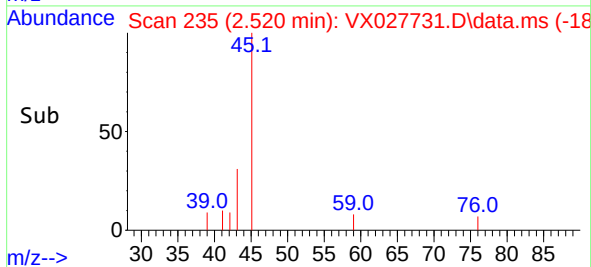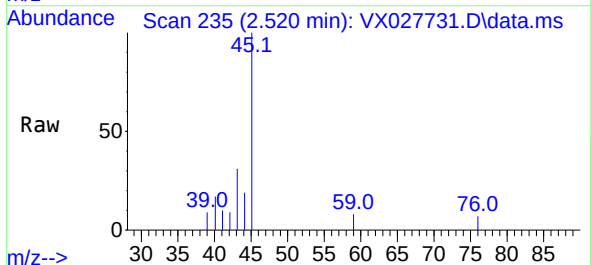



#18

Methyl Acetate

Concen: 0.086 ug/l

RT: 2.709 min Scan# 2

Delta R.T. 0.006 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :

MSVOA_X

ClientSampleId :





TB-20220322

Tgt Ion: 43 Resp: 95

Ion Ratio Lower Upper

43 100

74 0.0 22.8 34.2#

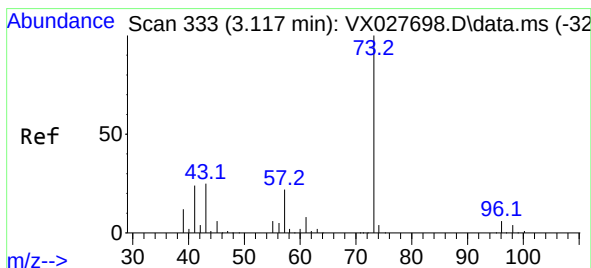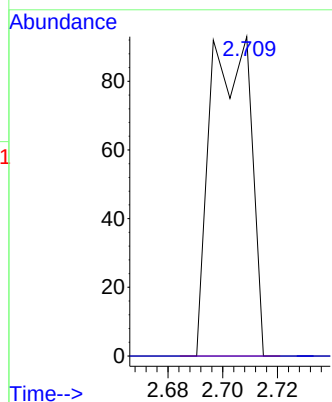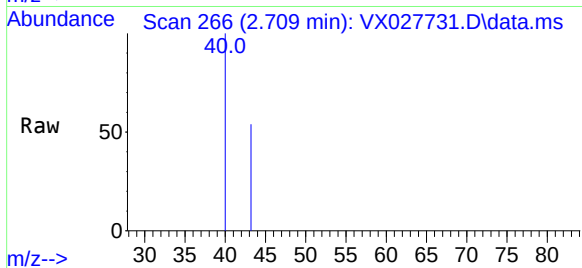

#19

Methyl tert-butyl Ether

Concen: 0.009 ug/l

RT: 2.934 min Scan# 303

Delta R.T. -0.183 min

Lab File: VX027731.D




Acq: 26 Mar 2022 16:50


Tgt Ion: 73 Resp: 23

Ion Ratio Lower Upper

73 100

57 0.0 16.8 25.2#

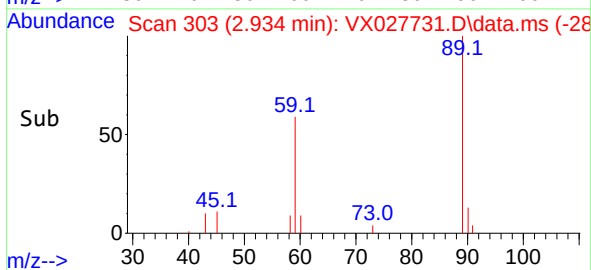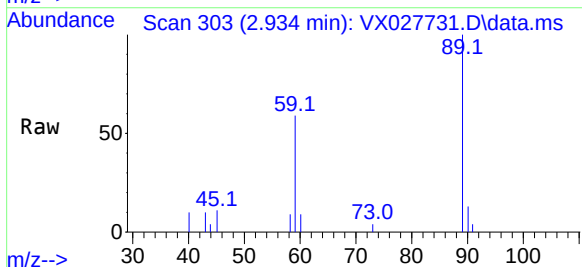







#20
Methylene Chloride
Concen: 0.240 ug/l
RT: 2.800 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Instrument :
MSVOA_X
ClientSampleId :
TB-20220322

Tgt Ion: 84 Resp: 185




Ion	Ratio	Lower	Upper
84	100		
49	94.5	85.5	128.3
51	0.0	26.6	39.8#
86	0.0	51.5	77.3#




#25
2-Butanone
Concen: 0.082 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.012 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 43 Resp: 57

Ion	Ratio	Lower	Upper
43	100		
72	0.0	24.4	36.6#

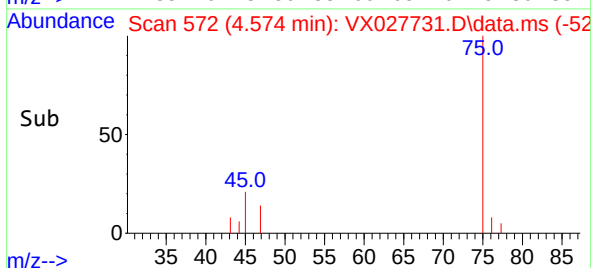

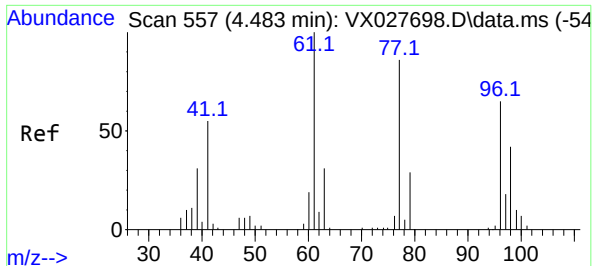

#26

2,2-Dichloropropane

Concen: 0.064 ug/l

RT: 4.580 min Scan# 51

Delta R.T. 0.097 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :

MSVOA_X

ClientSampleId :





TB-20220322

Tgt Ion: 77 Resp: 69

Ion Ratio Lower Upper

77 100

97 0.0 11.8 35.4#

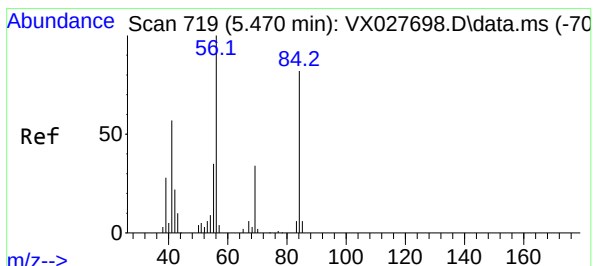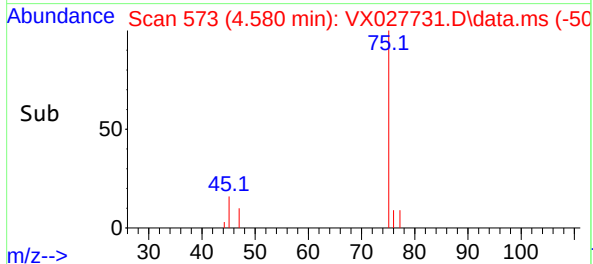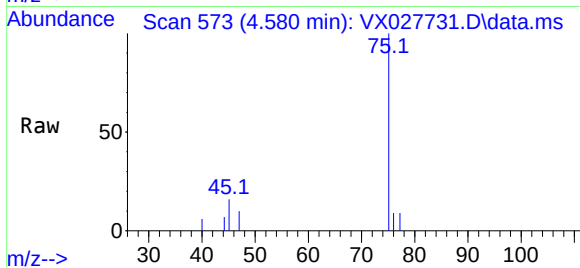

#31

Cyclohexane

Concen: 1.372 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.080 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50




Tgt Ion: 56 Resp: 1696


Ion Ratio Lower Upper

56 100

69 196.9 26.7 40.1#

84 90.9 77.2 115.8


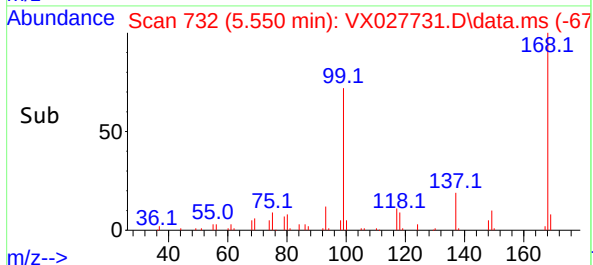
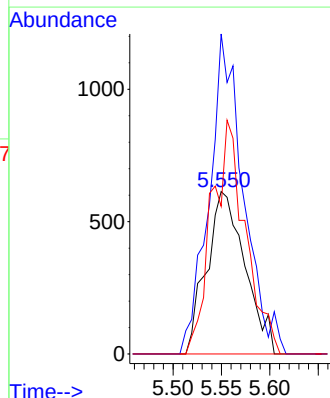
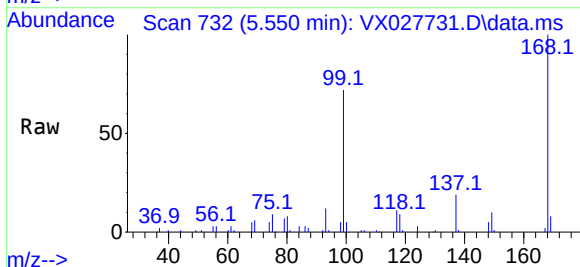


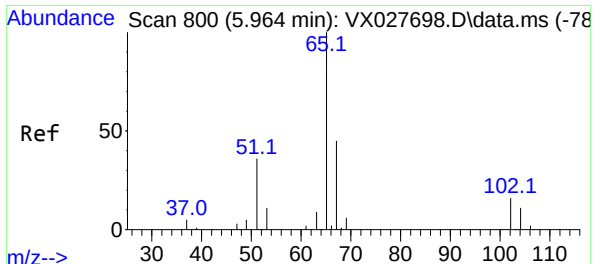

#33
1,2-Dichloroethane-d4
Concen: 50.298 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion: 65 Resp: 51280
Ion Ratio Lower Upper
65 100
67 51.5 0.0 107.4

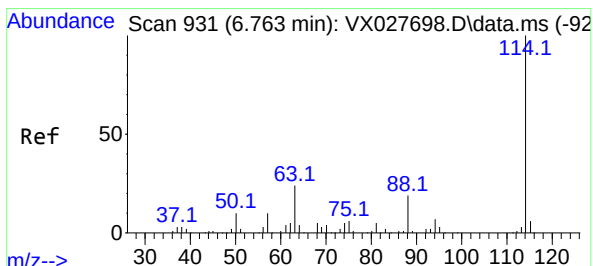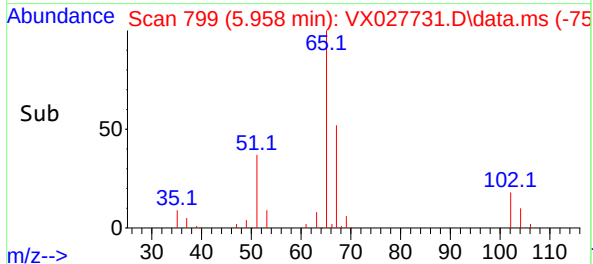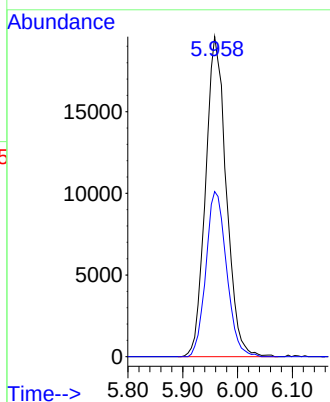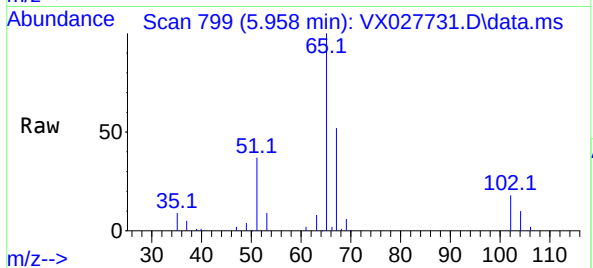

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 114 Resp: 112067
Ion Ratio Lower Upper
114 100
63 24.0 0.0 36.8
88 18.4 0.0 32.4


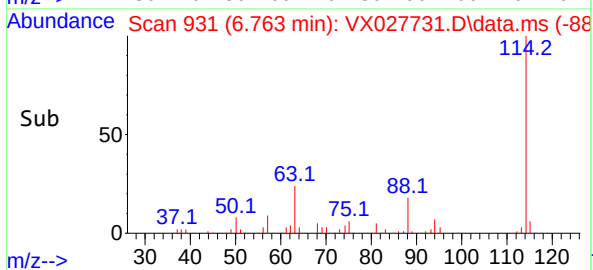

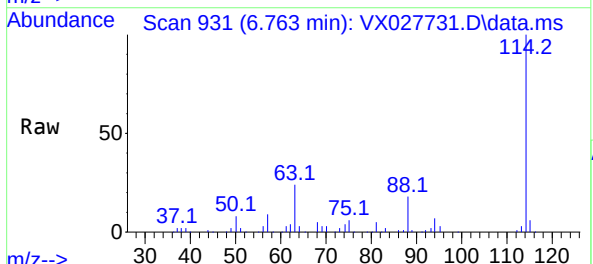


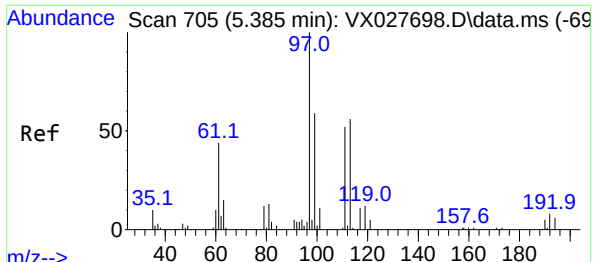

#35
Dibromofluoromethane
Concen: 50.390 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion:113 Resp: 37084
Ion Ratio Lower Upper
113 100
111 103.5 82.8 124.2
192 18.6 16.9 25.3

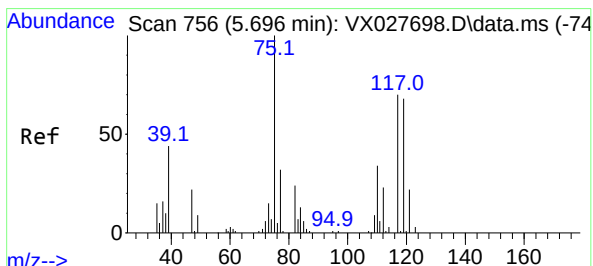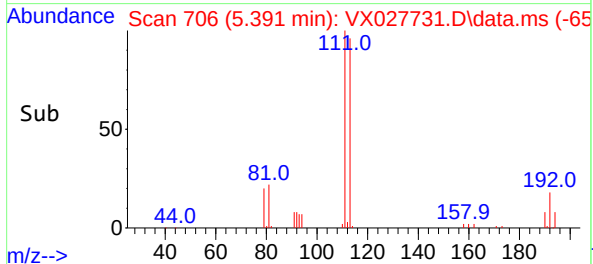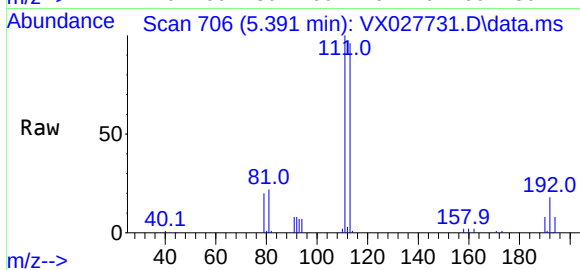

#36
1,1-Dichloropropene
Concen: 4.961 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 75 Resp: 5767
Ion Ratio Lower Upper
75 100
110 7.5 18.3 54.8#
77 0.0 24.8 37.2#

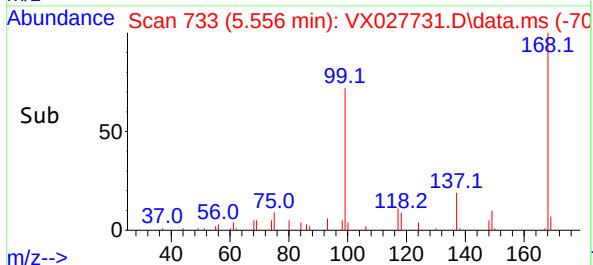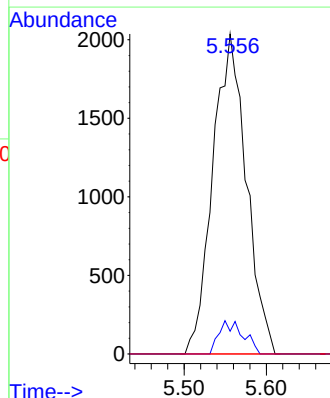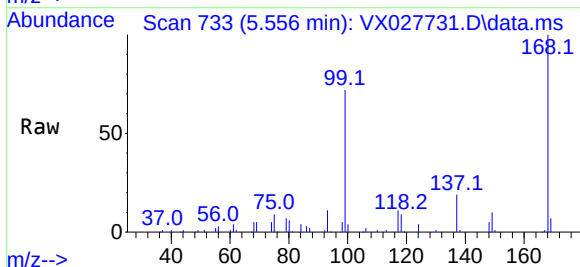



#37

Ethyl Acetate

Concen: 0.042 ug/l

RT: 4.574 min Scan# 51

Delta R.T. -0.147 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :

MSVOA_X

ClientSampleId :

TB-20220322





Tgt Ion: 43 Resp: 57

Ion Ratio Lower Upper

43 100

61 0.0 12.6 19.0#

70 0.0 10.2 15.2#

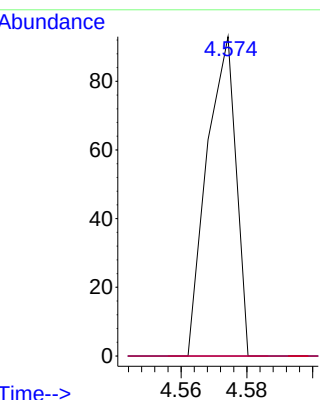

#38

Carbon Tetrachloride

Concen: 6.255 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.122 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50




Tgt Ion: 117 Resp: 7105


Ion Ratio Lower Upper

117 100

119 4.1 77.3 115.9#

121 0.0 24.2 36.2#

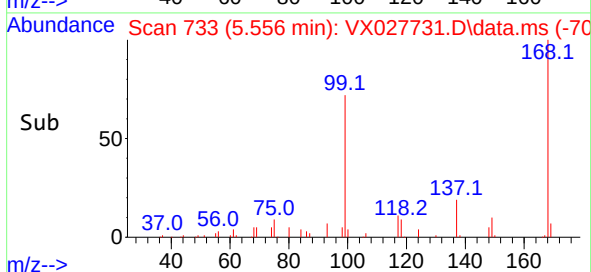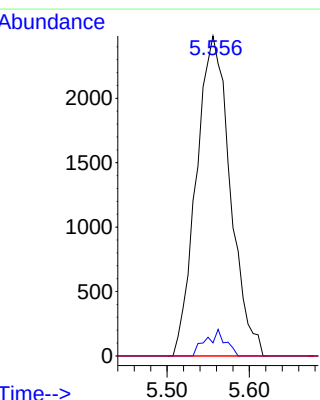

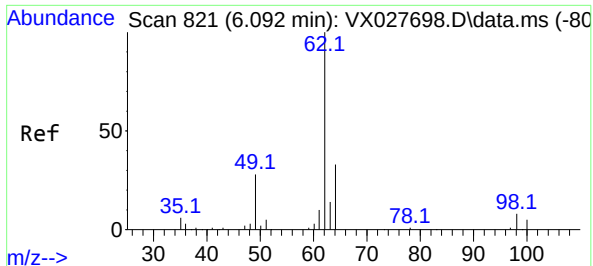

#42

1,2-Dichloroethane

Concen: 0.035 ug/l

RT: 6.098 min Scan# 81

Delta R.T. 0.006 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :

MSVOA_X

ClientSampleId :





TB-20220322

Tgt Ion: 62 Resp: 48

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

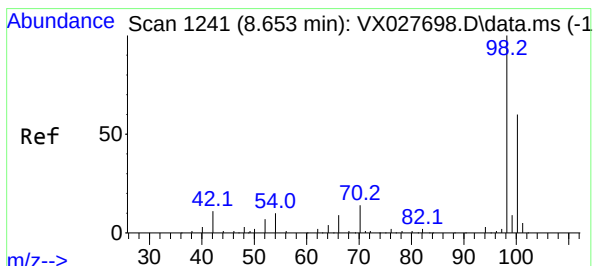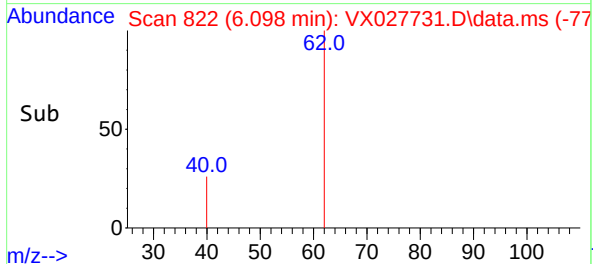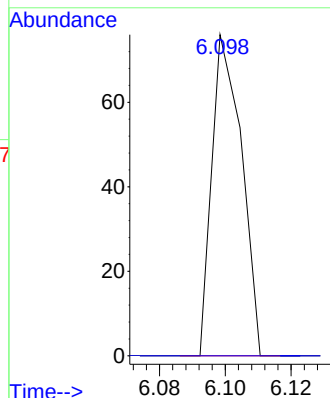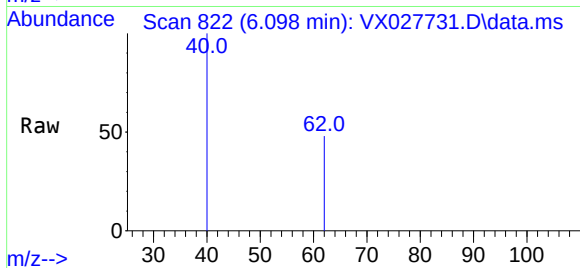

#50

Toluene-d8

Concen: 48.024 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX027731.D




Acq: 26 Mar 2022 16:50


Tgt Ion: 98 Resp: 136623

Ion Ratio Lower Upper

98 100

100 64.6 52.6 78.8

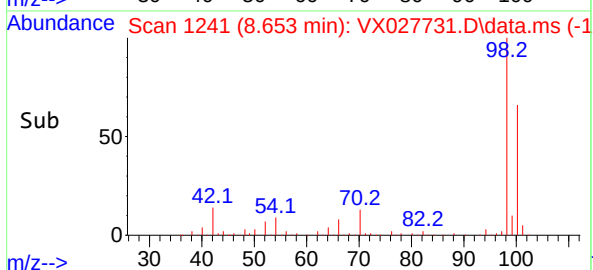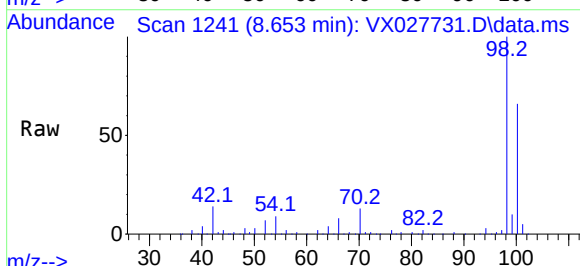

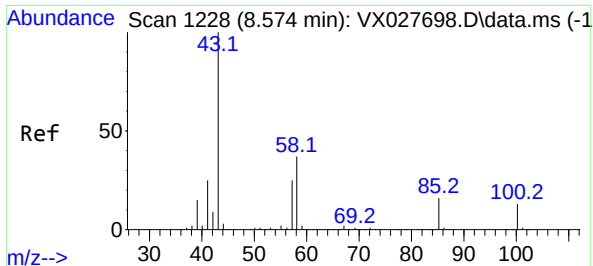

#51

4-Methyl-2-Pentanone

Concen: 0.434 ug/l

RT: 8.653 min Scan# 11

Delta R.T. 0.079 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :

MSVOA_X

ClientSampleId :





TB-20220322

Tgt Ion: 43 Resp: 609

Ion Ratio Lower Upper

43 100

58 193.3 36.1 54.1#

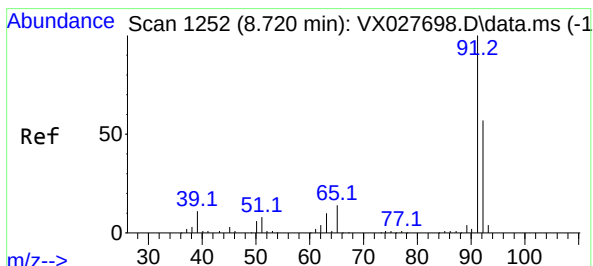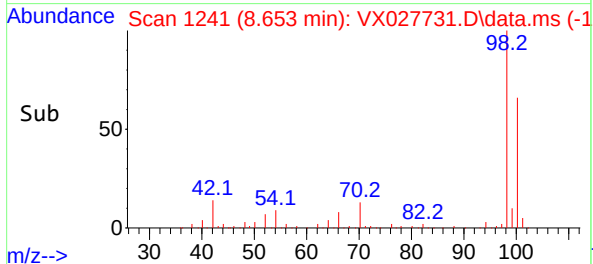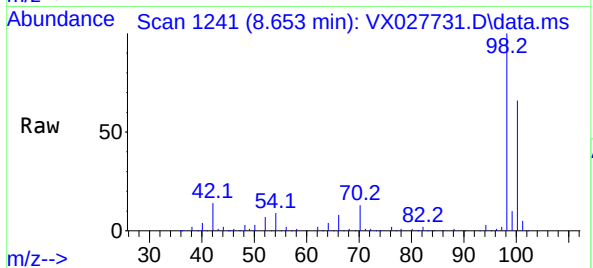

#52

Toluene

Concen: 0.037 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.006 min

Lab File: VX027731.D




Acq: 26 Mar 2022 16:50


Tgt Ion: 92 Resp: 75

Ion Ratio Lower Upper

92 100

91 310.7 137.5 206.3#

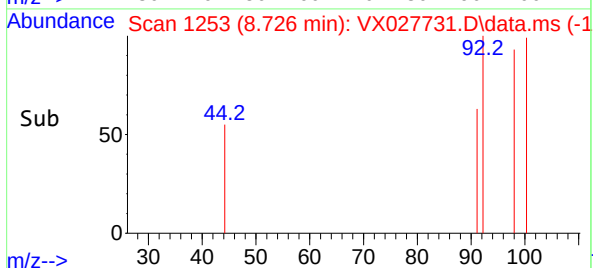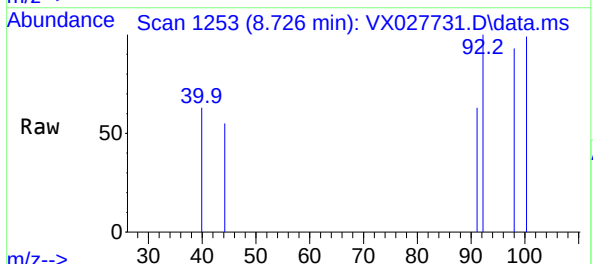



#62

4-Bromofluorobenzene

Concen: 45.776 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :

MSVOA_X

ClientSampleId :

TB-20220322





Tgt Ion: 95 Resp: 52842

Ion Ratio Lower Upper

95 100

174 64.4 0.0 163.0

176 61.4 0.0 155.0

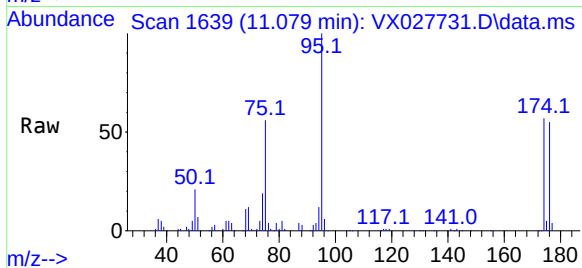

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50




Tgt Ion: 117 Resp: 101402


Ion Ratio Lower Upper

117 100

82 62.0 41.8 62.8

119 31.0 24.8 37.2


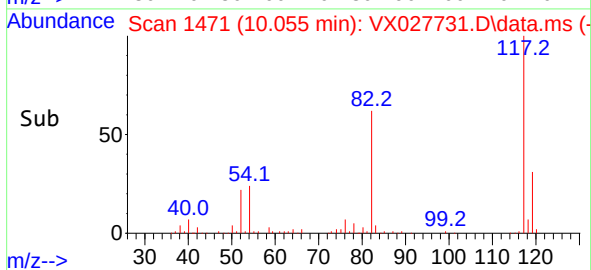

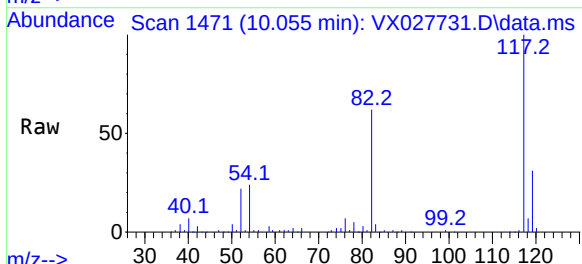




#67
Ethyl Benzene
Concen: 0.067 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.110 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion: 91 Resp: 266
Ion Ratio Lower Upper
91 100
106 0.0 24.6 36.8#



#68
m/p-Xylenes
Concen: 0.058 ug/l
RT: 10.293 min Scan# 1510
Delta R.T. -0.012 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 106 Resp: 83
Ion Ratio Lower Upper
106 100
91 320.5 160.4 240.6#


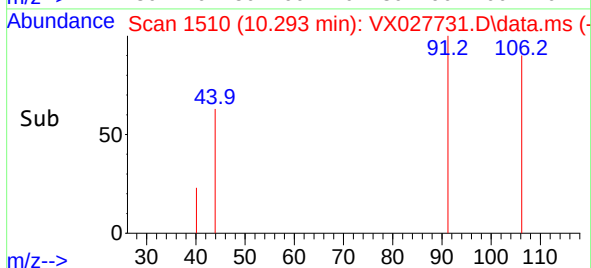
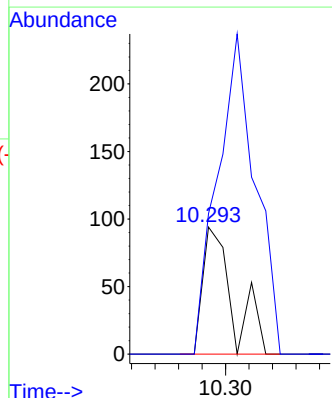





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion:152 Resp: 41541
Ion Ratio Lower Upper
152 100
115 67.8 37.5 112.7
150 159.6 0.0 338.2

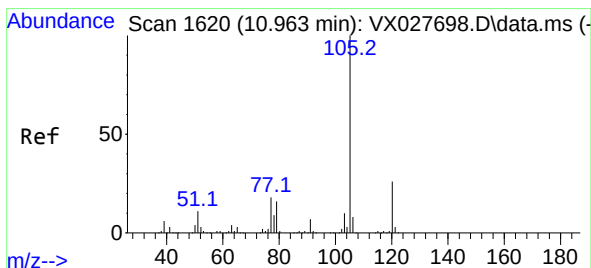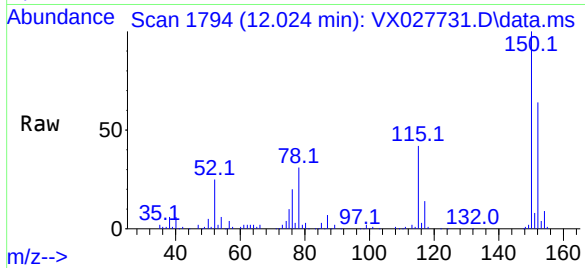

#73
Isopropylbenzene
Concen: 0.033 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.116 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion:105 Resp: 114
Ion Ratio Lower Upper
105 100
120 0.0 13.5 40.5#


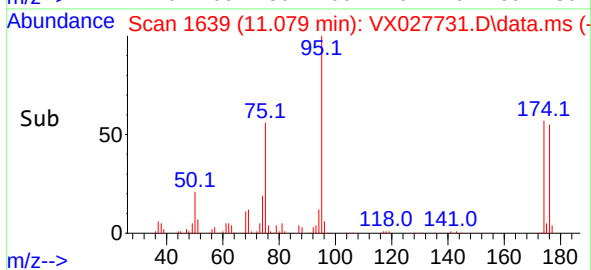

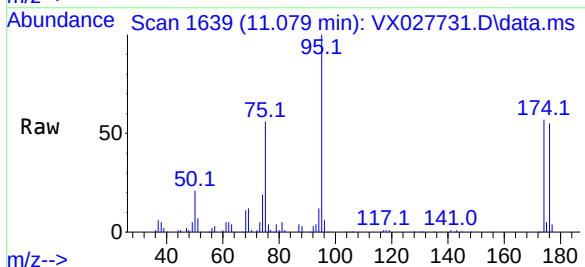




#76
1,2,3-Trichloropropane
Concen: 25.374 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion: 75 Resp: 29348
Ion Ratio Lower Upper
75 100
77 1.3 19.4 58.2#

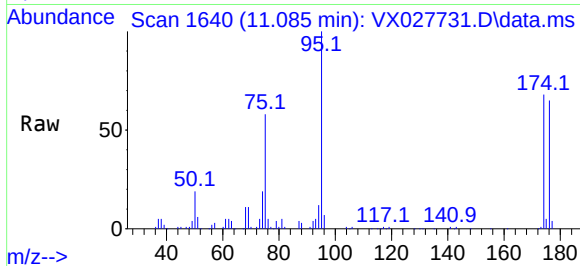

#78
n-propylbenzene
Concen: 0.012 ug/l
RT: 11.317 min Scan# 1678
Delta R.T. 0.012 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 91 Resp: 47
Ion Ratio Lower Upper
91 100
120 0.0 11.6 34.8#


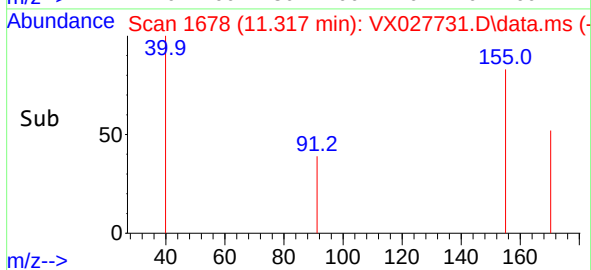

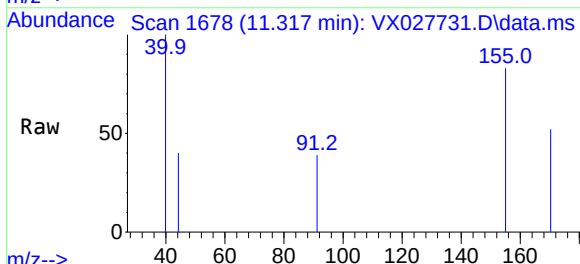




#79
2-Chlorotoluene
Concen: 0.018 ug/l
RT: 11.317 min Scan# 1687
Delta R.T. -0.049 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion: 91 Resp: 47
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

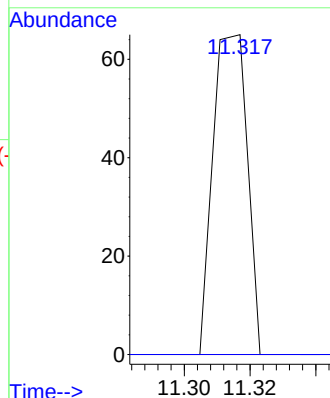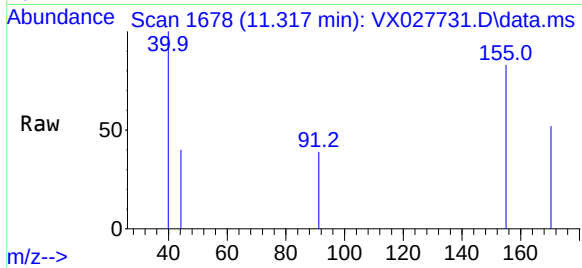

#80
1,3,5-Trimethylbenzene
Concen: 0.006 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. -0.067 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 105 Resp: 19
Ion Ratio Lower Upper
105 100
120 0.0 24.3 72.9#


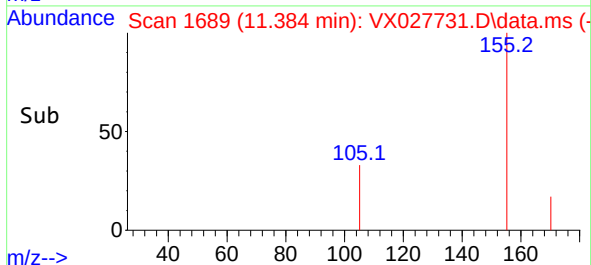
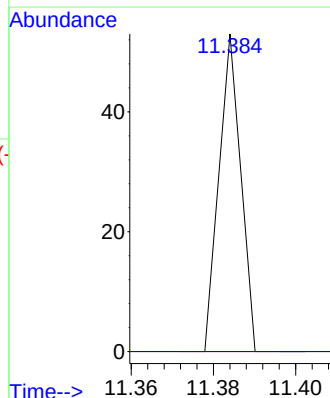
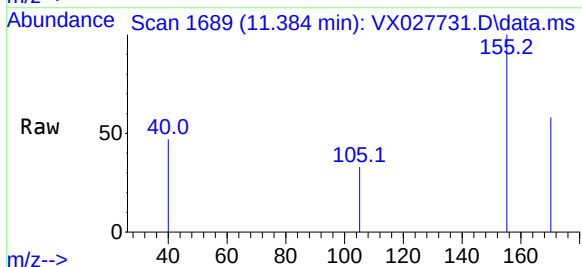




#81
trans-1,4-Dichloro-2-butene
Concen: 86.371 ug/l
RT: 11.085 min Scan# 11
Delta R.T. 0.061 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion: 75 Resp: 29348
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

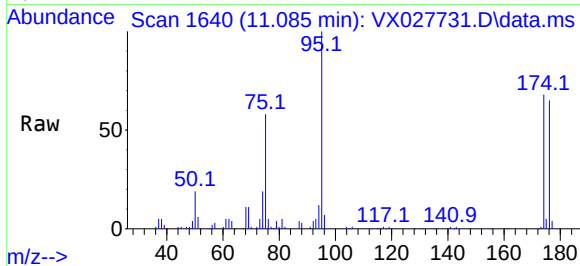

#82
4-Chlorotoluene
Concen: 0.016 ug/l
RT: 11.317 min Scan# 1678
Delta R.T. -0.140 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion: 91 Resp: 47
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


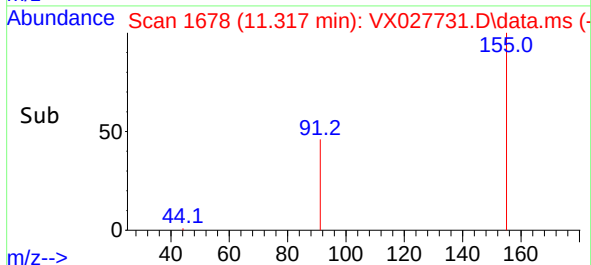

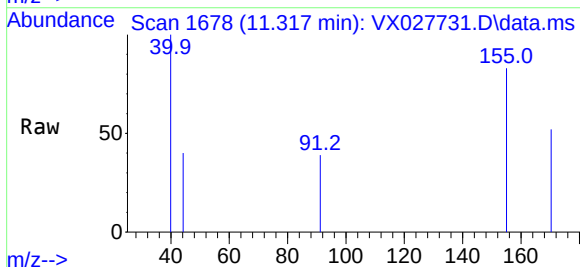




#84
1,2,4-Trimethylbenzene
Concen: 0.044 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50




Instrument :
MSVOA_X
ClientSampleId :
TB-20220322


Tgt Ion:105 Resp: 130
Ion Ratio Lower Upper
105 100
120 0.0 22.6 67.8#

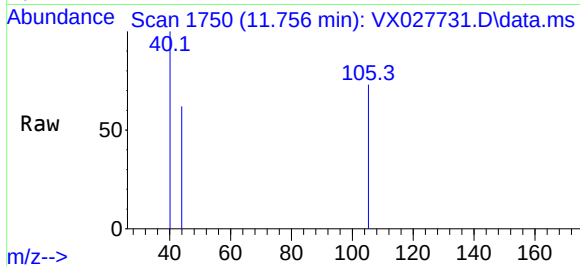

#85
sec-Butylbenzene
Concen: 0.037 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Tgt Ion:105 Resp: 130
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#

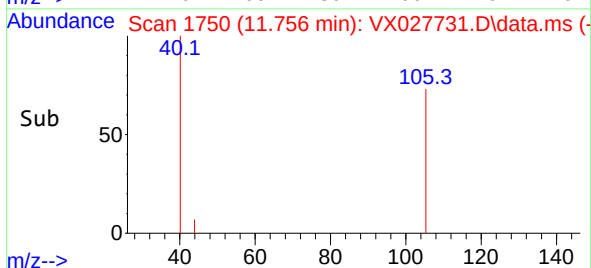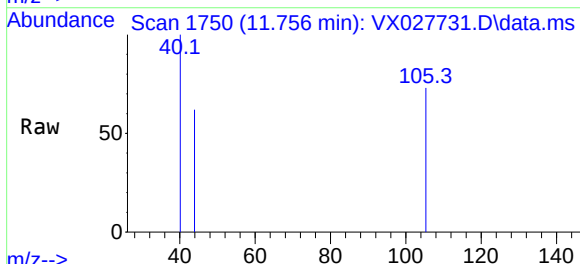



#87

1,3-Dichlorobenzene

Concen: 0.014 ug/l

RT: 12.042 min Scan# 1797

Delta R.T. 0.073 min

Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Instrument :





MSVOA_X

ClientSampleId :

TB-20220322

Tgt Ion:146 Resp: 20

Ion	Ratio	Lower	Upper
146	100		
111	3135.0	19.7	59.1#
148	1550.0	31.6	94.7#

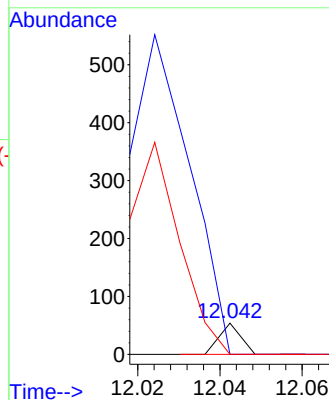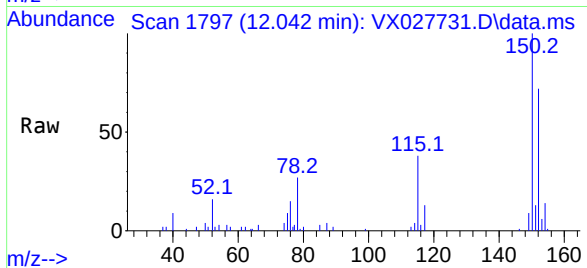

#88

1,4-Dichlorobenzene

Concen: 0.014 ug/l

RT: 12.042 min Scan# 1797




Delta R.T. 0.000 min


Lab File: VX027731.D

Acq: 26 Mar 2022 16:50

Tgt Ion:146 Resp: 20


Ion	Ratio	Lower	Upper
146	100		
111	3135.0	19.2	57.6#
148	1550.0	32.3	96.9#

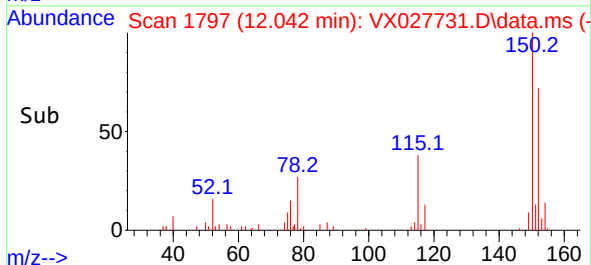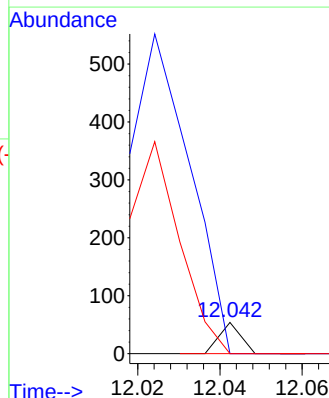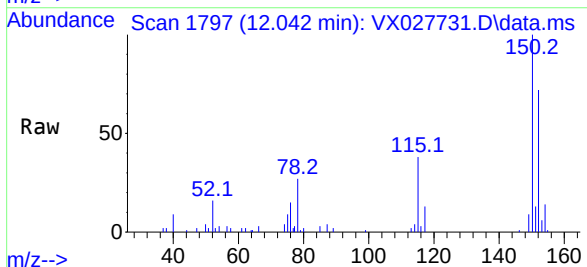

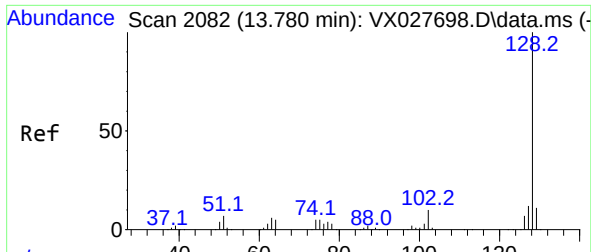

#95
Naphthalene
Concen: 0.015 ug/l
RT: 13.774 min Scan# 20
Delta R.T. -0.006 min
Lab File: VX027731.D
Acq: 26 Mar 2022 16:50

Instrument :
MSVOA_X
ClientSampleId :
TB-20220322

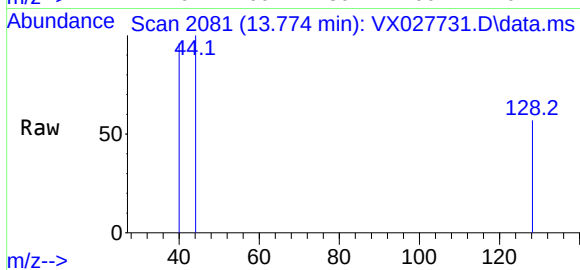

Tgt Ion:128 Resp: 43
Ion Ratio Lower Upper
128 100
127 0.0 10.2 15.4#
129 0.0 8.7 13.1#

