

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
 Data File : VX027731.D
 Acq On : 26 Mar 2022 16:50
 Operator : JC/MD
 Sample : N2076-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-20220322

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M

Title : SW846 8260

Signal : TIC: VX027731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	29	rBV2	2577	3924	1.05%	0.196%
2	2.538	231	238	246	rBV	8208	15699	4.21%	0.784%
3	2.947	297	305	315	rBV	4611	11168	2.99%	0.558%
4	4.580	565	573	590	rVB2	2084	7100	1.90%	0.354%
5	5.391	695	706	722	rBV	43113	124433	33.37%	6.212%
6	5.556	722	733	749	rVB	72063	201223	53.96%	10.046%
7	5.958	789	799	817	rVB	53320	138345	37.10%	6.907%
8	6.763	922	931	943	rBV	115133	273647	73.38%	13.662%
9	8.653	1234	1241	1250	rBV	235845	372911	100.00%	18.617%
10	10.055	1466	1471	1480	rVB	235210	324538	87.03%	16.202%
11	11.085	1634	1640	1651	rBV	182066	247745	66.44%	12.368%
12	12.024	1789	1794	1804	rVB	233416	282304	75.70%	14.094%




Sum of corrected areas: 2003037

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
Data File : VX027731.D
Acq On : 26 Mar 2022 16:50
Operator : JC/MD
Sample : N2076-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

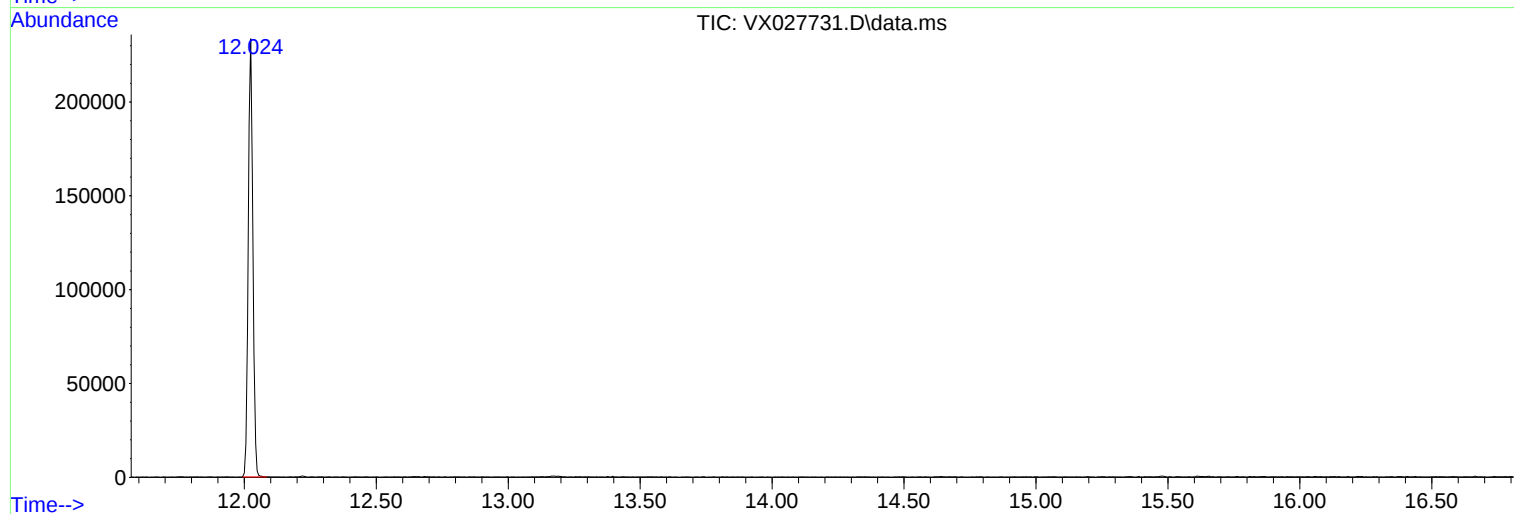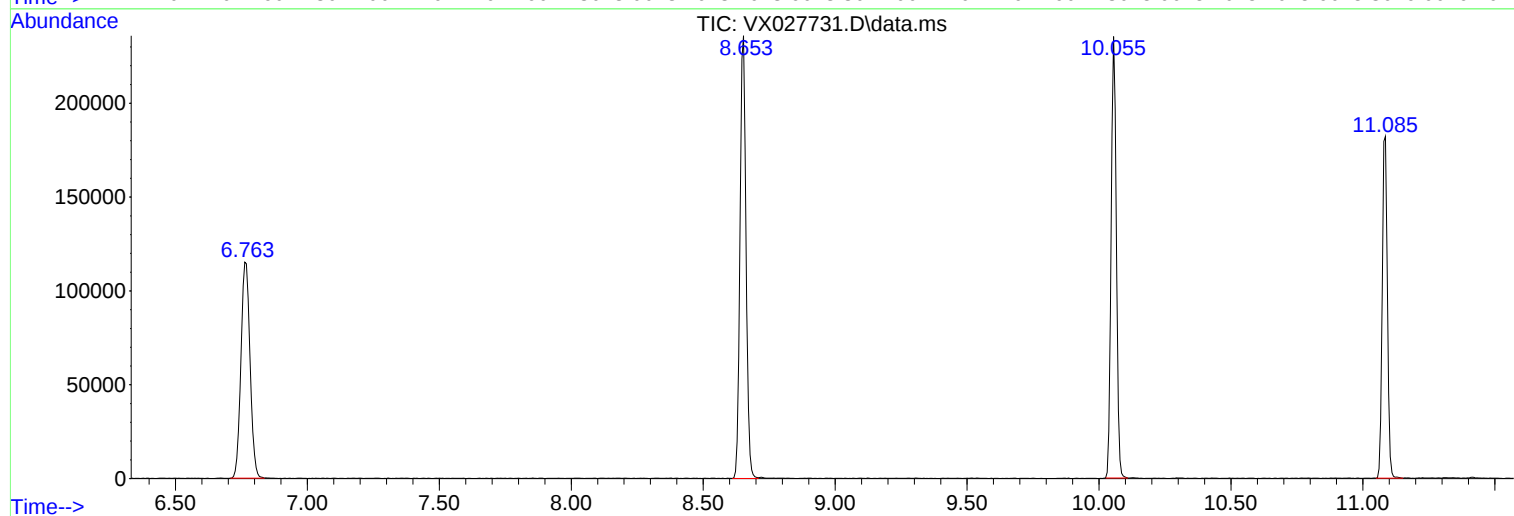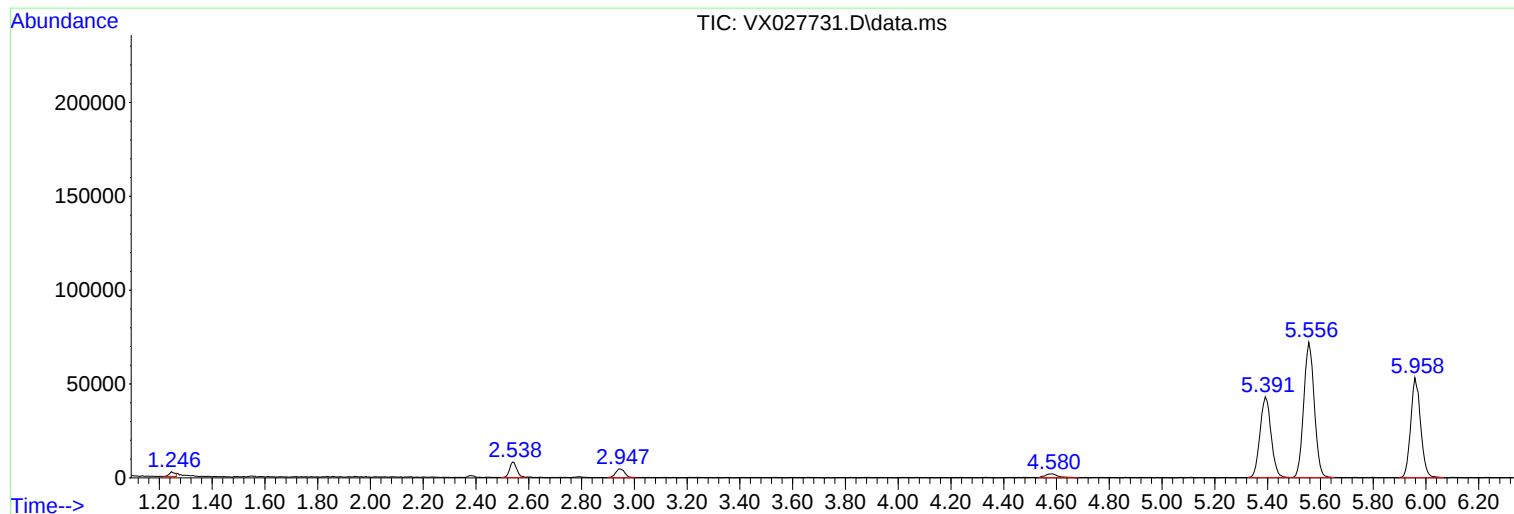

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
Data File : VX027731.D
Acq On : 26 Mar 2022 16:50
Operator : JC/MD
Sample : N2076-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
Data File : VX027731.D
Acq On : 26 Mar 2022 16:50
Operator : JC/MD
Sample : N2076-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------