

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
 Data File : VX027740.D
 Acq On : 26 Mar 2022 20:22
 Operator : JC/MD
 Sample : N1962-10
 Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C-23-25-28

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
 Title : SW846 8260

Signal : TIC: VX027740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	32	rBV3	7464	14340	3.85%	0.615%
2	5.391	696	706	721	rVB2	37281	109533	29.38%	4.698%
3	5.550	721	732	745	rBV2	68712	195027	52.31%	8.364%
4	5.958	788	799	809	rBV	44956	119433	32.03%	5.122%
5	6.373	860	867	875	rBV3	2458	6561	1.76%	0.281%
6	6.763	921	931	942	rBV	115843	274821	73.71%	11.786%
7	8.653	1234	1241	1250	rBV	233243	372864	100.00%	15.991%
8	10.055	1464	1471	1484	rBV	228762	330573	88.66%	14.178%
9	10.195	1489	1494	1500	rVB2	4303	6491	1.74%	0.278%
10	11.085	1634	1640	1650	rBV	203534	262751	70.47%	11.269%
11	11.384	1684	1689	1696	rBV2	5580	9169	2.46%	0.393%
12	11.616	1720	1727	1733	rBV4	2104	4027	1.08%	0.173%
13	11.756	1746	1750	1760	rVB	7061	9099	2.44%	0.390%
14	12.024	1789	1794	1800	rBV	241960	301756	80.93%	12.942%
15	12.091	1800	1805	1810	rVB	7238	9909	2.66%	0.425%
16	12.244	1824	1830	1837	rBV	31893	43296	11.61%	1.857%
17	12.426	1854	1860	1864	rBV3	3836	4964	1.33%	0.213%
18	12.615	1884	1891	1896	rBV3	2770	3939	1.06%	0.169%
19	12.981	1947	1951	1956	rVB6	2344	4368	1.17%	0.187%
20	13.292	1990	2002	2009	rBV6	11495	30100	8.07%	1.291%
21	13.384	2014	2017	2020	rBV4	3779	4631	1.24%	0.199%
22	13.426	2020	2024	2029	rVB6	3297	5092	1.37%	0.218%
23	13.506	2031	2037	2041	rBV8	2739	6198	1.66%	0.266%
24	13.780	2077	2082	2088	rVV	38398	52755	14.15%	2.263%
25	13.847	2089	2093	2096	rVB5	3491	4358	1.17%	0.187%
26	14.213	2150	2153	2160	rVB9	3844	7978	2.14%	0.342%
27	14.414	2184	2186	2193	rVB8	2726	5528	1.48%	0.237%
28	14.640	2216	2223	2227	rBV5	13060	28108	7.54%	1.205%
29	14.786	2240	2247	2251	rBV	13472	20440	5.48%	0.877%
30	14.963	2275	2276	2281	rVB5	4852	4913	1.32%	0.211%
31	15.182	2309	2312	2315	rBV5	2896	4646	1.25%	0.199%
32	15.213	2315	2317	2321	rVB4	5191	5767	1.55%	0.247%
33	15.383	2341	2345	2348	rBV6	4296	7140	1.91%	0.306%
34	15.420	2348	2351	2355	rVB6	11462	17209	4.62%	0.738%
35	15.481	2358	2361	2367	rBV7	6078	9656	2.59%	0.414%
36	15.584	2375	2378	2380	rBV4	3180	4507	1.21%	0.193%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
Data File : VX027740.D
Acq On : 26 Mar 2022 20:22
Operator : JC/MD
Sample : N1962-10
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C-23-25-28

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M

Title : SW846 8260

37	15.621	2380	2384	2387	rVB5	6813	10413	2.79%	0.447%
38	15.749	2399	2405	2409	rBV9	4825	8864	2.38%	0.380%
39	15.981	2440	2443	2445	rBV4	3018	4540	1.22%	0.195%
40	16.603	2540	2545	2549	rVB7	3140	5905	1.58%	0.253%


Sum of corrected areas: 2331669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
Data File : VX027740.D
Acq On : 26 Mar 2022 20:22
Operator : JC/MD
Sample : N1962-10
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C-23-25-28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

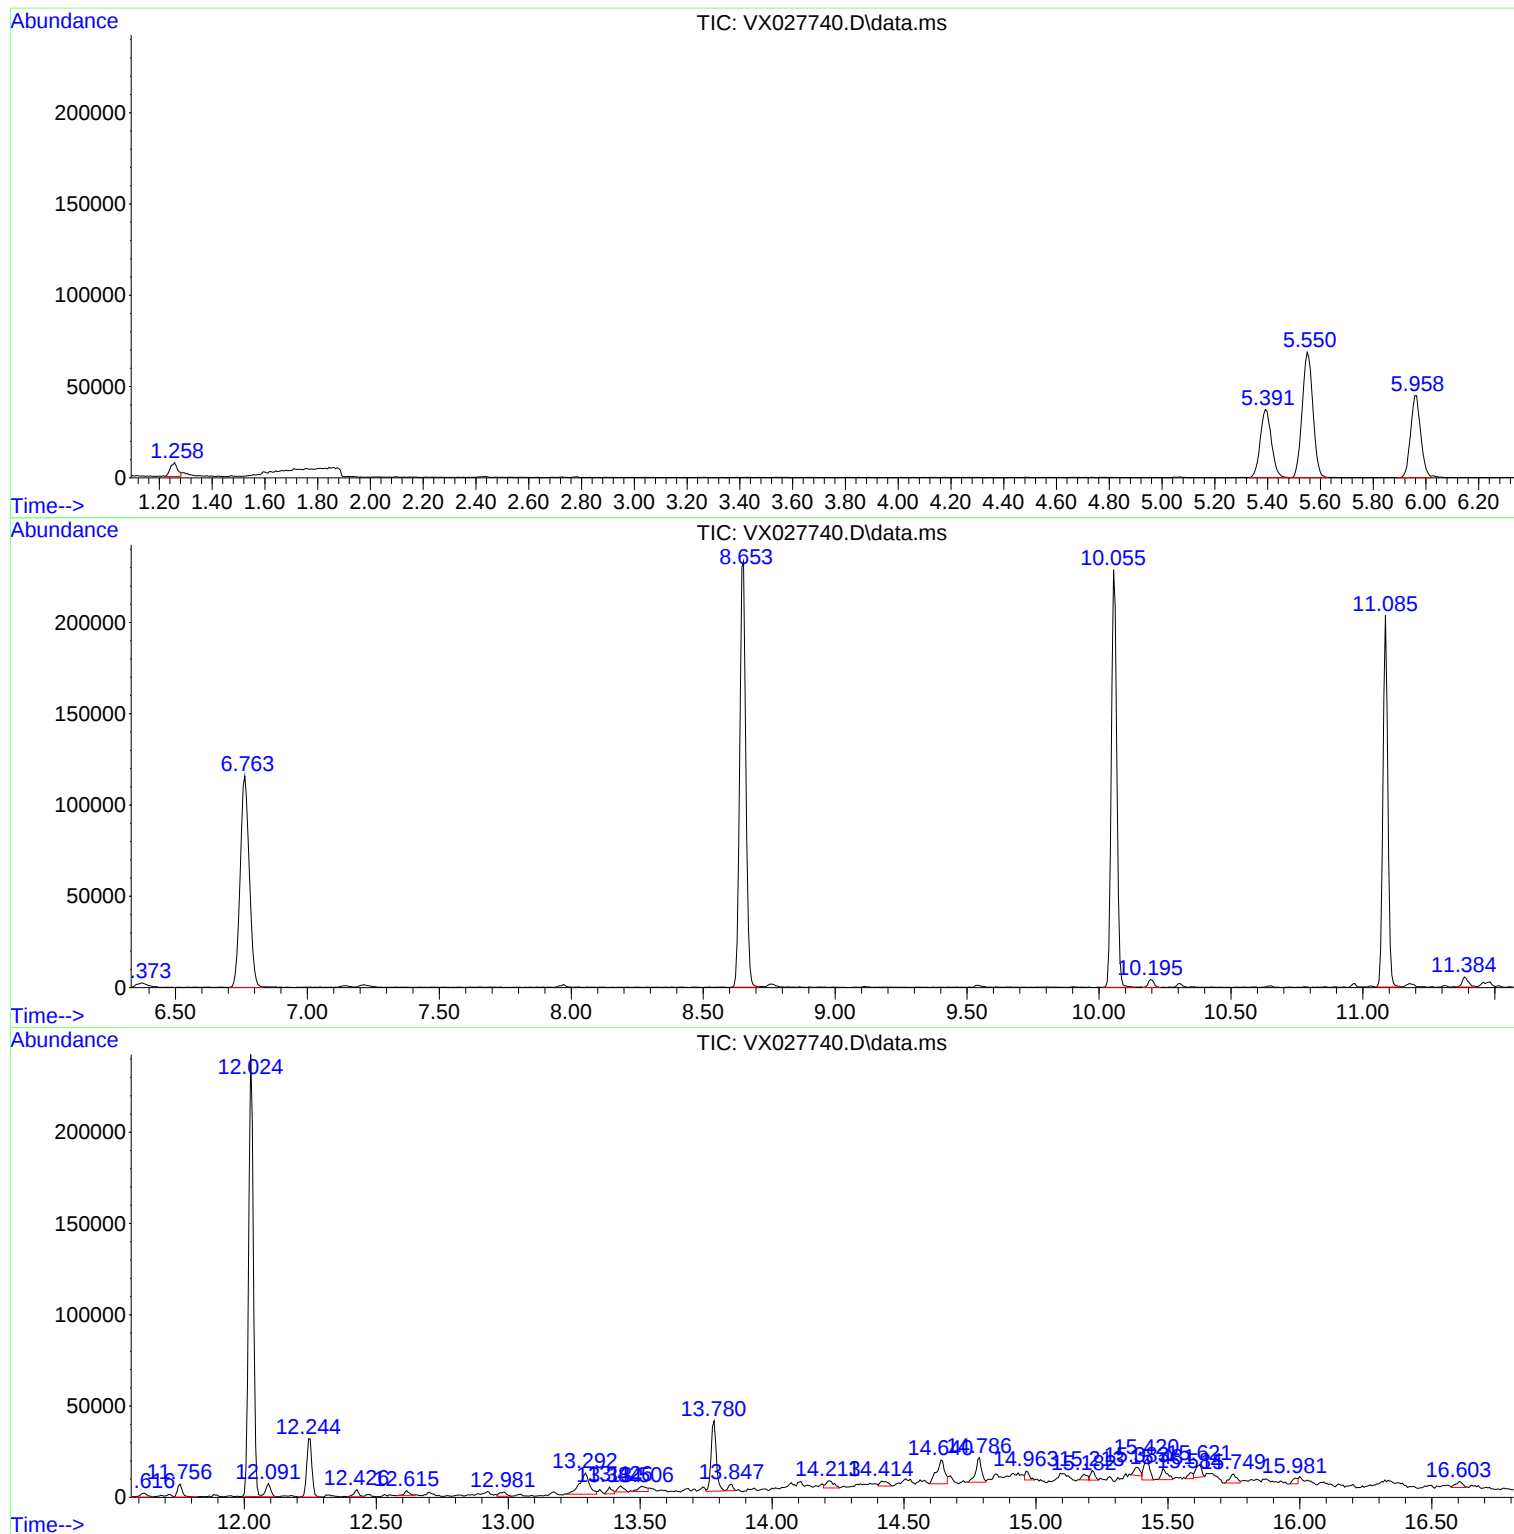

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
Data File : VX027740.D
Acq On : 26 Mar 2022 20:22
Operator : JC/MD
Sample : N1962-10
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C-23-25-28










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.244	7.17 ug/l	43296	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	94
2			Benzene, 2-propenyl-	118	C9H10	000300-57-2	76
3			Benzene, cyclopropyl-	118	C9H10	000873-49-4	76
4			Tetracyclo[3.3.1.0(2,8).0(4,6)]-...	118	C9H10	1000191-13-7	59
5			Benzene, 1-ethenyl-2-methyl-	118	C9H10	000611-15-4	58

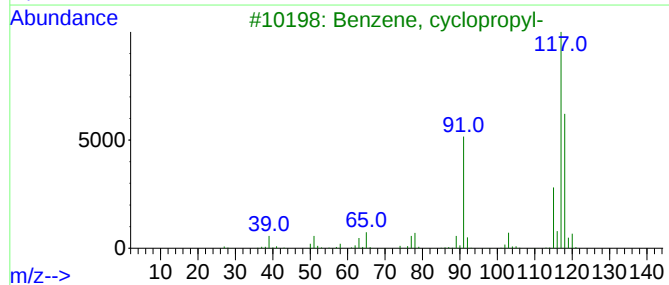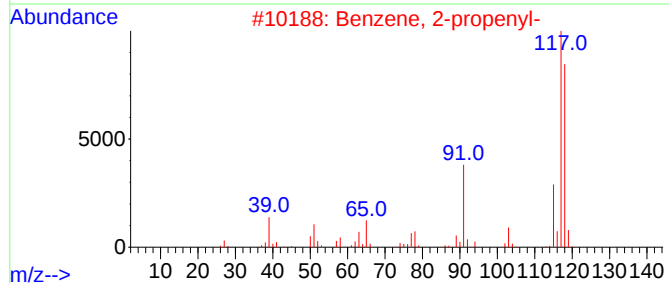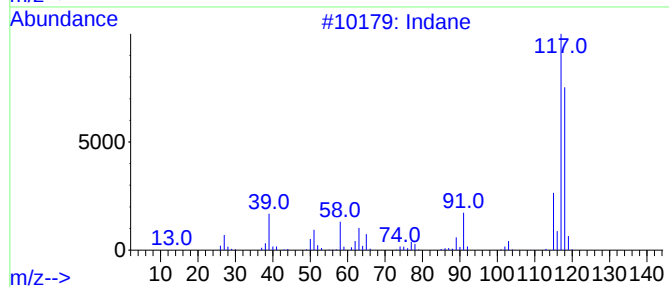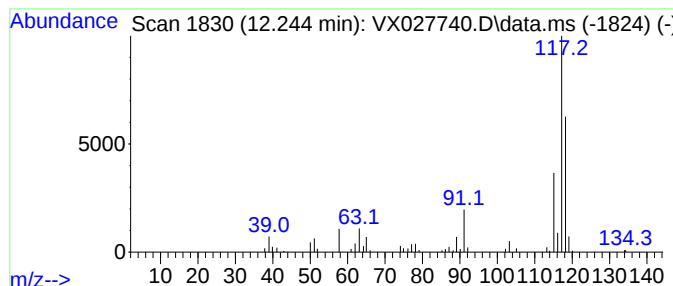

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032622\
Data File : VX027740.D
Acq On : 26 Mar 2022 20:22
Operator : JC/MD
Sample : N1962-10
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C-23-25-28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.244	7.2	ug/l	43296	4	12.024	301756	50.0