


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032624\
Data File : VX040790.D
Acq On : 26 Mar 2024 08:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032124W.M
Title : SW846 8260
Last Update : Fri Mar 22 02:44:48 2024

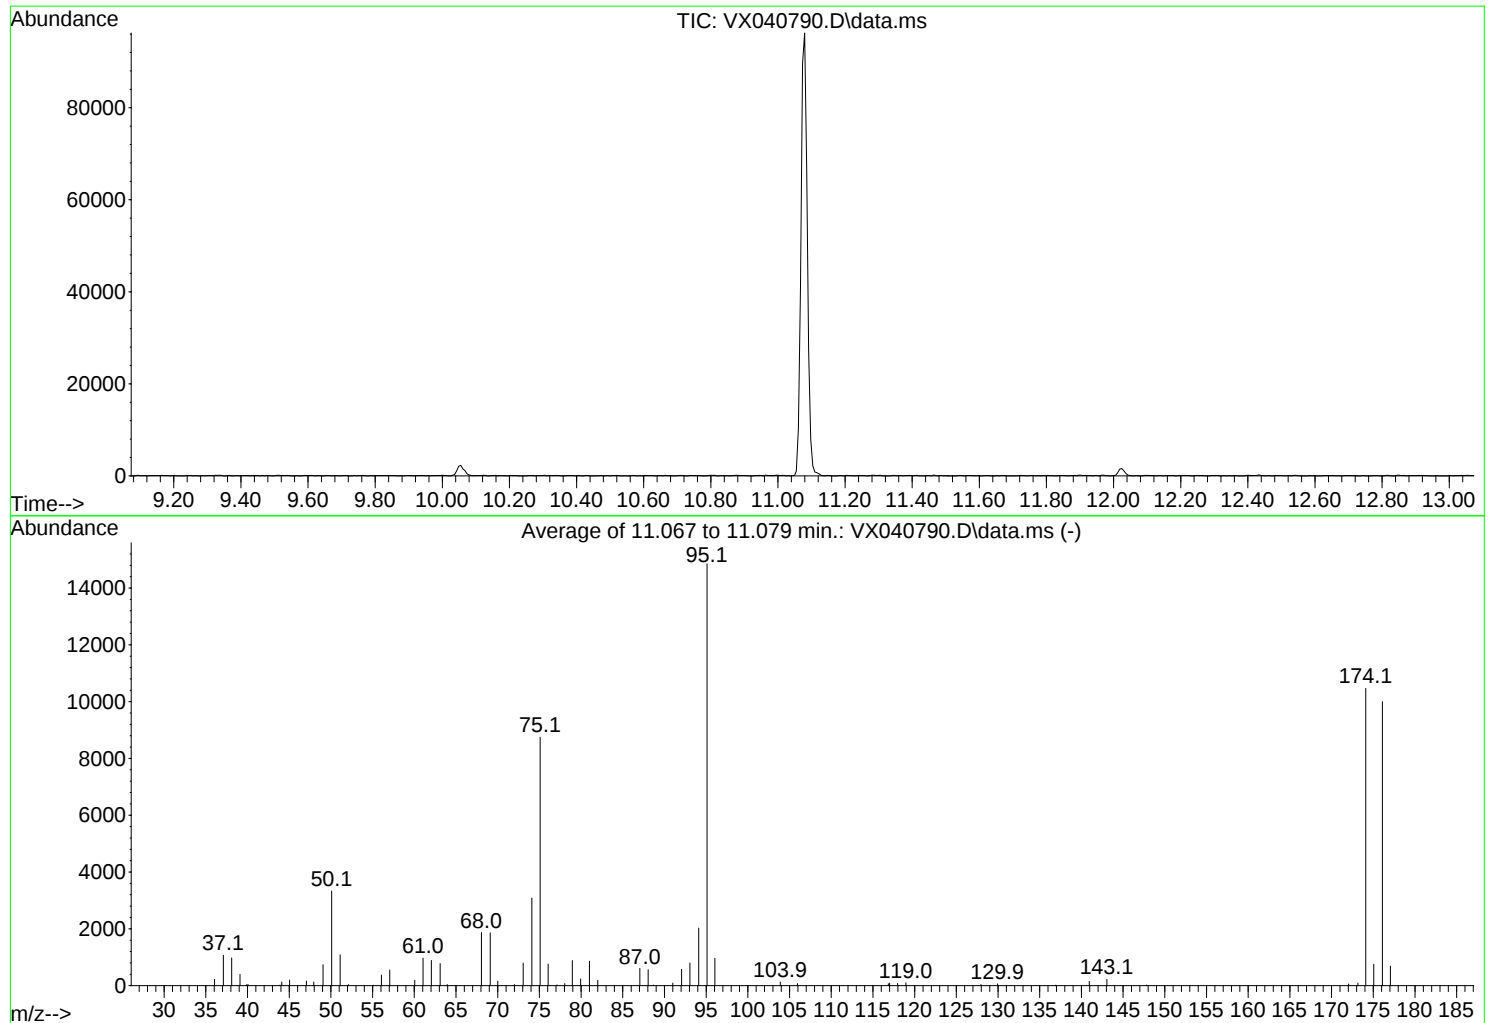

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.4	3328	PASS
75	95	30	60	58.9	8751	PASS
95	95	100	100	100.0	14854	PASS
96	95	5	9	6.5	963	PASS
173	174	0.00	2	0.9	92	PASS
174	95	50	100	70.5	10470	PASS
175	174	5	9	7.2	754	PASS
176	174	95	101	95.5	10003	PASS
177	176	5	9	6.9	686	PASS