

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032625\
 Data File : VX045469.D
 Acq On : 26 Mar 2025 14:53
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Mar 27 01:40:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	60498	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	119457	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	108100	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	41598	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	57484	59.735	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 119.480%	
35) Dibromofluoromethane	5.379	113	42339	53.005	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 106.000%	
50) Toluene-d8	8.647	98	147049	50.779	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 101.560%	
62) 4-Bromofluorobenzene	11.079	95	51013	53.161	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 106.320%	


Target Compounds				Qvalue		
3) Chloromethane	1.301	50	358	0.384	ug/l #	43
5) Bromomethane	1.593	94	237	0.652	ug/l #	40
9) 1,1,2-Trichlorotrifluo...	2.319	101	184	0.262	ug/l #	68
11) Tert butyl alcohol	2.934	59	655	3.593	ug/l #	73
13) Acrolein	2.227	56	128	0.607	ug/l #	44
15) Acrylonitrile	3.075	53	371	0.759	ug/l #	59
16) Acetone	2.386	43	796	1.783	ug/l #	75
17) Carbon Disulfide	2.502	76	1823	0.921	ug/l	98
18) Methyl Acetate	2.715	43	310	0.289	ug/l #	54
20) Methylene Chloride	2.788	84	249	0.282	ug/l #	87
21) trans-1,2-Dichloroethene	3.081	96	223	0.304	ug/l #	66
36) 1,1-Dichloropropene	5.702	75	223	0.204	ug/l #	42
38) Carbon Tetrachloride	5.544	117	7077	6.363	ug/l #	16
44) Trichloroethene	7.135	130	164	0.202	ug/l	56
64) Tetrachloroethene	9.281	164	193	0.279	ug/l #	48
68) m/p-Xylenes	10.305	106	474	0.325	ug/l	89
76) 1,2,3-Trichloropropane	11.079	75	29466	30.434	ug/l #	36
81) trans-1,4-Dichloro-2-b...	11.079	75	29466	104.150	ug/l #	6
82) 4-Chlorotoluene	11.457	91	862	0.339	ug/l	87
84) 1,2,4-Trimethylbenzene	11.756	105	591	0.224	ug/l	77
85) sec-Butylbenzene	11.890	105	717	0.222	ug/l	100
86) p-Isopropyltoluene	12.012	119	638	0.244	ug/l #	73
87) 1,3-Dichlorobenzene	11.969	146	424	0.310	ug/l	91
88) 1,4-Dichlorobenzene	11.969	146	424	0.307	ug/l	89
89) n-Butylbenzene	12.341	91	807	0.359	ug/l #	80
91) 1,2-Dichlorobenzene	12.341	146	370	0.270	ug/l	87
93) 1,2,4-Trichlorobenzene	13.591	180	609	0.780	ug/l	94
94) Hexachlorobutadiene	13.725	225	119	0.372	ug/l #	59
95) Naphthalene	13.780	128	2823	0.941	ug/l #	96
96) 1,2,3-Trichlorobenzene	13.963	180	766	0.930	ug/l	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032625\
Data File : VX045469.D
Acq On : 26 Mar 2025 14:53
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Mar 27 01:40:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




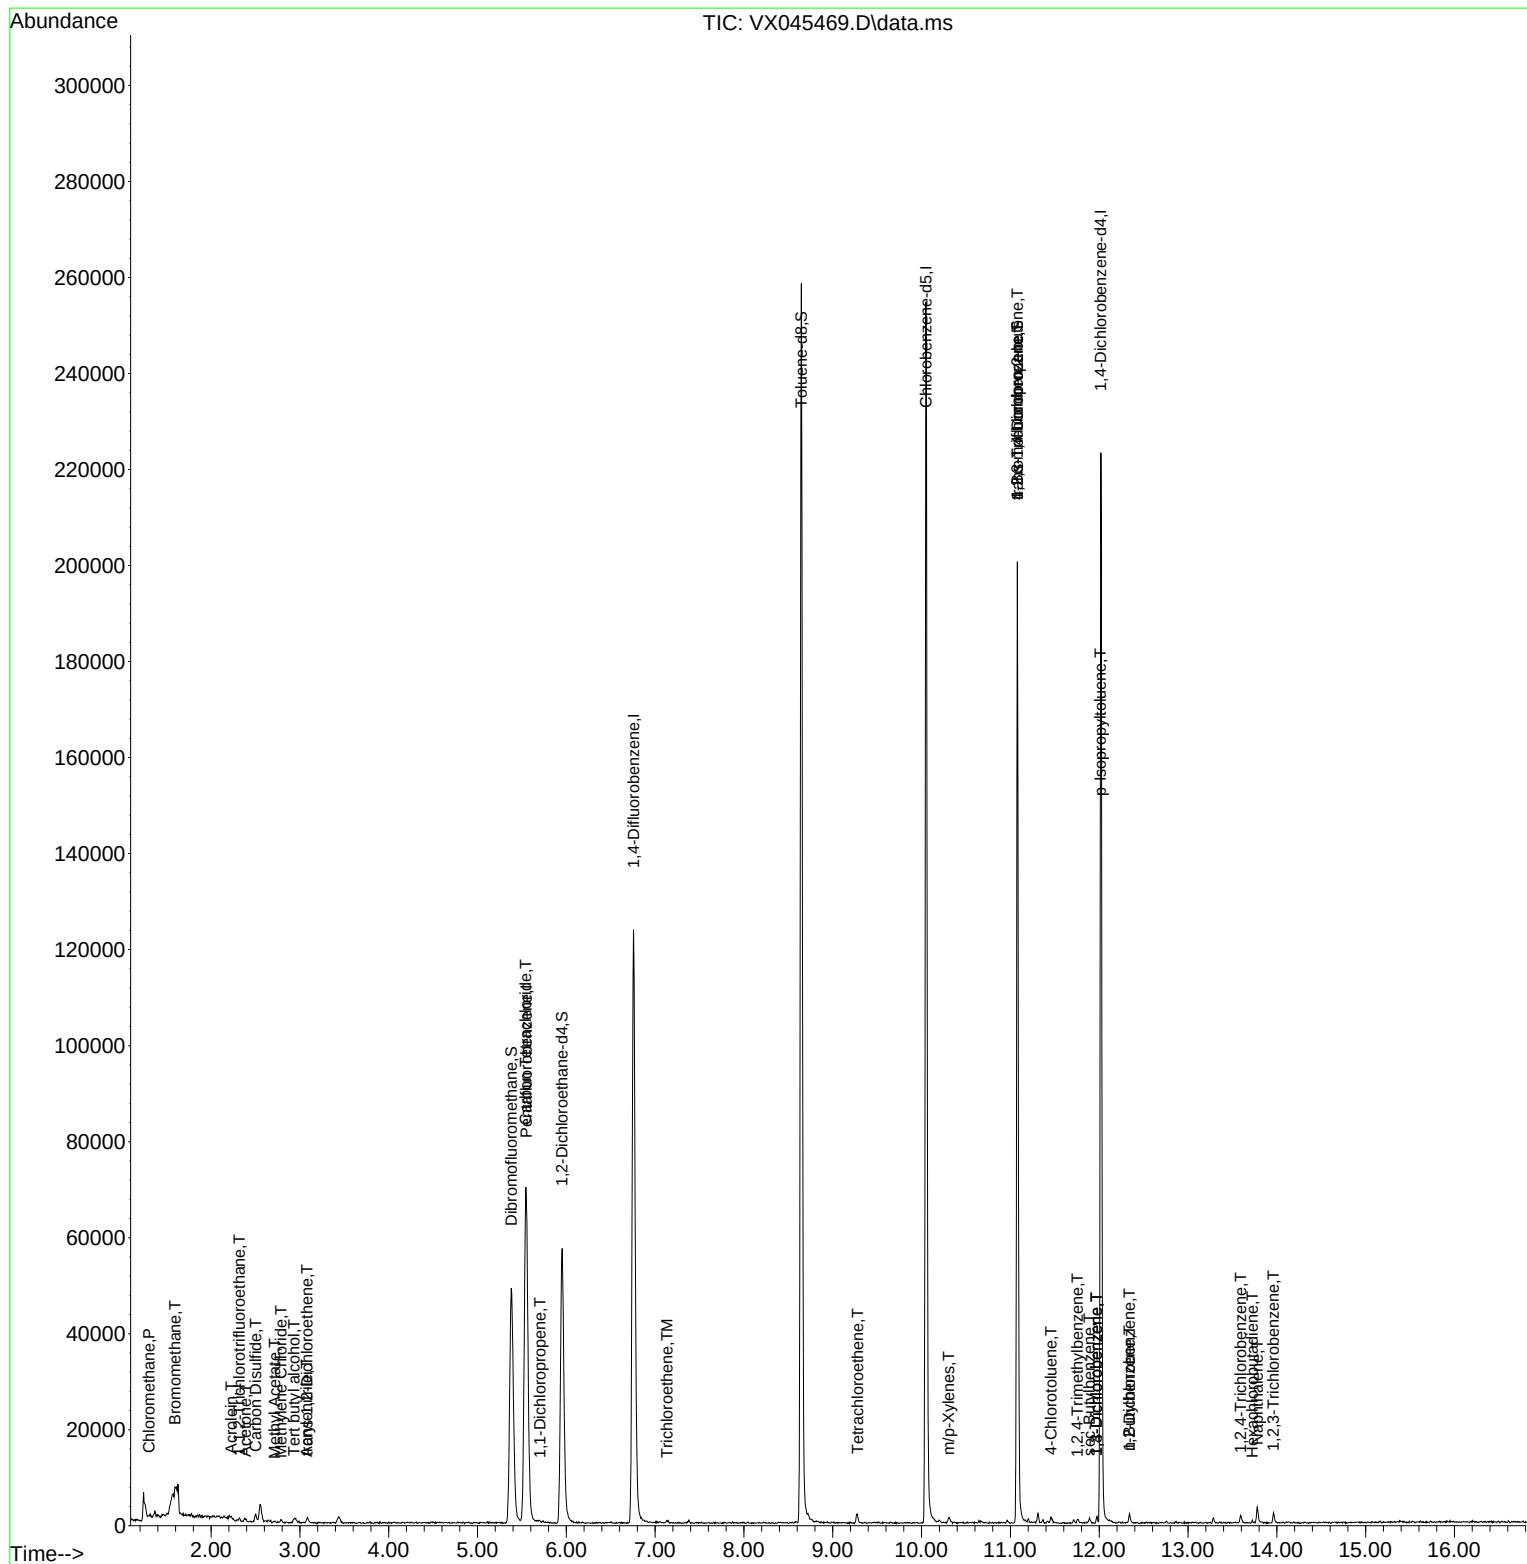




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 60498
Ion Ratio Lower Upper
168 100
99 65.0 48.2 72.4

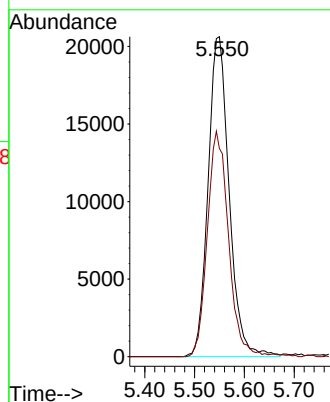

#3
Chloromethane
Concen: 0.384 ug/l
RT: 1.301 min Scan# 35
Delta R.T. -0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion: 50 Resp: 358
Ion Ratio Lower Upper
50 100
52 0.0 25.0 37.4#


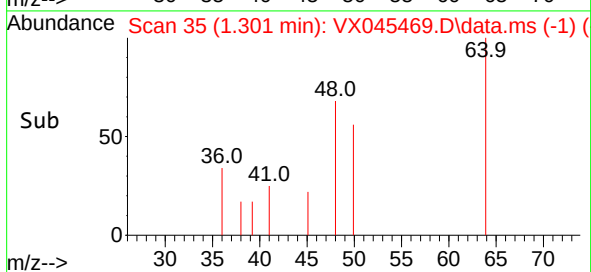
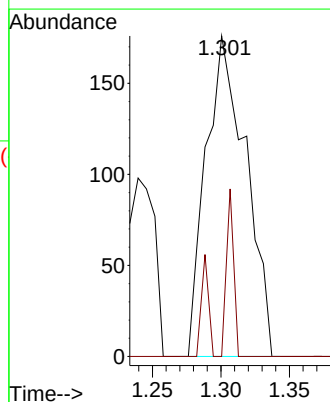



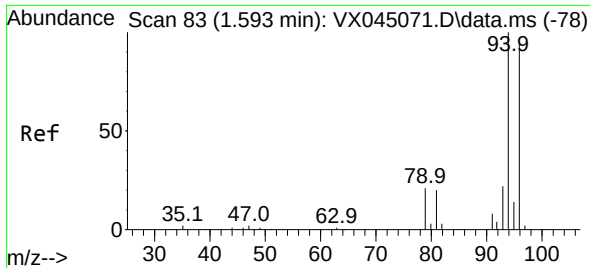

#5
Bromomethane
Concen: 0.652 ug/l
RT: 1.593 min Scan# 81
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 94 Resp: 237
Ion Ratio Lower Upper
94 100
96 35.9 75.0 112.4#

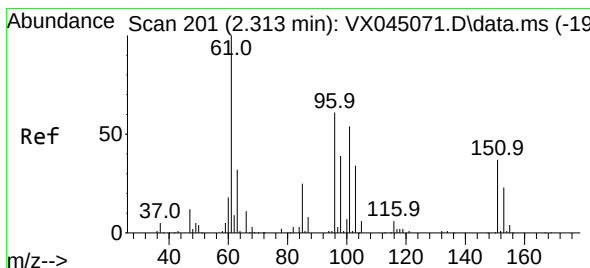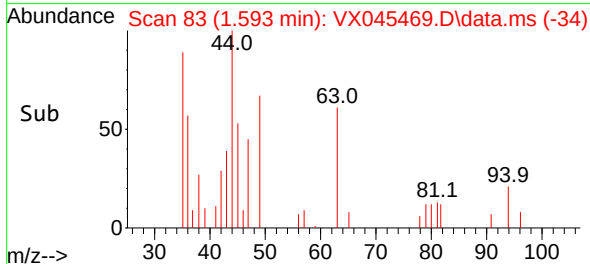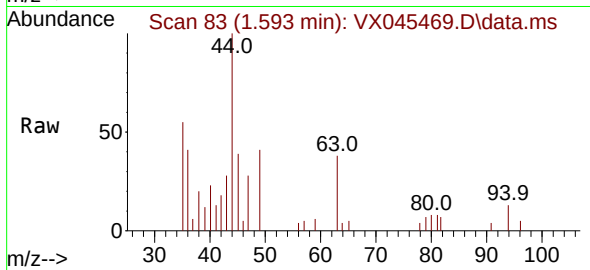

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.262 ug/l
RT: 2.319 min Scan# 202
Delta R.T. 0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion:101 Resp: 184
Ion Ratio Lower Upper
101 100
85 22.8 36.2 54.4#
151 45.1 56.4 84.6#

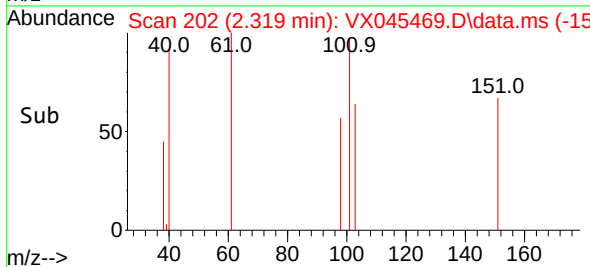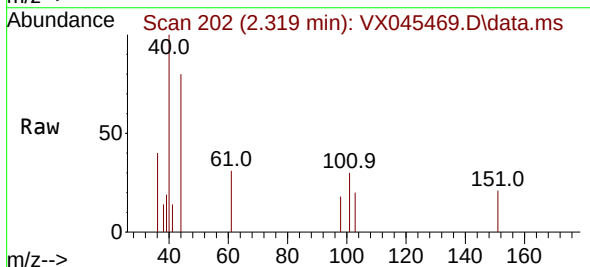

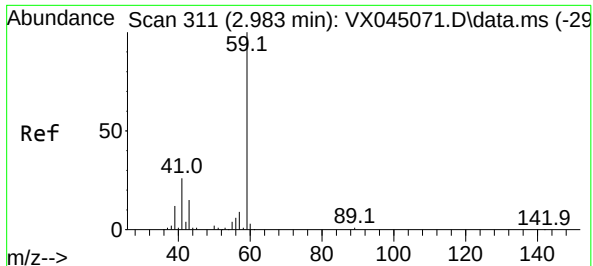

#11

Tert butyl alcohol

Concen: 3.593 ug/l

RT: 2.934 min Scan# 30

Delta R.T. -0.049 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 59 Resp: 655

Ion Ratio Lower Upper

59 100

57 0.0 7.8 11.8#

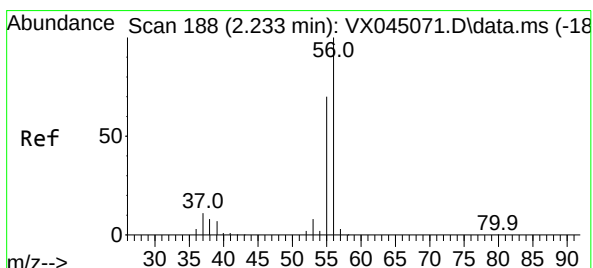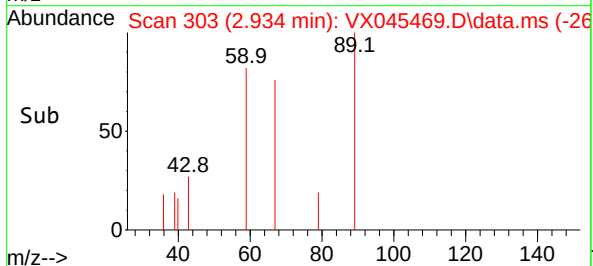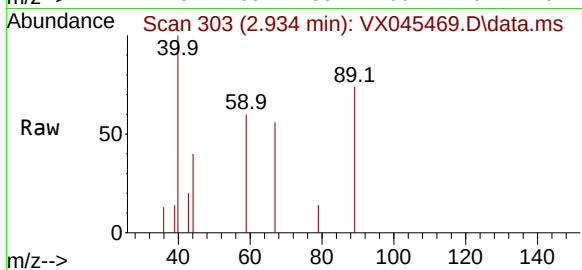

#13

Acrolein

Concen: 0.607 ug/l

RT: 2.227 min Scan# 187

Delta R.T. -0.006 min

Lab File: VX045469.D




Acq: 26 Mar 2025 14:53


Tgt Ion: 56 Resp: 128

Ion Ratio Lower Upper

56 100

55 24.2 56.2 84.4#


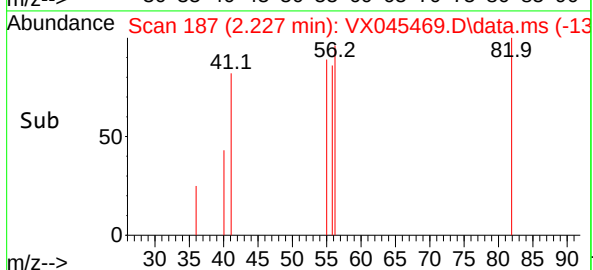

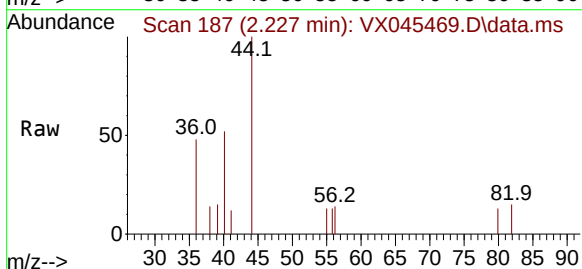




#15
 Acrylonitrile
 Concen: 0.759 ug/l
 RT: 3.075 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: VX045469.D
 Acq: 26 Mar 2025 14:53




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion	Ratio	Lower	Upper
53	100		
52	41.5	66.2	99.2#
51	18.9	29.0	43.4#

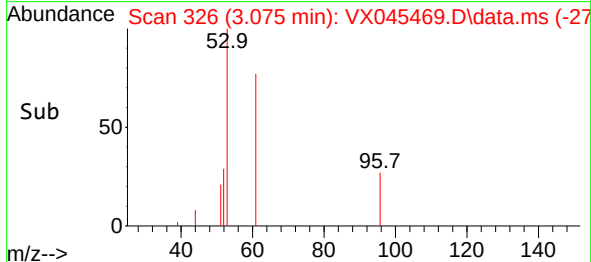

#16
 Acetone
 Concen: 1.783 ug/l
 RT: 2.386 min Scan# 213
 Delta R.T. -0.000 min
 Lab File: VX045469.D
 Acq: 26 Mar 2025 14:53

Tgt Ion	Ratio	Lower	Upper
43	100		
58	16.6	24.2	36.4#




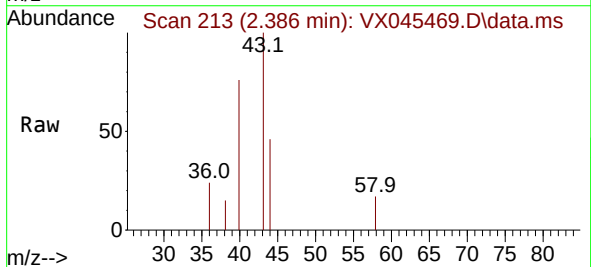




#17
Carbon Disulfide
Concen: 0.921 ug/l
RT: 2.502 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 76 Resp: 1823
Ion Ratio Lower Upper
76 100
78 8.9 6.6 9.8

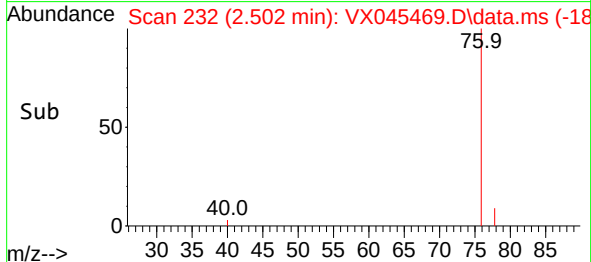

#18
Methyl Acetate
Concen: 0.289 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.012 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion: 43 Resp: 310
Ion Ratio Lower Upper
43 100
74 0.0 17.4 26.2#




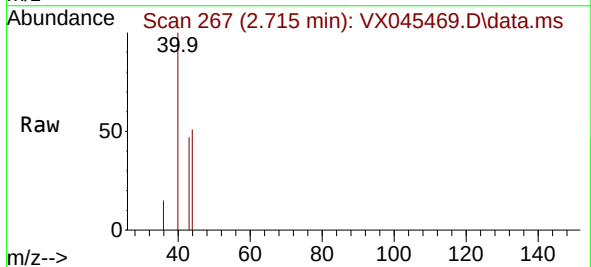




#20
Methylene Chloride
Concen: 0.282 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:	84	Resp:	249
Ion	Ratio	Lower	Upper
84	100		
49	131.5	106.5	159.7
51	0.0	32.1	48.1#
86	67.3	50.0	75.0

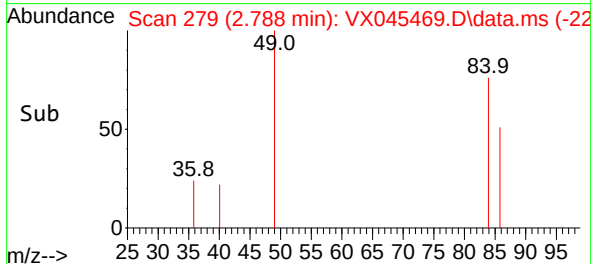

#21
trans-1,2-Dichloroethene
Concen: 0.304 ug/l
RT: 3.081 min Scan# 327
Delta R.T. -0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion:	96	Resp:	223
Ion	Ratio	Lower	Upper
96	100		
61	132.0	117.0	175.4
98	0.0	53.4	80.2#

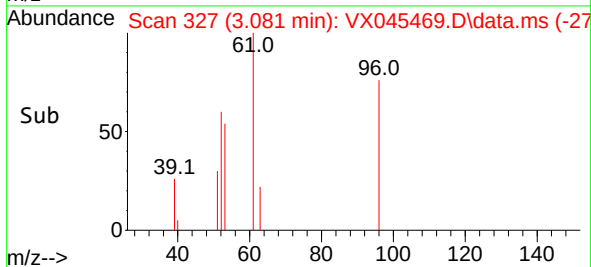



#33

1,2-Dichloroethane-d4

Concen: 59.735 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 65 Resp: 57484

Ion Ratio Lower Upper

65 100

67 48.6 0.0 106.2

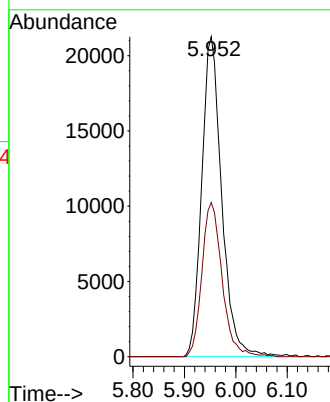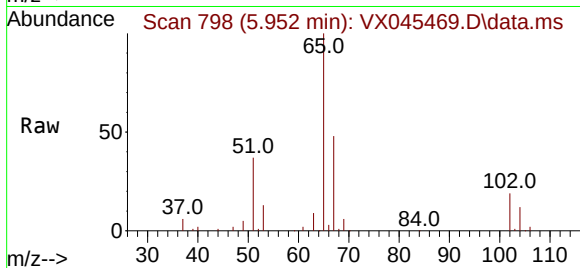

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53




Tgt Ion: 114 Resp: 119457


Ion Ratio Lower Upper

114 100

63 24.0 0.0 41.8

88 16.9 0.0 32.8


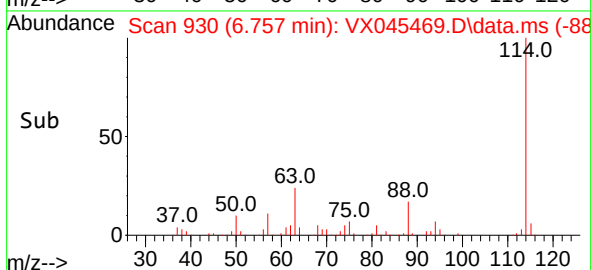

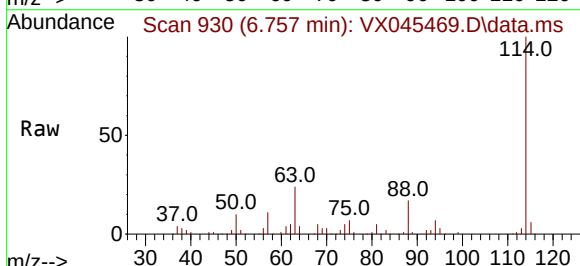


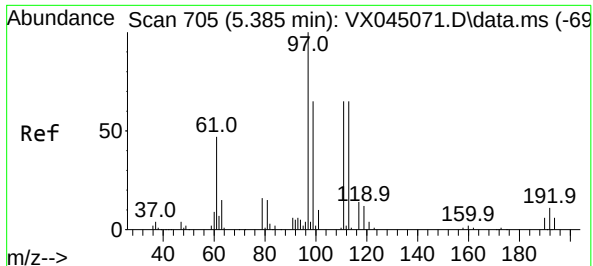

#35
Dibromofluoromethane
Concen: 53.005 ug/l
RT: 5.379 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:113 Resp: 42339
Ion Ratio Lower Upper
113 100
111 103.3 81.8 122.6
192 17.0 14.3 21.5

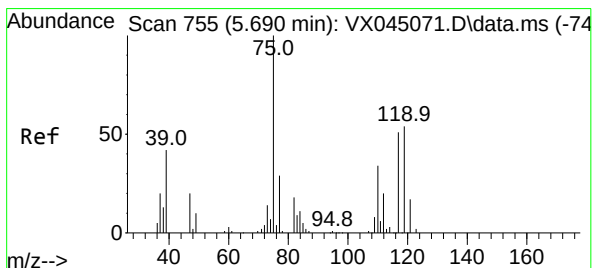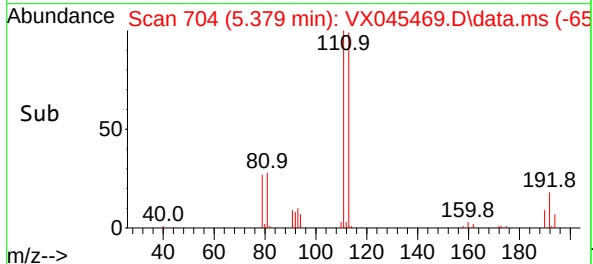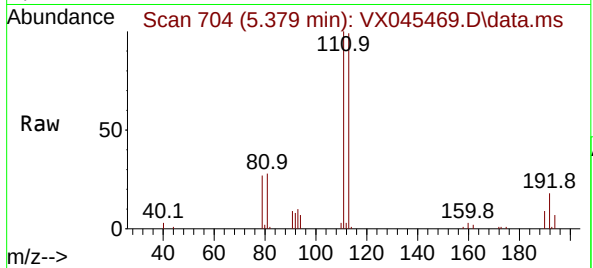

#36
1,1-Dichloropropene
Concen: 0.204 ug/l
RT: 5.702 min Scan# 757
Delta R.T. 0.012 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53


Tgt Ion: 75 Resp: 223
Ion Ratio Lower Upper
75 100
110 0.0 16.9 50.6#
77 0.0 24.5 36.7#

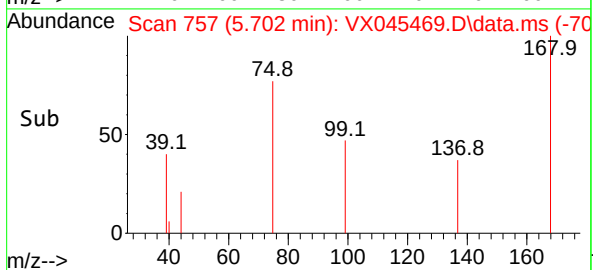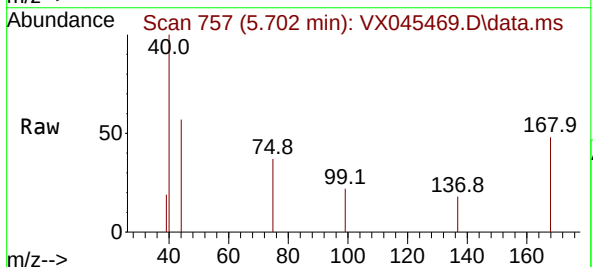






#38
Carbon Tetrachloride
Concen: 6.363 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Instrument :
MSVOA_X
ClientSampleId :
IBLK







Tgt Ion:117 Resp: 7077
Ion Ratio Lower Upper
117 100
119 5.2 76.7 115.1#
121 0.0 25.5 38.3#

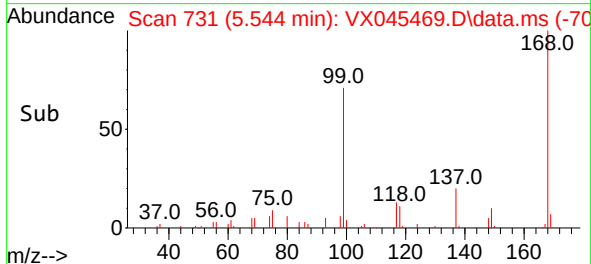

#44
Trichloroethene
Concen: 0.202 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.012 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion:130 Resp: 164
Ion Ratio Lower Upper
130 100
95 147.2 0.0 205.0


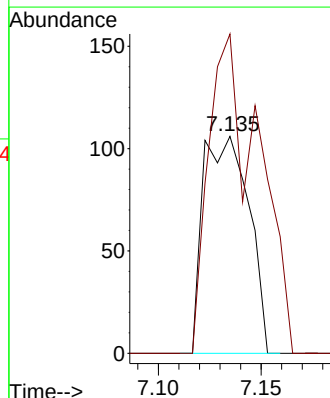

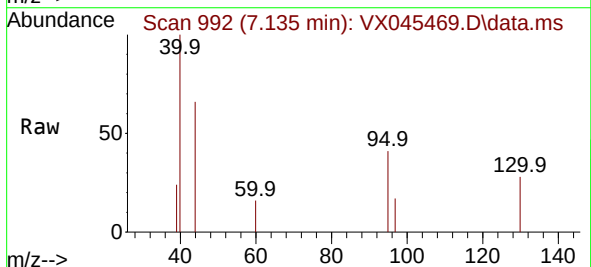




#50
Toluene-d8
Concen: 50.779 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 147049
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

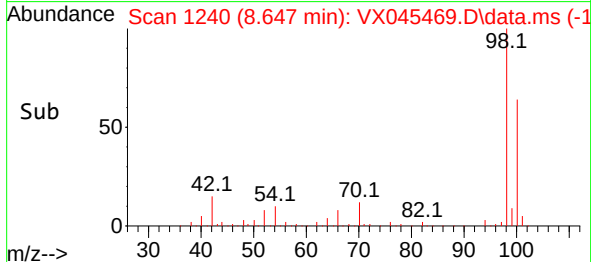

#62
4-Bromofluorobenzene
Concen: 53.161 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion: 95 Resp: 51013
Ion Ratio Lower Upper
95 100
174 69.8 0.0 148.2
176 67.0 0.0 141.4



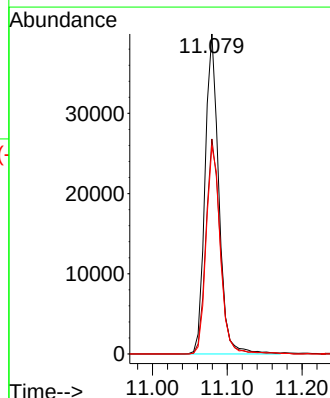





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 108100
Ion Ratio Lower Upper
117 100
82 62.0 46.3 69.5
119 32.6 25.7 38.5

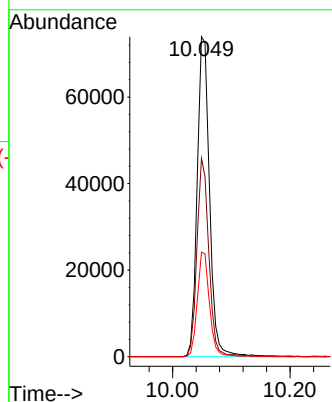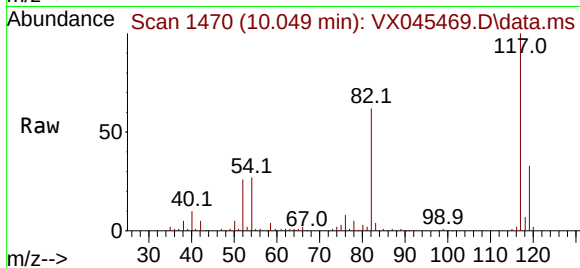

#64
Tetrachloroethene
Concen: 0.279 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.012 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion:164 Resp: 193
Ion Ratio Lower Upper
164 100
166 59.2 103.6 155.4#
129 73.5 82.7 124.1#
131 35.4 80.5 120.7#


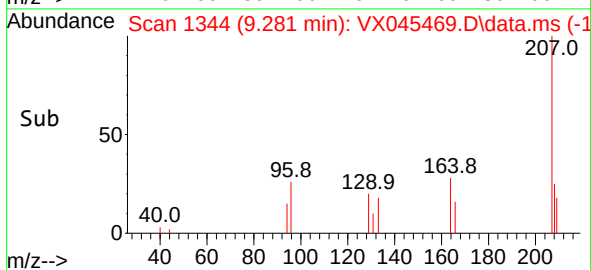

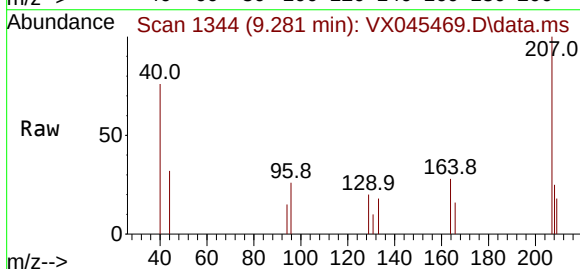




#68
m/p-Xylenes
Concen: 0.325 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:106 Resp: 474
Ion Ratio Lower Upper
106 100
91 190.3 165.4 248.0

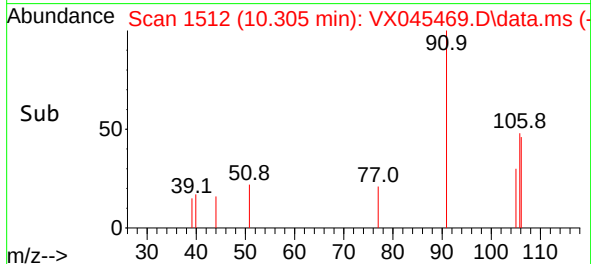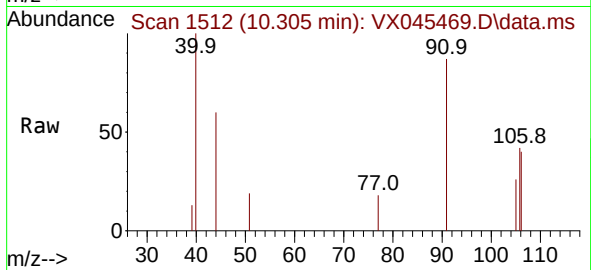

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion:152 Resp: 41598
Ion Ratio Lower Upper
152 100
115 62.8 44.2 132.6
150 157.2 0.0 349.0


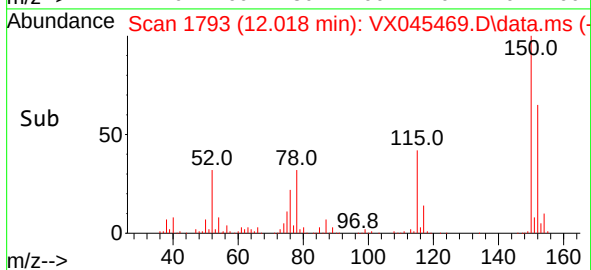

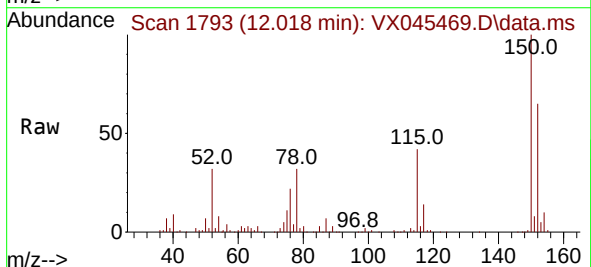




#76
1,2,3-Trichloropropane
Concen: 30.434 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 75 Resp: 29466
Ion Ratio Lower Upper
75 100
77 1.1 20.7 62.1#

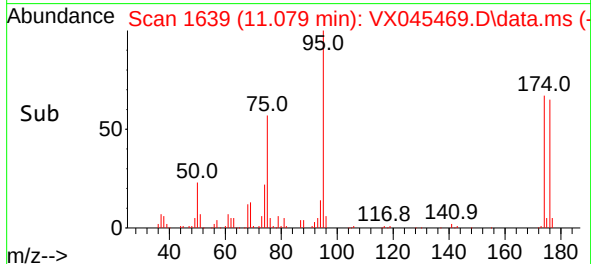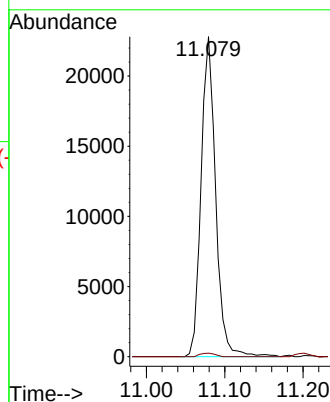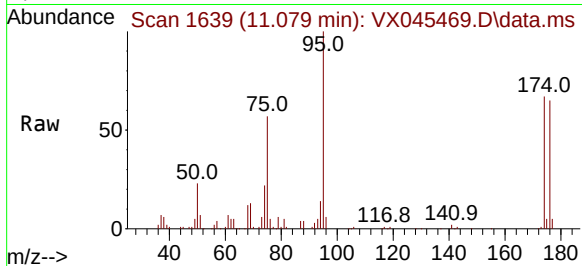

#81
trans-1,4-Dichloro-2-butene
Concen: 104.150 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion: 75 Resp: 29466
Ion Ratio Lower Upper
75 100
53 0.0 88.5 132.7#
89 0.0 36.2 54.4#




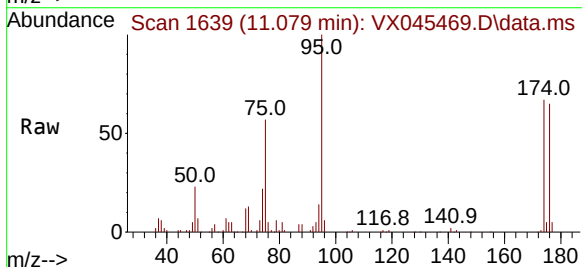




#82
4-Chlorotoluene
Concen: 0.339 ug/l
RT: 11.457 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 91 Resp: 862
Ion Ratio Lower Upper
91 100
126 21.7 14.1 42.4

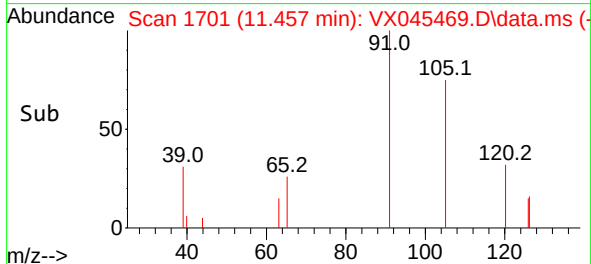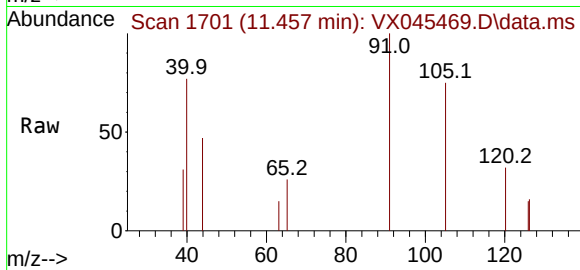

#84
1,2,4-Trimethylbenzene
Concen: 0.224 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion: 105 Resp: 591
Ion Ratio Lower Upper
105 100
120 29.1 22.1 66.1




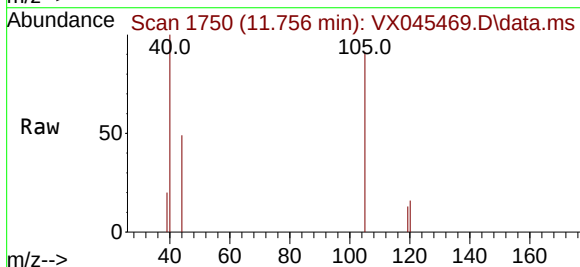




#85
 sec-Butylbenzene
 Concen: 0.222 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. -0.000 min
 Lab File: VX045469.D
 Acq: 26 Mar 2025 14:53




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion:105 Resp: 717
 Ion Ratio Lower Upper
 105 100
 134 19.8 9.8 29.4

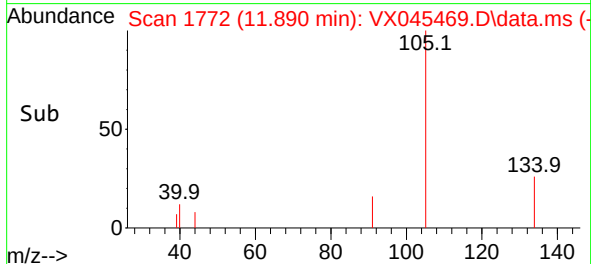

#86
 p-Isopropyltoluene
 Concen: 0.244 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.006 min
 Lab File: VX045469.D
 Acq: 26 Mar 2025 14:53

Tgt Ion:119 Resp: 638
 Ion Ratio Lower Upper
 119 100
 134 22.1 12.9 38.6
 91 48.7 12.7 38.0#


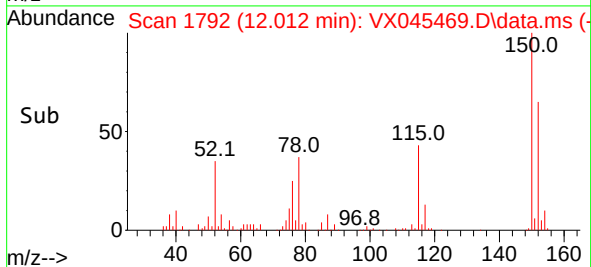






#87
1,3-Dichlorobenzene
Concen: 0.310 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.000 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:146 Resp: 424
Ion Ratio Lower Upper
146 100
111 47.2 21.1 63.4
148 71.9 31.9 95.7

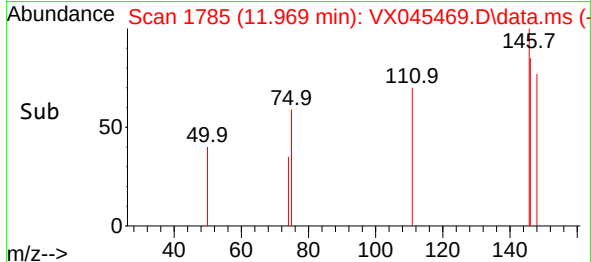

#88
1,4-Dichlorobenzene
Concen: 0.307 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.067 min
Lab File: VX045469.D
Acq: 26 Mar 2025 14:53

Tgt Ion:146 Resp: 424
Ion Ratio Lower Upper
146 100
111 47.2 20.2 60.5
148 71.9 31.9 95.9

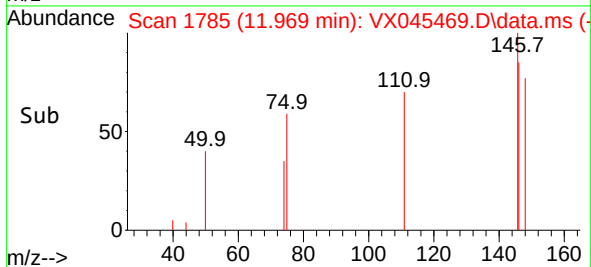



#89

n-Butylbenzene

Concen: 0.359 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.012 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion: 91 Resp: 807

Ion Ratio Lower Upper

91 100

92 45.6 26.7 80.0

134 3.8 12.2 36.6#

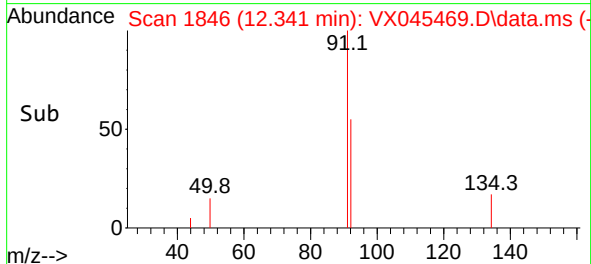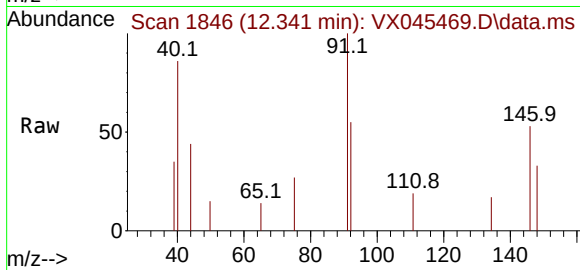

#91

1,2-Dichlorobenzene

Concen: 0.270 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.006 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53




Tgt Ion:146 Resp: 370


Ion Ratio Lower Upper

146 100

111 33.0 21.6 65.0

148 54.9 31.9 95.9

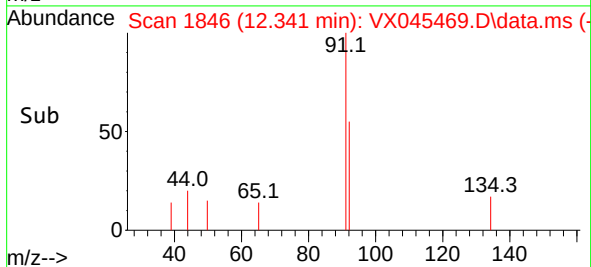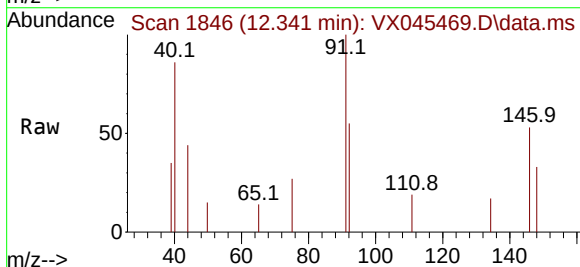



#93

1,2,4-Trichlorobenzene

Concen: 0.780 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:180 Resp: 609

Ion Ratio Lower Upper

180 100

182 93.6 47.3 141.9

145 21.7 16.3 48.9

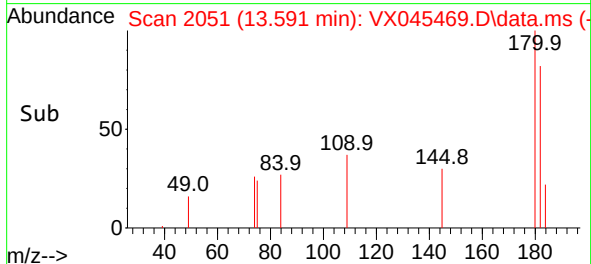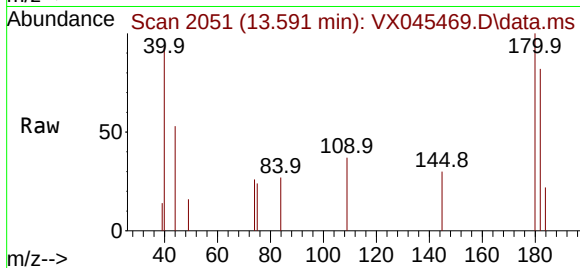

#94

Hexachlorobutadiene

Concen: 0.372 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. -0.000 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53




Tgt Ion:225 Resp: 119


Ion Ratio Lower Upper

225 100

223 41.2 31.9 95.7

227 21.0 31.4 94.0#

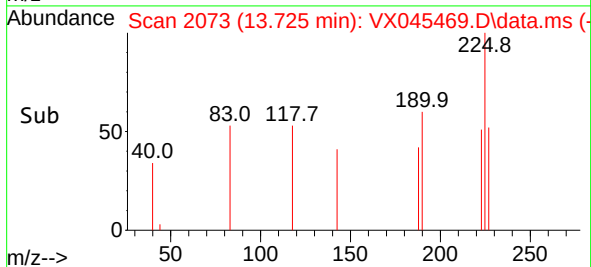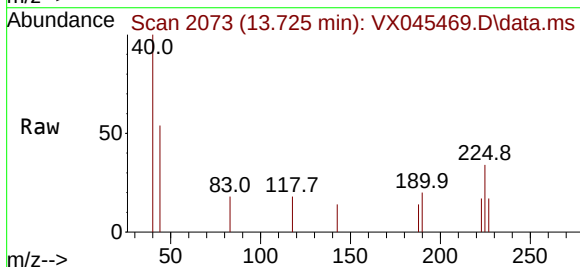



#95

Naphthalene

Concen: 0.941 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:128 Resp: 2823

Ion Ratio Lower Upper

128 100

127 12.3 10.3 15.5

129 7.9 8.7 13.1#

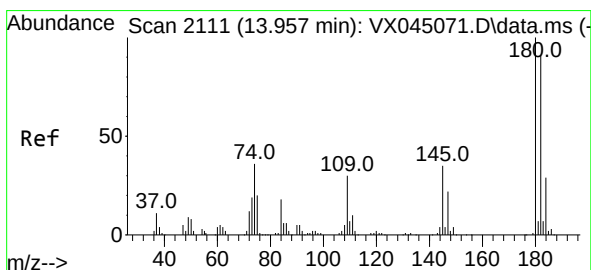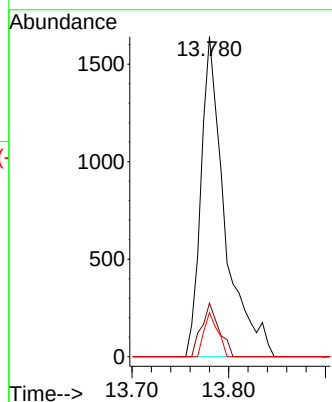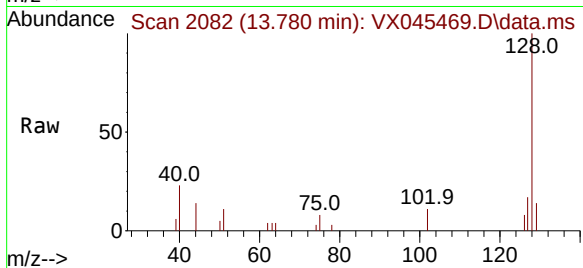

#96

1,2,3-Trichlorobenzene

Concen: 0.930 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. 0.006 min

Lab File: VX045469.D

Acq: 26 Mar 2025 14:53

Tgt Ion:180 Resp: 766

Ion Ratio Lower Upper

180 100

182 66.4 47.5 142.6

145 26.9 17.0 50.9

