

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032719\
 Data File : VX008486.D
 Acq On : 27 Mar 2019 16:39
 Operator : JC/SP
 Sample : K2099-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-C02-SETTLED-1H-A

Quant Time: Mar 28 10:01:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X032719W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Mar 27 12:01:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.01	128	35432	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.86	114	204473	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.11	117	173754	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.06	65	90054	30.38	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	101.27%
60) 4-Bromofluorobenzene	11.13	95	87712	28.97	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	96.57%
63) Toluene-d8	8.71	98	253796	30.77	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	102.57%


Target Compounds					Ovalue
15) Acetone	2.44	58	3508	6.766 ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032719\
Data File : VX008486.D
Acq On : 27 Mar 2019 16:39
Operator : JC/SP
Sample : K2099-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-C02-SETTLED-1H-A

Quant Time: Mar 28 10:01:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X032719W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Mar 27 12:01:15 2019
Response via : Initial Calibration

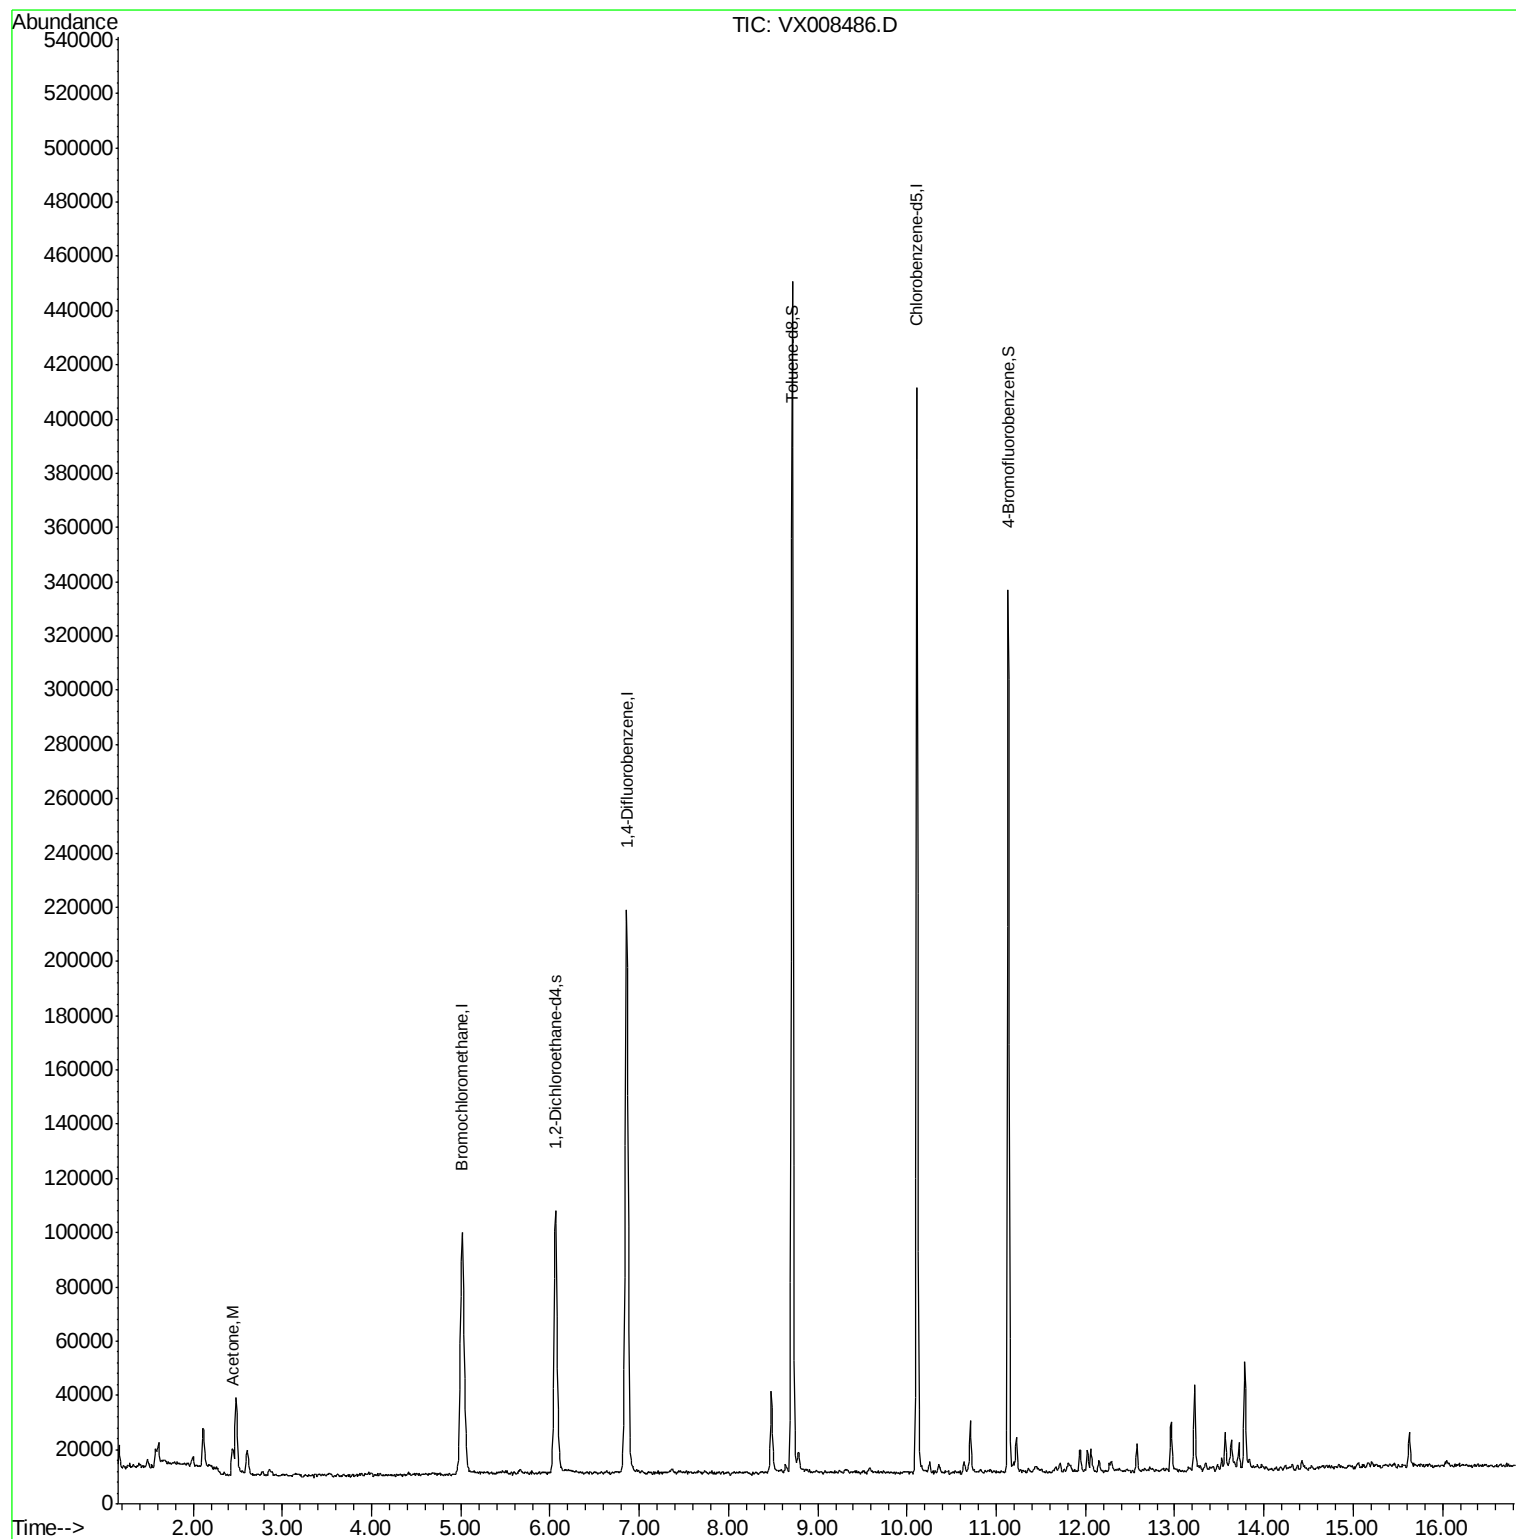

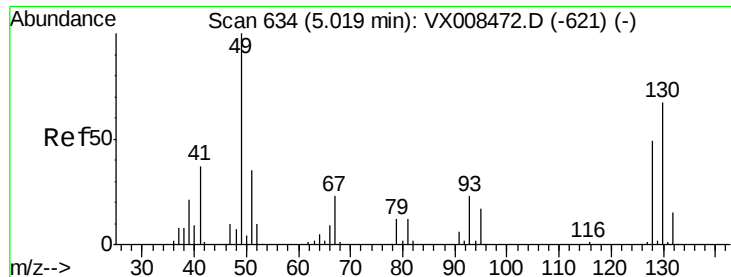

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.01 min Scan# 633

Delta R.T. -0.01 min

Lab File: VX008486.D

Acq: 27 Mar 2019 16:39

Instrument :

MSVOA_X

ClientSampleId :

MH-C02-SETTLED-1H-A


Tot Ion:128 Resp: 35432

Ion Ratio Lower Upper

128 100

49 205.0 0.0 350.8




130 128.4 0.0 325.8

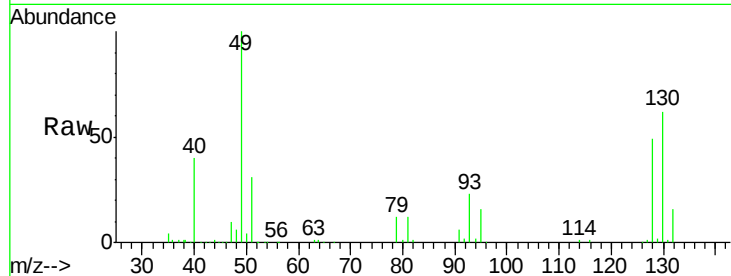

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

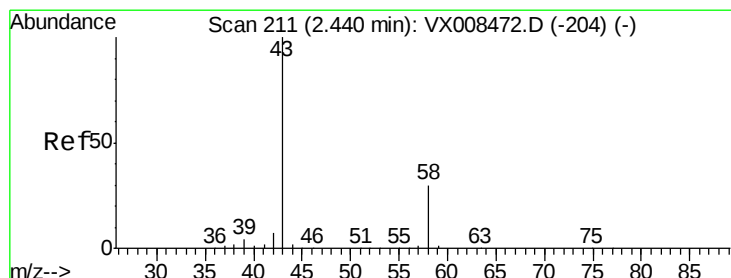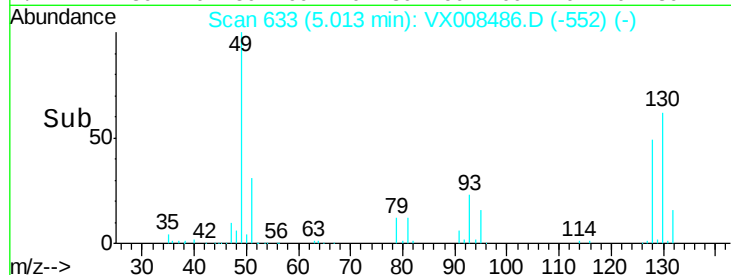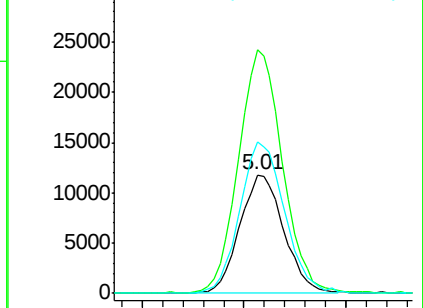

#15

Acetone

Concen: 6.766 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.00 min

Lab File: VX008486.D


Acq: 27 Mar 2019 16:39

Tgt Ion: 58 Resp: 3508

Ion Ratio Lower Upper



58 100


43 334.0 249.8 374.6

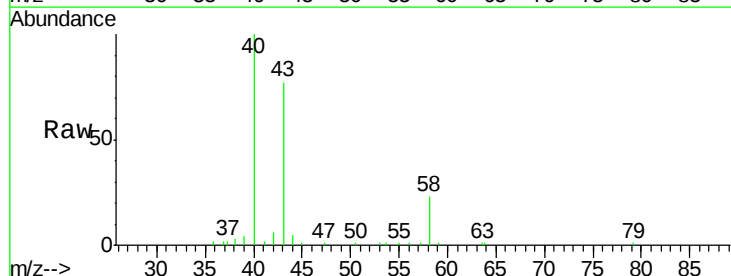

Abundance Ion 58.00 (57.70 to 58.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

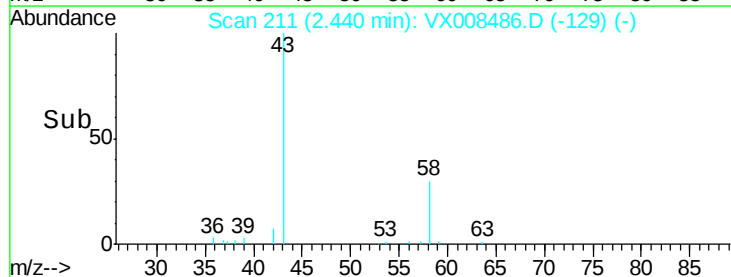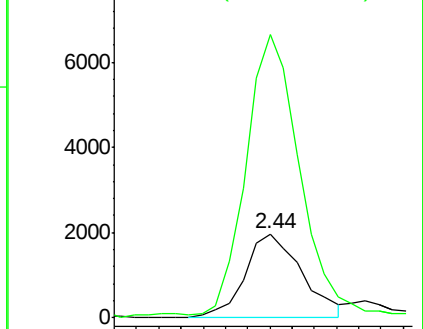

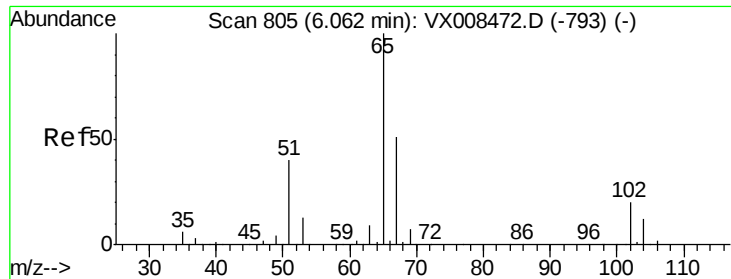

#27

1,2-Dichloroethane-d4

Concen: 30.382 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX008486.D

Acq: 27 Mar 2019 16:39

Instrument :

MSVOA_X

ClientSampleId :





MH-C02-SETTLED-1H-A

Tot Ion: 65 Resp: 90054

Ion Ratio Lower Upper

65 100

67 53.6 42.9 64.3

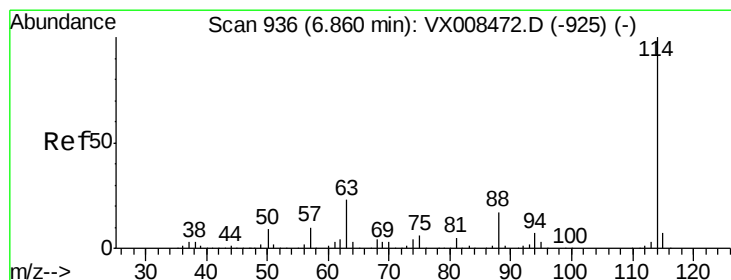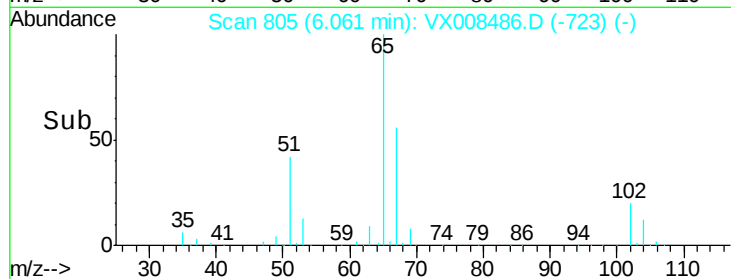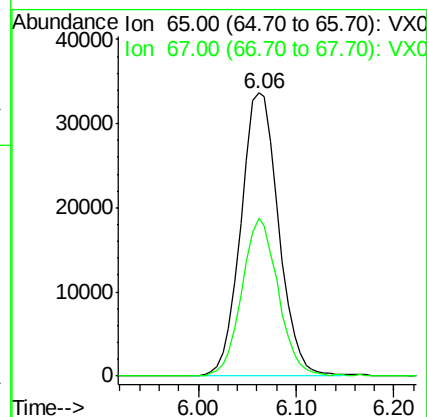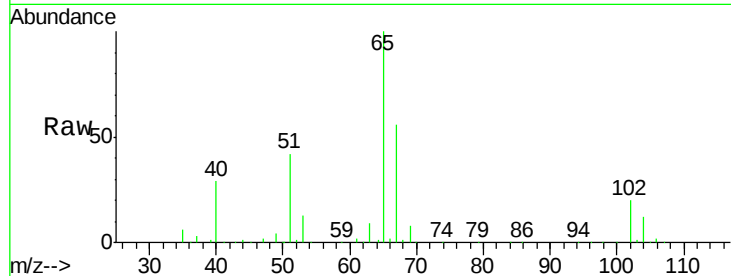

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX008486.D

Acq: 27 Mar 2019 16:39




Tgt Ion: 114 Resp: 204473


Ion Ratio Lower Upper

114 100

63 23.5 14.2 21.4#

88 16.6 11.9 17.9


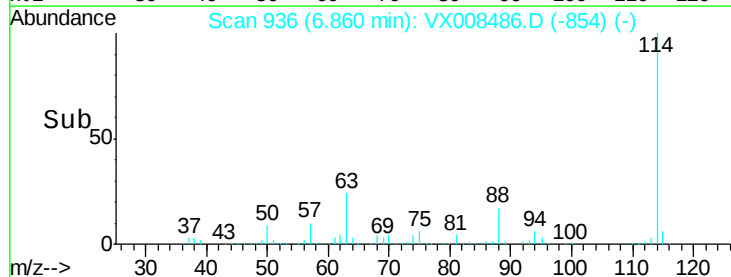
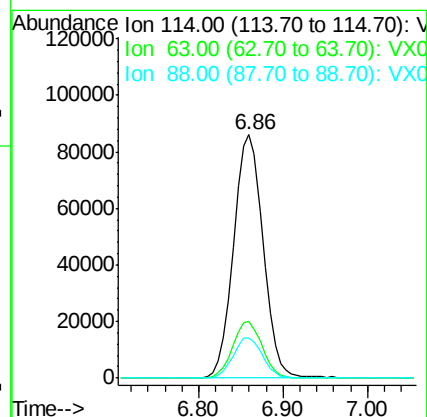
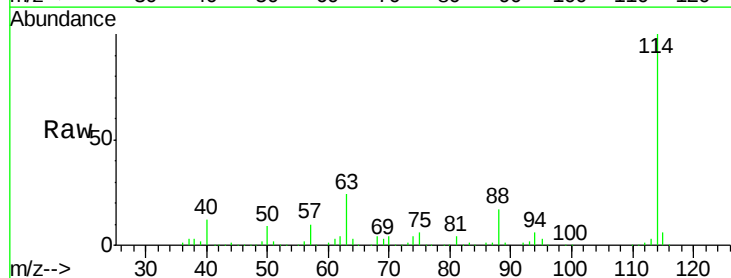


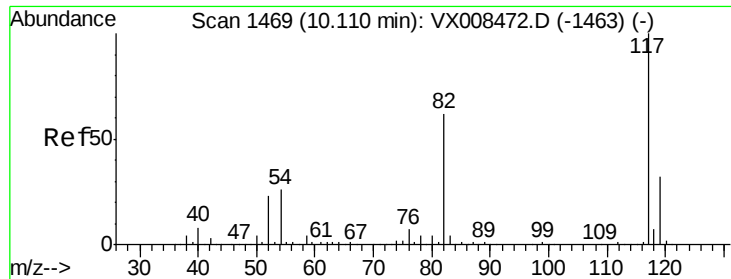

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX008486.D
Acq: 27 Mar 2019 16:39




Instrument :
MSVOA_X
ClientSampleId :
MH-C02-SETTLED-1H-A


Tot Ion:117 Resp: 173754
Ion Ratio Lower Upper
117 100
82 60.9 40.4 60.6#
119 32.1 25.8 38.6

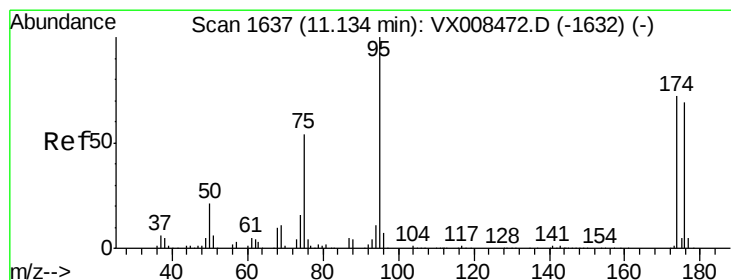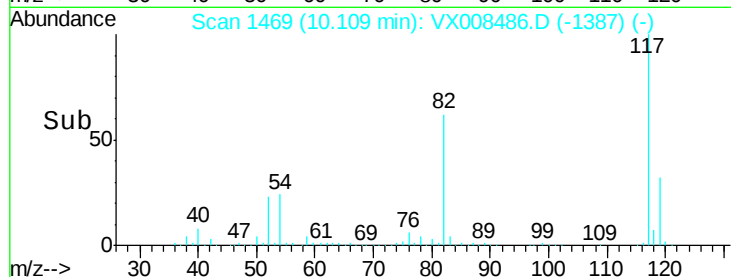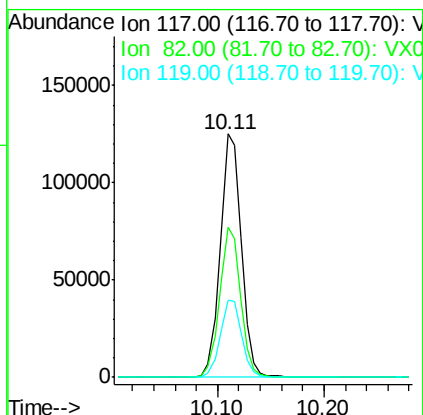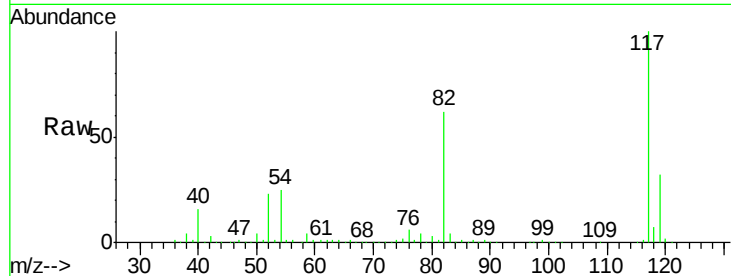

#60
4-Bromofluorobenzene
Concen: 28.973 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX008486.D
Acq: 27 Mar 2019 16:39

Tgt Ion: 95 Resp: 87712
Ion Ratio Lower Upper
95 100
174 73.4 74.9 112.3#
176 71.8 70.7 106.1

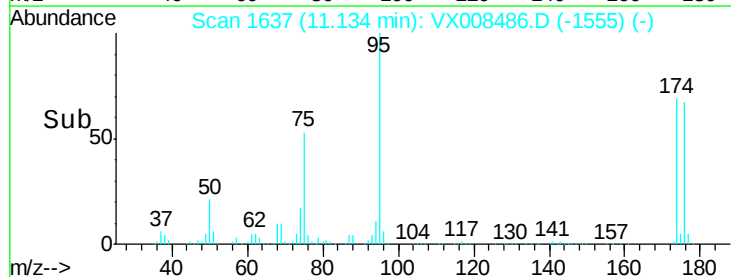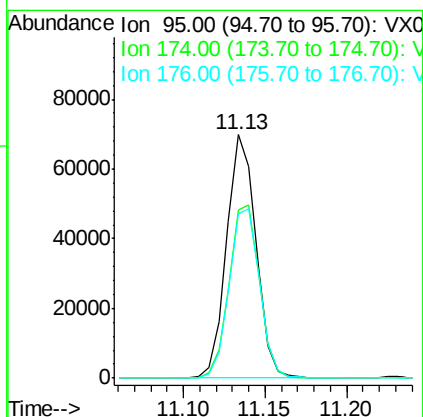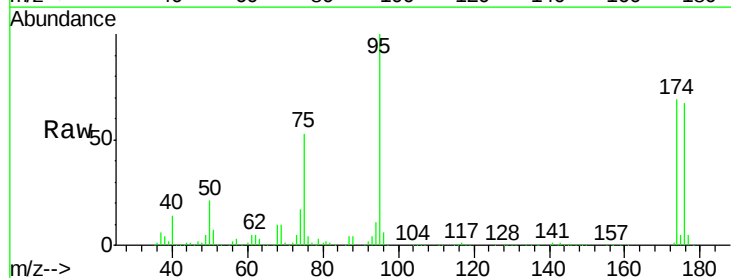

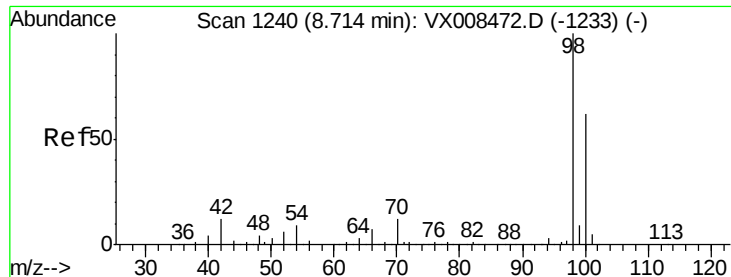

#63

Toluene-d8

Concen: 30.772 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX008486.D

Acq: 27 Mar 2019 16:39

Instrument :

MSVOA_X

ClientSampleId :


MH-C02-SETTLED-1H-A

Tot Ion: 98 Resp: 253796

Ion Ratio Lower Upper

98 100

100 63.9 50.9 76.3

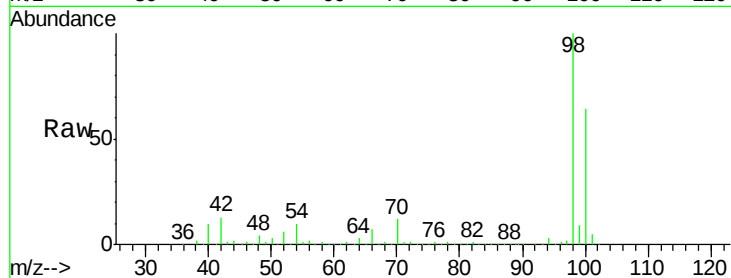

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

