

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032719\
 Data File : VX008503.D
 Acq On : 27 Mar 2019 23:12
 Operator : JC/SP
 Sample : K2137-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SEWER-OUTLET-02

Integration Parameters: RTEINT3.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X032719W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.440	204	211	230	rBV	1256745	2136716	8.52%	7.085%
2	2.629	230	242	264	rBV	11067723	25083641	100.00%	83.176%
3	5.013	622	633	645	rBV	85713	261773	1.04%	0.868%
4	6.061	792	805	819	rBV	94199	253067	1.01%	0.839%
5	6.860	926	936	947	rBV	206453	491426	1.96%	1.630%
6	8.713	1232	1240	1247	rBV	437853	675674	2.69%	2.240%
7	10.109	1464	1469	1477	rBV	400138	548693	2.19%	1.819%
8	11.133	1631	1637	1649	rVB	327640	418162	1.67%	1.387%
9	12.024	1778	1783	1787	rBV	251543	288281	1.15%	0.956%




Sum of corrected areas: 30157433

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032719\
Data File : VX008503.D
Acq On : 27 Mar 2019 23:12
Operator : JC/SP
Sample : K2137-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SEWER-OUTLET-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X032719W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

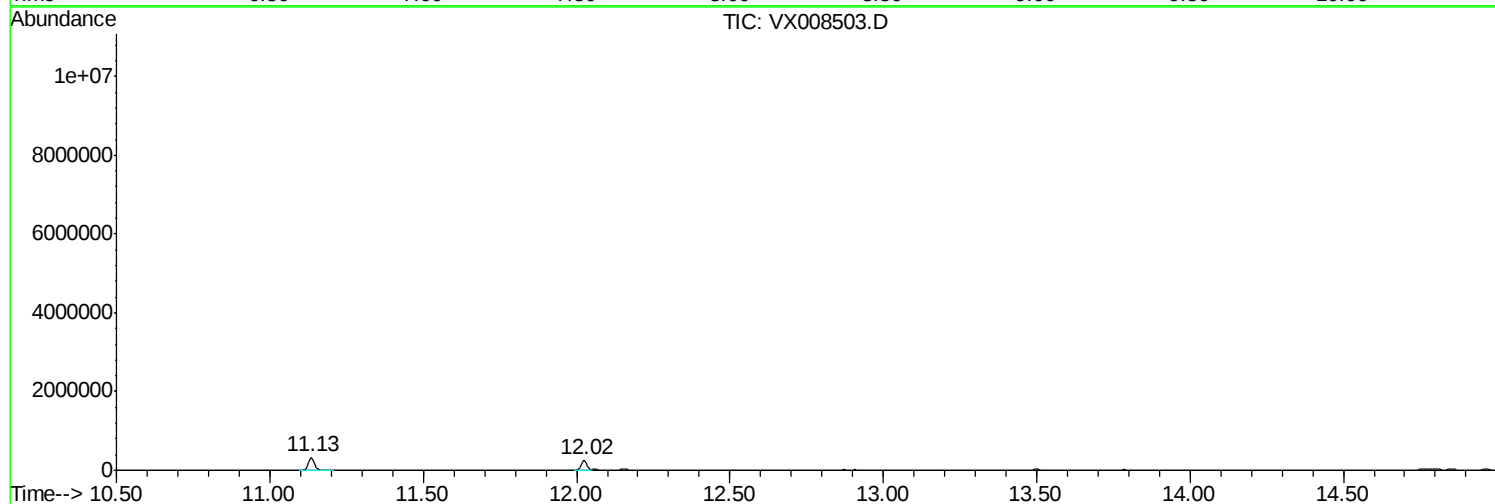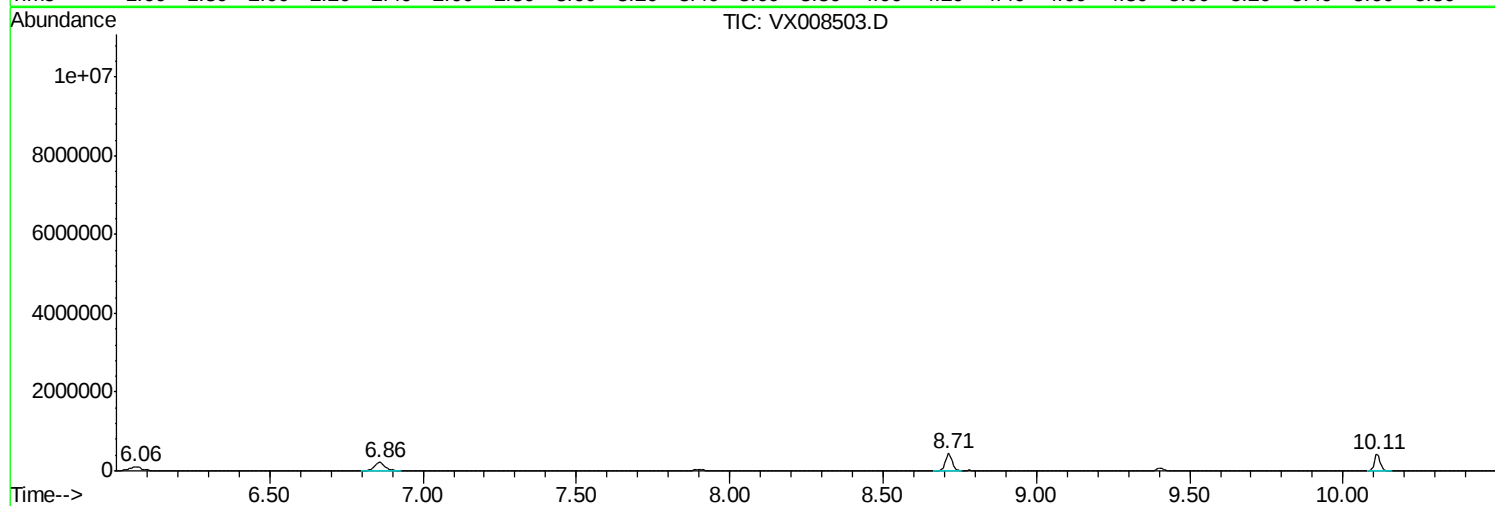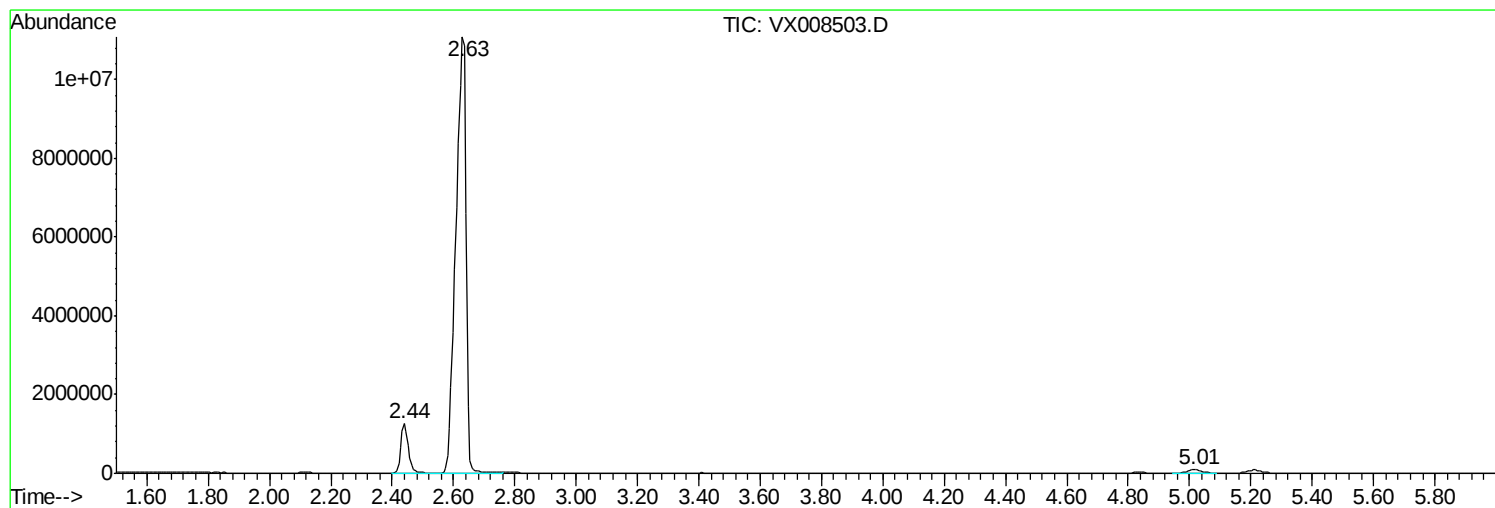

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX032719\
Data File : VX008503.D
Acq On : 27 Mar 2019 23:12
Operator : JC/SP
Sample : K2137-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 35 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
SEWER-OUTLET-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X032719W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.63	2874.66 ug/l	25083600	Bromochloromethane	5.01
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Isopropyl Alcohol	60 C3H8O	000067-63-0	86
2	Isopropyl Alcohol	60 C3H8O	000067-63-0	78
3	Isopropyl Alcohol	60 C3H8O	000067-63-0	78
4	Hydrazine, ethyl-	60 C2H8N2	000624-80-6	9
5	Hydrazine, 1,2-dimethyl-	60 C2H8N2	000540-73-8	9

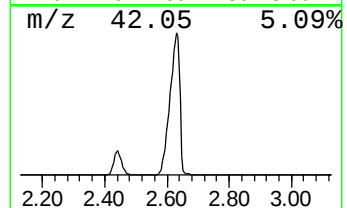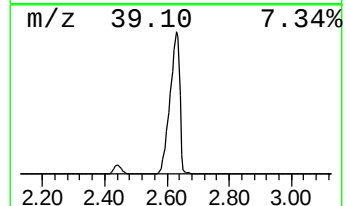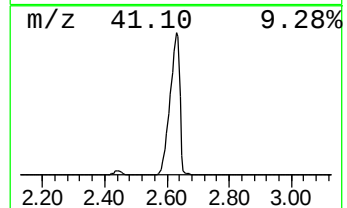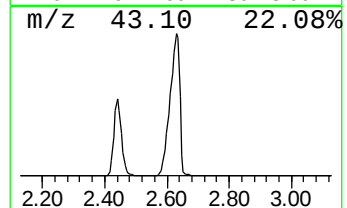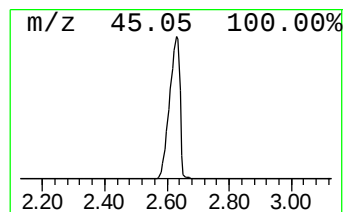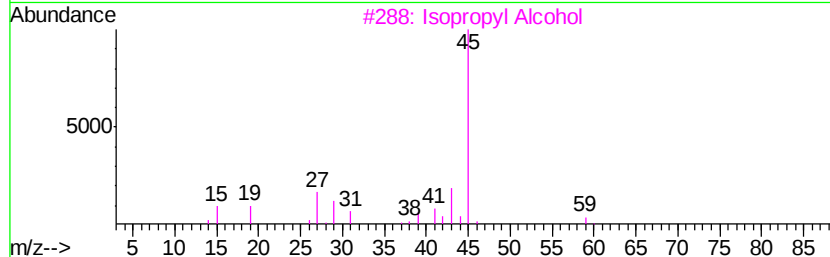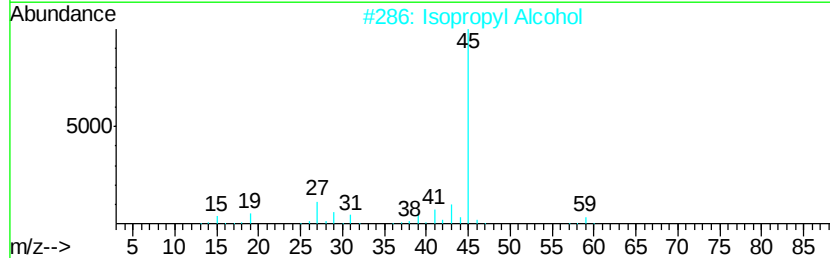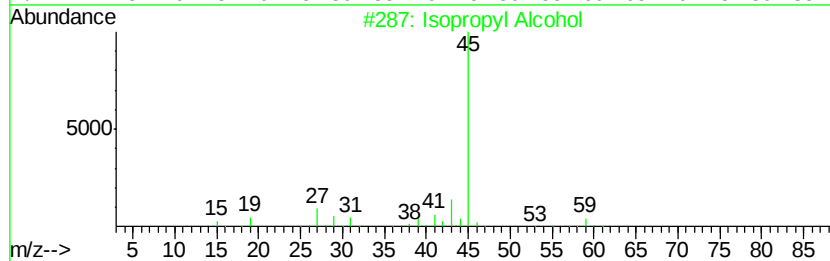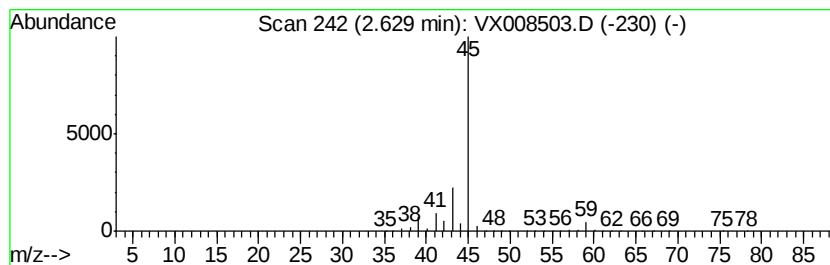

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX032719\
Data File : VX008503.D
Acq On : 27 Mar 2019 23:12
Operator : JC/SP
Sample : K2137-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SEWER-OUTLET-02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\624X032719W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
Isopropyl Alcohol	2.63	2874.7	ug/l	25083600	1	5.01	261773	30.0