


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032719\
Data File : VX008469.D
Acq On : 27 Mar 2019 09:05
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X032719W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Mar 27 12:01:15 2019

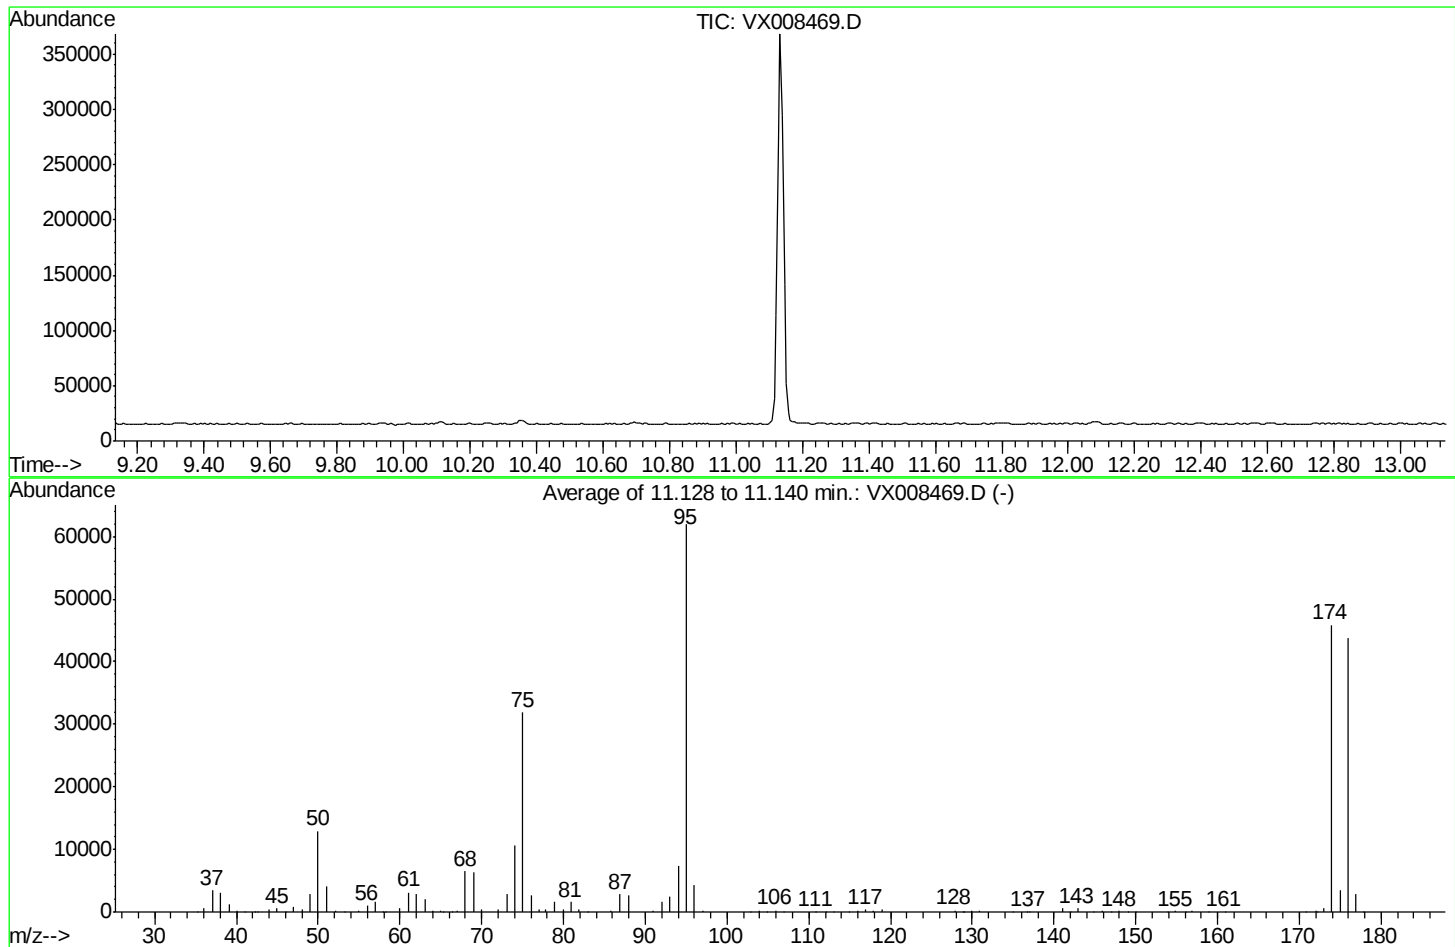

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	12967	PASS
75	95	30	60	51.4	31853	PASS
95	95	100	100	100.0	61930	PASS
96	95	5	9	6.8	4204	PASS
173	174	0.00	2	1.2	536	PASS
174	95	50	100	74.1	45898	PASS
175	174	5	9	7.5	3435	PASS
176	174	95	101	95.5	43824	PASS
177	176	5	9	6.6	2904	PASS