


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032719\
 Data File : VX008477.D
 Acq On : 27 Mar 2019 12:45
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X032719W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Mar 27 12:01:15 2019

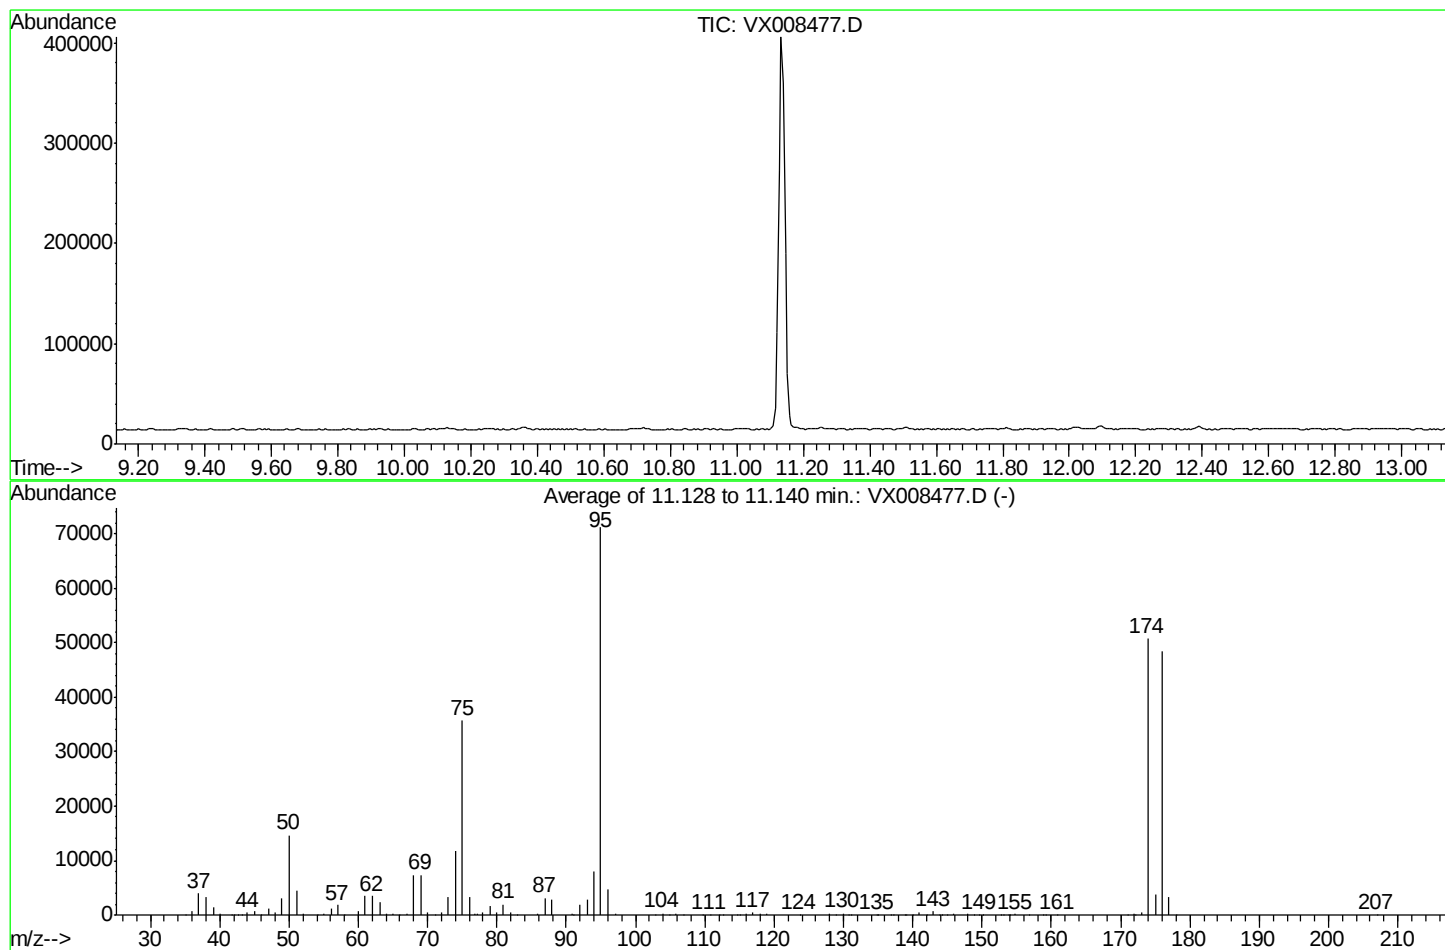

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	14600	PASS
75	95	30	60	50.1	35712	PASS
95	95	100	100	100.0	71213	PASS
96	95	5	9	6.8	4820	PASS
173	174	0.00	2	0.7	376	PASS
174	95	50	100	71.3	50765	PASS
175	174	5	9	7.6	3834	PASS
176	174	95	101	95.5	48464	PASS
177	176	5	9	6.9	3320	PASS