


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX032720\
 Data File : VX015397.D
 Acq On : 27 Mar 2020 21:53
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
 Title : SW846 8260
 Last Update : Fri Mar 27 09:35:51 2020

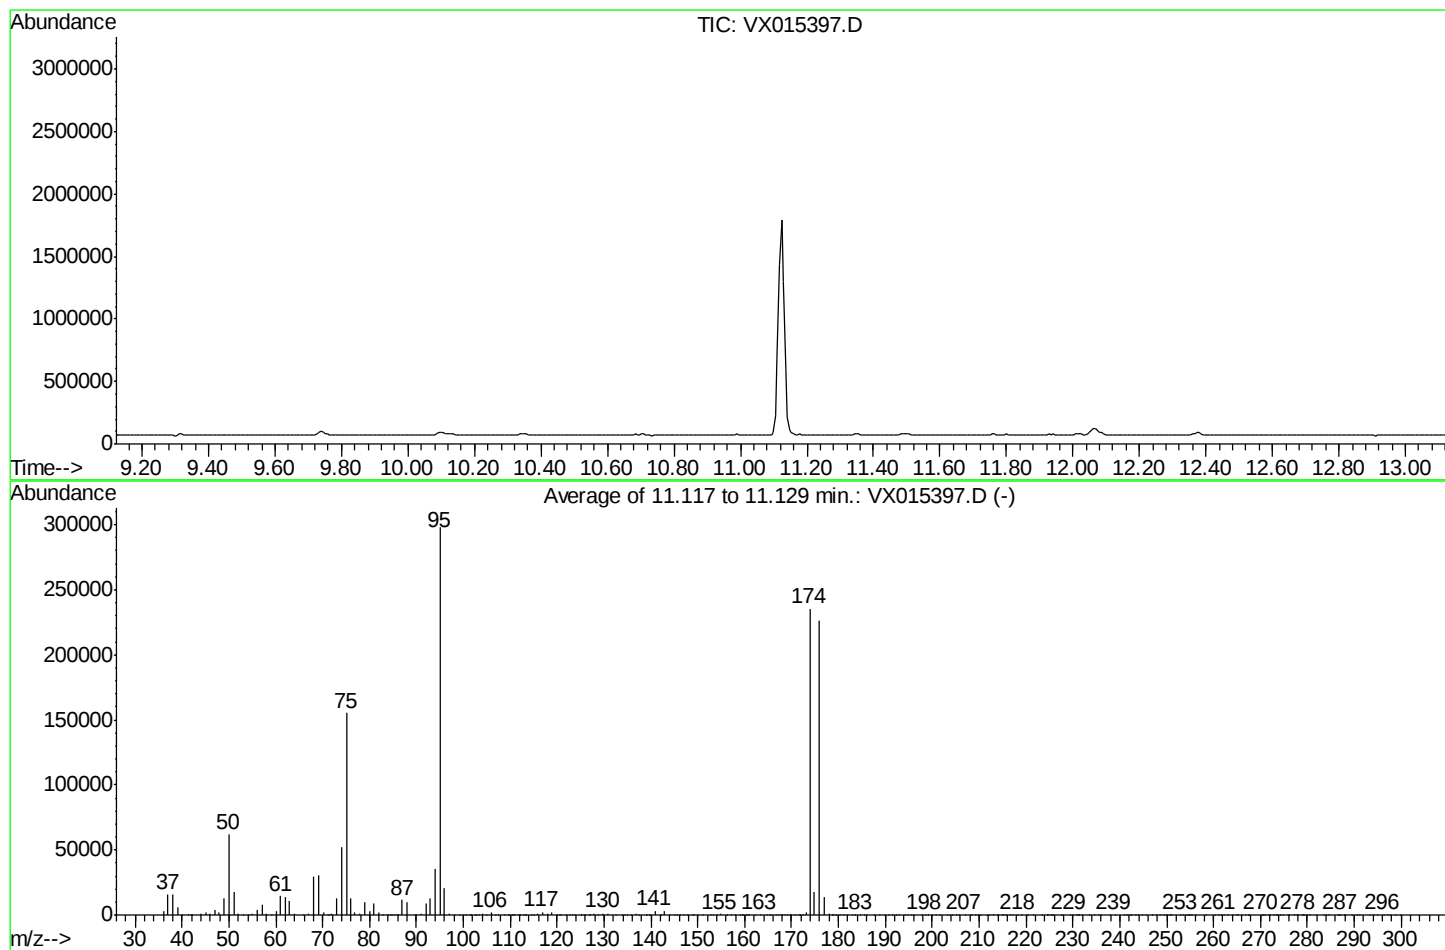

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1668

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	61887	PASS
75	95	30	60	52.1	155121	PASS
95	95	100	100	100.0	298016	PASS
96	95	5	9	6.9	20586	PASS
173	174	0.00	2	0.9	2218	PASS
174	95	50	100	79.0	235405	PASS
175	174	5	9	7.4	17456	PASS
176	174	95	101	96.3	226773	PASS
177	176	5	9	6.2	14113	PASS