

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034747.D
Acq On : 27 Mar 2023 13:53
Operator : JC/MD
Sample : 02100-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB08

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	230	240	252	rBV2	15131	46928	2.71%	0.500%
2	5.007	634	643	659	rBV2	32597	104852	6.06%	1.118%
3	5.385	692	705	720	rBV2	190949	557832	32.24%	5.949%
4	5.549	720	732	748	rVV	338714	980220	56.65%	10.453%
5	5.952	786	798	811	rBV	223512	606664	35.06%	6.469%
6	6.763	920	931	952	rBV	534291	1284254	74.22%	13.695%
7	8.646	1233	1240	1248	rBV	1083590	1730359	100.00%	18.452%
8	8.720	1248	1252	1269	rVB	37126	65207	3.77%	0.695%
9	10.055	1465	1471	1490	rBV	1100261	1483770	85.75%	15.823%
10	10.305	1506	1512	1523	rVB	19196	29960	1.73%	0.319%
11	11.079	1634	1639	1656	rBV	867679	1143102	66.06%	12.190%
12	12.024	1788	1794	1803	rBV	1051840	1344239	77.69%	14.335%




Sum of corrected areas: 9377387

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034747.D
Acq On : 27 Mar 2023 13:53
Operator : JC/MD
Sample : 02100-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

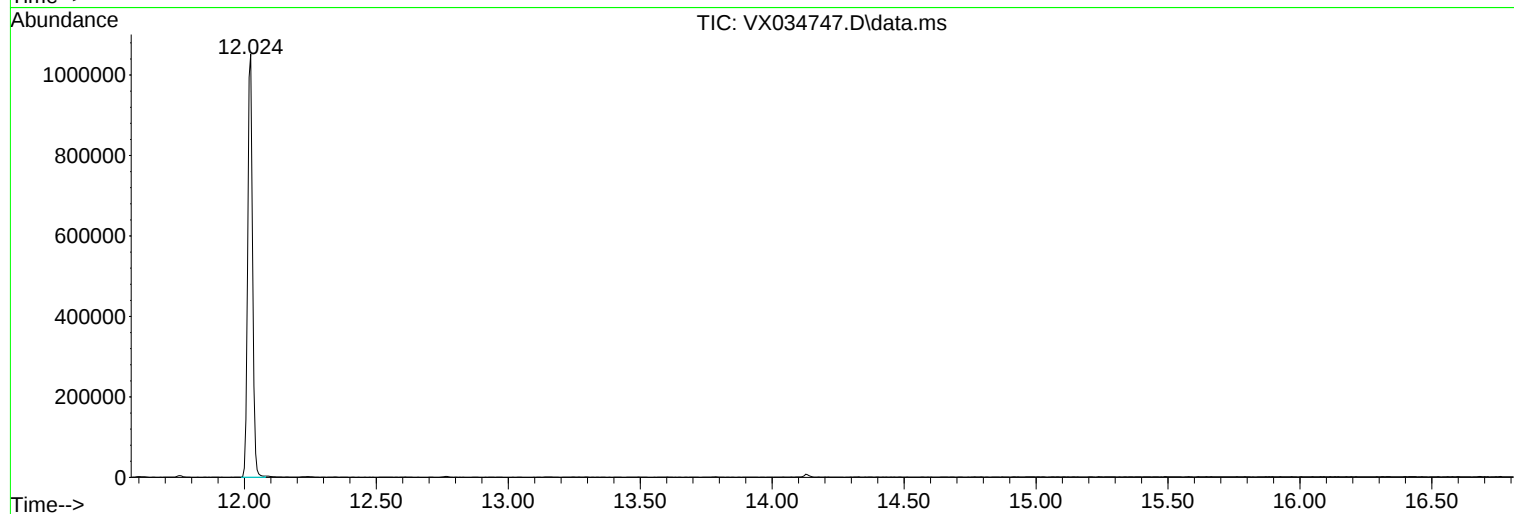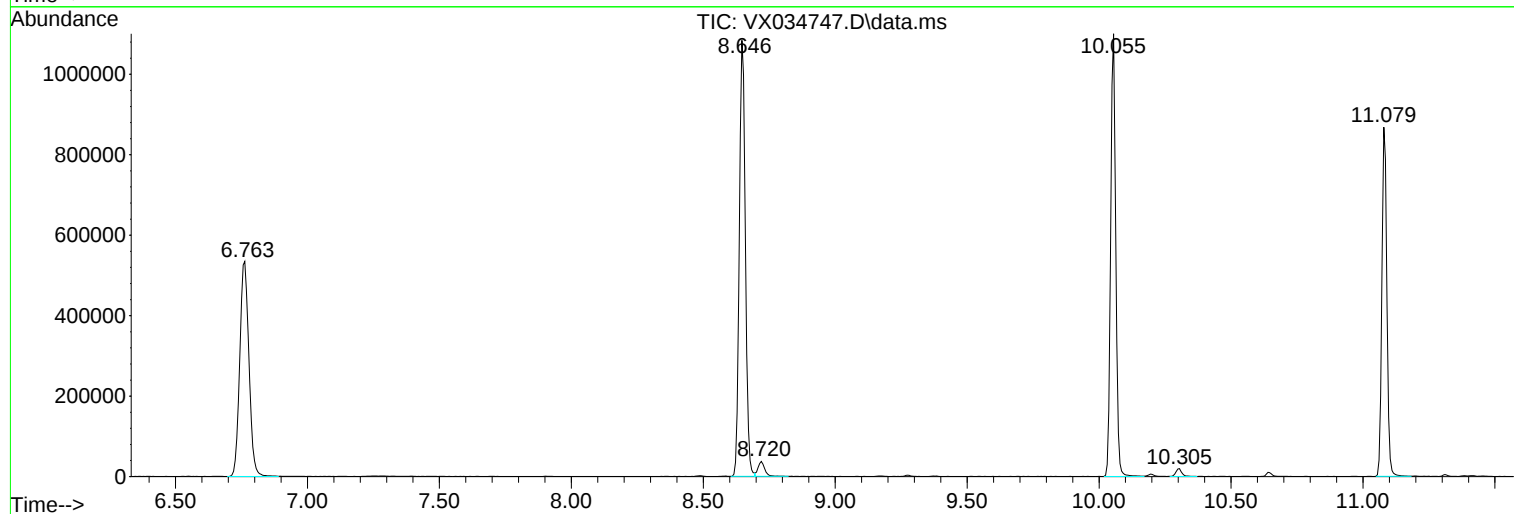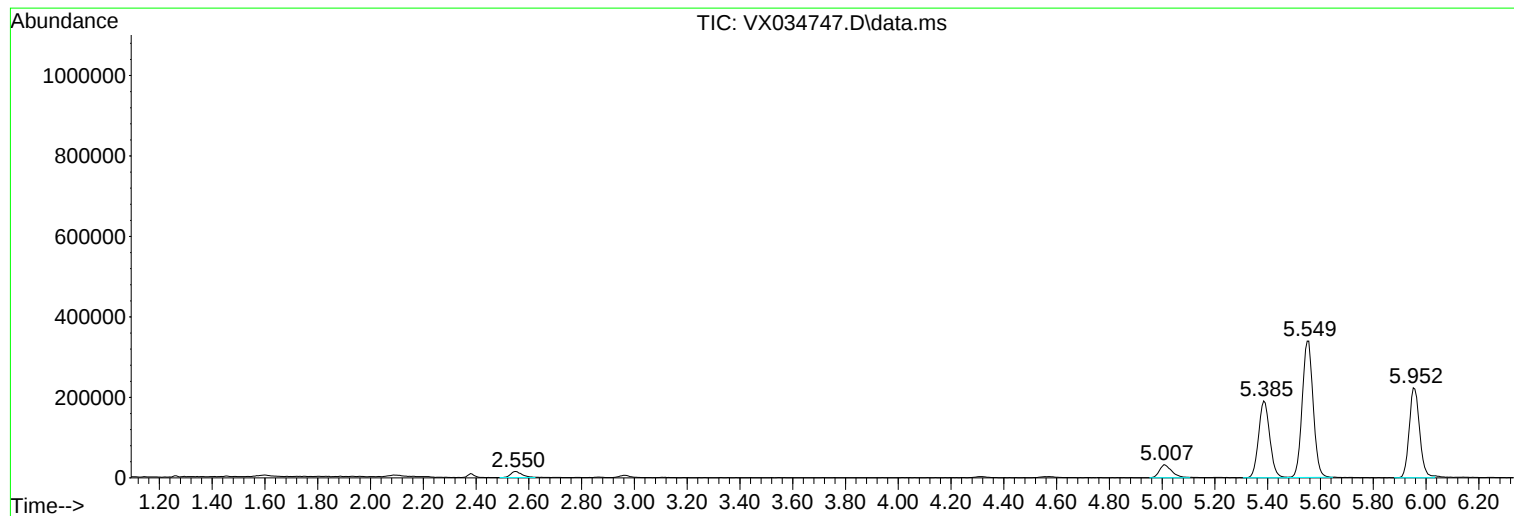

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034747.D
Acq On : 27 Mar 2023 13:53
Operator : JC/MD
Sample : 02100-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034747.D
Acq On : 27 Mar 2023 13:53
Operator : JC/MD
Sample : 02100-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------