

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034755.D
Acq On : 27 Mar 2023 17:22
Operator : JC/MD
Sample : 02073-04 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1660

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	31	34	48	rBV3	5565	19053	1.46%	0.258%
2	2.380	204	212	231	rBV	280968	469053	36.03%	6.360%
3	5.385	694	705	722	rBV	144839	421872	32.41%	5.721%
4	5.550	722	732	749	rVB	249410	715609	54.97%	9.704%
5	5.958	788	799	814	rBV	172480	457246	35.12%	6.200%
6	6.763	920	931	947	rBV	401441	963647	74.03%	13.067%
7	8.647	1234	1240	1247	rBV	833078	1301768	100.00%	17.652%
8	8.720	1247	1252	1263	rVB	75803	122442	9.41%	1.660%
9	10.055	1465	1471	1482	rBV	799394	1113235	85.52%	15.096%
10	11.079	1634	1639	1649	rBV	641413	820559	63.03%	11.127%
11	12.024	1788	1794	1805	rBV	748659	970073	74.52%	13.154%




Sum of corrected areas: 7374557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034755.D
Acq On : 27 Mar 2023 17:22
Operator : JC/MD
Sample : 02073-04 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

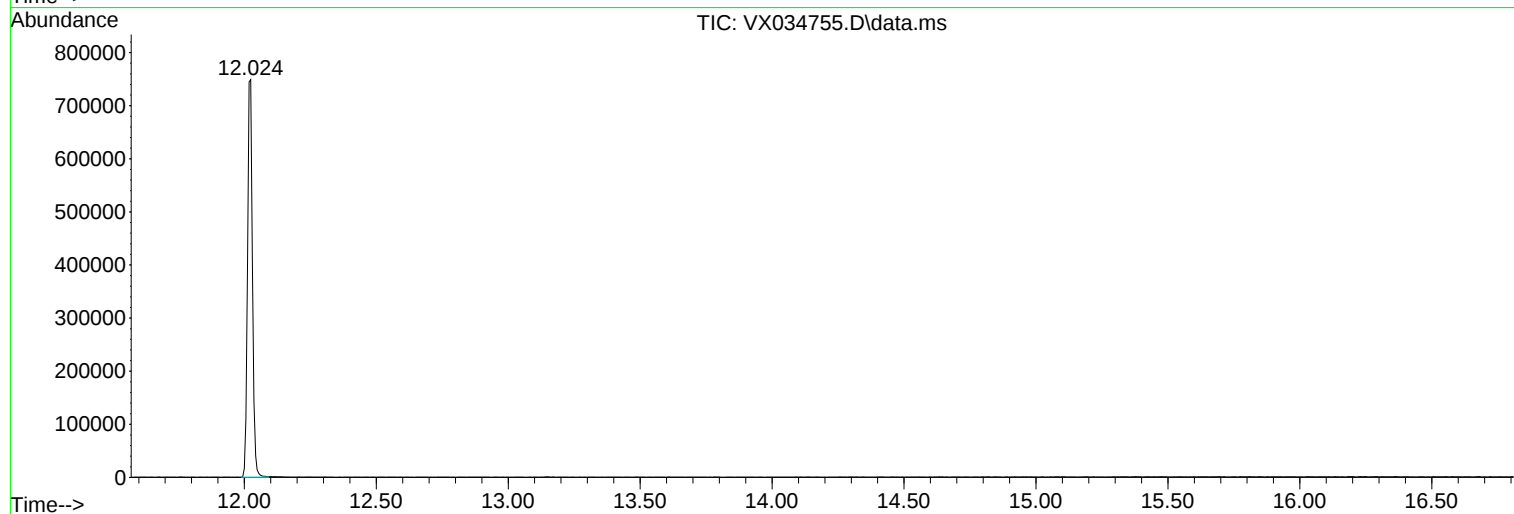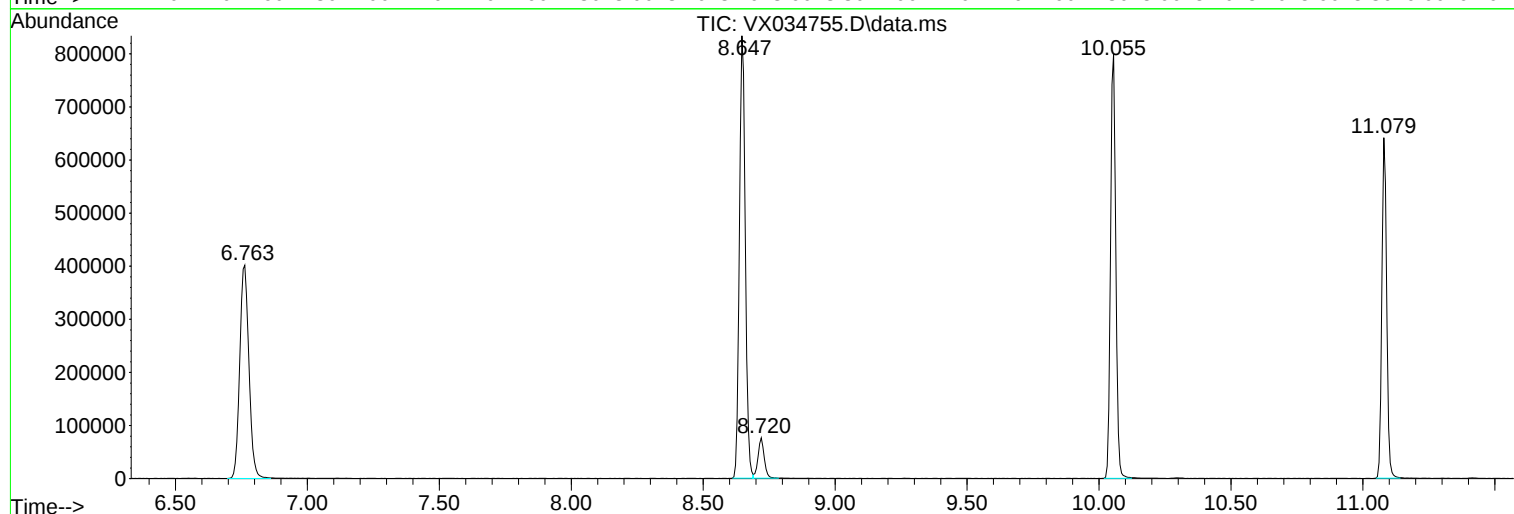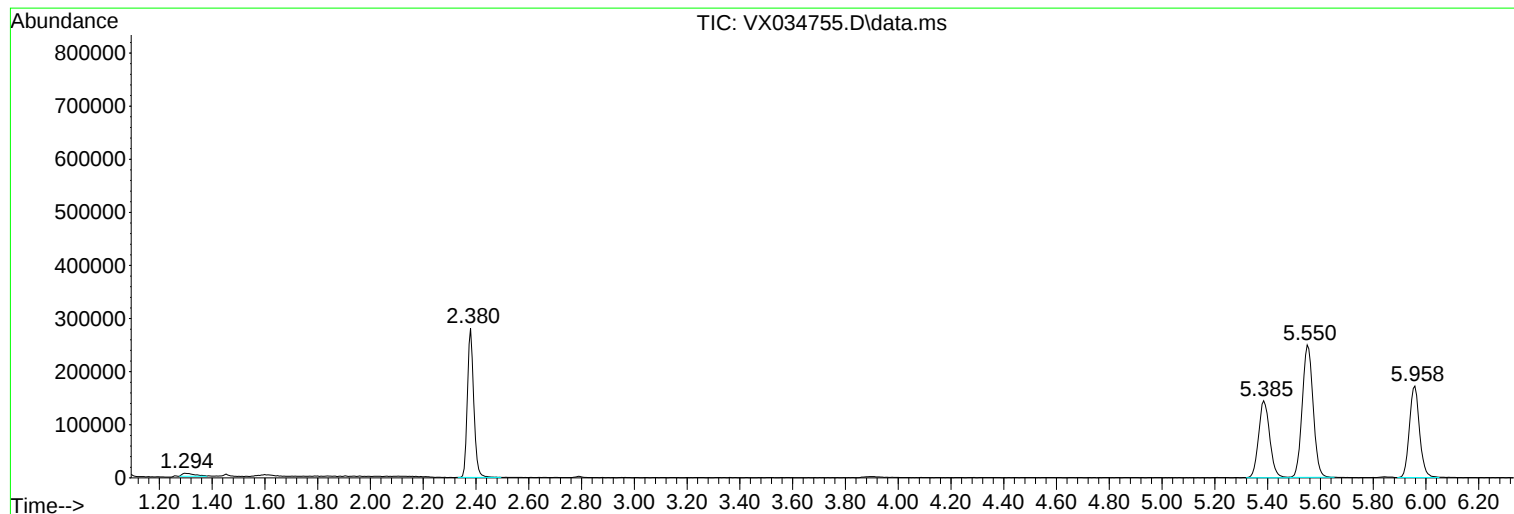

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034755.D
Acq On : 27 Mar 2023 17:22
Operator : JC/MD
Sample : 02073-04 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032723\
Data File : VX034755.D
Acq On : 27 Mar 2023 17:22
Operator : JC/MD
Sample : 02073-04 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------