

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032724\
 Data File : VX040807.D
 Acq On : 27 Mar 2024 12:53
 Operator : JC/MD
 Sample : PB159779TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB159779TB

Quant Time: Mar 28 03:53:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 22 02:44:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	42050	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	74043	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	75030	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	34780	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	34526	48.831	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.660%		
35) Dibromofluoromethane	5.385	113	25399	45.844	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	91.680%		
50) Toluene-d8	8.647	98	95343	50.259	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	100.520%		
62) 4-Bromofluorobenzene	11.079	95	35238	47.015	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	94.040%		
Target Compounds						Qvalue
6) Chloroethane	1.715	64	188	0.508	ug/l #	43
11) Tert butyl alcohol	2.959	59	900	7.949	ug/l #	95
13) Acrolein	2.239	56	75	1.119	ug/l #	14
15) Acrylonitrile	3.075	53	58	0.208	ug/l #	17
16) Acetone	2.380	43	31769	126.853	ug/l	99
17) Carbon Disulfide	2.514	76	420	0.294	ug/l #	76
18) Methyl Acetate	2.703	43	517	0.770	ug/l #	82
20) Methylene Chloride	2.788	84	2128	3.887	ug/l	97
25) 2-Butanone	4.568	43	3265	8.323	ug/l	96
29) Tetrahydrofuran	5.013	42	53	0.203	ug/l #	34
31) Cyclohexane	5.550	56	1065	1.268	ug/l #	7
36) 1,1-Dichloropropene	5.556	75	3915	4.799	ug/l #	49
37) Ethyl Acetate	4.727	43	1190	1.285	ug/l #	72
38) Carbon Tetrachloride	5.550	117	4739	5.161	ug/l #	14
43) Isopropyl Acetate	6.336	43	37894	26.051	ug/l	97
48) Methyl methacrylate	7.793	41	34095	51.283	ug/l #	50
51) 4-Methyl-2-Pentanone	8.543	43	29564	32.773	ug/l #	46
53) t-1,3-Dichloropropene	8.952	75	190	0.215	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	10921	11.935	ug/l #	66
56) Ethyl methacrylate	9.244	69	266	0.291	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	1394	1.493	ug/l #	42
59) 2-Hexanone	9.482	43	22177	31.736	ug/l #	51
74) N-amyl acetate	10.823	43	263	0.202	ug/l #	44
76) 1,2,3-Trichloropropane	11.079	75	20739	27.725	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	20739	70.139	ug/l #	5
93) 1,2,4-Trichlorobenzene	13.585	180	240	0.282	ug/l #	87
94) Hexachlorobutadiene	13.725	225	171	0.509	ug/l	77
95) Naphthalene	13.780	128	674	0.250	ug/l #	80
96) 1,2,3-Trichlorobenzene	13.963	180	239	0.286	ug/l #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032724\
Data File : VX040807.D
Acq On : 27 Mar 2024 12:53
Operator : JC/MD
Sample : PB159779TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB159779TB

Quant Time: Mar 28 03:53:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032124W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 22 02:44:48 2024
Response via : Initial Calibration




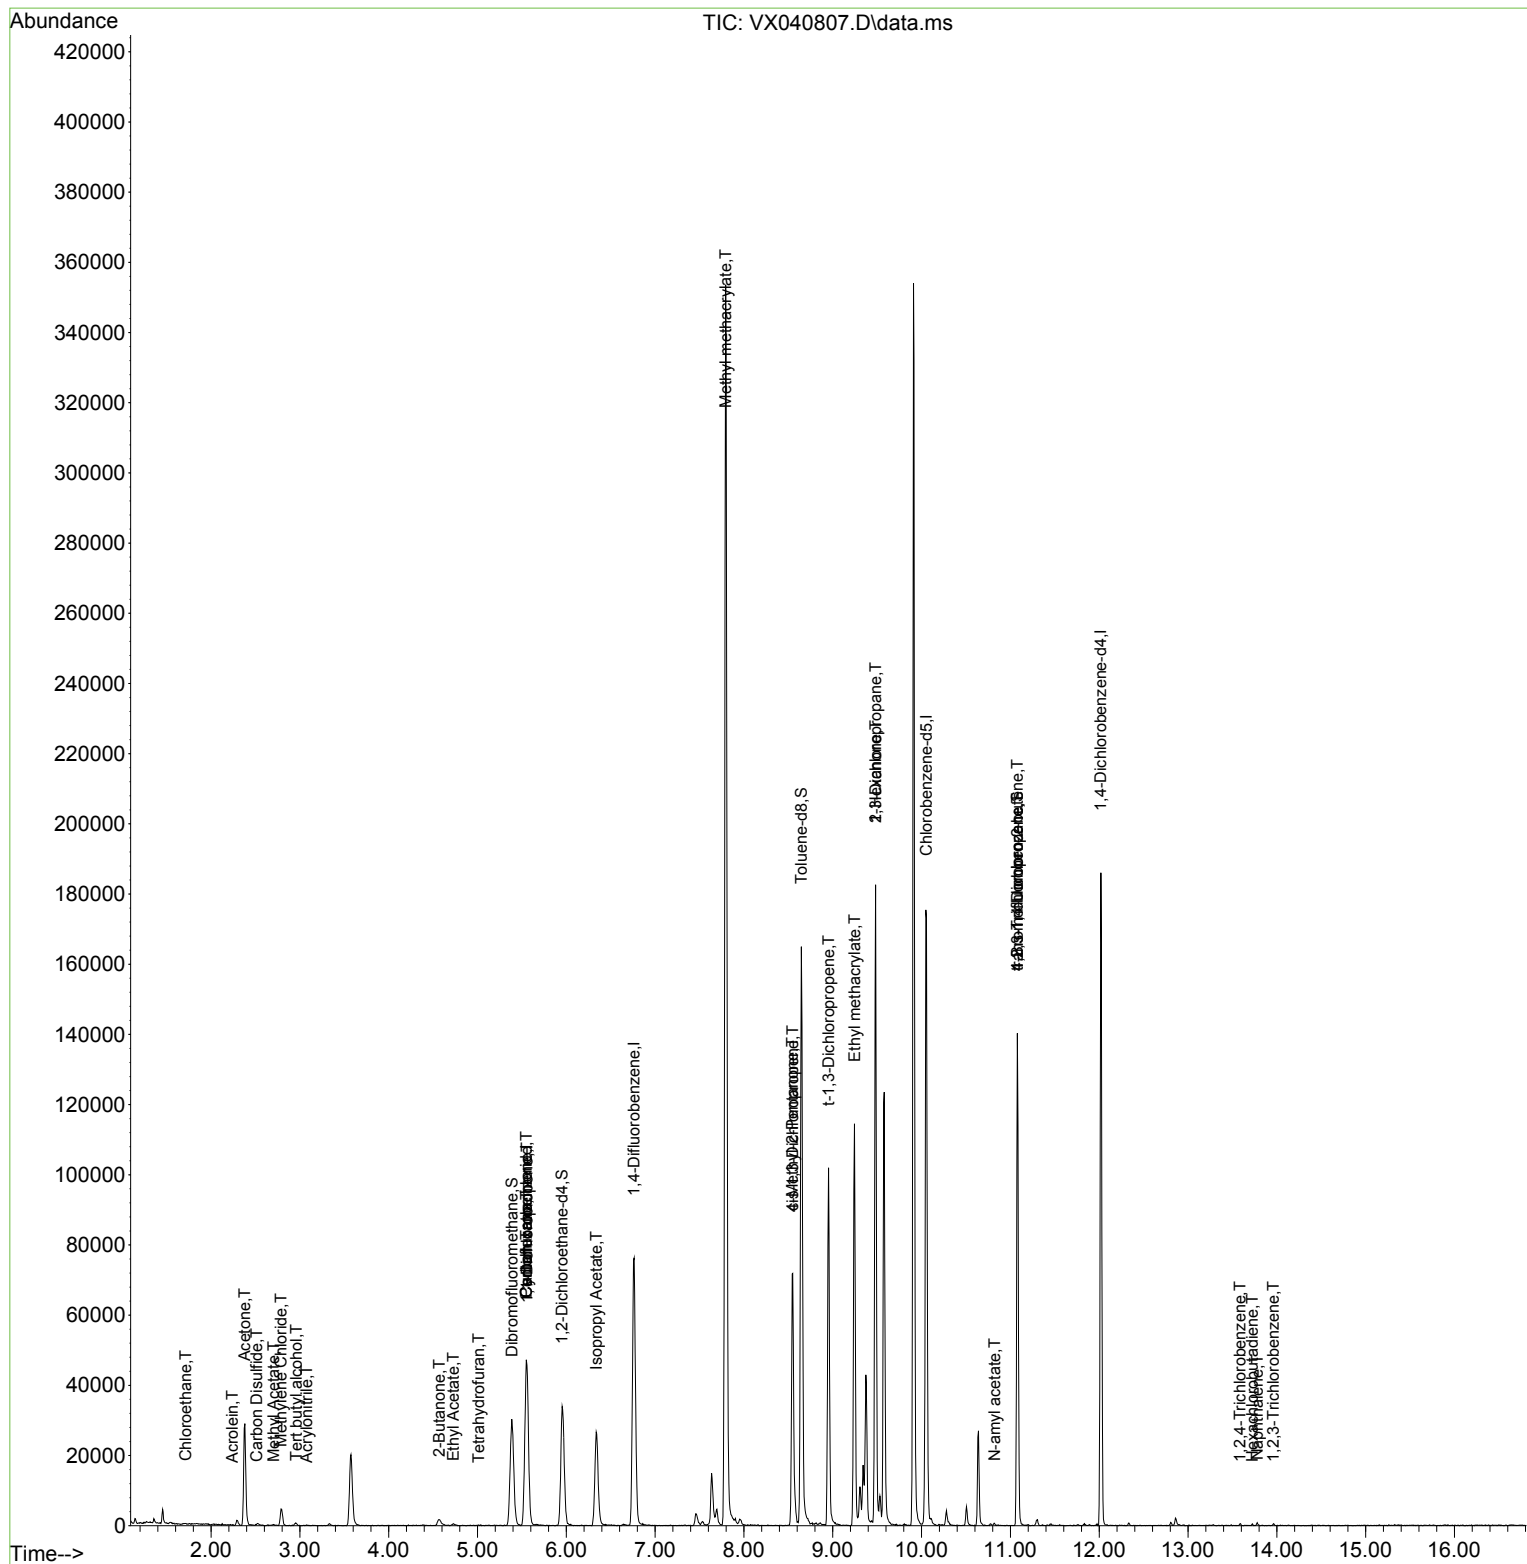




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion:168 Resp: 42050
Ion Ratio Lower Upper
168 100
99 67.5 56.6 85.0

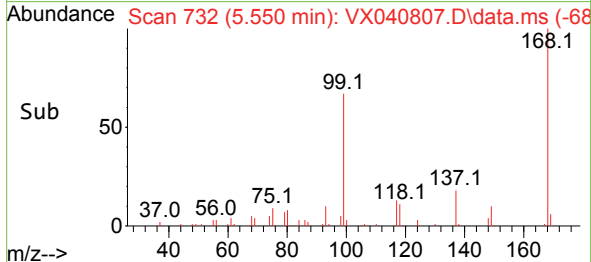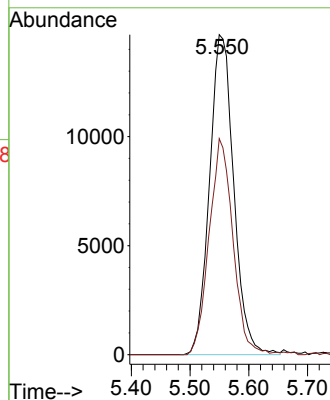

#6
Chloroethane
Concen: 0.508 ug/l
RT: 1.715 min Scan# 103
Delta R.T. 0.030 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 64 Resp: 188
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

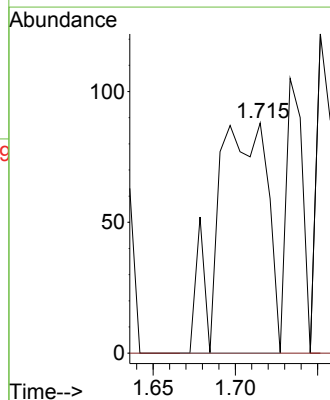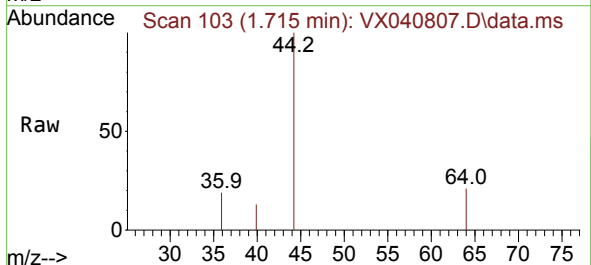

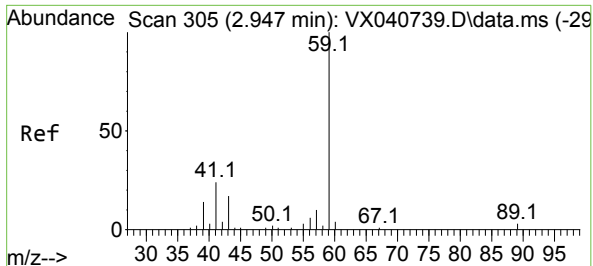

#11

Tert butyl alcohol

Concen: 7.949 ug/l

RT: 2.959 min Scan# 305

Delta R.T. 0.012 min

Lab File: VX040807.D

Acq: 27 Mar 2024 12:53

Instrument :

MSVOA_X

ClientSampleId :





PB159779TB

Tgt Ion: 59 Resp: 900

Ion Ratio Lower Upper

59 100

57 5.8 6.0 9.0#

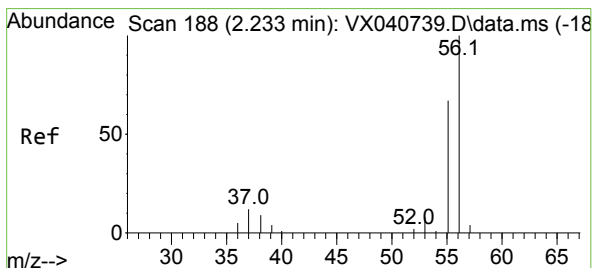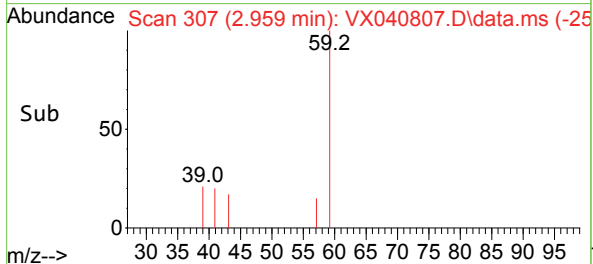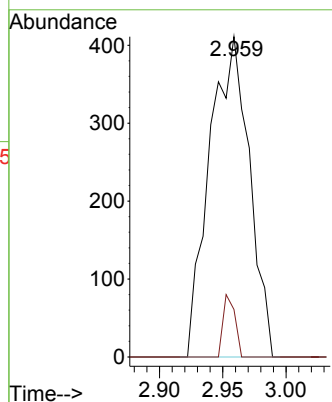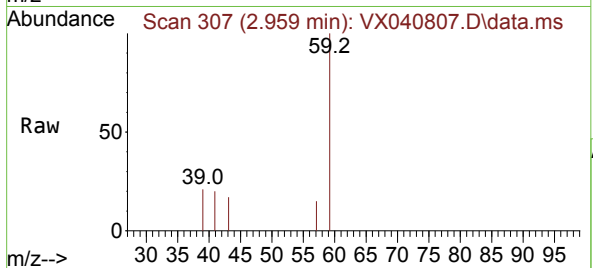

#13

Acrolein

Concen: 1.119 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.006 min

Lab File: VX040807.D




Acq: 27 Mar 2024 12:53


Tgt Ion: 56 Resp: 75

Ion Ratio Lower Upper

56 100

55 0.0 57.1 85.7#


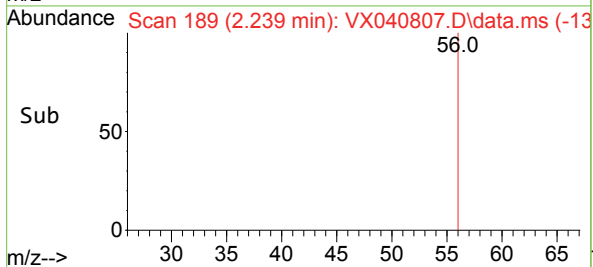
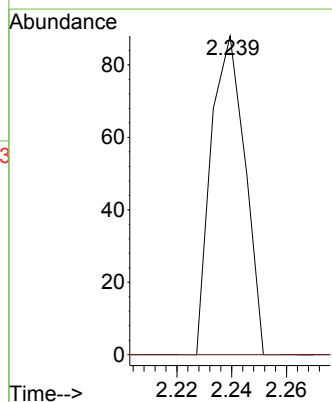
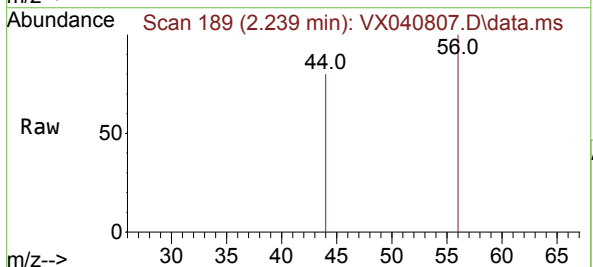




#15
Acrylonitrile
Concen: 0.208 ug/l
RT: 3.075 min Scan# 31
Delta R.T. 0.019 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion: 53 Resp: 58
Ion Ratio Lower Upper
53 100
52 0.0 66.0 99.0#
51 0.0 29.8 44.6#

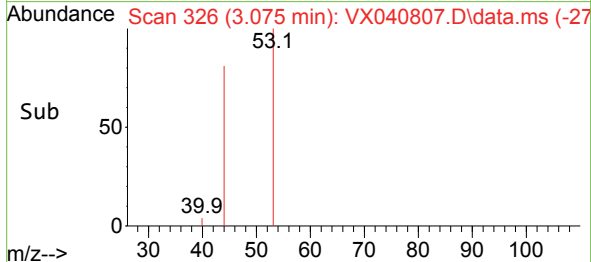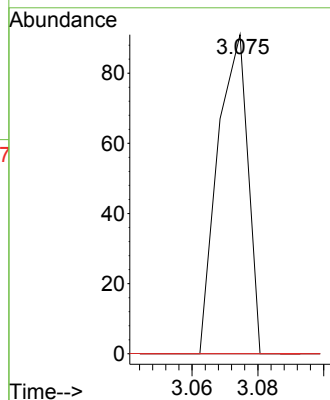

#16
Acetone
Concen: 126.853 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53


Tgt Ion: 43 Resp: 31769
Ion Ratio Lower Upper
43 100
58 26.9 21.9 32.9

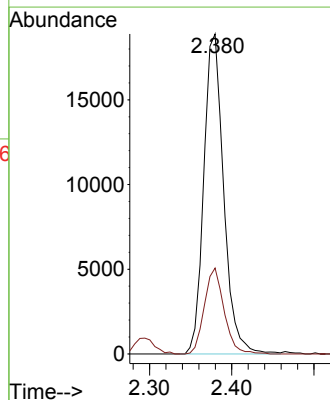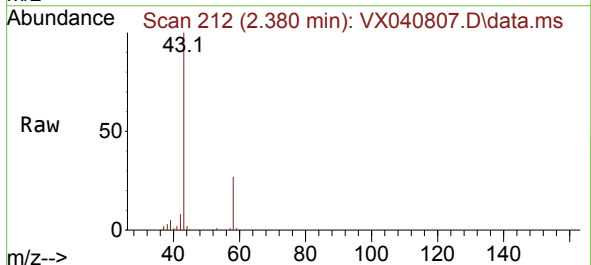






#17
Carbon Disulfide
Concen: 0.294 ug/l
RT: 2.514 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53


Instrument :
MSVOA_X
ClientSampleId :
PB159779TB





Tgt Ion: 76 Resp: 420
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#




#18
Methyl Acetate
Concen: 0.770 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53



Tgt Ion: 43 Resp: 517
Ion Ratio Lower Upper
43 100
74 13.7 17.8 26.8#



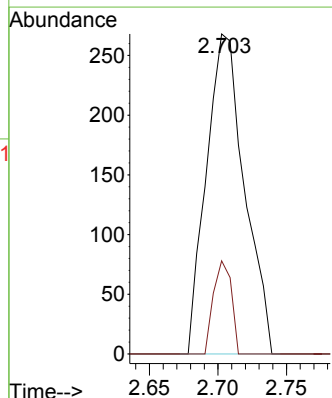





#20
Methylene Chloride
Concen: 3.887 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion: 84	Resp: 2128
Ion Ratio	Lower Upper
84 100	
49 130.5	103.6 155.4
51 46.9	33.8 50.6
86 64.6	49.4 74.0



#25
2-Butanone
Concen: 8.323 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.024 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53


Tgt Ion: 43	Resp: 3265		
Ion Ratio	Lower	Upper	
43 100			
72 26.3	19.4	29.2	

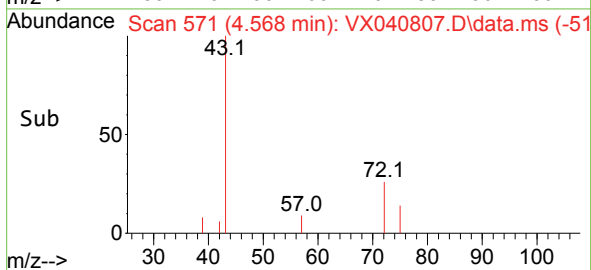



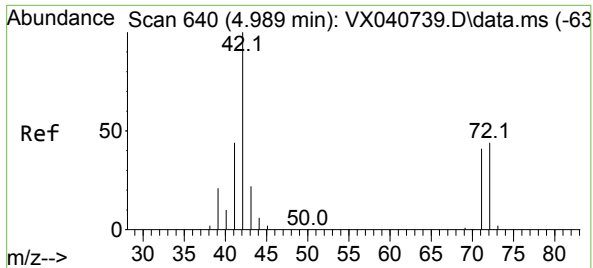


#29
Tetrahydrofuran
Concen: 0.203 ug/l
RT: 5.013 min Scan# 64
Delta R.T. 0.024 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Instrument :
MSVOA_X
ClientSampleId :
PB159779TB



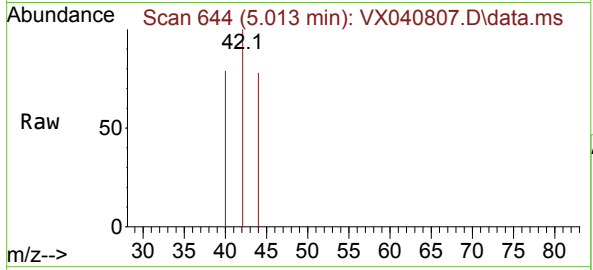



Tgt Ion: 42 Resp: 53
Ion Ratio Lower Upper
42 100
72 0.0 34.2 51.4#
71 0.0 32.2 48.2#

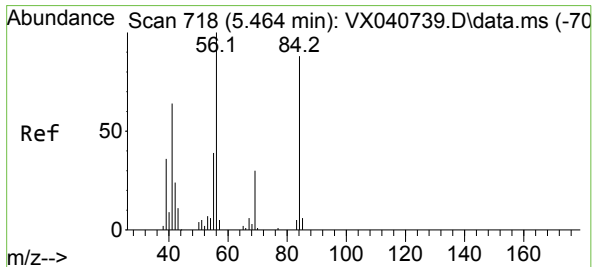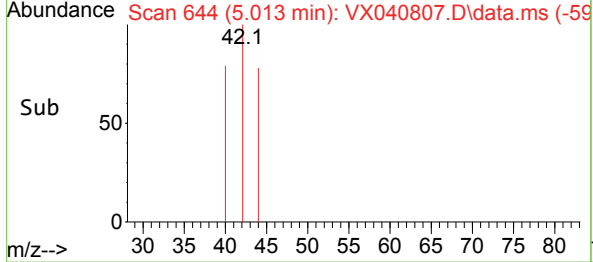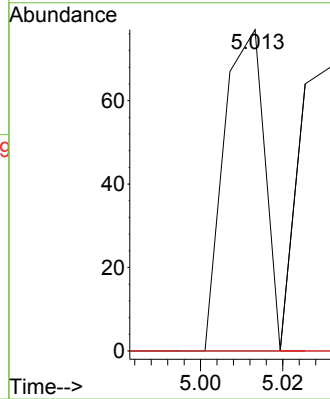

#31
Cyclohexane
Concen: 1.268 ug/l
RT: 5.550 min Scan# 732
Delta R.T. 0.086 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 56 Resp: 1065
Ion Ratio Lower Upper
56 100
69 149.1 23.4 35.2#
84 124.1 65.9 98.9#

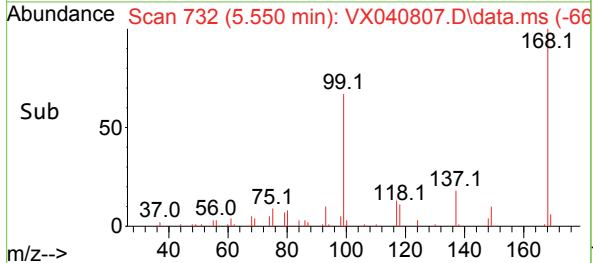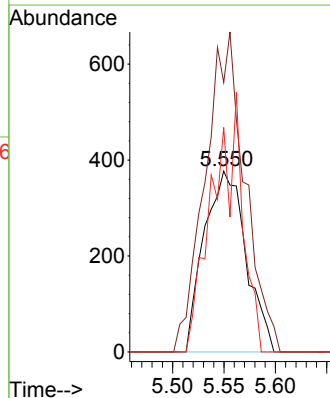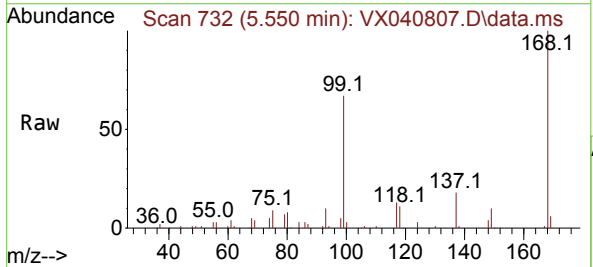



#33

1,2-Dichloroethane-d4

Concen: 48.831 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX040807.D

Acq: 27 Mar 2024 12:53

Instrument :

MSVOA_X

ClientSampleId :





PB159779TB

Tgt Ion: 65 Resp: 34526

Ion Ratio Lower Upper

65 100

67 50.3 0.0 100.2

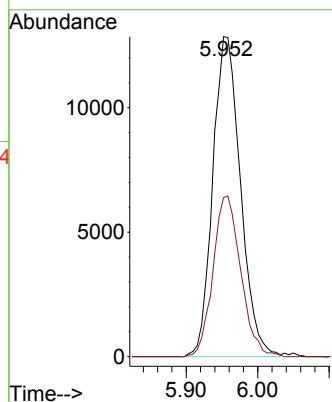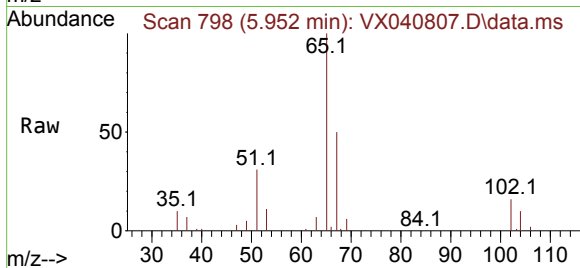

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX040807.D

Acq: 27 Mar 2024 12:53




Tgt Ion: 114 Resp: 74043


Ion Ratio Lower Upper

114 100

63 22.6 0.0 45.0

88 15.5 0.0 36.6


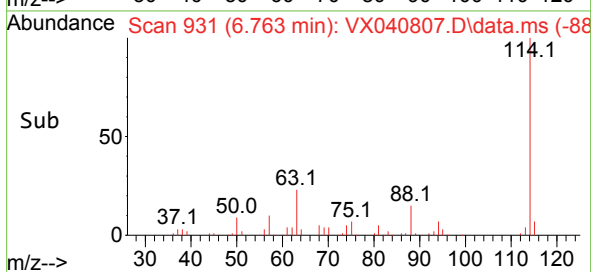

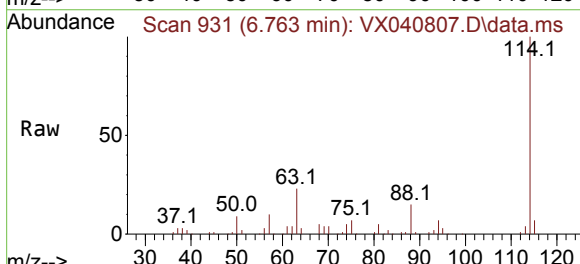


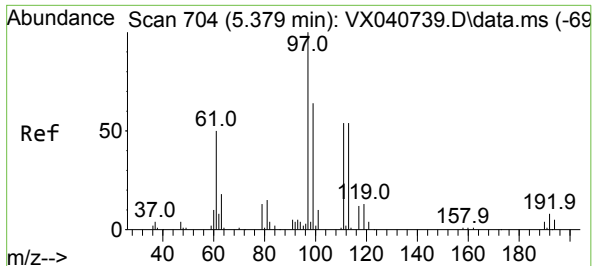

#35
Dibromofluoromethane
Concen: 45.844 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion:113 Resp: 25399
Ion Ratio Lower Upper
113 100
111 101.4 82.9 124.3
192 17.1 13.3 19.9

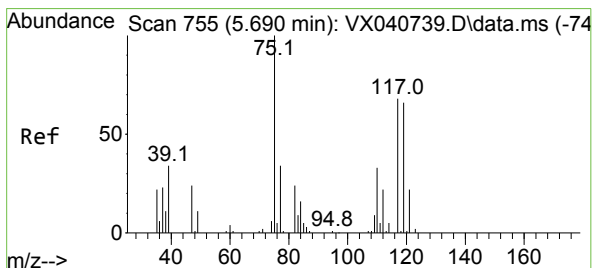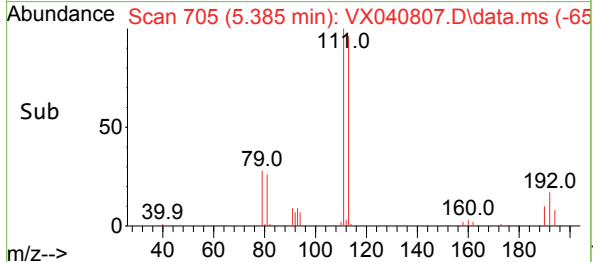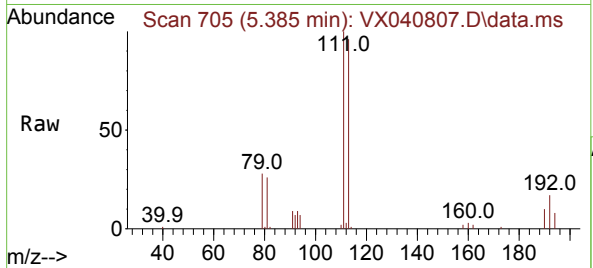

#36
1,1-Dichloropropene
Concen: 4.799 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 75 Resp: 3915
Ion Ratio Lower Upper
75 100
110 7.3 17.0 50.9#
77 0.0 24.7 37.1#

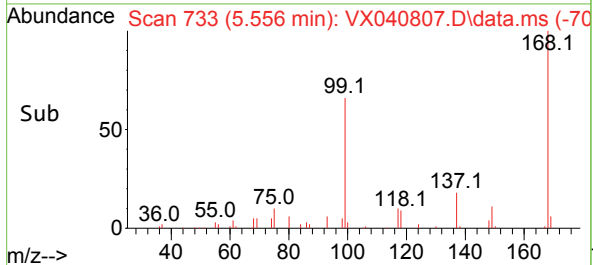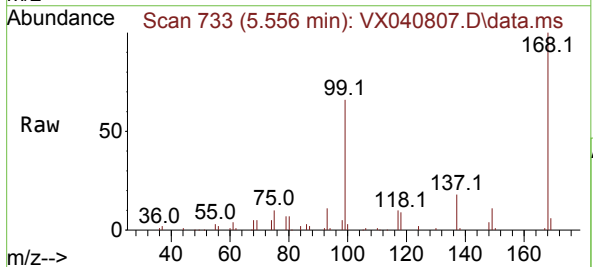



#37

Ethyl Acetate

Concen: 1.285 ug/l

RT: 4.727 min Scan# 597

Delta R.T. 0.024 min

Lab File: VX040807.D

Acq: 27 Mar 2024 12:53

Instrument :

MSVOA_X

ClientSampleId :

PB159779TB





Tgt Ion: 43 Resp: 1190

Ion Ratio Lower Upper

43 100

61 2.2 10.6 16.0#

70 0.0 8.3 12.5#

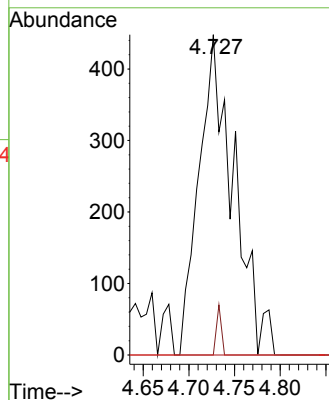

#38

Carbon Tetrachloride

Concen: 5.161 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.122 min

Lab File: VX040807.D

Acq: 27 Mar 2024 12:53




Tgt Ion: 117 Resp: 4739


Ion Ratio Lower Upper

117 100

119 3.0 78.2 117.2#

121 0.0 24.4 36.6#



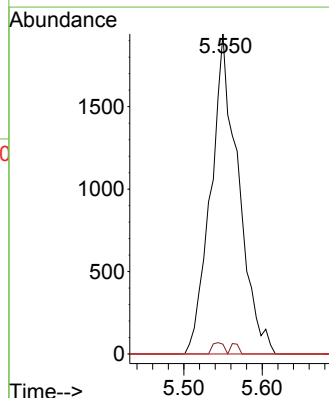





#43
Isopropyl Acetate
Concen: 26.051 ug/l
RT: 6.336 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion: 43 Resp: 37894
Ion Ratio Lower Upper
43 100
61 16.9 15.2 22.8
87 11.6 9.8 14.6

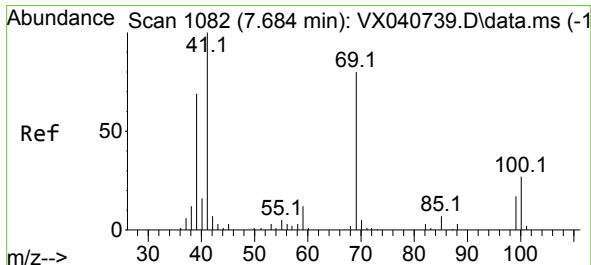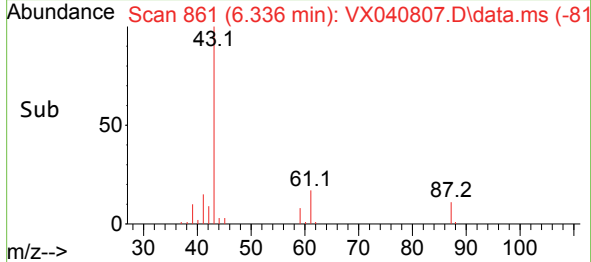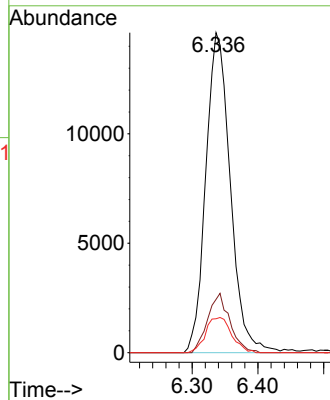

#48
Methyl methacrylate
Concen: 51.283 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.110 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 41 Resp: 34095
Ion Ratio Lower Upper
41 100
69 0.1 59.2 88.8#
39 57.7 47.7 71.5



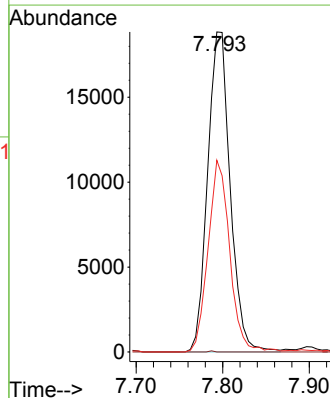
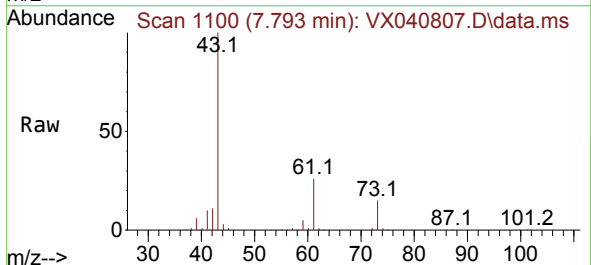




#50
Toluene-d8
Concen: 50.259 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion: 98 Resp: 95343
Ion Ratio Lower Upper
98 100
100 63.6 53.1 79.7



#51
4-Methyl-2-Pentanone
Concen: 32.773 ug/l
RT: 8.543 min Scan# 1223
Delta R.T. -0.024 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 43 Resp: 29564
Ion Ratio Lower Upper
43 100
58 5.4 30.4 45.6#


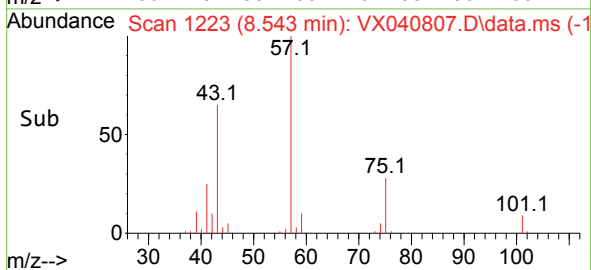






#53
 t-1,3-Dichloropropene
 Concen: 0.215 ug/l
 RT: 8.952 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX040807.D
 Acq: 27 Mar 2024 12:53




Instrument :
 MSVOA_X
 ClientSampleId :
 PB159779TB


Tgt Ion: 75 Resp: 190
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.7 38.5#



#54
 cis-1,3-Dichloropropene
 Concen: 11.935 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.189 min
 Lab File: VX040807.D
 Acq: 27 Mar 2024 12:53

Tgt Ion: 75 Resp: 10921
 Ion Ratio Lower Upper
 75 100
 77 0.8 25.3 37.9#
 39 41.4 46.7 70.1#


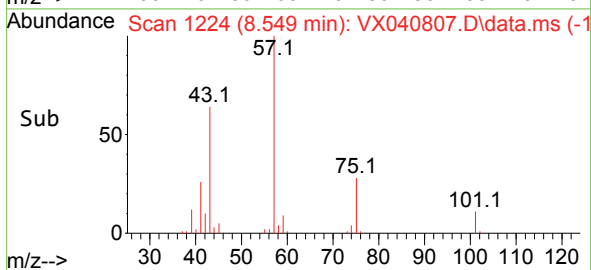






#56
Ethyl methacrylate
Concen: 0.291 ug/l
RT: 9.244 min Scan# 1338
Delta R.T. 0.134 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion: 69 Resp: 266
Ion Ratio Lower Upper
69 100
41 7403.0 56.8 85.2#
39 3419.2 32.0 48.0#

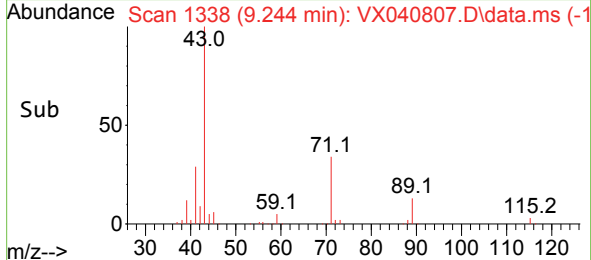

#57
1,3-Dichloropropane
Concen: 1.493 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 76 Resp: 1394
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#




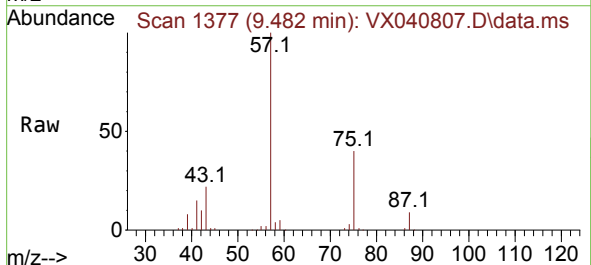




#59
2-Hexanone
Concen: 31.736 ug/l
RT: 9.482 min Scan# 11
Delta R.T. 0.055 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion: 43 Resp: 22177
Ion Ratio Lower Upper
43 100
58 18.0 26.2 78.5#

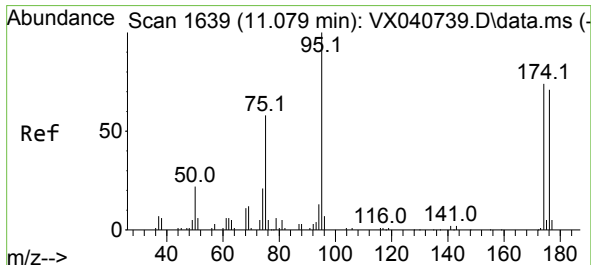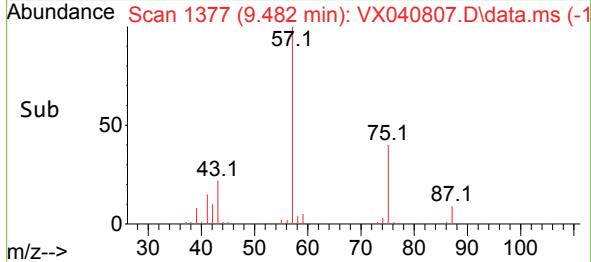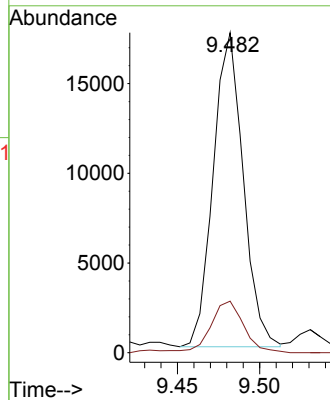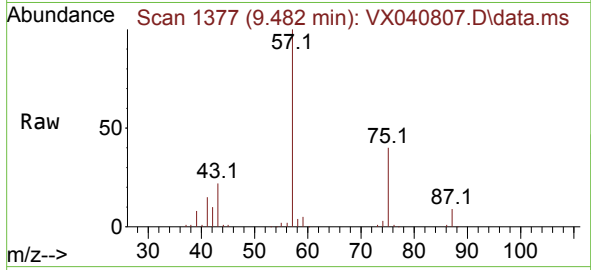

#62
4-Bromofluorobenzene
Concen: 47.015 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 95 Resp: 35238
Ion Ratio Lower Upper
95 100
174 74.7 0.0 135.6
176 71.5 0.0 131.0



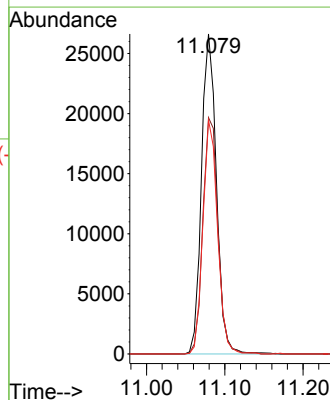
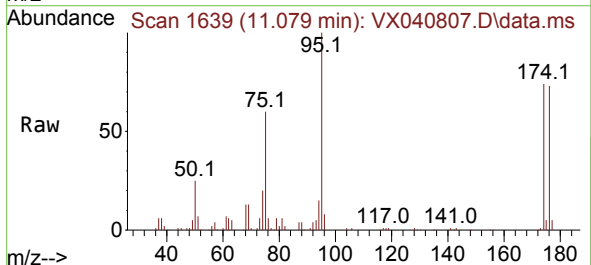




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion:117 Resp: 75030
Ion Ratio Lower Upper
117 100
82 57.6 46.2 69.4
119 32.0 25.5 38.3

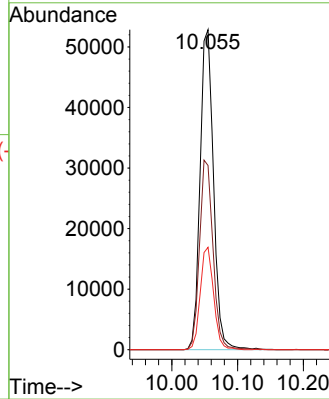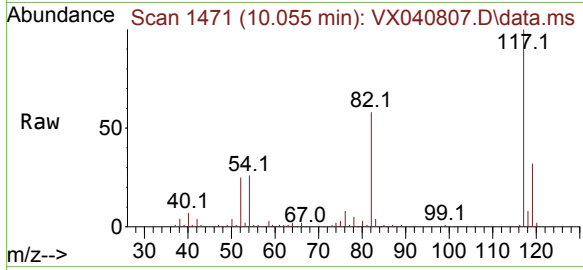

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion:152 Resp: 34780
Ion Ratio Lower Upper
152 100
115 63.5 43.3 129.9
150 155.8 0.0 345.0



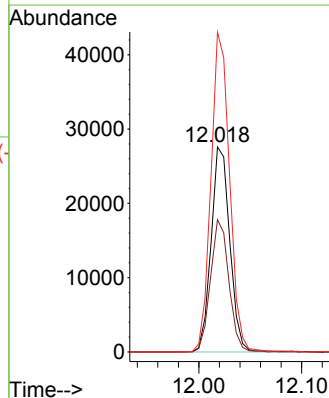
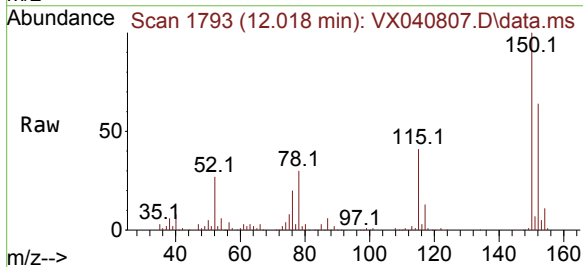




#74
N-amy1 acetate
Concen: 0.202 ug/l
RT: 10.823 min Scan# 1639
Delta R.T. -0.018 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53




Instrument :
MSVOA_X
ClientSampleId :
PB159779TB


Tgt Ion: 43 Resp: 263
Ion Ratio Lower Upper
43 100
70 0.0 32.9 49.3#
55 0.0 19.3 28.9#
61 0.0 18.8 28.2#



#76
1,2,3-Trichloropropane
Concen: 27.725 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

Tgt Ion: 75 Resp: 20739
Ion Ratio Lower Upper
75 100
77 0.8 19.1 57.5#









#81
 trans-1,4-Dichloro-2-butene
 Concen: 70.139 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.061 min
 Lab File: VX040807.D
 Acq: 27 Mar 2024 12:53




Instrument :
 MSVOA_X
 ClientSampleId :
 PB159779TB


Tgt Ion: 75 Resp: 20739
 Ion Ratio Lower Upper
 75 100
 53 0.0 90.5 135.7#
 89 0.1 36.9 55.3#

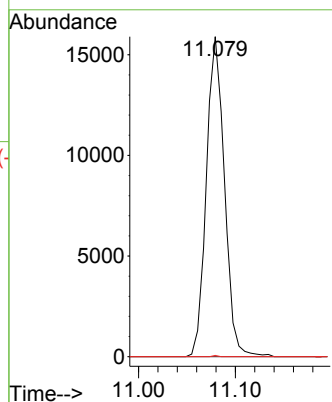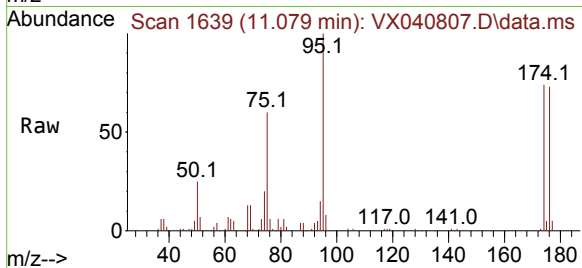

#93
 1,2,4-Trichlorobenzene
 Concen: 0.282 ug/l
 RT: 13.585 min Scan# 2050
 Delta R.T. -0.000 min
 Lab File: VX040807.D
 Acq: 27 Mar 2024 12:53


Tgt Ion:180 Resp: 240
 Ion Ratio Lower Upper
 180 100
 182 99.2 48.3 144.8
 145 11.7 18.0 54.0#

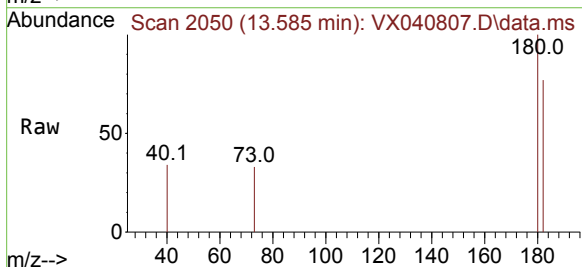






#94
Hexachlorobutadiene
Concen: 0.509 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53


Instrument :
MSVOA_X
ClientSampleId :
PB159779TB

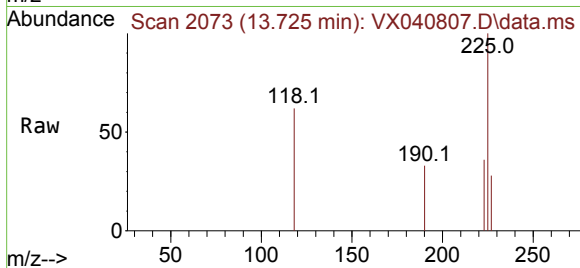



Tgt Ion:225 Resp: 171
Ion Ratio Lower Upper
225 100
223 50.9 31.1 93.2
227 39.8 32.5 97.5

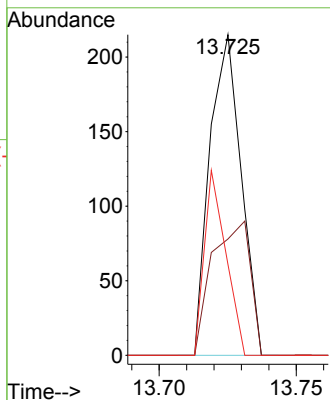


#95
Naphthalene
Concen: 0.250 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX040807.D
Acq: 27 Mar 2024 12:53

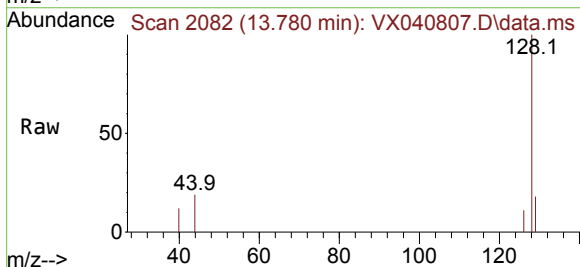

Tgt Ion:128 Resp: 674
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 13.1 8.8 13.2

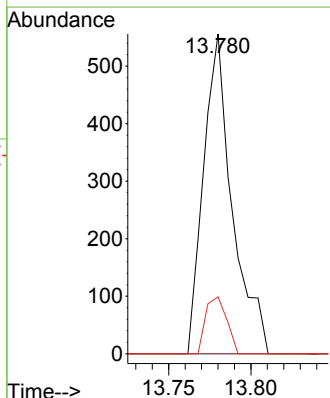



#96

1,2,3-Trichlorobenzene

Concen: 0.286 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX040807.D


Acq: 27 Mar 2024 12:53

Instrument :

MSVOA_X

ClientSampleId :

PB159779TB

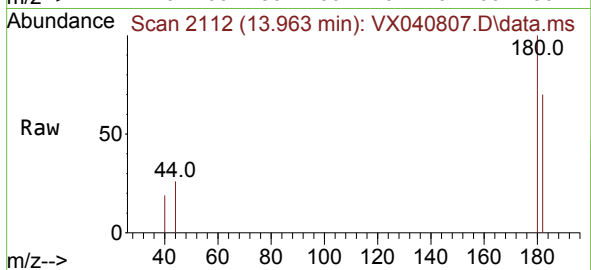

Tgt Ion:180 Resp: 239

Ion Ratio Lower Upper

180 100

182 78.7 46.9 140.6

145 0.0 17.8 53.5#

