


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX032819\  
Data File : VX008506.D  
Acq On : 28 Mar 2019 08:55  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X032519W.M  
Title : SW846 8260  
Last Update : Tue Mar 26 07:57:20 2019

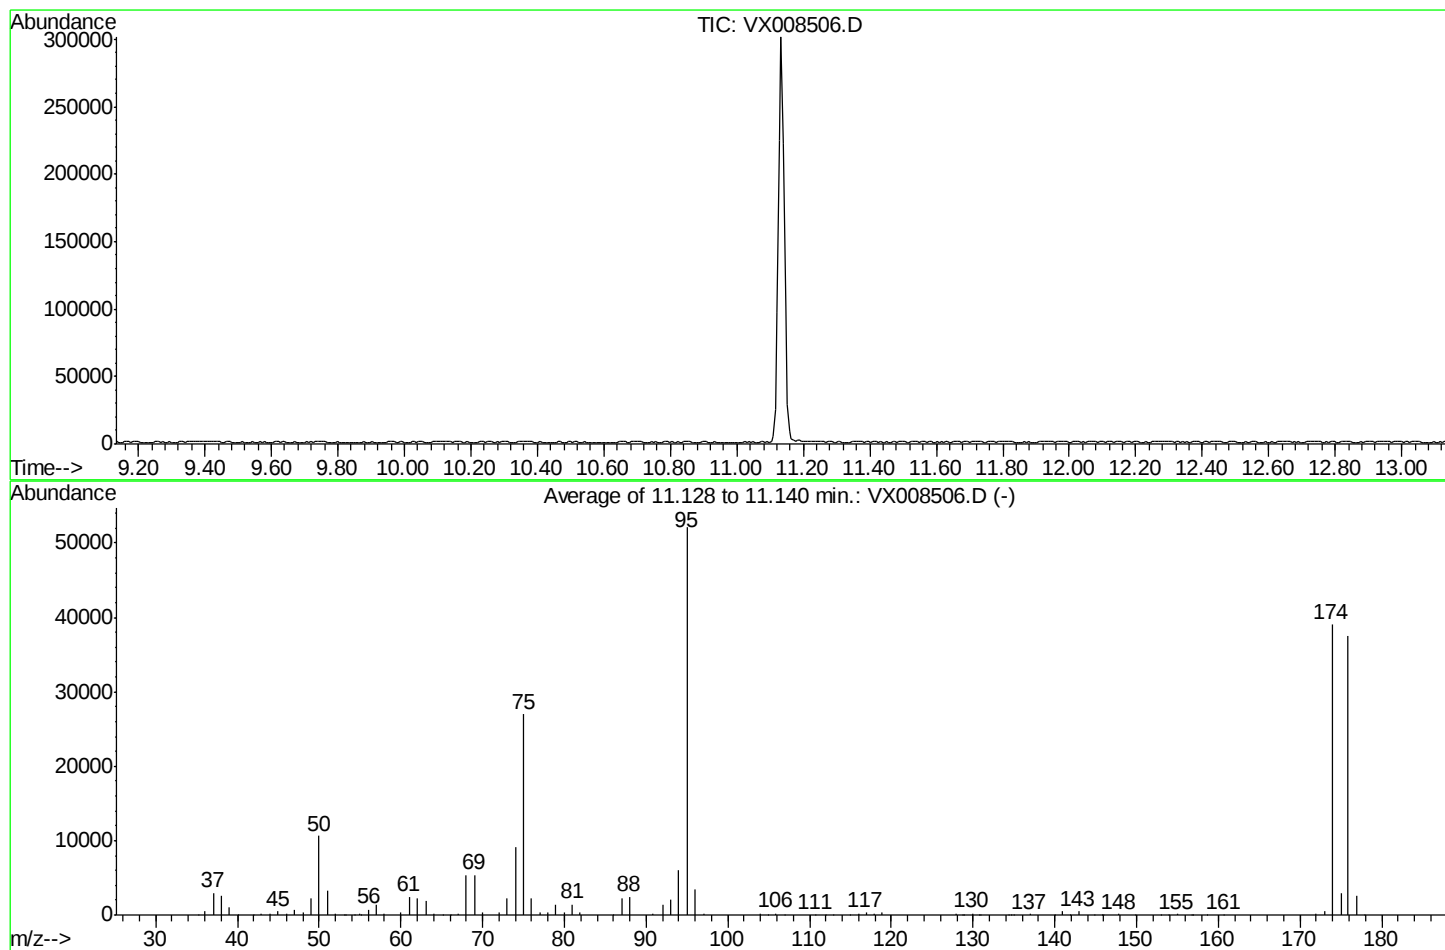

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.3      | 10604   | PASS             |
| 75          | 95           | 30           | 60           | 51.7      | 26938   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 52114   | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 3408    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 480     | PASS             |
| 174         | 95           | 50           | 100          | 74.9      | 39048   | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 2980    | PASS             |
| 176         | 174          | 95           | 101          | 95.9      | 37464   | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 2563    | PASS             |