

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
 Data File : VX027757.D
 Acq On : 28 Mar 2022 18:05
 Operator : JC/MD
 Sample : N2123-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 20220344-MODIFIED-ELUTRIATE

Quant Time: Mar 29 05:40:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 25 16:26:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	68963	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	120007	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	112664	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	49567	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	51972	45.949	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	91.900%		
35) Dibromofluoromethane	5.391	113	40670	51.607	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	103.220%		
50) Toluene-d8	8.653	98	148575	48.770	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	97.540%		
62) 4-Bromofluorobenzene	11.079	95	62234	50.345	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	100.700%		
Target Compounds						Qvalue
6) Chloroethane	1.697	64	245	0.480	ug/l	# 43
10) Methyl Iodide	2.465	142	23	2.893	ug/l	# 41
11) Tert butyl alcohol	2.953	59	2071	9.834	ug/l	# 85
16) Acetone	2.380	43	21172	44.260	ug/l	95
25) 2-Butanone	4.562	43	5677	7.390	ug/l	# 89
36) 1,1-Dichloropropene	5.550	75	5932	4.766	ug/l	# 47
37) Ethyl Acetate	4.562	43	5677	3.918	ug/l	# 65
38) Carbon Tetrachloride	5.562	117	7362	6.052	ug/l	# 17
39) Methylcyclohexane	7.379	83	986	0.689	ug/l	# 83
40) Benzene	6.050	78	1210	0.352	ug/l	95
48) Methyl methacrylate	7.659	41	142	Below Cal	#	68
52) Toluene	8.720	92	2870	1.335	ug/l	96
55) 1,1,2-Trichloroethane	9.104	97	236	0.270	ug/l	# 16
67) Ethyl Benzene	10.195	91	38679	8.749	ug/l	93
68) m/p-Xylenes	10.305	106	11585	7.230	ug/l	88
69) o-Xylene	10.646	106	10601	6.583	ug/l	84
70) Styrene	10.640	104	835	0.326	ug/l	# 1
73) Isopropylbenzene	10.963	105	10309	2.532	ug/l	97
74) N-amyl acetate	10.860	43	505	0.258	ug/l	# 28
76) 1,2,3-Trichloropropane	11.079	75	33110	23.992	ug/l	# 38
78) n-propylbenzene	11.311	91	3232	0.669	ug/l	97
79) 2-Chlorotoluene	11.384	91	5074	1.666	ug/l	# 47
80) 1,3,5-Trimethylbenzene	11.451	105	6644	1.899	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.079	75	33110	81.664	ug/l	# 15
82) 4-Chlorotoluene	11.616	91	2316	0.661	ug/l	81
83) tert-Butylbenzene	11.969	119	4603	1.432	ug/l	76
84) 1,2,4-Trimethylbenzene	11.756	105	37172	10.466	ug/l	97
85) sec-Butylbenzene	11.756	105	37172	8.827	ug/l	# 56
86) p-Isopropyltoluene	12.012	119	7142	2.155	ug/l	91
89) n-Butylbenzene	12.323	91	2015	0.642	ug/l	# 16
90) Hexachloroethane	12.555	117	1330	2.515	ug/l	# 10
92) 1,2-Dibromo-3-Chloropr...	12.969	75	137	0.390	ug/l	# 1
95) Naphthalene	13.780	128	593227	168.059	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027757.D
Acq On : 28 Mar 2022 18:05
Operator : JC/MD
Sample : N2123-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Quant Time: Mar 29 05:40:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 25 16:26:59 2022
Response via : Initial Calibration

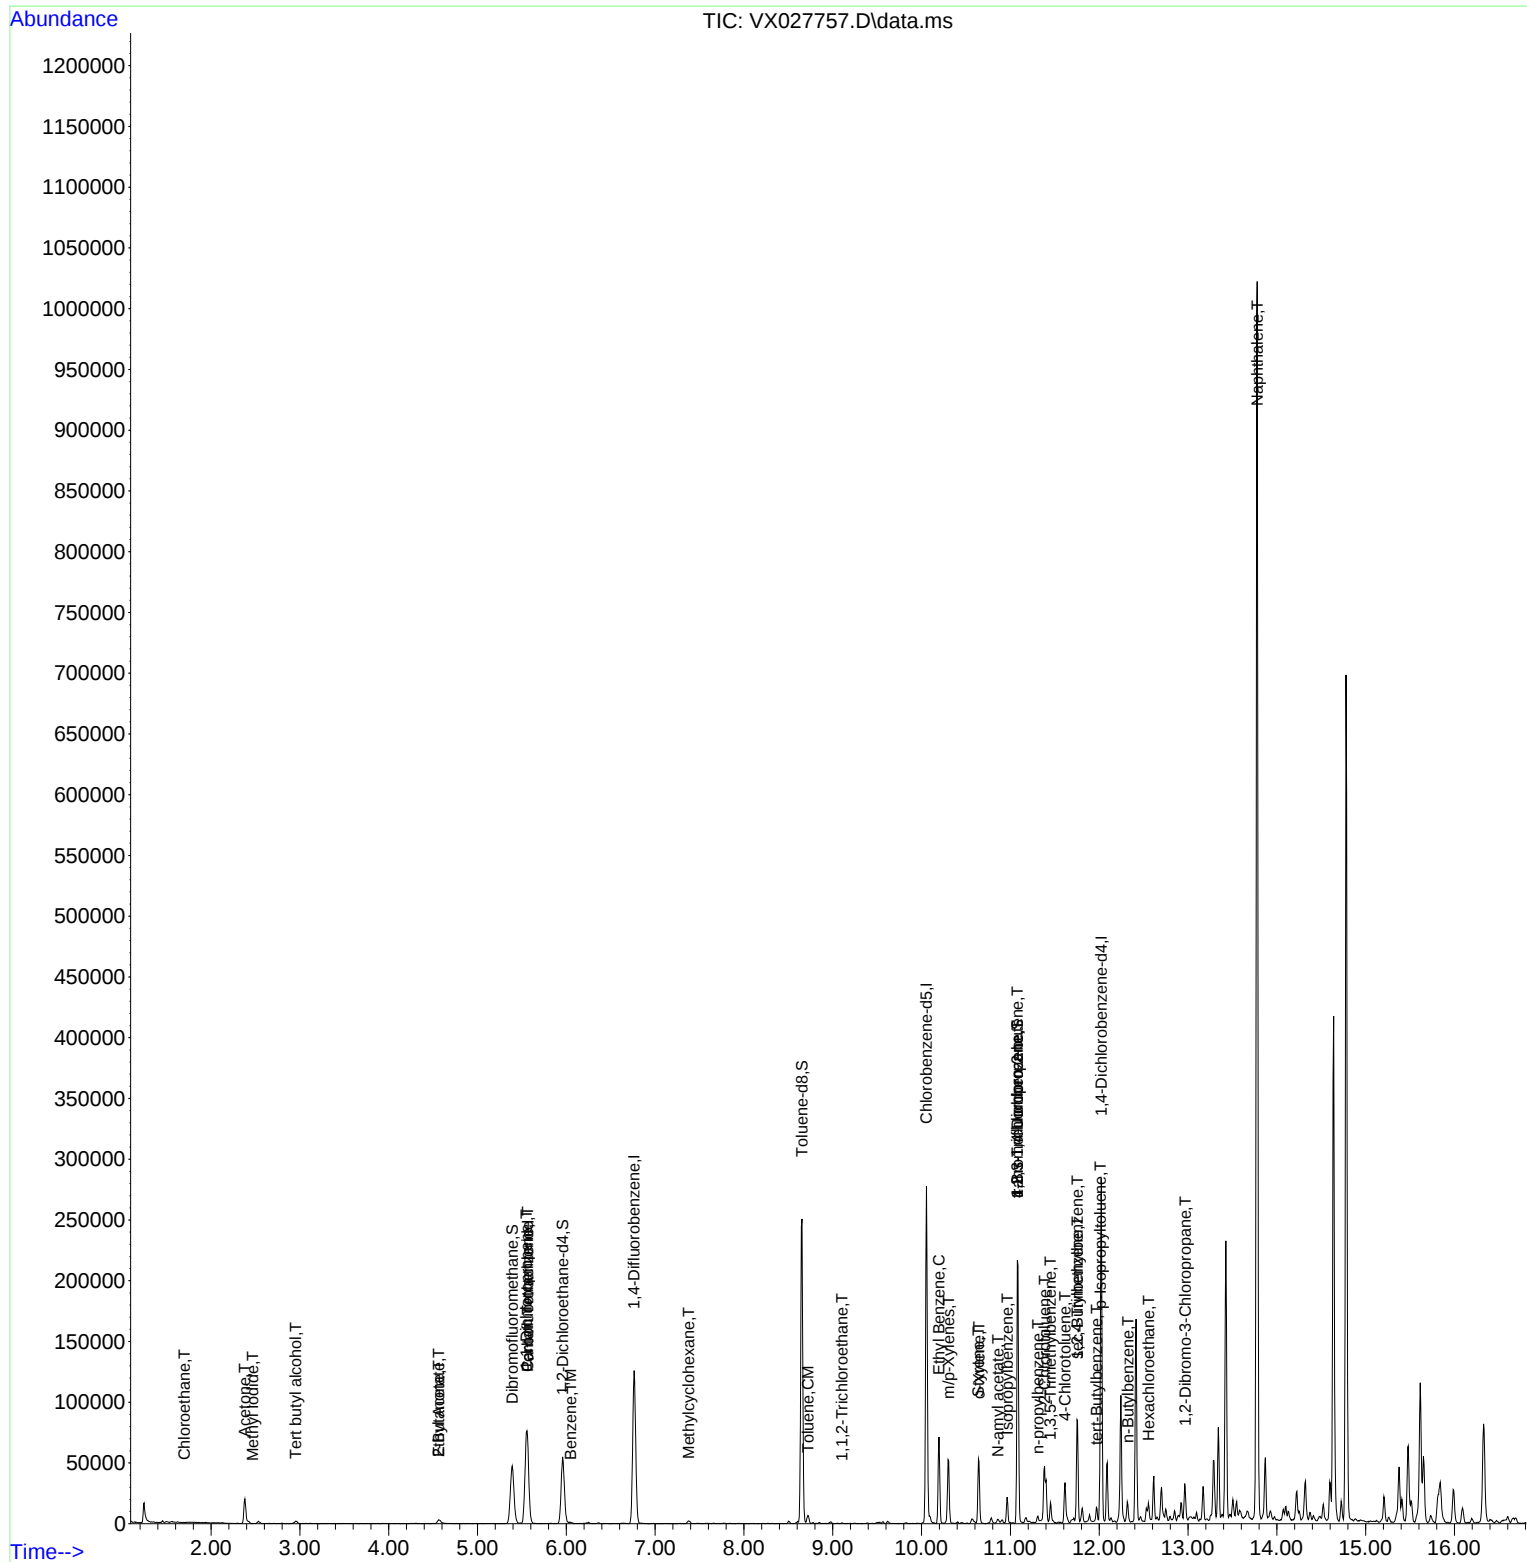






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE







Tgt Ion:168 Resp: 68963
Ion Ratio Lower Upper
168 100
99 64.7 41.7 62.5#



#6
Chloroethane
Concen: 0.480 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.019 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 64 Resp: 245
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#


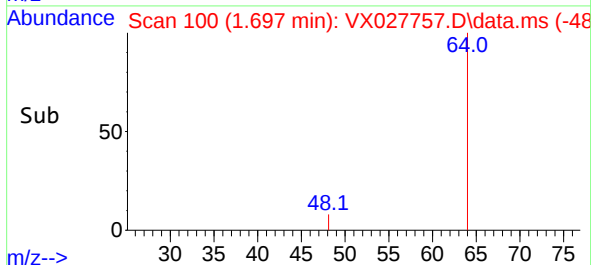
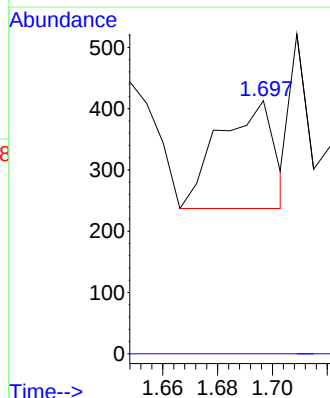
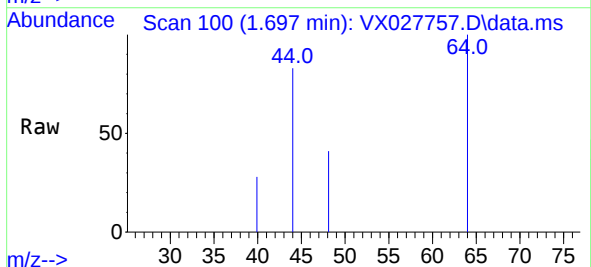




#10
Methyl Iodide
Concen: 2.893 ug/l
RT: 2.465 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion:142 Resp: 23
Ion Ratio Lower Upper
142 100
127 0.0 33.9 50.9#
141 0.0 11.4 17.2#

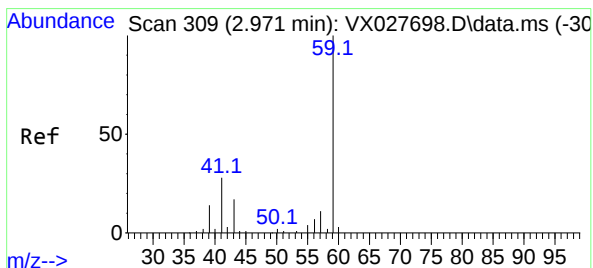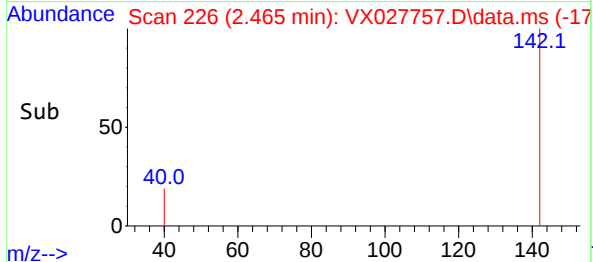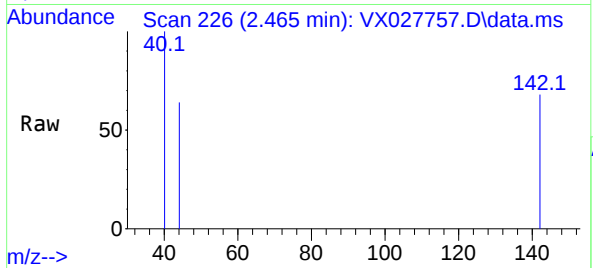

#11
Tert butyl alcohol
Concen: 9.834 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.018 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 59 Resp: 2071
Ion Ratio Lower Upper
59 100
57 4.9 8.3 12.5#


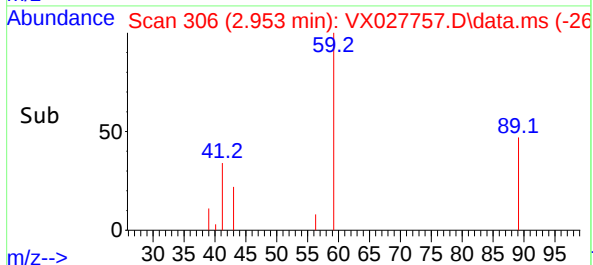
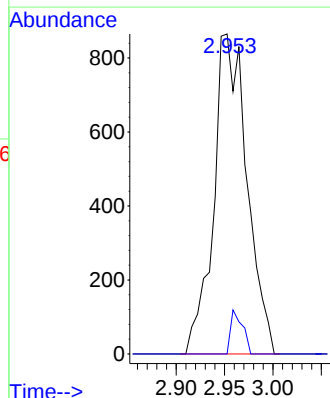
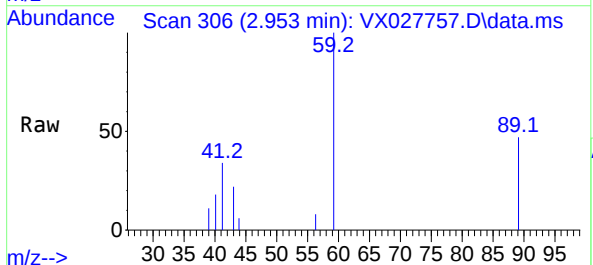




#16
Acetone
Concen: 44.260 ug/l
RT: 2.380 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion: 43 Resp: 21172
Ion Ratio Lower Upper
43 100
58 32.8 28.8 43.2

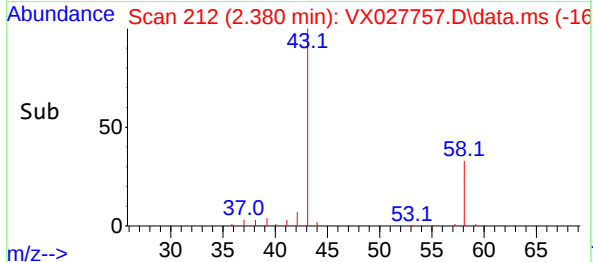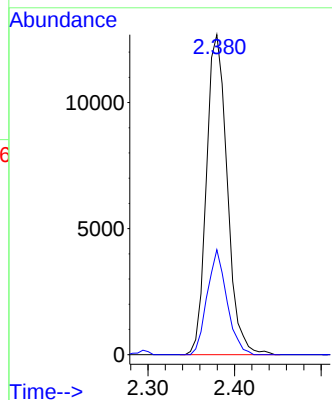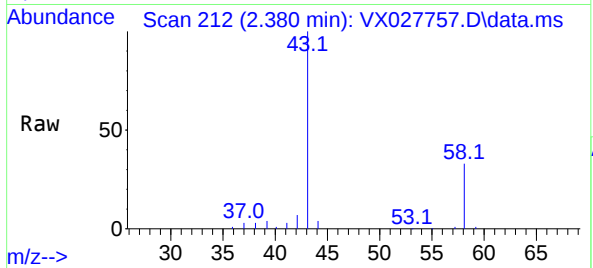

#25
2-Butanone
Concen: 7.390 ug/l
RT: 4.562 min Scan# 570
Delta R.T. 0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 43 Resp: 5677
Ion Ratio Lower Upper
43 100
72 24.3 24.4 36.6#

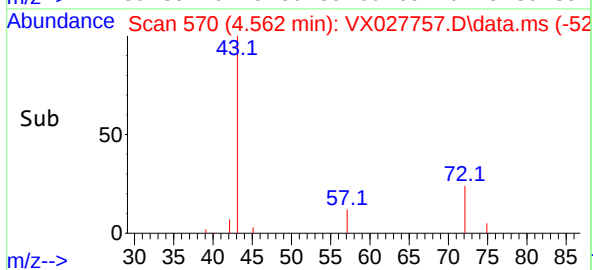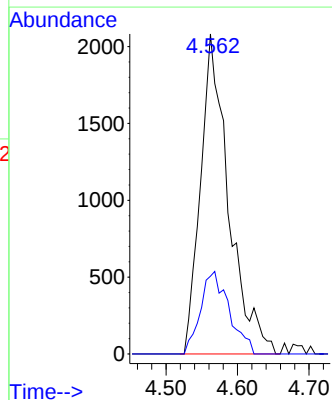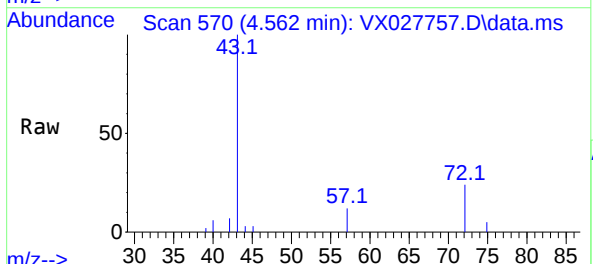

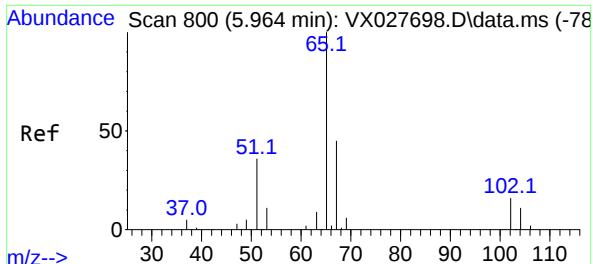

#33

1,2-Dichloroethane-d4

Concen: 45.949 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05

Instrument :

MSVOA_X

ClientSampleId :





20220344-MODIFIED-ELUTRIATE

Tgt Ion: 65 Resp: 51972

Ion Ratio Lower Upper

65 100

67 52.2 0.0 107.4

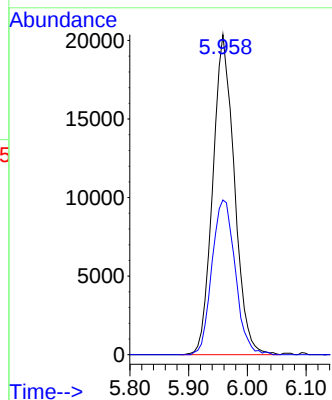

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05




Tgt Ion: 114 Resp: 120007


Ion Ratio Lower Upper

114 100

63 24.0 0.0 36.8

88 17.4 0.0 32.4


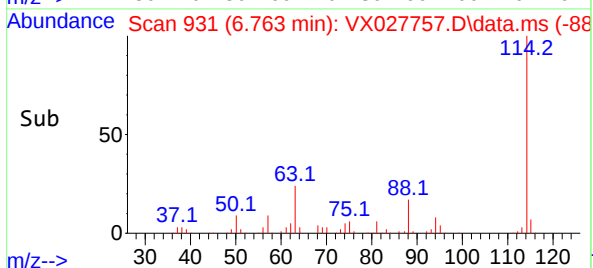
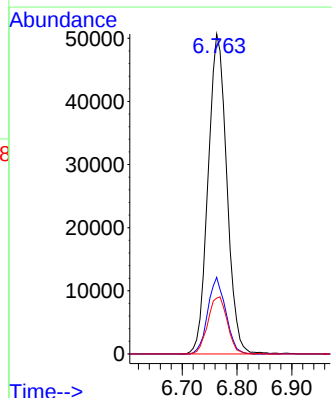
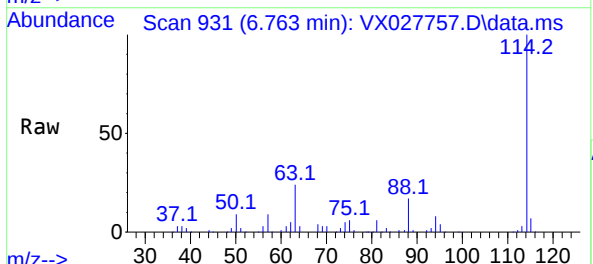


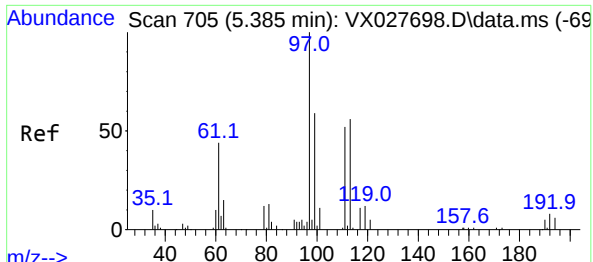

#35
Dibromofluoromethane
Concen: 51.607 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion:113 Resp: 40670
Ion Ratio Lower Upper
113 100
111 101.0 82.8 124.2
192 18.5 16.9 25.3

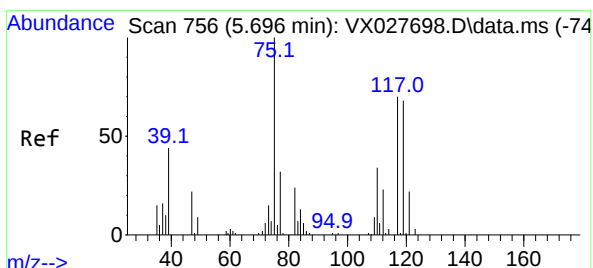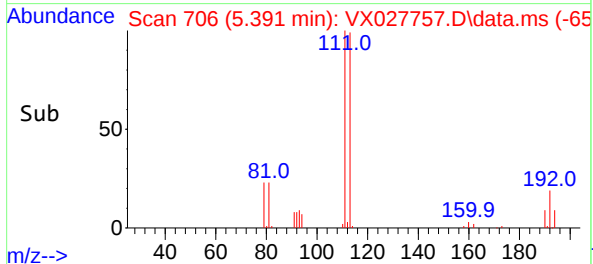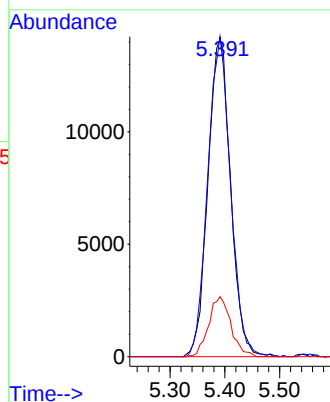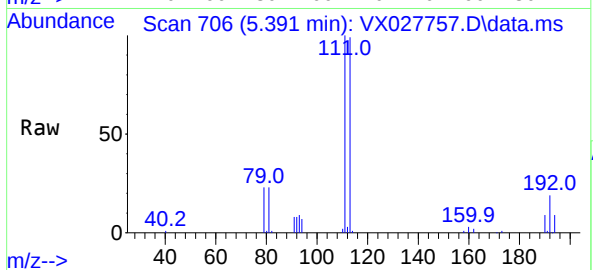

#36
1,1-Dichloropropene
Concen: 4.766 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.146 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 75 Resp: 5932
Ion Ratio Lower Upper
75 100
110 6.8 18.3 54.8#
77 0.0 24.8 37.2#

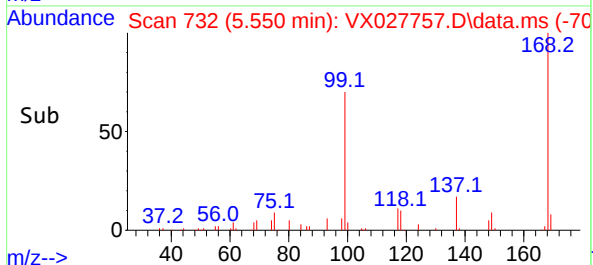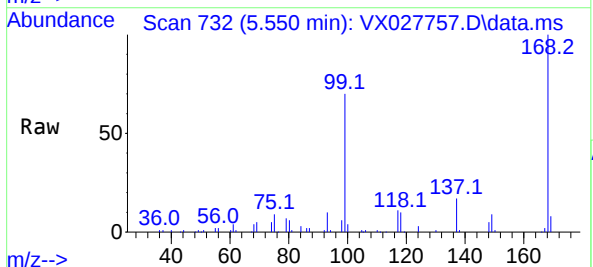



#37

Ethyl Acetate

Concen: 3.918 ug/l

RT: 4.562 min Scan# 51

Delta R.T. -0.159 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05

Instrument :

MSVOA_X

ClientSampleId :

20220344-MODIFIED-ELUTRIATE





Tgt Ion: 43 Resp: 5677

Ion Ratio Lower Upper

43 100

61 0.0 12.6 19.0#

70 0.0 10.2 15.2#

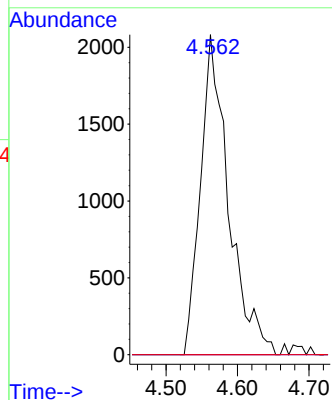

#38

Carbon Tetrachloride

Concen: 6.052 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.116 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05




Tgt Ion: 117 Resp: 7362


Ion Ratio Lower Upper

117 100

119 6.7 77.3 115.9#

121 0.0 24.2 36.2#

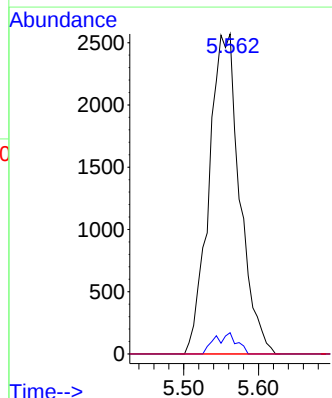



#39

Methylcyclohexane

Concen: 0.689 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.006 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05





Instrument :

MSVOA_X

ClientSampleId :

20220344-MODIFIED-ELUTRIATE

Tgt Ion: 83	Resp: 986
Ion Ratio	Lower Upper
83	100
55	77.1 54.6 81.8
98	30.2 37.4 56.2#

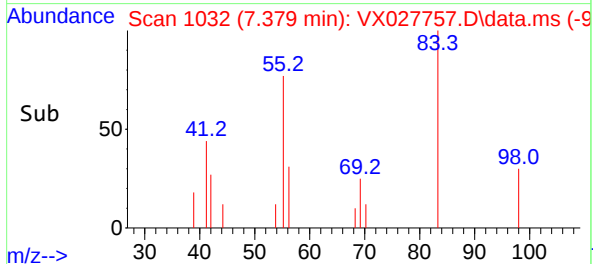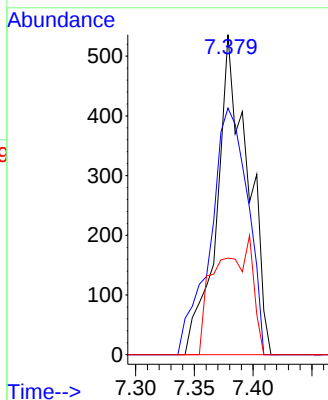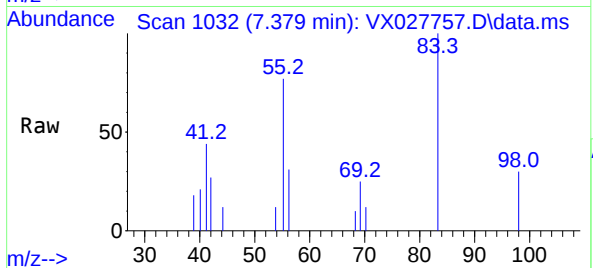

#40

Benzene

Concen: 0.352 ug/l




RT: 6.050 min Scan# 814


Delta R.T. 0.006 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05

Tgt Ion: 78	Resp: 1210
Ion Ratio	Lower Upper
78	100
77	21.4 19.3 28.9

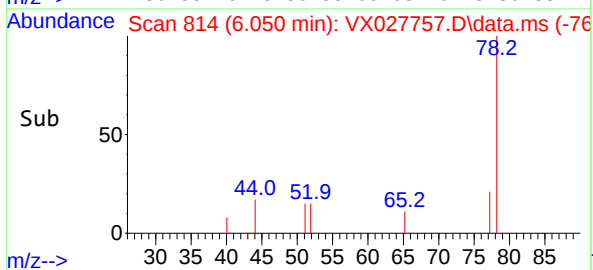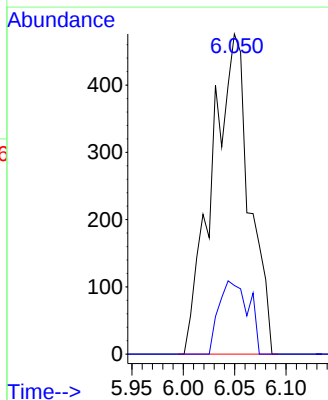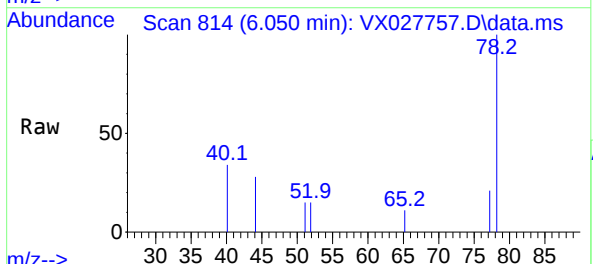



#48

Methyl methacrylate

Concen: Below Cal

RT: 7.659 min Scan# 1084

Delta R.T. -0.037 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05

Instrument :

MSVOA_X

ClientSampleId :

20220344-MODIFIED-ELUTRIATE





Tgt Ion: 41 Resp: 142

Ion Ratio Lower Upper

41 100

69 93.7 82.5 123.7

39 0.0 43.8 65.8#

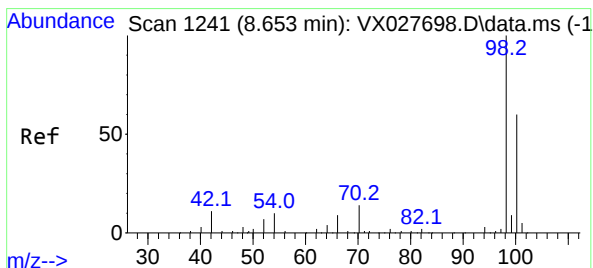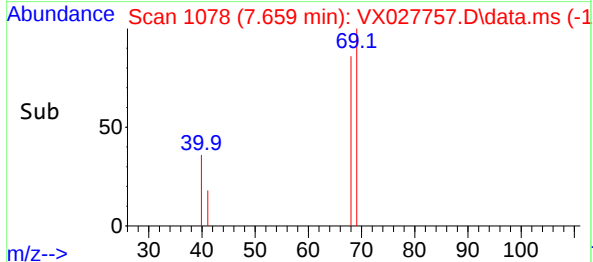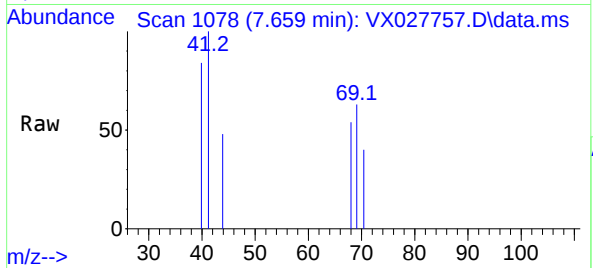

#50

Toluene-d8

Concen: 48.770 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX027757.D




Acq: 28 Mar 2022 18:05


Tgt Ion: 98 Resp: 148575

Ion Ratio Lower Upper

98 100

100 65.3 52.6 78.8


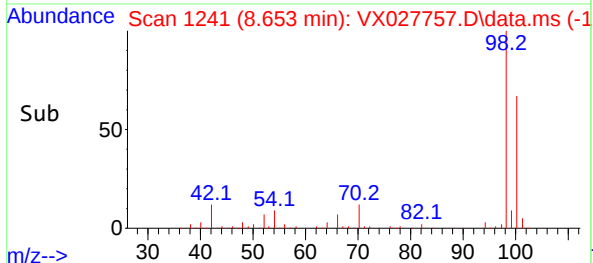
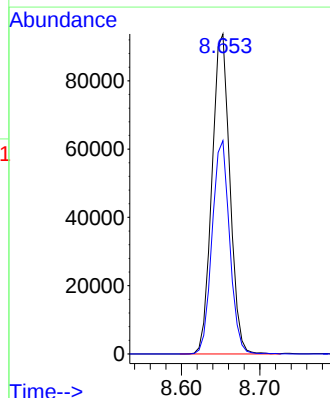
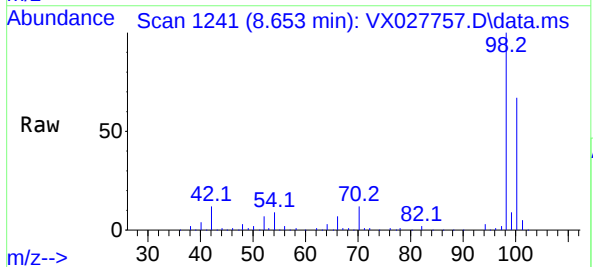




#52
Toluene
Concen: 1.335 ug/l
RT: 8.720 min Scan# 1315
Delta R.T. -0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument : MSVOA_X
ClientSampleId : 20220344-MODIFIED-ELUTRIATE


Tgt Ion: 92 Resp: 2870
Ion Ratio Lower Upper
92 100
91 166.0 137.5 206.3

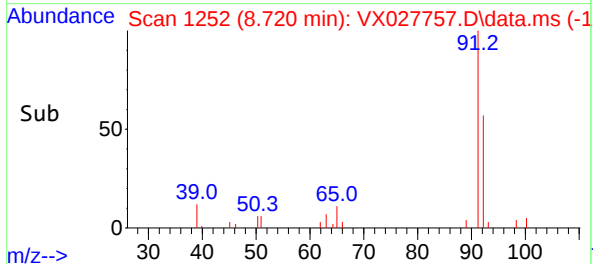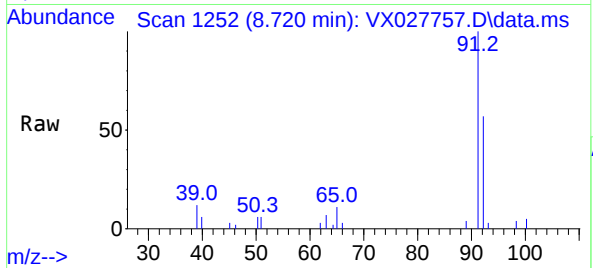

#55
1,1,2-Trichloroethane
Concen: 0.270 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 97 Resp: 236
Ion Ratio Lower Upper
97 100
83 0.0 66.2 99.4#
85 0.0 42.9 64.3#
99 0.0 49.0 73.6#


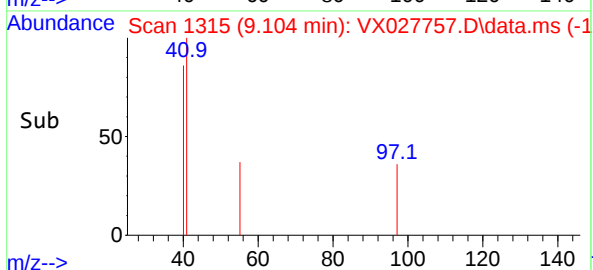
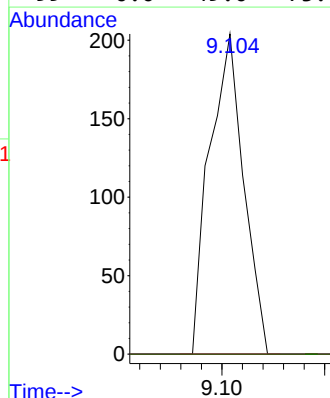





#62
4-Bromofluorobenzene
Concen: 50.345 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion: 95 Resp: 62234
Ion Ratio Lower Upper
95 100
174 64.2 0.0 163.0
176 62.5 0.0 155.0

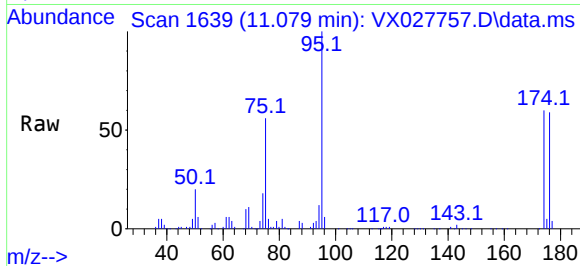

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 117 Resp: 112664
Ion Ratio Lower Upper
117 100
82 61.7 41.8 62.8
119 32.2 24.8 37.2

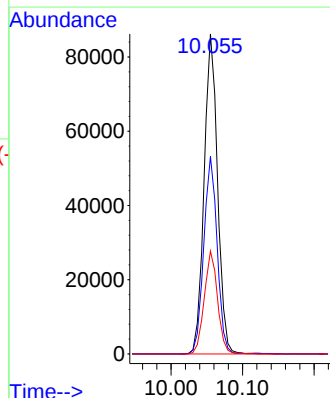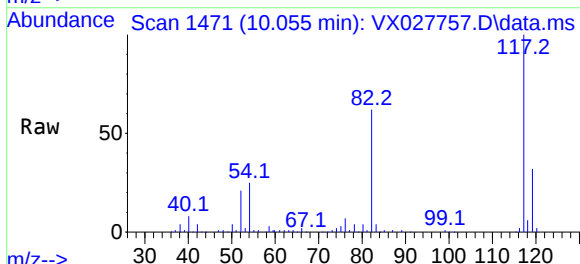



#67

Ethyl Benzene

Concen: 8.749 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX027757.D

Acq: 28 Mar 2022 18:05

Instrument :

MSVOA_X

ClientSampleId :





20220344-MODIFIED-ELUTRIATE

Tgt Ion: 91 Resp: 38679

Ion Ratio Lower Upper

91 100

106 34.5 24.6 36.8

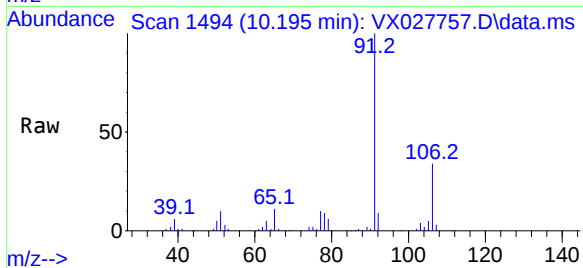

#68

m/p-Xylenes

Concen: 7.230 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX027757.D




Acq: 28 Mar 2022 18:05


Tgt Ion:106 Resp: 11585

Ion Ratio Lower Upper

106 100

91 218.8 160.4 240.6



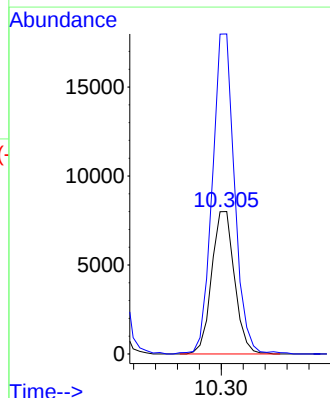
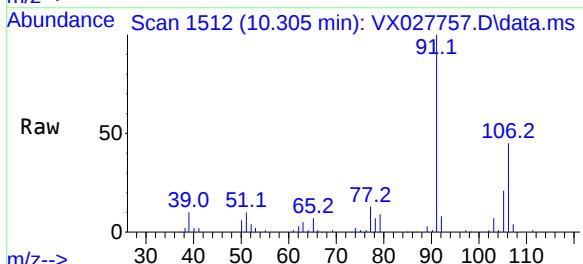




#69
o-Xylene
Concen: 6.583 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion:106 Resp: 10601
Ion Ratio Lower Upper
106 100
91 238.0 106.1 318.1

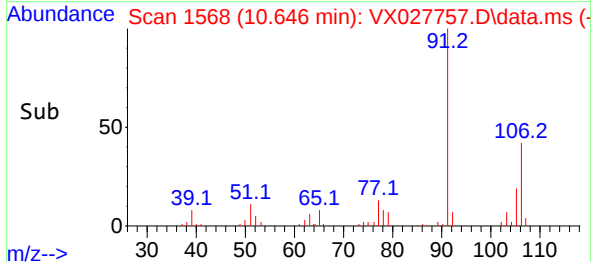

#70
Styrene
Concen: 0.326 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.019 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion:104 Resp: 835
Ion Ratio Lower Upper
104 100
78 258.9 38.6 57.8#
103 213.1 43.8 65.8#


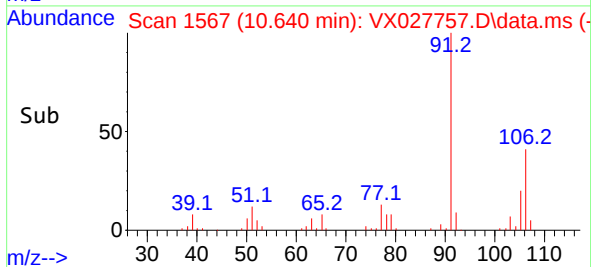

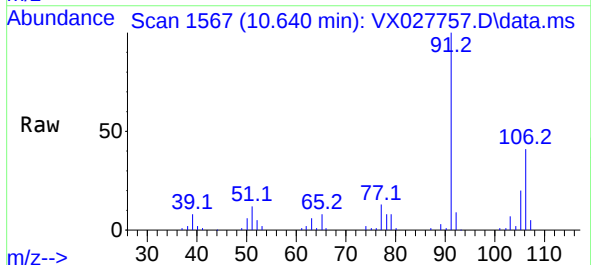




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion:152 Resp: 49567
Ion Ratio Lower Upper
152 100
115 69.5 37.5 112.7
150 156.7 0.0 338.2

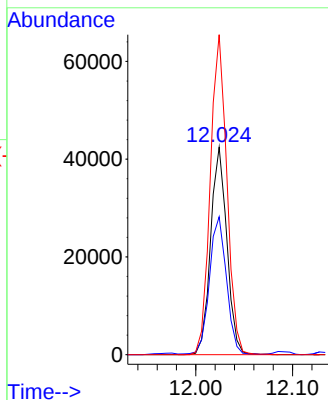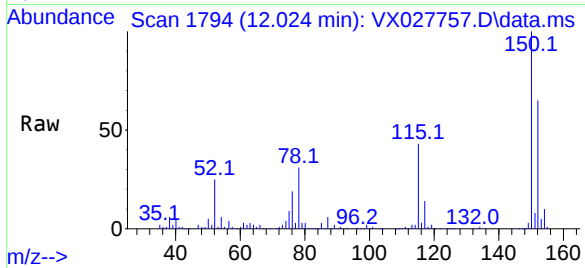

#73
Isopropylbenzene
Concen: 2.532 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion:105 Resp: 10309
Ion Ratio Lower Upper
105 100
120 25.4 13.5 40.5


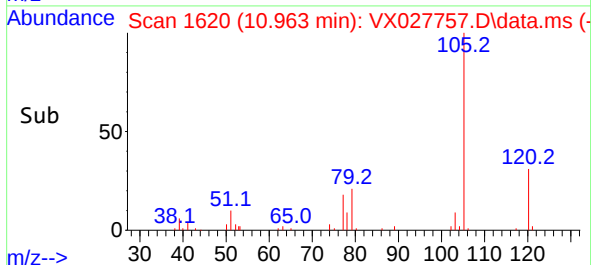
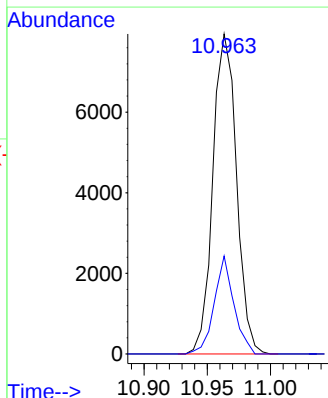
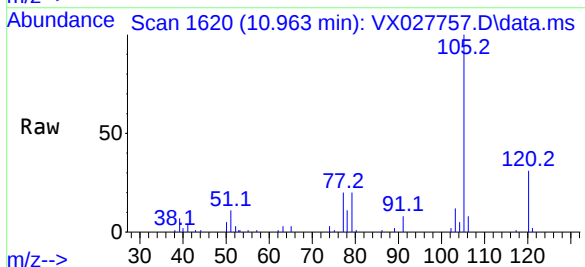




#74
N-amy1 acetate
Concen: 0.258 ug/l
RT: 10.860 min Scan# 1
Delta R.T. 0.012 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion: 43	Resp: 505
Ion Ratio	Lower Upper
43	100
70	47.9 42.5 63.7
55	140.0 23.1 34.7#
61	0.0 22.8 34.2#

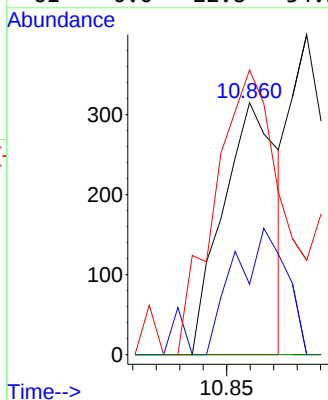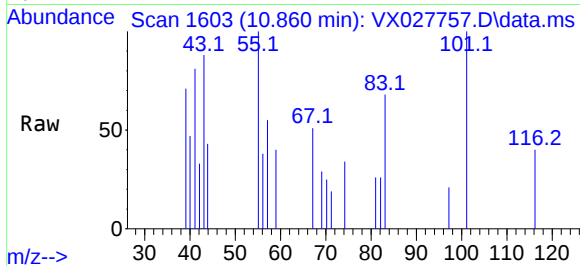

#76
1,2,3-Trichloropropane
Concen: 23.992 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 75	Resp: 33110
Ion Ratio	Lower Upper
75	100
77	1.2 19.4 58.2#


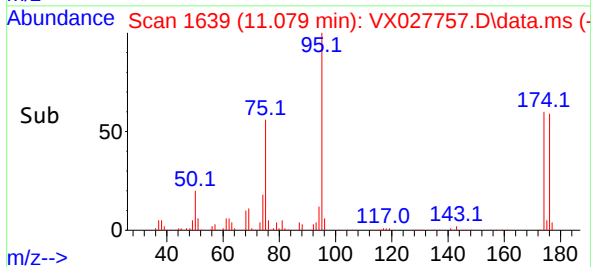
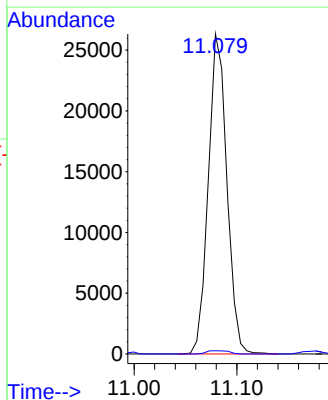
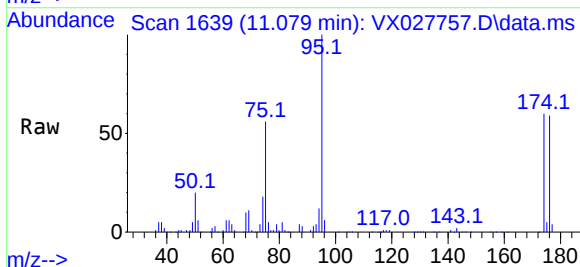




#78
n-propylbenzene
Concen: 0.669 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.006 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion: 91 Resp: 3232
Ion Ratio Lower Upper
91 100
120 21.5 11.6 34.8



#79
2-Chlorotoluene
Concen: 1.666 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 91 Resp: 5074
Ion Ratio Lower Upper
91 100
126 4.0 17.3 51.9#


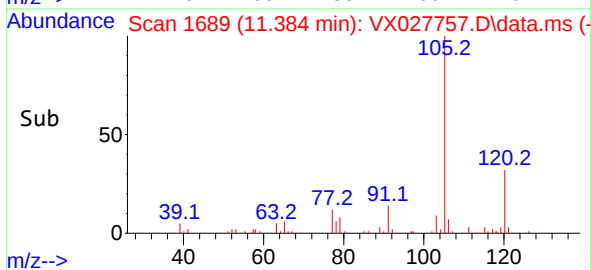

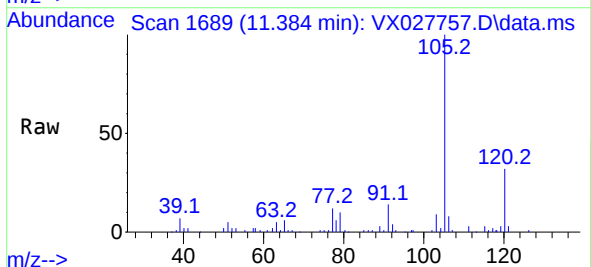




#80
1,3,5-Trimethylbenzene
Concen: 1.899 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion:105 Resp: 6644
Ion Ratio Lower Upper
105 100
120 46.1 24.3 72.9

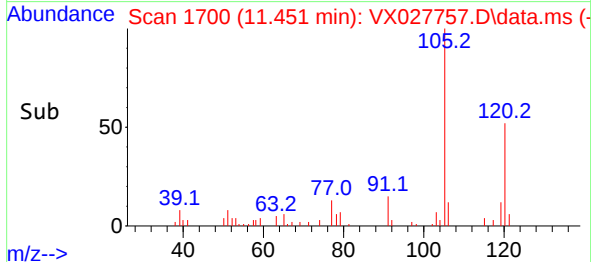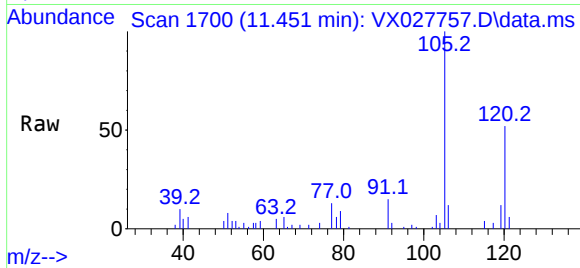

#81
trans-1,4-Dichloro-2-butene
Concen: 81.664 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 75 Resp: 33110
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#


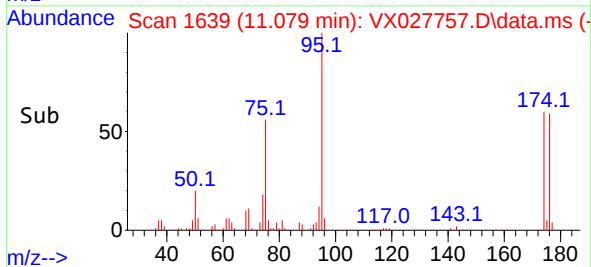

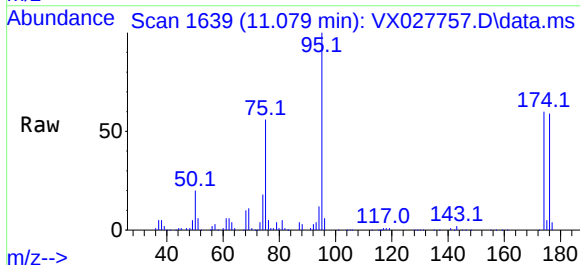




#82
4-Chlorotoluene
Concen: 0.661 ug/l
RT: 11.616 min Scan# 11
Delta R.T. 0.159 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion: 91 Resp: 2316
Ion Ratio Lower Upper
91 100
126 19.3 14.9 44.5

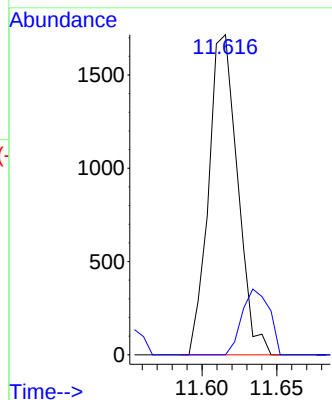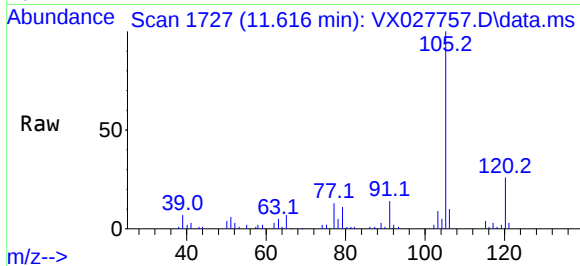

#83
tert-Butylbenzene
Concen: 1.432 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.250 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 119 Resp: 4603
Ion Ratio Lower Upper
119 100
91 30.6 26.9 80.6
134 25.5 11.4 34.2


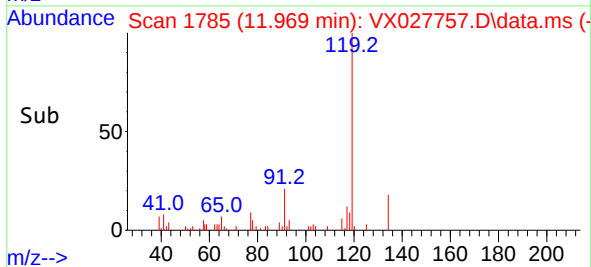
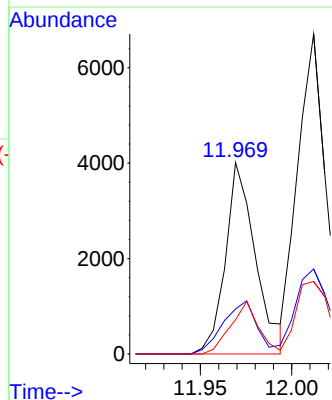
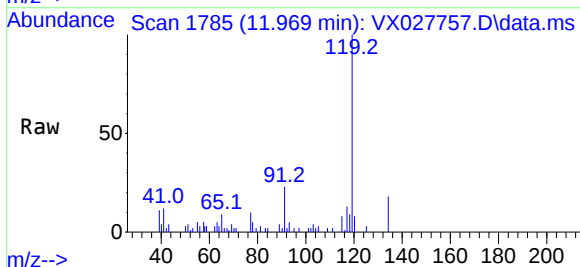




#84
1,2,4-Trimethylbenzene
Concen: 10.466 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion:105 Resp: 37172
Ion Ratio Lower Upper
105 100
120 43.0 22.6 67.8

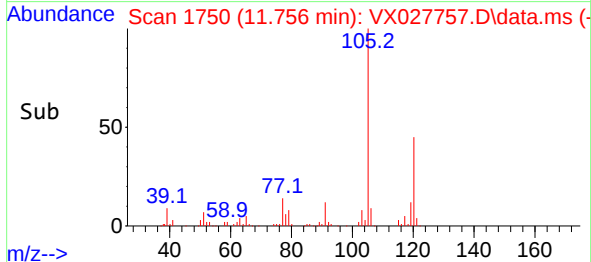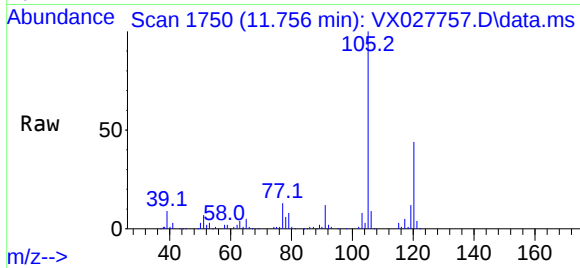

#85
sec-Butylbenzene
Concen: 8.827 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion:105 Resp: 37172
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#


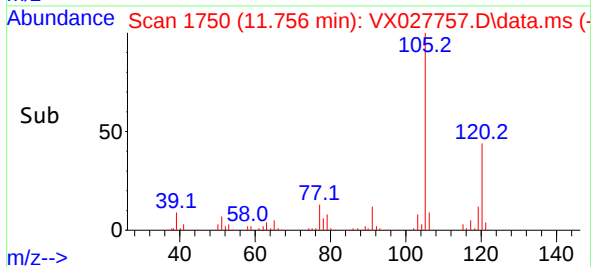

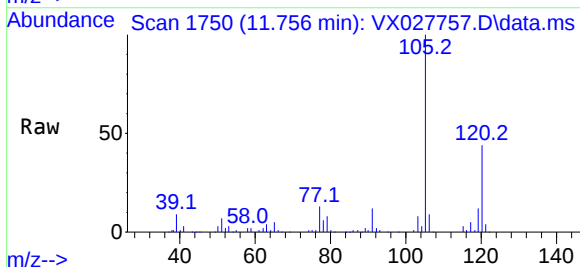




#86
p-Isopropyltoluene
Concen: 2.155 ug/l
RT: 12.012 min Scan# 119
Delta R.T. -0.000 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument : MSVOA_X
ClientSampleId : 20220344-MODIFIED-ELUTRIATE


Tgt Ion:	119	Resp:	7142
Ion	Ratio	Lower	Upper
119	100		
134	25.7	13.0	39.0
91	31.7	11.3	33.9

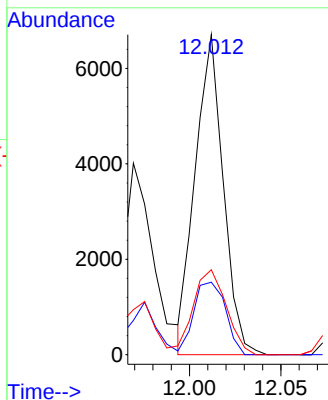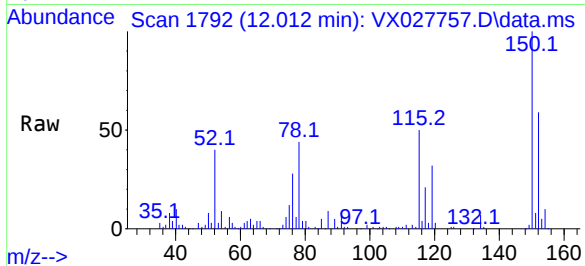

#89
n-Butylbenzene
Concen: 0.642 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion:	91	Resp:	2015
Ion	Ratio	Lower	Upper
91	100		
92	18.1	27.8	83.3#
134	104.4	13.3	39.8#


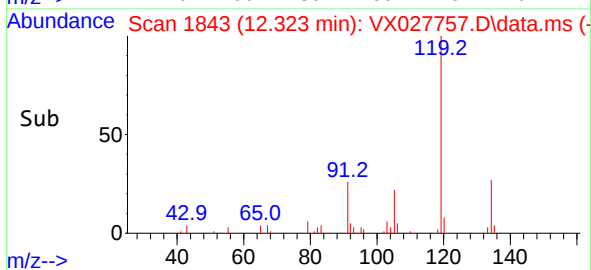
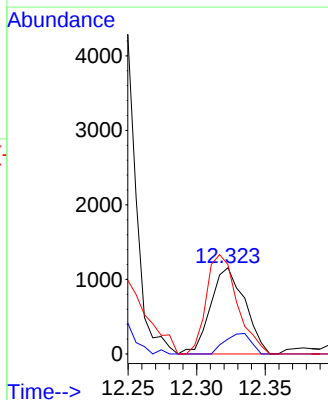
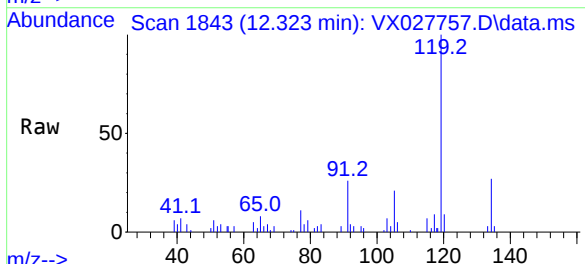




#90
Hexachloroethane
Concen: 2.515 ug/l
RT: 12.555 min Scan# 1881
Delta R.T. 0.013 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05




Instrument :
MSVOA_X
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Tgt Ion:117 Resp: 1330
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

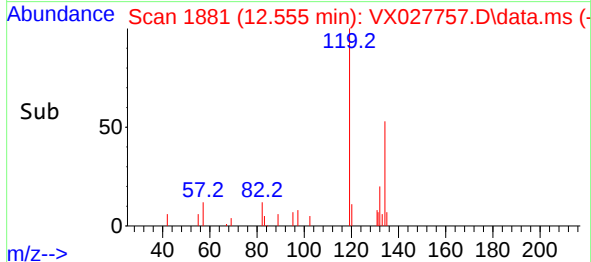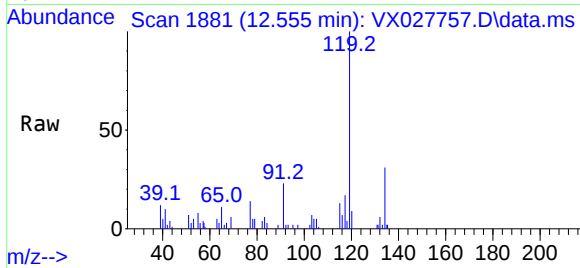

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.390 ug/l
RT: 12.969 min Scan# 1949
Delta R.T. 0.024 min
Lab File: VX027757.D
Acq: 28 Mar 2022 18:05

Tgt Ion: 75 Resp: 137
Ion Ratio Lower Upper
75 100
155 0.0 47.0 141.2#
157 0.0 57.9 173.6#

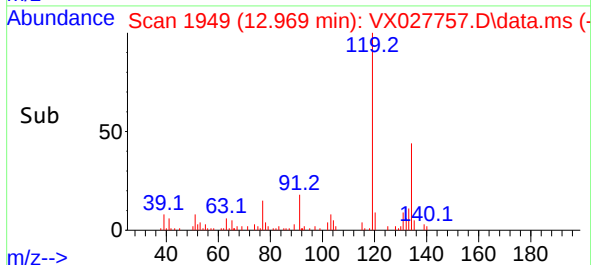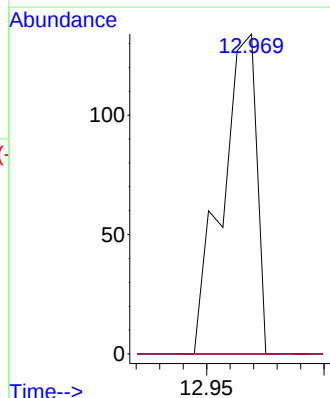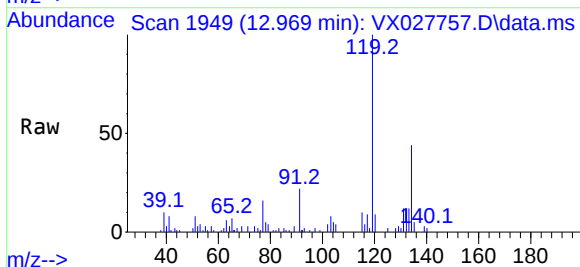



#95

Naphthalene

Concen: 168.059 ug/l

RT: 13.780 min Scan# 20

Delta R.T. -0.000 min

Lab File: VX027757.D


Acq: 28 Mar 2022 18:05

Instrument :

MSVOA_X

ClientSampleId :

20220344-MODIFIED-ELUTRIATE



Tgt Ion:128 Resp: 593227

Ion Ratio Lower Upper

128 100

127 13.2 10.2 15.4

129 11.0 8.7 13.1

