

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
 Data File : VX027759.D
 Acq On : 28 Mar 2022 18:52
 Operator : JC/MD
 Sample : N2041-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-20220316

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M

Title : SW846 8260

Signal : TIC: VX027759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	39	rBV	13572	24354	5.94%	1.084%
2	2.532	231	237	251	rBV	7596	14157	3.45%	0.630%
3	2.947	296	305	312	rVB3	2047	5073	1.24%	0.226%
4	5.391	695	706	722	rBV3	48212	140460	34.25%	6.250%
5	5.550	722	732	748	rVV3	77415	222928	54.36%	9.920%
6	5.958	790	799	813	rBV	57774	154661	37.71%	6.882%
7	6.763	922	931	944	rBV	129989	306647	74.77%	13.645%
8	8.653	1234	1241	1251	rBV	258824	410100	100.00%	18.248%
9	10.055	1464	1471	1484	rBV	266893	356208	86.86%	15.850%
10	11.079	1634	1639	1647	rBV	213301	280541	68.41%	12.483%
11	12.024	1789	1794	1802	rBV	272081	332181	81.00%	14.781%




Sum of corrected areas: 2247310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027759.D
Acq On : 28 Mar 2022 18:52
Operator : JC/MD
Sample : N2041-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

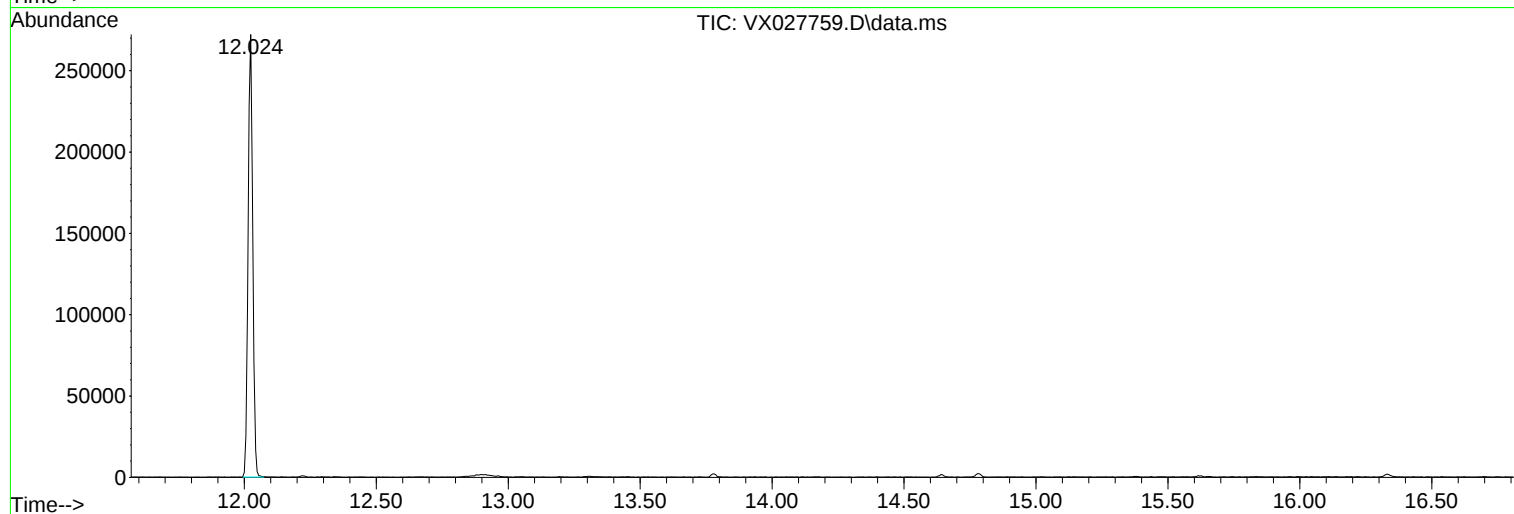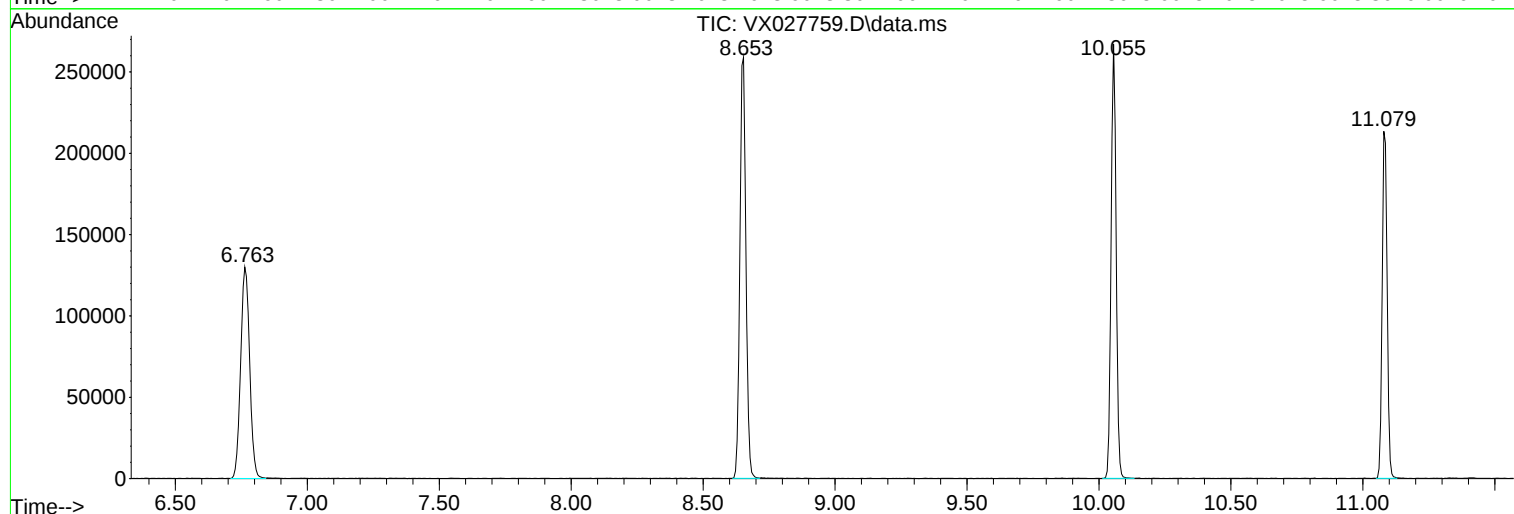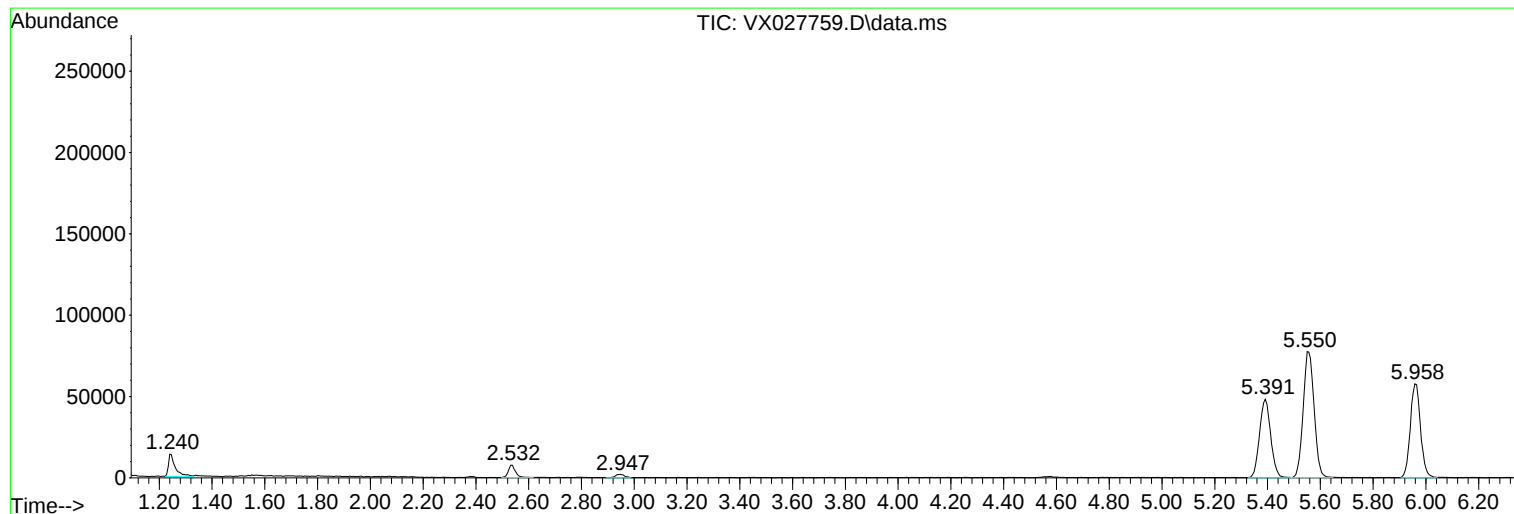

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027759.D
Acq On : 28 Mar 2022 18:52
Operator : JC/MD
Sample : N2041-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027759.D
Acq On : 28 Mar 2022 18:52
Operator : JC/MD
Sample : N2041-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------