

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027761.D
Acq On : 28 Mar 2022 19:39
Operator : JC/MD
Sample : N2041-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20220316

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M

Title : SW846 8260

Signal : TIC: VX027761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	197	204	212	rBV2	37111	73401	2.82%	1.548%
2	5.391	693	706	721	rBB	43342	127366	4.89%	2.686%
3	5.556	721	733	747	rBV2	73748	210975	8.11%	4.448%
4	5.958	790	799	813	rBV2	47612	127303	4.89%	2.684%
5	6.763	922	931	942	rBV	116666	279913	10.75%	5.902%
6	7.129	979	991	1007	rBV	1220929	2602651	100.00%	54.878%
7	8.653	1234	1241	1250	rBV	243968	380081	14.60%	8.014%
8	9.275	1337	1343	1348	rBB	21386	31229	1.20%	0.658%
9	10.055	1465	1471	1481	rBV	254344	340134	13.07%	7.172%
10	11.085	1634	1640	1652	rVB	199941	263444	10.12%	5.555%
11	12.024	1789	1794	1805	rVB	249569	306119	11.76%	6.455%




Sum of corrected areas: 4742616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027761.D
Acq On : 28 Mar 2022 19:39
Operator : JC/MD
Sample : N2041-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

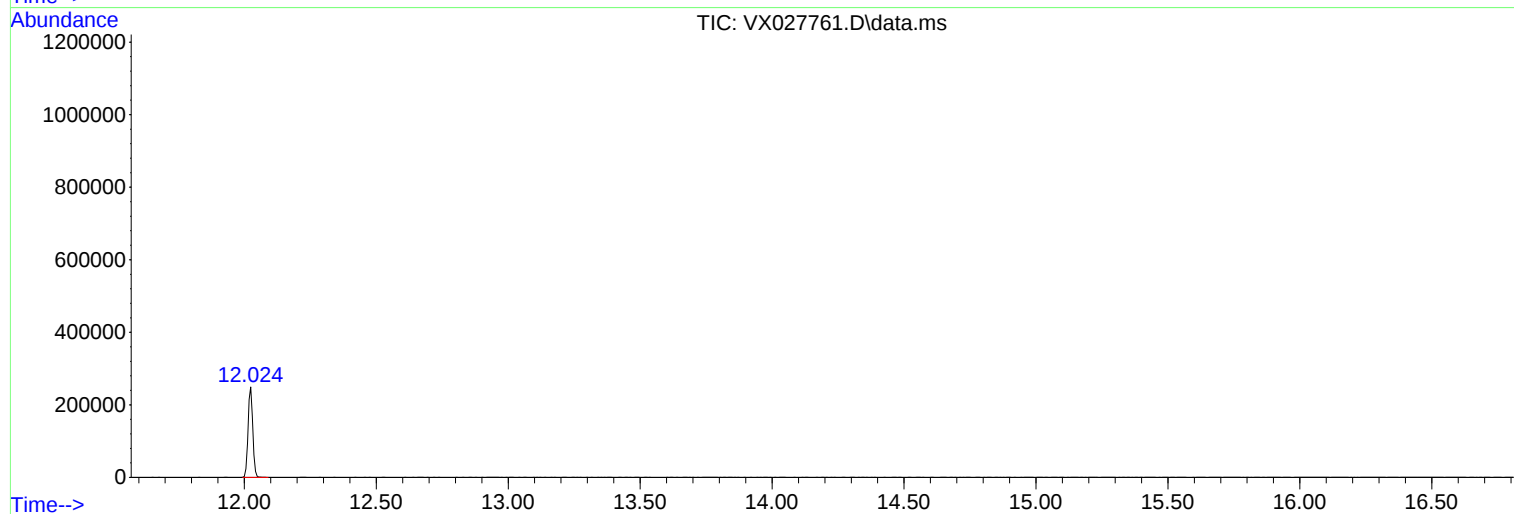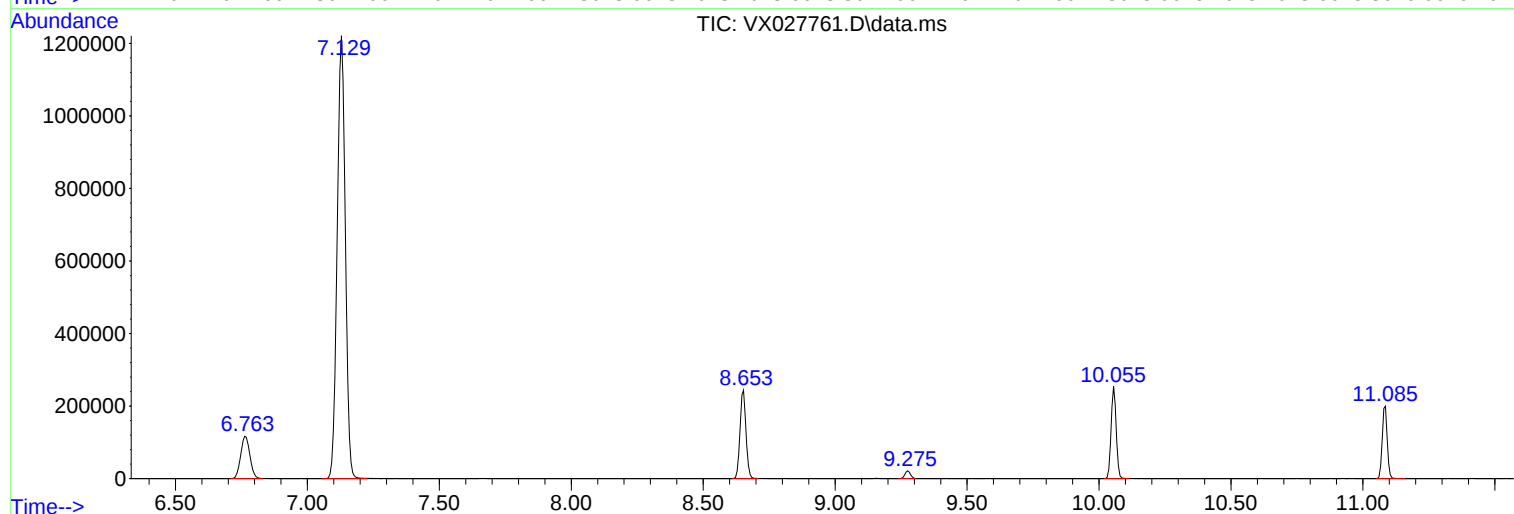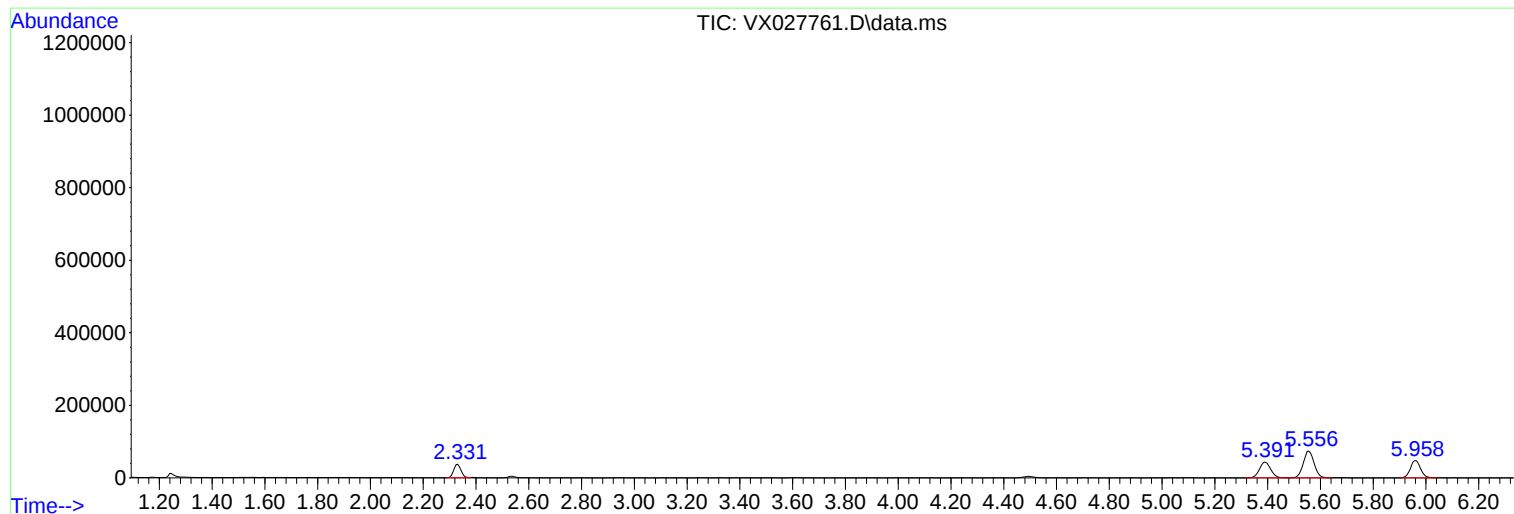

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027761.D
Acq On : 28 Mar 2022 19:39
Operator : JC/MD
Sample : N2041-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027761.D
Acq On : 28 Mar 2022 19:39
Operator : JC/MD
Sample : N2041-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20220316

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------