
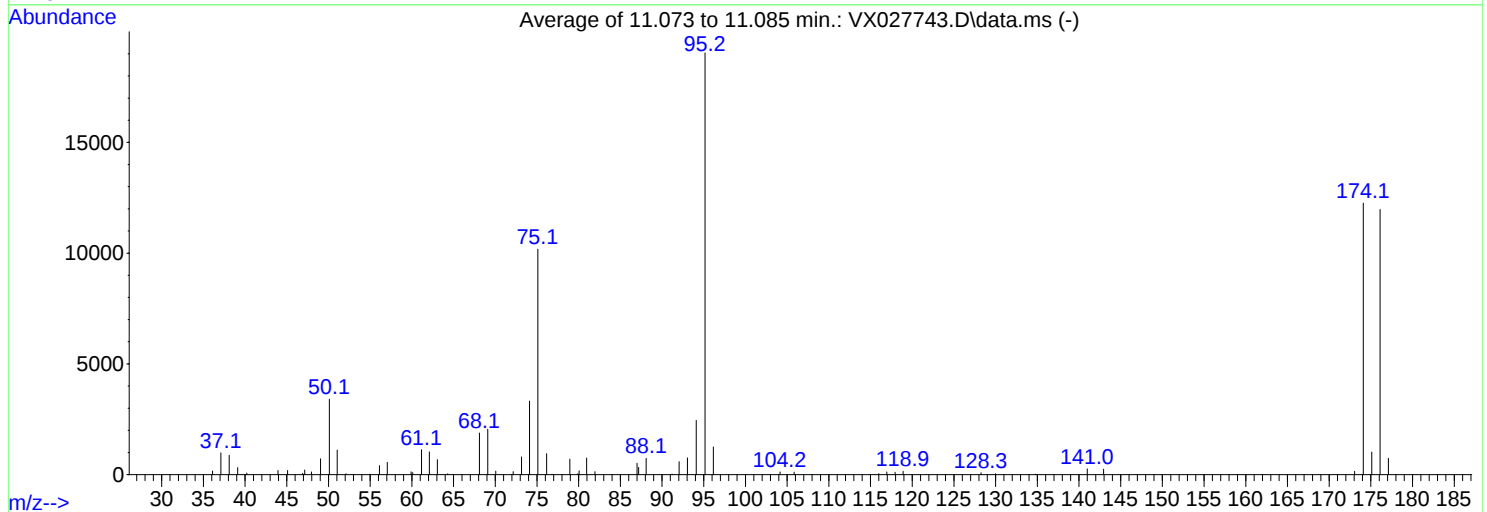


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
Data File : VX027743.D
Acq On : 28 Mar 2022 10:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
Title : SW846 8260
Last Update : Fri Mar 25 16:26:59 2022

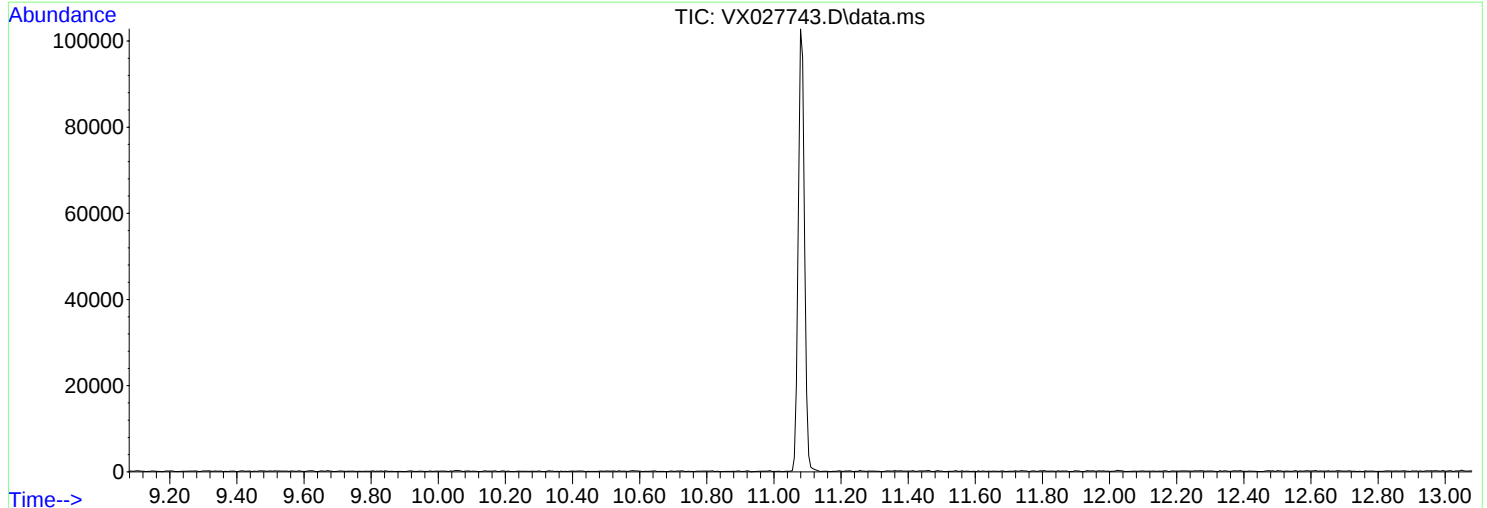

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	3410	PASS
75	95	30	60	53.5	10178	PASS
95	95	100	100	100.0	19042	PASS
96	95	5	9	6.6	1253	PASS
173	174	0.00	2	1.3	155	PASS
174	95	50	100	64.4	12255	PASS
175	174	5	9	8.3	1019	PASS
176	174	95	101	97.7	11968	PASS
177	176	5	9	6.2	738	PASS