
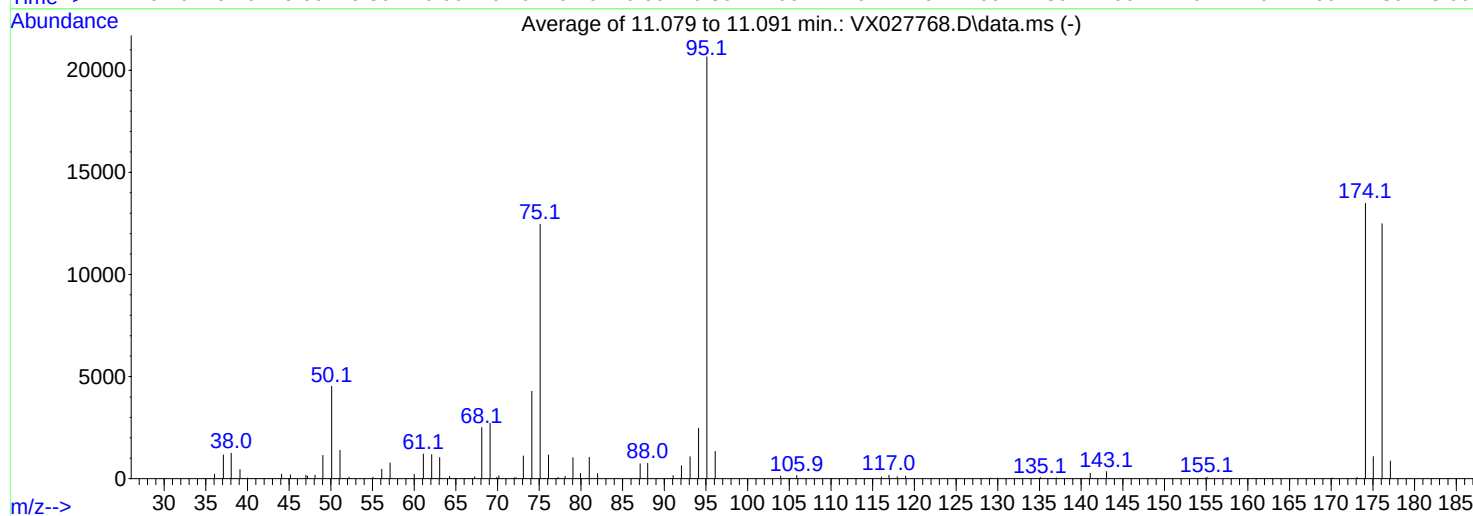


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032822\
 Data File : VX027768.D
 Acq On : 28 Mar 2022 22:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032522W.M
 Title : SW846 8260
 Last Update : Fri Mar 25 16:26:59 2022

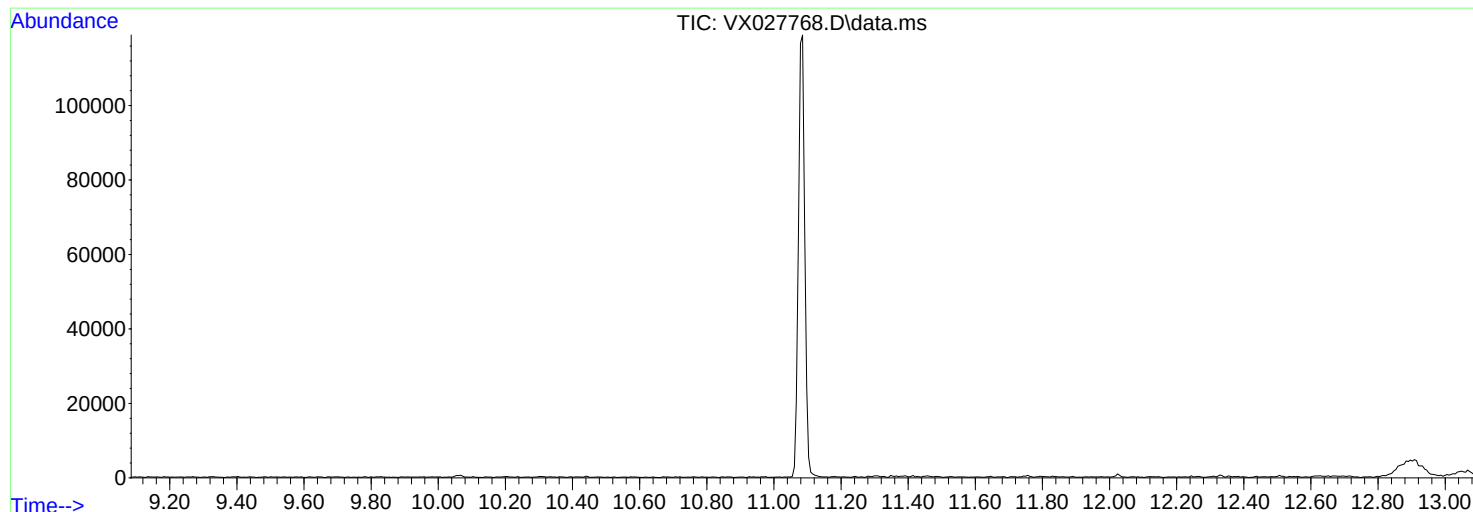

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	4519	PASS
75	95	30	60	60.3	12460	FAIL*
95	95	100	100	100.0	20656	PASS
96	95	5	9	6.4	1329	PASS
173	174	0.00	2	0.4	60	PASS
174	95	50	100	65.3	13479	PASS
175	174	5	9	8.0	1083	PASS
176	174	95	101	92.6	12484	FAIL*
177	176	5	9	6.9	863	PASS