

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034801.D
Acq On : 28 Mar 2023 18:23
Operator : JC/MD
Sample : 02109-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-03-26

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	207	213	220	rBV	34041	60925	4.02%	0.758%
2	2.788	273	279	286	rBV2	7881	15253	1.01%	0.190%
3	5.385	694	705	719	rBV	165631	483936	31.94%	6.017%
4	5.550	721	732	748	rVB	292970	836429	55.20%	10.400%
5	5.952	788	798	817	rBV	205148	537149	35.45%	6.679%
6	6.757	921	930	946	rBV	458305	1109575	73.23%	13.796%
7	8.647	1234	1240	1249	rBV	980087	1515147	100.00%	18.839%
8	10.055	1465	1471	1485	rBV	953796	1297834	85.66%	16.137%
9	11.079	1634	1639	1654	rBV	776360	982733	64.86%	12.219%
10	12.024	1788	1794	1805	rBV	892912	1178340	77.77%	14.651%
11	15.640	2379	2387	2392	rBV9	9299	25219	1.66%	0.314%




Sum of corrected areas: 8042540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034801.D
Acq On : 28 Mar 2023 18:23
Operator : JC/MD
Sample : 02109-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-03-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

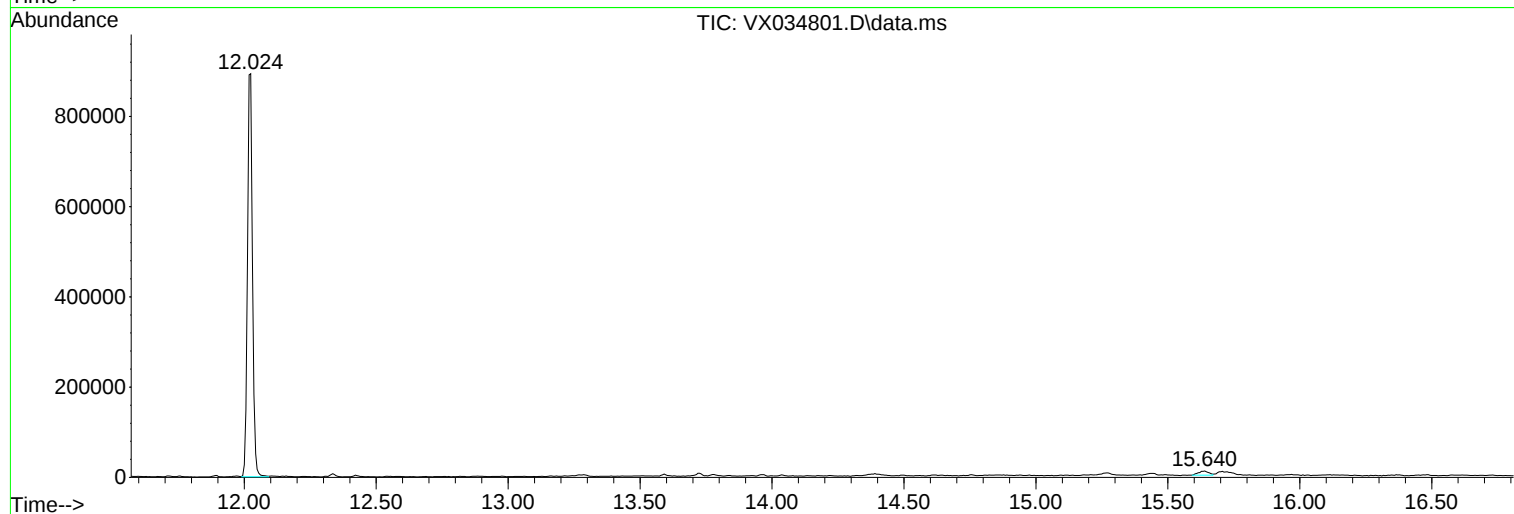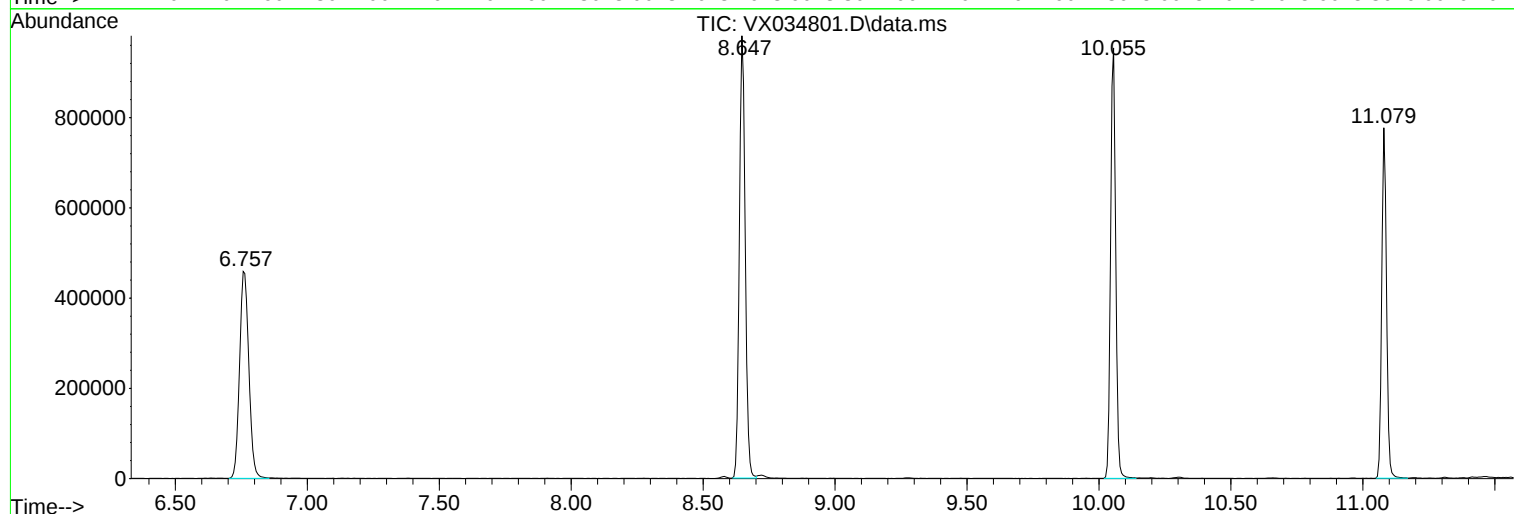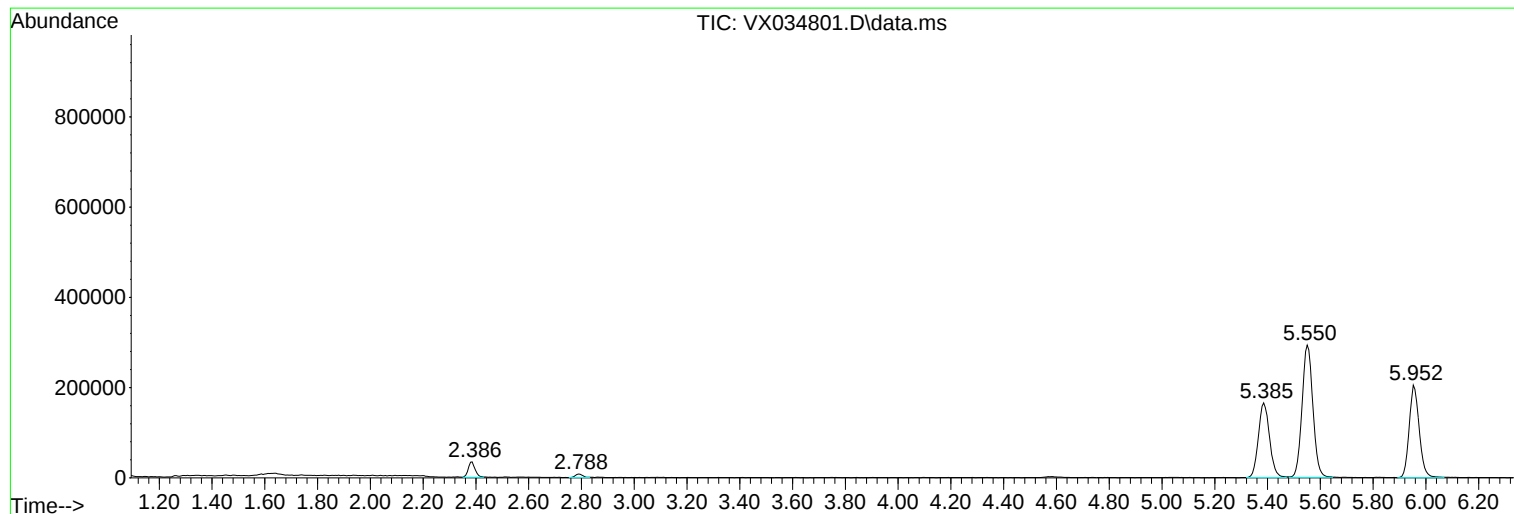

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034801.D
Acq On : 28 Mar 2023 18:23
Operator : JC/MD
Sample : 02109-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-03-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034801.D
Acq On : 28 Mar 2023 18:23
Operator : JC/MD
Sample : 02109-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-03-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------