

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
 Data File : VX034807.D
 Acq On : 28 Mar 2023 20:42
 Operator : JC/MD
 Sample : 01950-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PT-VOA-WP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.618	82	87	99	rBV	423501	536779	13.49%	1.033%
2	1.892	126	132	141	rBV	439334	632027	15.89%	1.217%
3	2.319	195	202	209	rBV	352555	554717	13.95%	1.068%
4	2.386	209	213	230	rVB	88720	173738	4.37%	0.334%
5	2.788	272	279	297	rBV	121715	245514	6.17%	0.473%
6	3.099	319	330	347	rBV2	803908	2044199	51.39%	3.935%
7	4.489	547	558	563	rBV	187844	502863	12.64%	0.968%
8	4.556	563	569	591	rVB	252779	752289	18.91%	1.448%
9	5.093	642	657	673	rBV	349238	1061561	26.69%	2.044%
10	5.385	691	705	721	rBV2	336839	1036594	26.06%	1.996%
11	5.550	721	732	743	rVV	252575	717648	18.04%	1.382%
12	5.678	743	753	770	rVB	258581	766797	19.28%	1.476%
13	5.952	787	798	804	rBV	187538	492297	12.38%	0.948%
14	6.038	804	812	831	rVB	994891	2604818	65.49%	5.014%
15	6.757	920	930	950	rBV	404093	971423	24.42%	1.870%
16	7.824	1094	1105	1121	rBV	426085	798343	20.07%	1.537%
17	8.366	1187	1194	1213	rBV	1024314	1620996	40.75%	3.121%
18	8.574	1221	1228	1235	rBV	1461776	2298908	57.80%	4.426%
19	8.647	1235	1240	1250	rVB	855687	1334136	33.54%	2.568%
20	8.976	1289	1294	1312	rBV	194613	288576	7.25%	0.556%
21	9.275	1336	1343	1357	rBV	772614	1139425	28.65%	2.193%
22	9.427	1363	1368	1377	rBV	656639	931545	23.42%	1.793%
23	9.519	1377	1383	1392	rVV	582208	844094	21.22%	1.625%
24	9.610	1392	1398	1411	rVB	213871	306129	7.70%	0.589%
25	10.055	1465	1471	1472	rBV	863148	1081242	27.18%	2.081%
26	10.079	1472	1475	1483	rVV	1155292	1572168	39.52%	3.027%
27	10.165	1483	1489	1490	rVV	648043	853561	21.46%	1.643%
28	10.195	1490	1494	1505	rVV	2335012	3127268	78.62%	6.020%
29	10.299	1505	1511	1526	rVB	2461192	3379496	84.96%	6.506%
30	10.640	1561	1567	1579	rBV	3094501	3977685	100.00%	7.657%
31	11.079	1634	1639	1655	rBV	774922	964372	24.24%	1.856%
32	11.213	1655	1661	1670	rBV	1569602	2022547	50.85%	3.894%
33	11.451	1695	1700	1715	rVB	1279700	1539365	38.70%	2.963%
34	11.750	1740	1749	1763	rBV	2077715	2485516	62.49%	4.785%
35	11.969	1779	1785	1789	rBV	1017589	1229095	30.90%	2.366%
36	12.036	1789	1796	1802	rVB2	1065507	2355636	59.22%	4.535%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034807.D
Acq On : 28 Mar 2023 20:42
Operator : JC/MD
Sample : 01950-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260

37	12.335	1839	1845	1858	rBV	2480791	3052986	76.75%	5.877%
38	12.945	1939	1945	1953	rBV	115058	152330	3.83%	0.293%
39	13.585	2045	2050	2064	rBV	1197176	1497057	37.64%	2.882%




Sum of corrected areas: 51945740

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034807.D
Acq On : 28 Mar 2023 20:42
Operator : JC/MD
Sample : 01950-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

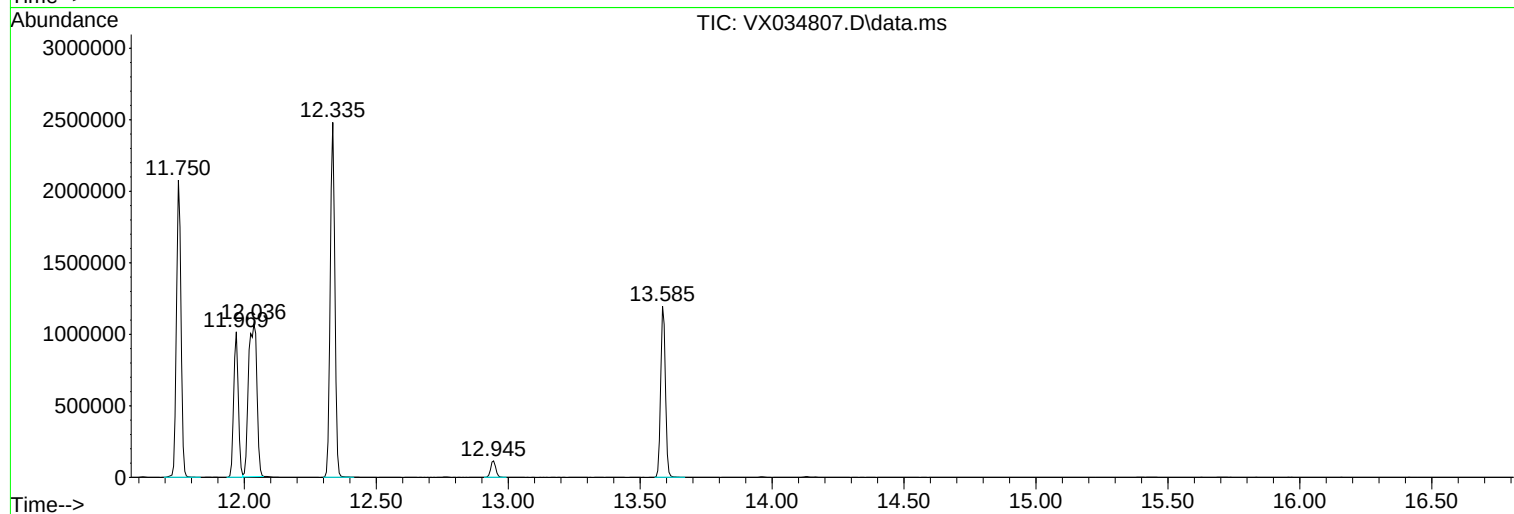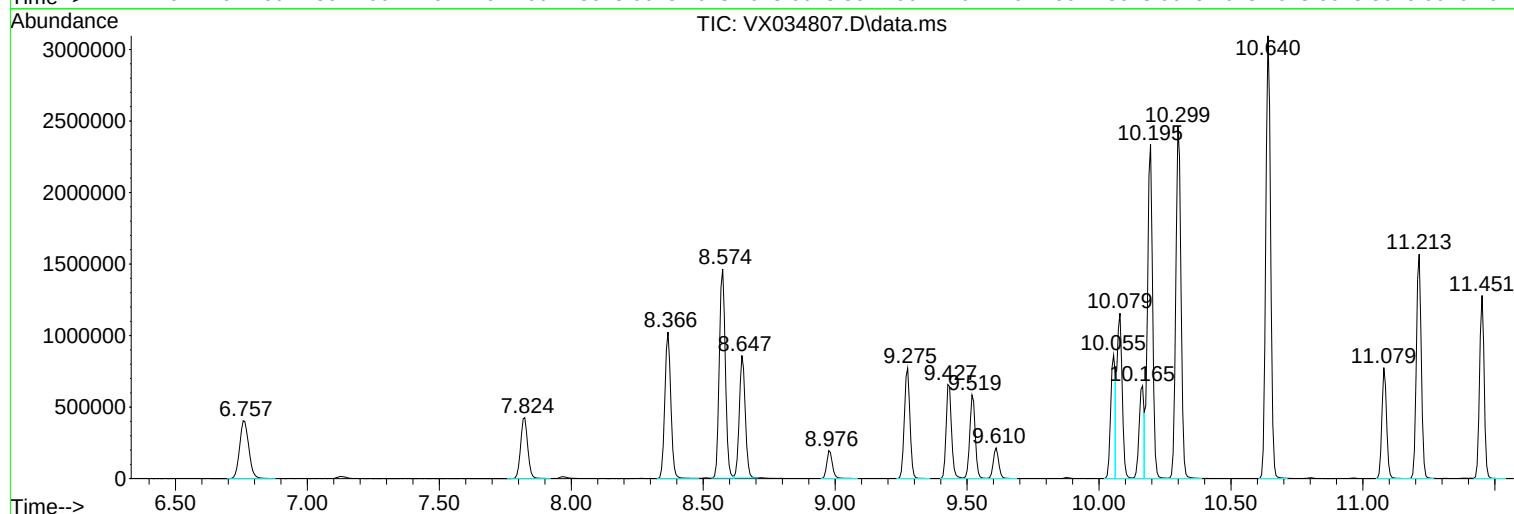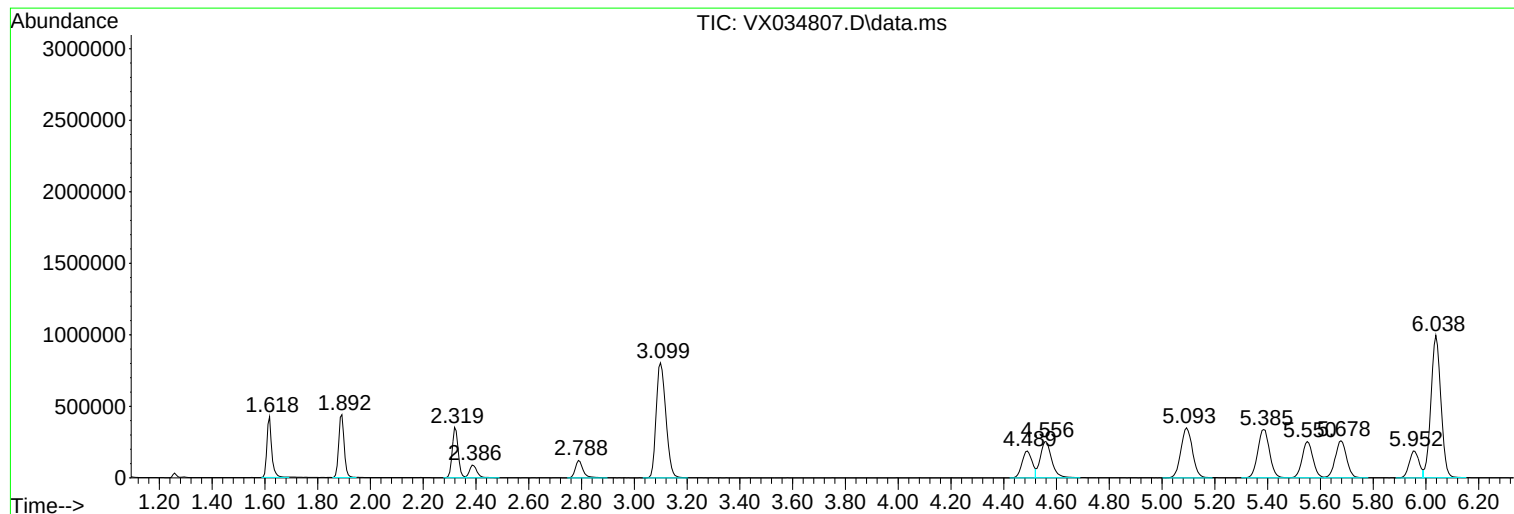

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034807.D
Acq On : 28 Mar 2023 20:42
Operator : JC/MD
Sample : 01950-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034807.D
Acq On : 28 Mar 2023 20:42
Operator : JC/MD
Sample : 01950-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------