
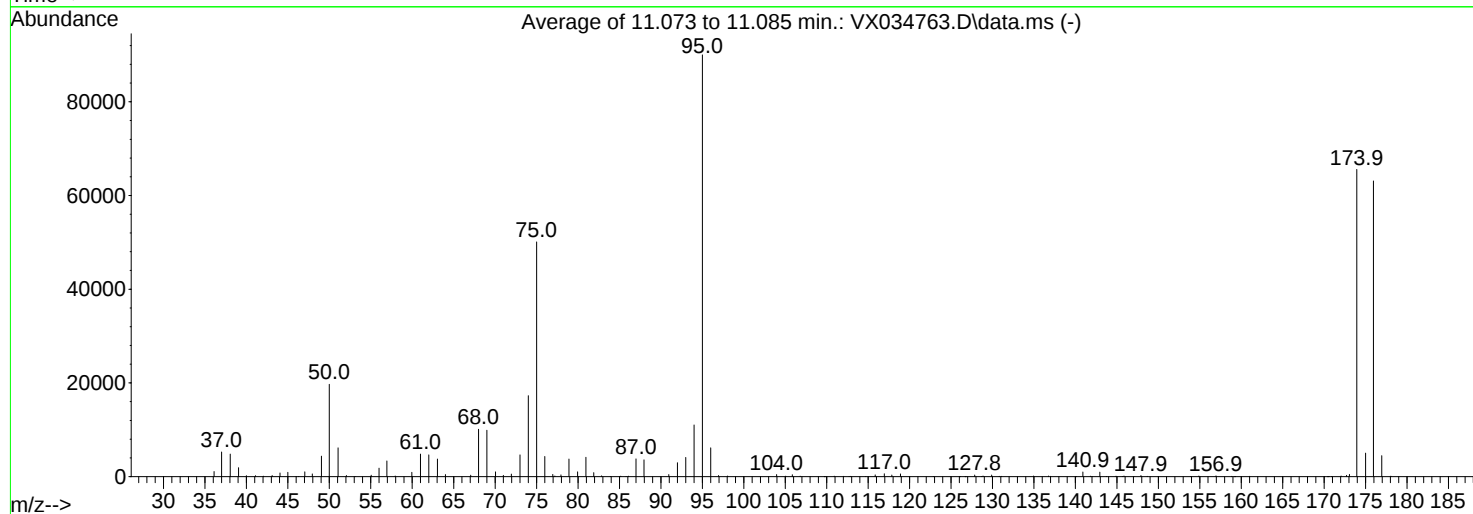


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032823\
Data File : VX034763.D
Acq On : 27 Mar 2023 21:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Title : SW846 8260
Last Update : Mon Mar 13 10:29:32 2023

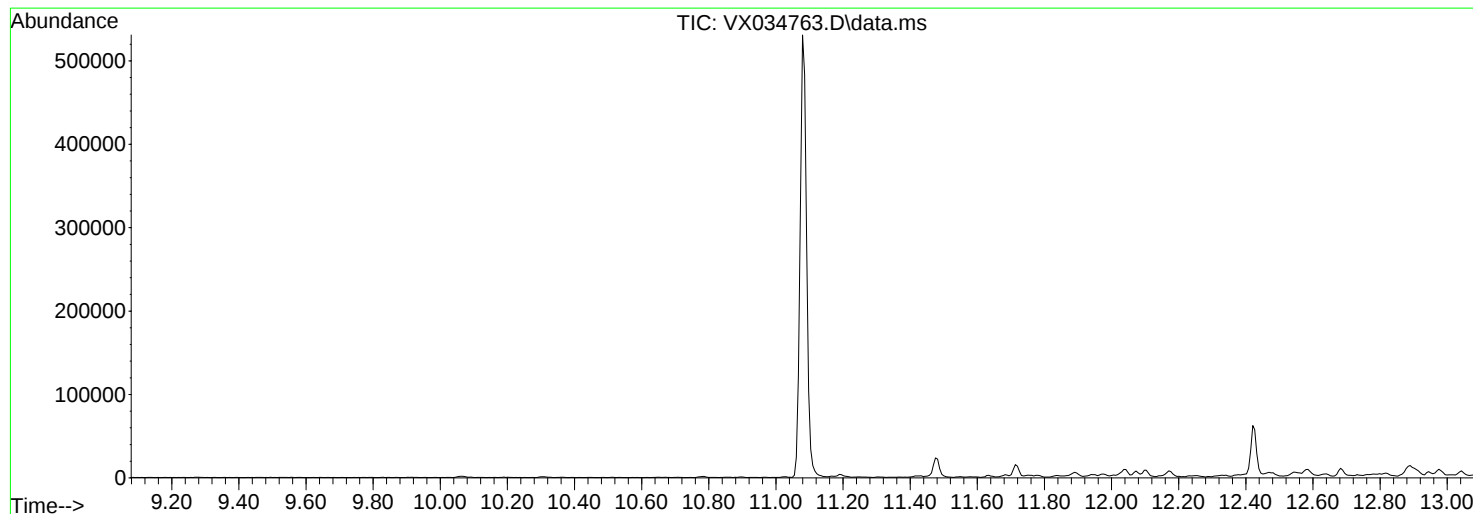

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	19705	PASS
75	95	30	60	55.7	50101	PASS
95	95	100	100	100.0	90021	PASS
96	95	5	9	6.8	6151	PASS
173	174	0.00	2	0.7	467	PASS
174	95	50	100	72.8	65552	PASS
175	174	5	9	7.6	5012	PASS
176	174	95	101	96.3	63112	PASS
177	176	5	9	7.1	4463	PASS