
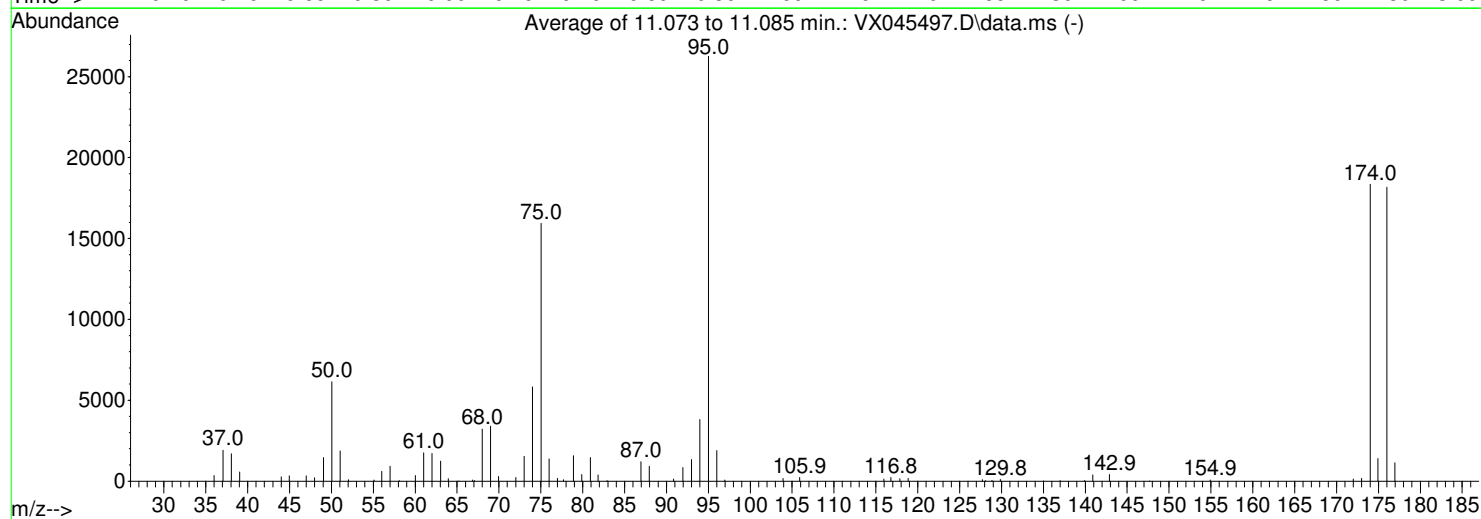


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032825\
Data File : VX045497.D
Acq On : 28 Mar 2025 08:25
Operator : JC/MD
Sample : BFB717
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB717

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM032825WMA.M
Title : VOC Analysis
Last Update : Fri Mar 28 14:43:26 2025

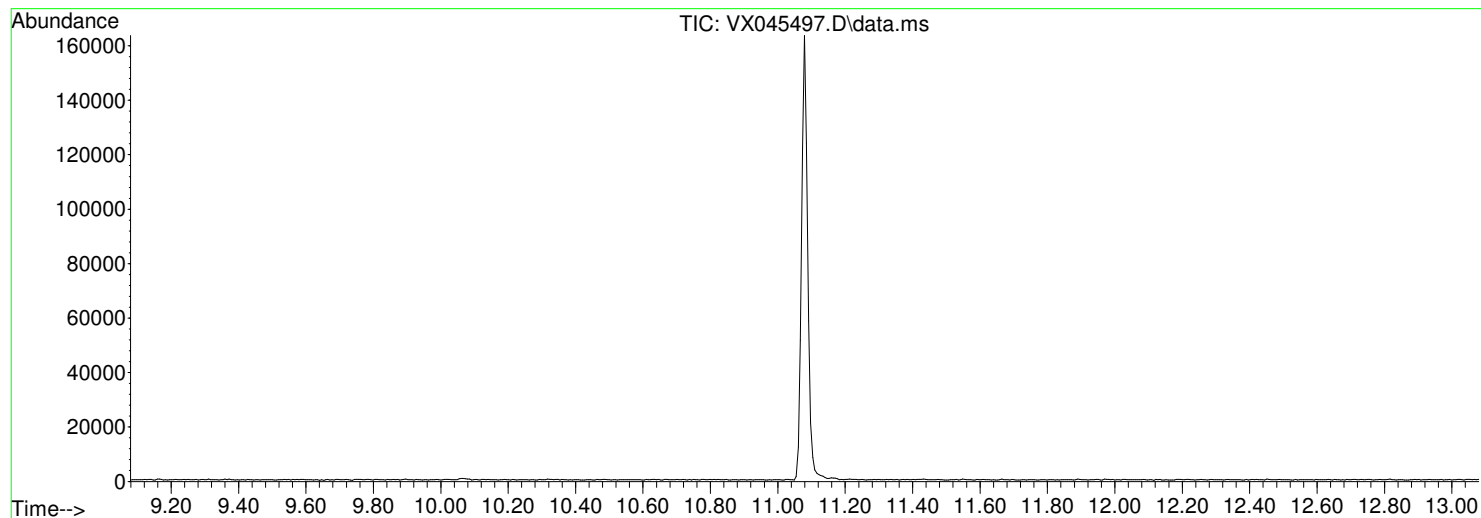

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	6143	PASS
75	95	30	80	60.7	15938	PASS
95	95	100	100	100.0	26261	PASS
96	95	5	9	7.2	1880	PASS
173	174	0.00	2	0.9	174	PASS
174	95	50	120	69.8	18342	PASS
175	174	5	9	7.7	1405	PASS
176	174	95	101	99.1	18173	PASS
177	176	5	9	6.3	1144	PASS

Scan 1633 (11.043 min): VX045497.D\data.ms
BFB717

m/z	Abundance
39.10	96.0
39.90	413.0
44.00	155.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717

m/z	Abundance
36.00	412.0
37.00	1901.0
38.10	1564.0
39.10	660.0
40.00	443.0
44.00	433.0
45.00	288.0
47.10	392.0
48.00	228.0
49.00	1435.0
50.10	5925.0
51.00	1705.0
52.10	105.0
55.10	111.0
56.10	648.0
57.00	893.0
58.10	54.0
60.00	339.0
61.00	1707.0
62.00	1567.0
63.10	1370.0
64.00	172.0
65.20	57.0
67.10	82.0
68.00	3162.0
69.00	3410.0
70.00	260.0
72.10	172.0
73.00	1728.0
74.00	5772.0
75.00	14989.0
76.00	1482.0
77.00	169.0
77.70	99.0
78.90	1412.0
79.90	287.0
80.90	1285.0
81.80	352.0
87.00	1046.0
88.00	856.0
90.80	121.0
91.90	800.0
93.00	1158.0
94.00	3519.0
95.00	24400.0
96.00	1808.0
96.90	93.0
104.00	189.0
105.90	158.0
116.00	110.0
116.90	165.0
117.80	120.0
118.80	144.0
129.90	113.0
140.90	267.0
142.90	411.0
154.90	61.0
172.00	121.0
173.10	130.0
174.00	14002.0
174.90	1019.0
176.00	13566.0
176.90	968.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717

m/z	Abundance
36.00	396.0
37.00	2356.0
38.00	2131.0
39.10	658.0
40.00	369.0
44.00	474.0
45.00	380.0
46.90	400.0
48.00	296.0
49.10	1834.0
50.00	7545.0
51.00	2245.0
52.00	133.0
55.10	124.0
56.00	637.0
57.00	999.0
58.10	50.0
60.10	363.0
61.00	1907.0
62.00	2210.0
63.00	1327.0
64.00	152.0
66.80	112.0
68.00	3626.0
69.00	4202.0
70.00	401.0
72.00	261.0
73.00	1726.0
74.00	6889.0
75.00	18792.0
76.00	1497.0
77.00	224.0
77.60	91.0
78.90	1825.0
79.90	601.0
80.90	1767.0
81.90	550.0
82.90	76.0
86.90	1457.0
87.90	1197.0
90.90	146.0
92.00	969.0
93.00	1675.0
94.00	4756.0
95.00	30936.0
96.00	2339.0
97.00	58.0
103.90	184.0
105.90	270.0
115.90	195.0
116.70	279.0
117.90	188.0
118.90	167.0
127.70	103.0
128.10	80.0
128.90	76.0
129.90	124.0
135.00	52.0
139.90	92.0
140.80	488.0
142.90	430.0
147.70	56.0
154.90	53.0
172.00	186.0
173.00	239.0
174.00	22408.0
175.00	1705.0
176.00	21856.0
176.90	1425.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717

m/z	Abundance
36.00	250.0
37.10	1453.0
38.00	1389.0
39.00	657.0
40.00	369.0
44.00	375.0
44.90	294.0
47.00	200.0
47.90	116.0
49.10	1112.0
50.00	4960.0
51.10	1658.0
52.00	55.0
55.90	536.0
57.00	848.0
59.90	353.0
61.00	1648.0
62.00	1377.0
63.10	988.0
63.90	119.0
66.90	119.0
68.00	2842.0
69.00	2589.0
69.90	230.0
71.90	233.0
73.00	1144.0
74.00	4812.0
75.10	14034.0
76.00	1155.0
77.00	123.0
77.80	97.0
78.90	1454.0
79.90	350.0
80.90	1331.0
81.80	242.0
87.00	1084.0
87.90	681.0
90.80	107.0
92.00	738.0
93.00	1196.0
94.00	3144.0
95.00	23448.0
96.00	1494.0
97.00	73.0
103.80	157.0
105.90	229.0
116.00	100.0
116.90	233.0
117.80	130.0
118.80	200.0
127.70	170.0
128.80	52.0
129.70	71.0
137.00	63.0
141.00	434.0
142.90	349.0
154.90	72.0
172.00	107.0
172.90	152.0
174.00	18616.0
174.90	1492.0
176.00	19096.0
177.00	1039.0

Instrument :
MSVOA_X
ClientSampleId :
BFB717