


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX032919\  
 Data File : VX008534.D  
 Acq On : 29 Mar 2019 08:57  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X032519W.M  
 Title : SW846 8260  
 Last Update : Tue Mar 26 07:57:20 2019

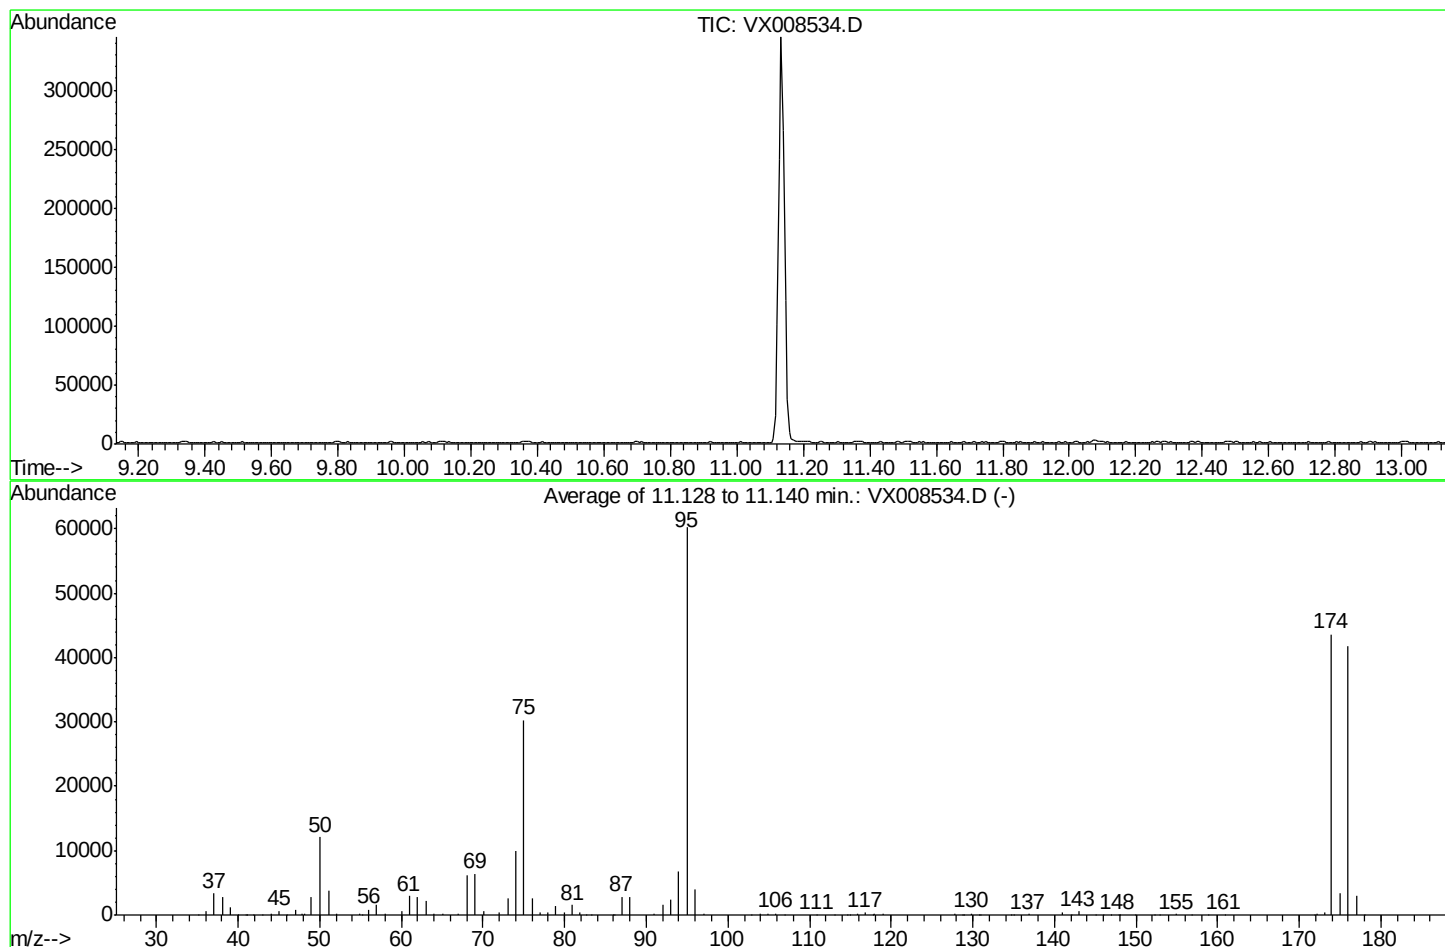

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.0      | 12072   | PASS             |
| 75          | 95           | 30           | 60           | 50.2      | 30261   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 60226   | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 4011    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 451     | PASS             |
| 174         | 95           | 50           | 100          | 72.4      | 43624   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 3474    | PASS             |
| 176         | 174          | 95           | 101          | 95.8      | 41802   | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 2914    | PASS             |