

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021571.D
 Acq On : 29 Mar 2021 12:55
 Operator : JC/MD
 Sample : M1785-10 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1

Quant Time: Mar 30 03:26:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 24 12:25:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	58534	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	105367	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	106458	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	48214	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.035	65	49320	50.64	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 101.28%			
35) Dibromofluoromethane	5.458	113	37501	50.10	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 100.20%			
50) Toluene-d8	8.694	98	133624	50.10	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 100.20%			
62) 4-Bromofluorobenzene	11.118	95	54349	52.41	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 104.82%			
Target Compounds						Qvalue
3) Chloromethane	1.317	50	1417	1.96	ug/l #	81
5) Bromomethane	1.634	94	69	0.26	ug/l #	2
10) Methyl Iodide	2.499	142	49	6.73	ug/l #	42
13) Acrolein	2.170	56	28	4.64	ug/l #	1
16) Acetone	2.423	43	418	1.14	ug/l #	76
18) Methyl Acetate	2.746	43	241	0.23	ug/l #	47
20) Methylene Chloride	2.829	84	277	0.39	ug/l #	75
29) Tetrahydrofuran	5.099	42	120	0.33	ug/l #	27
36) 1,1-Dichloropropene	5.623	75	5205	5.04	ug/l #	49
38) Carbon Tetrachloride	5.623	117	6423	5.79	ug/l #	15
44) Trichloroethene	7.188	130	993	1.28	ug/l	87
55) 1,1,2-Trichloroethane	9.141	97	319	0.42	ug/l #	15
56) Ethyl methacrylate	9.135	69	120	2.17	ug/l #	1
67) Ethyl Benzene	10.235	91	5238	1.34	ug/l	91
68) m/p-Xylenes	10.341	106	2963	2.13	ug/l	92
69) o-Xylene	10.683	106	301	0.22	ug/l	92
71) Bromoform	11.112	173	154	0.23	ug/l #	29
73) Isopropylbenzene	11.000	105	102371	30.22	ug/l	99
74) N-amyl acetate	10.894	43	1080	0.66	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.259	83	919	0.77	ug/l #	33
76) 1,2,3-Trichloropropane	11.341	75	1484	1.32	ug/l #	1
78) n-propylbenzene	11.341	91	200026	50.00	ug/l	97
79) 2-Chlorotoluene	11.341	91	200026	82.42	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.436	105	9454	3.27	ug/l	77
81) trans-1,4-Dichloro-2-b...	11.000	75	1482	4.02	ug/l #	61
82) 4-Chlorotoluene	11.341	91	200026	69.42	ug/l #	45
83) tert-Butylbenzene	11.753	119	10295	3.65	ug/l	81
84) 1,2,4-Trimethylbenzene	11.789	105	235955	80.88	ug/l	98
85) sec-Butylbenzene	11.930	105	43181	13.29	ug/l	98
86) p-Isopropyltoluene	12.218	119	17888	6.05	ug/l	90
89) n-Butylbenzene	12.371	91	16860	6.22	ug/l #	81
90) Hexachloroethane	12.653	117	6780	12.70	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	13.001	75	105	2.30	ug/l #	1
95) Naphthalene	13.812	128	10784	3.43	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021571.D
Acq On : 29 Mar 2021 12:55
Operator : JC/MD
Sample : M1785-10 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Time: Mar 30 03:26:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021571.D
Acq On : 29 Mar 2021 12:55
Operator : JC/MD
Sample : M1785-10 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Time: Mar 30 03:26:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration




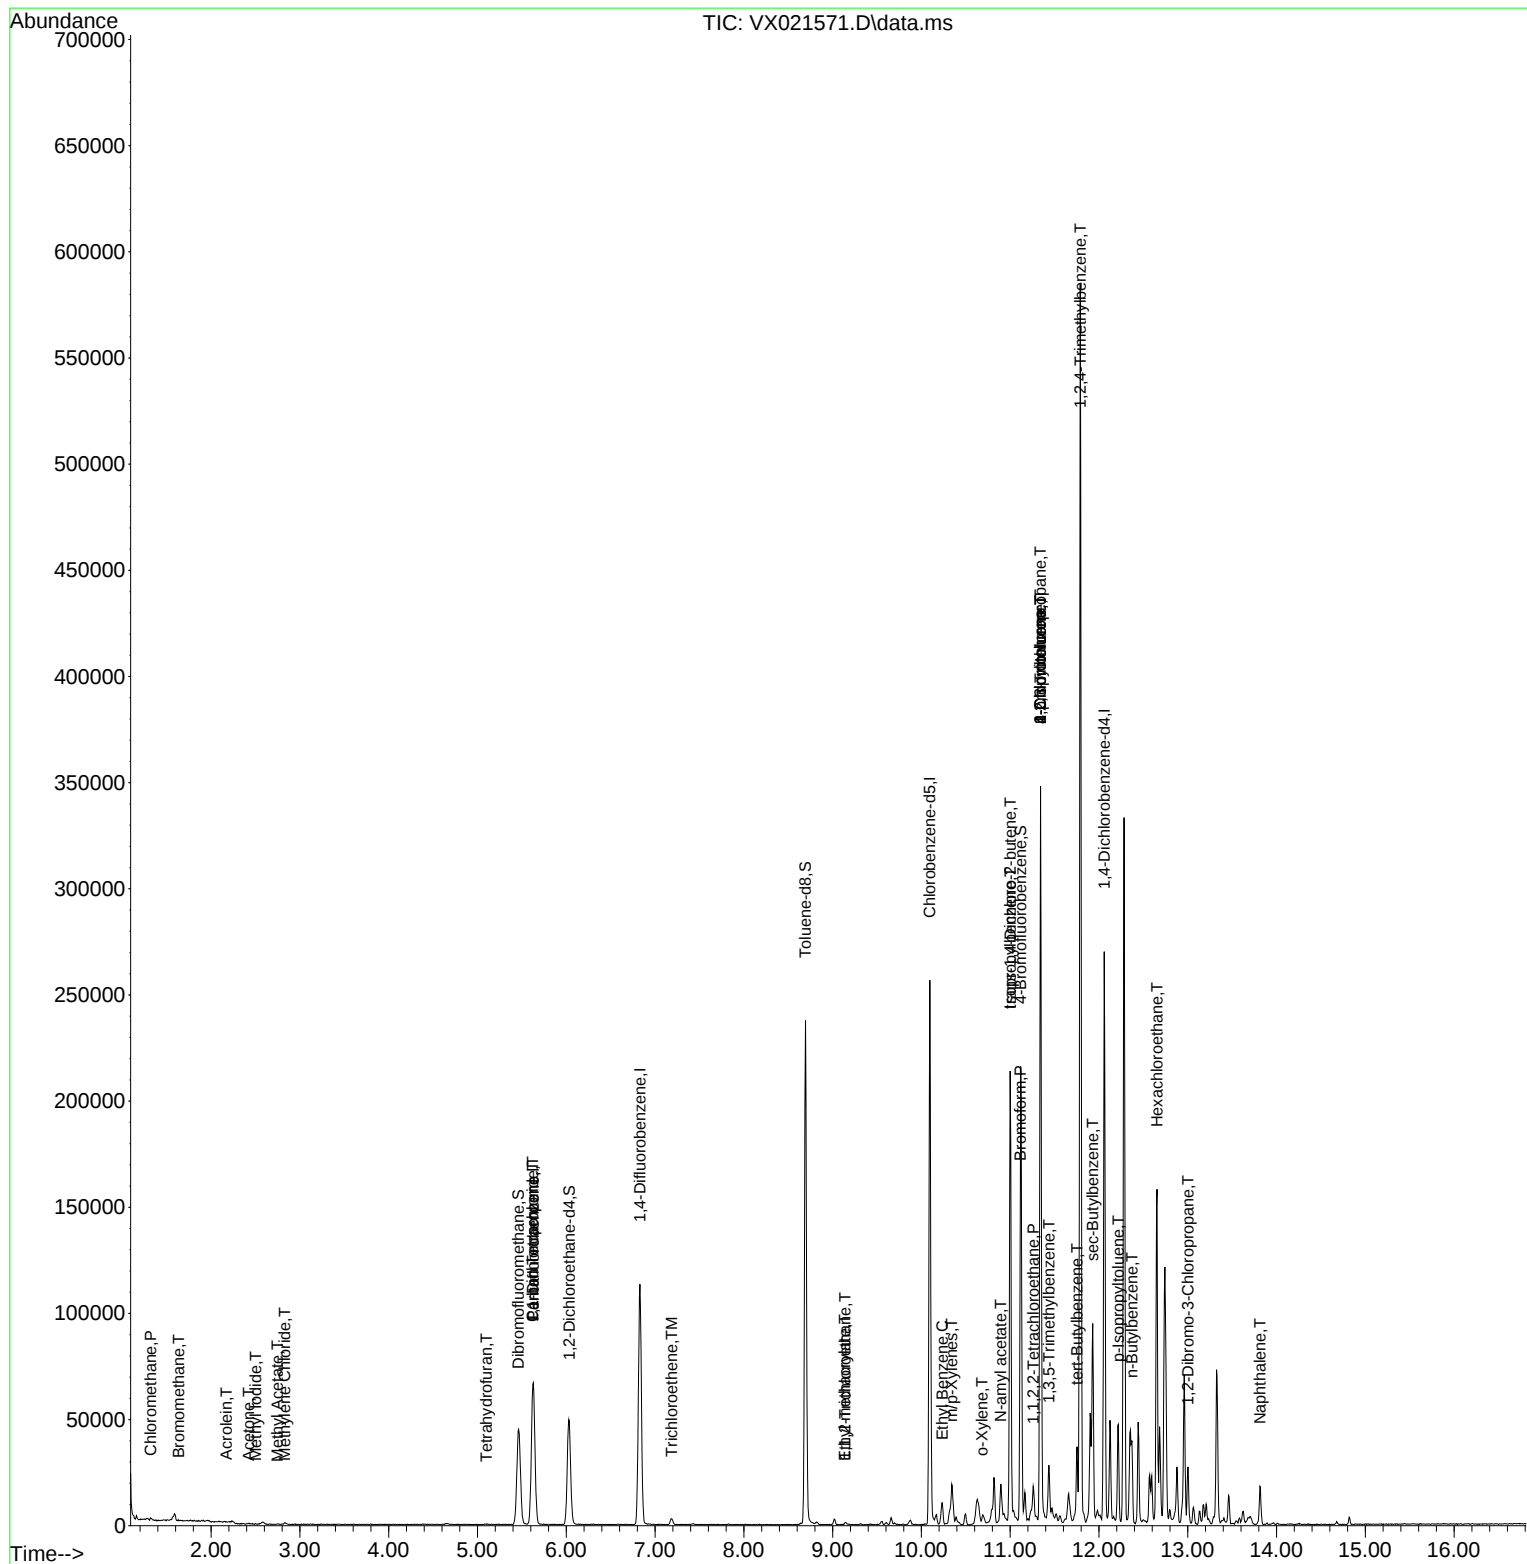




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion:168 Resp: 58534
Ion Ratio Lower Upper
168 100
99 64.7 45.8 68.6

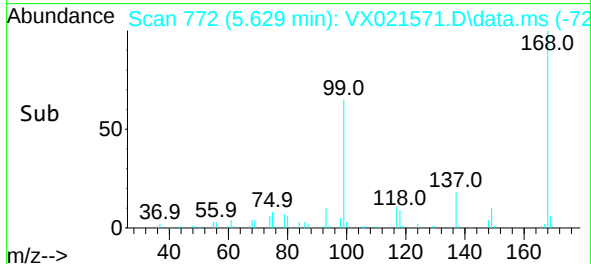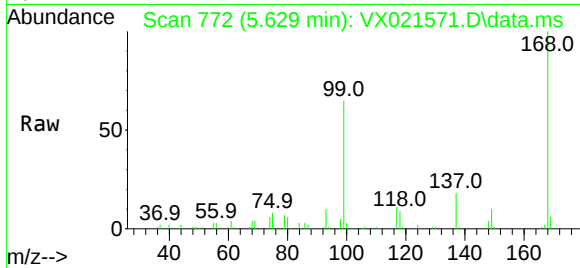

#3
Chloromethane
Concen: 1.96 ug/l
RT: 1.317 min Scan# 39
Delta R.T. 0.006 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 50 Resp: 1417
Ion Ratio Lower Upper
50 100
52 43.5 26.4 39.6#


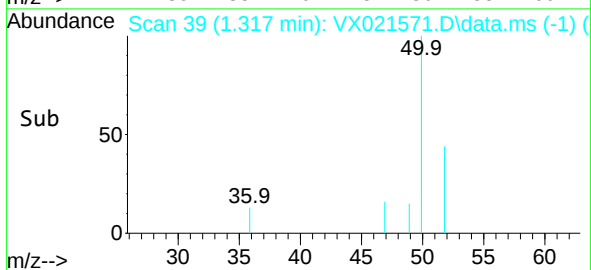

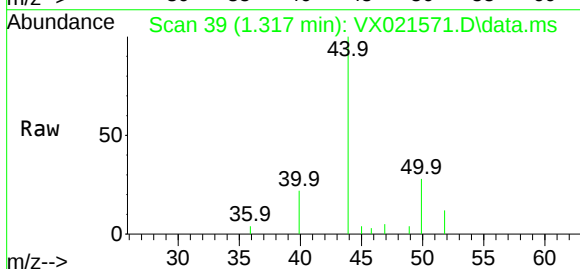


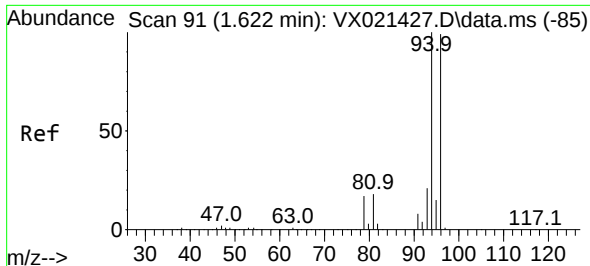

#5
Bromomethane
Concen: 0.26 ug/l
RT: 1.634 min Scan# 93
Delta R.T. 0.012 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 94 Resp: 69
Ion Ratio Lower Upper
94 100
96 0.0 76.4 114.6#

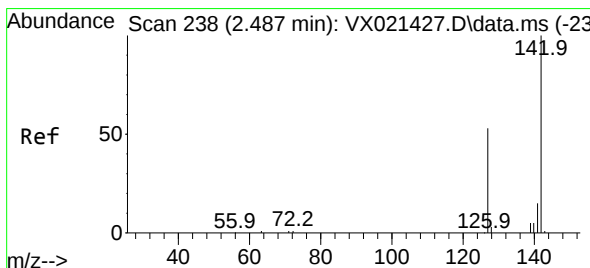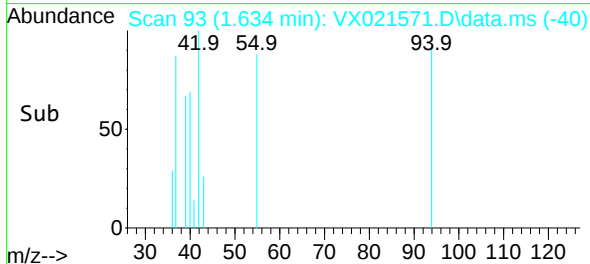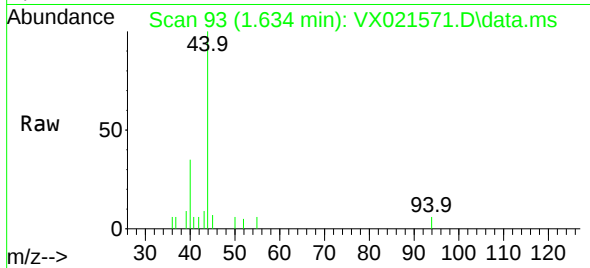

#10
Methyl Iodide
Concen: 6.73 ug/l
RT: 2.499 min Scan# 240
Delta R.T. 0.012 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion:142 Resp: 49
Ion Ratio Lower Upper
142 100
127 0.0 33.3 49.9#
141 0.0 11.4 17.0#


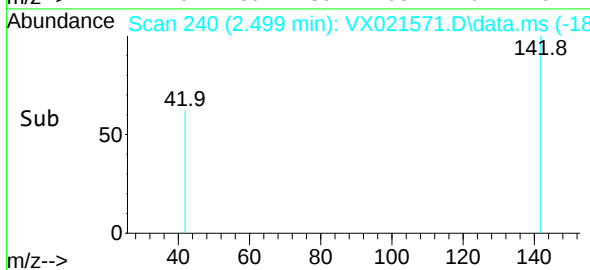

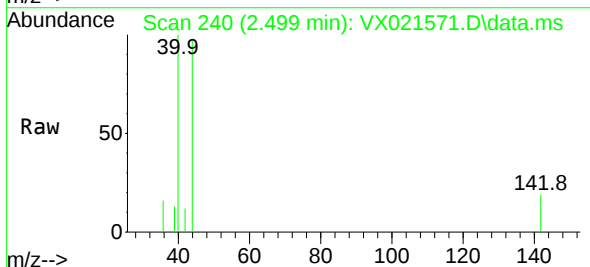


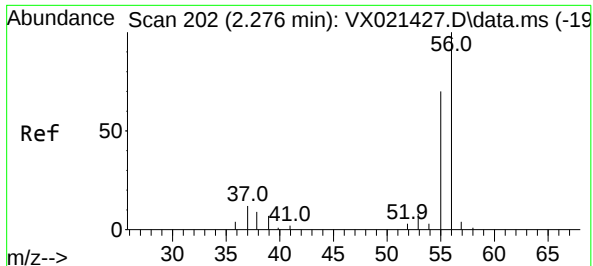

#13
Acrolein
Concen: 4.64 ug/l
RT: 2.170 min Scan# 184
Delta R.T. -0.106 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 56 Resp: 28
Ion Ratio Lower Upper
56 100
55 300.0 56.4 84.6#

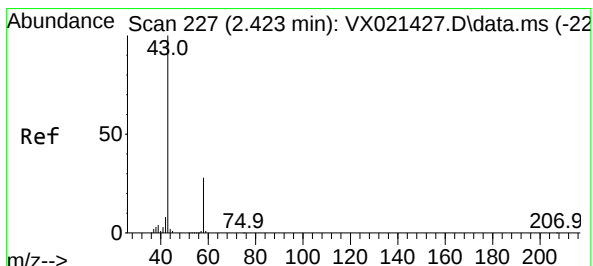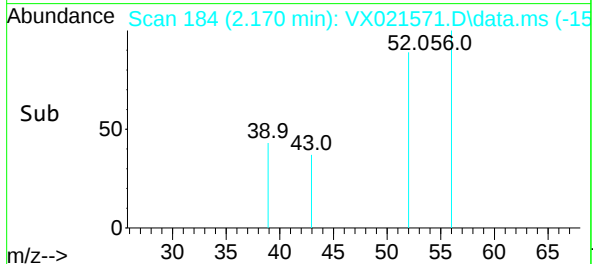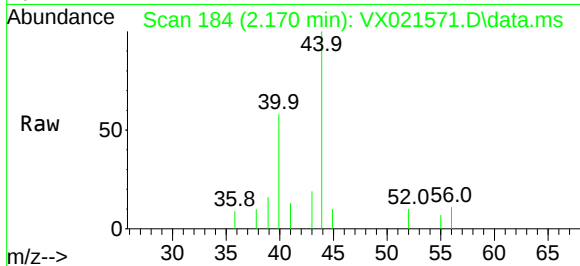

#16
Acetone
Concen: 1.14 ug/l
RT: 2.423 min Scan# 227
Delta R.T. -0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 43 Resp: 418
Ion Ratio Lower Upper
43 100
58 20.9 27.8 41.8#


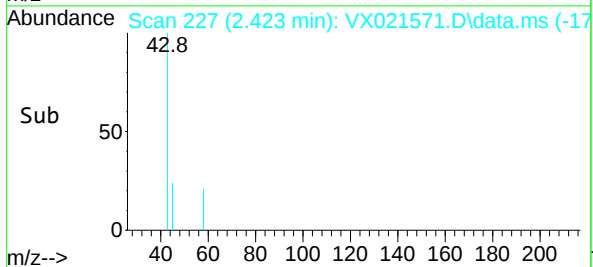

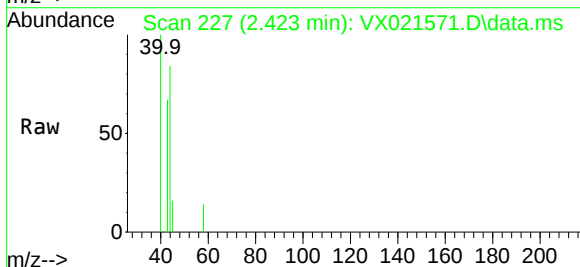


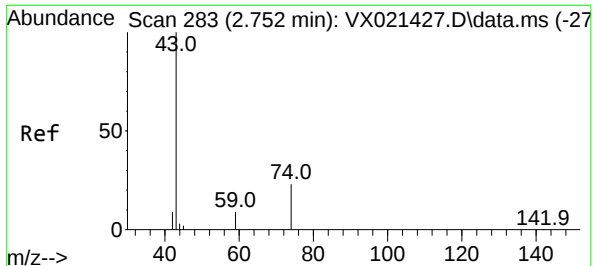

#18
Methyl Acetate
Concen: 0.23 ug/l
RT: 2.746 min Scan# 282
Delta R.T. -0.006 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 43 Resp: 241
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

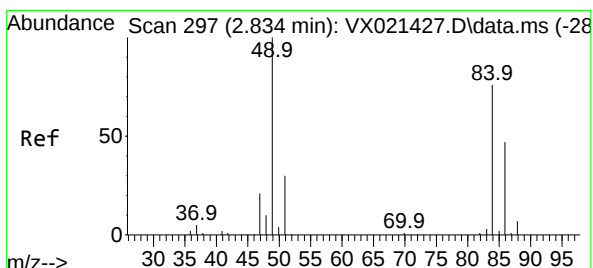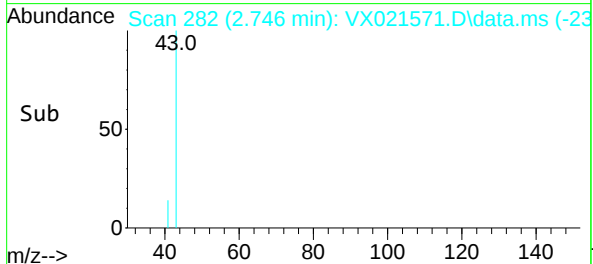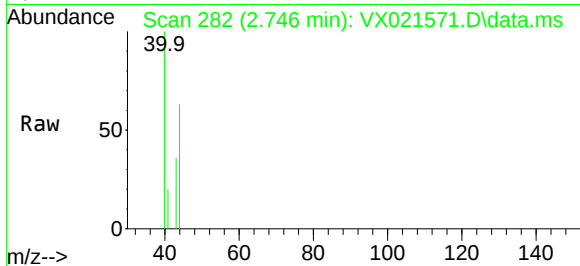

#20
Methylene Chloride
Concen: 0.39 ug/l
RT: 2.829 min Scan# 296
Delta R.T. -0.005 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 84 Resp: 277
Ion Ratio Lower Upper
84 100
49 89.8 88.6 132.8
51 21.3 27.0 40.6#
86 34.3 50.3 75.5#

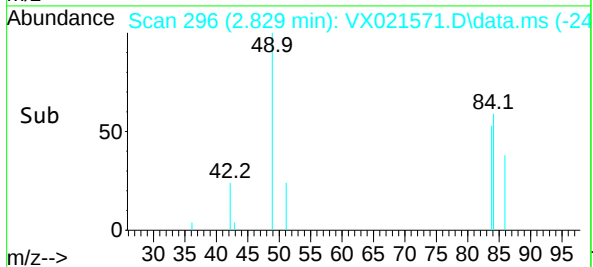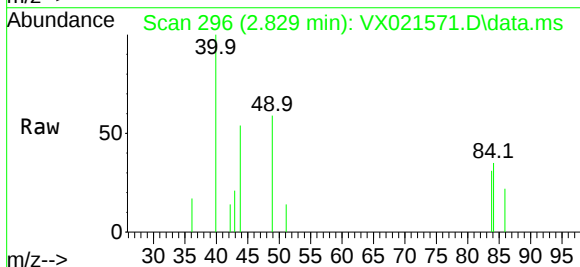



#29

Tetrahydrofuran

Concen: 0.33 ug/l

RT: 5.099 min Scan# 682

Delta R.T. 0.011 min

Lab File: VX021571.D


Acq: 29 Mar 2021 12:55

Instrument :




MSVOA_X

ClientSampleId :

MW-1

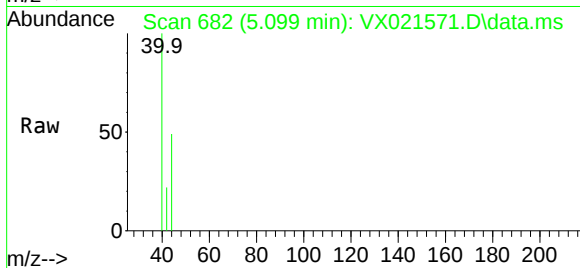

Tgt Ion: 42	Resp: 120
Ion Ratio	Lower Upper
42	100
72	0.0 41.7 62.5#
71	0.0 38.4 57.6#

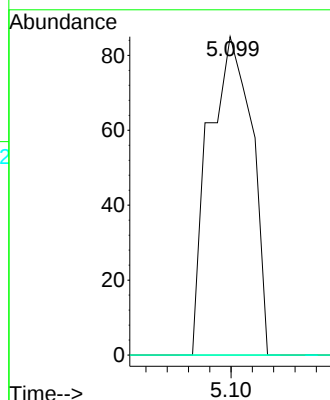

#33

1,2-Dichloroethane-d4

Concen: 50.64 ug/l




RT: 6.035 min Scan# 841


Delta R.T. 0.006 min

Lab File: VX021571.D

Acq: 29 Mar 2021 12:55

Tgt Ion: 65	Resp: 49320
Ion Ratio	Lower Upper
65	100
67	50.4 0.0 105.4

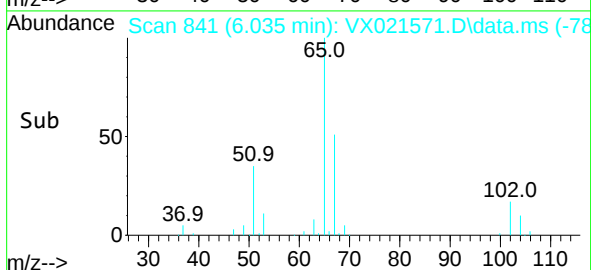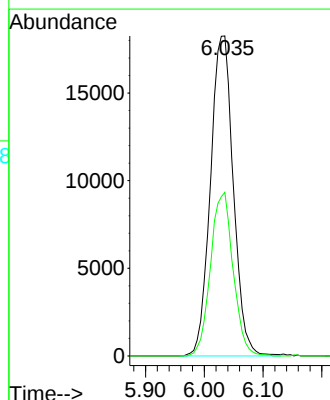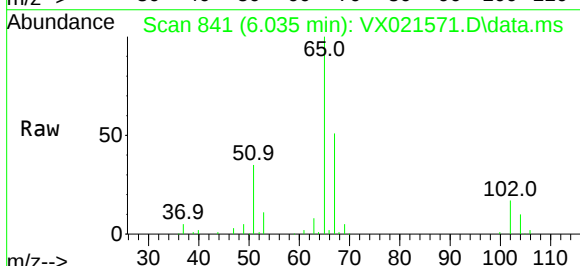

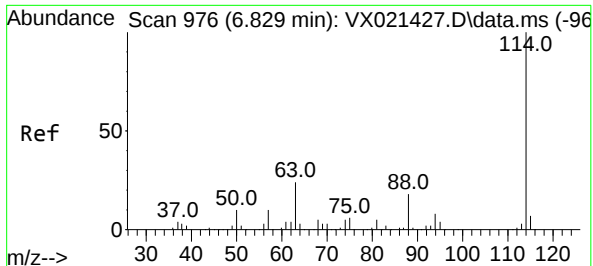

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.829 min Scan# 976

Delta R.T. 0.000 min

Lab File: VX021571.D

Acq: 29 Mar 2021 12:55





Tgt Ion:114 Resp: 105367

Ion Ratio Lower Upper

114 100

63 23.2 0.0 40.8

88 16.3 0.0 32.8

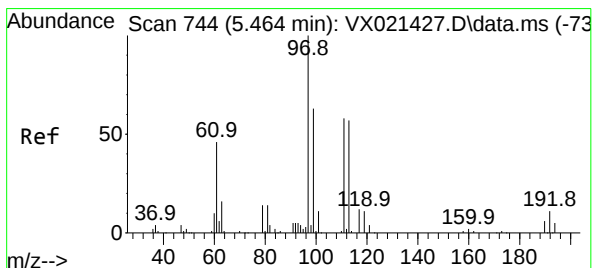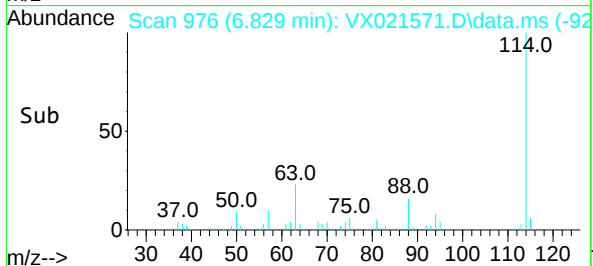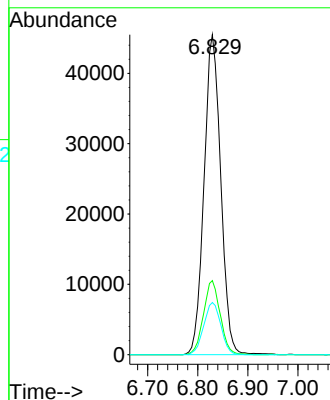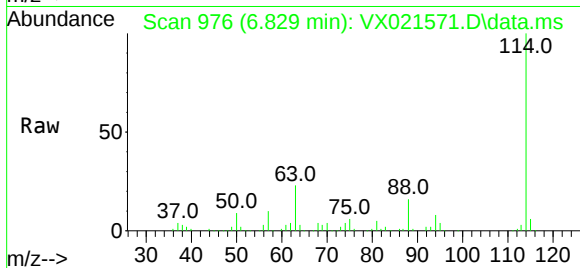

#35

Dibromofluoromethane

Concen: 50.10 ug/l

RT: 5.458 min Scan# 743

Delta R.T. -0.006 min

Lab File: VX021571.D

Acq: 29 Mar 2021 12:55




Tgt Ion:113 Resp: 37501


Ion Ratio Lower Upper

113 100

111 101.9 81.9 122.9

192 18.8 16.7 25.1


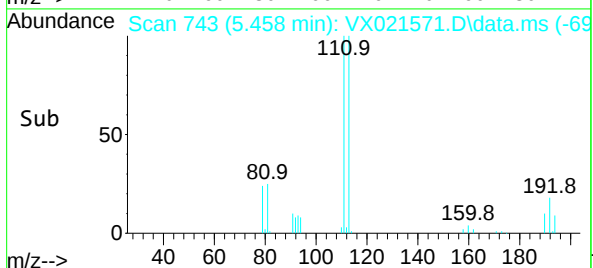
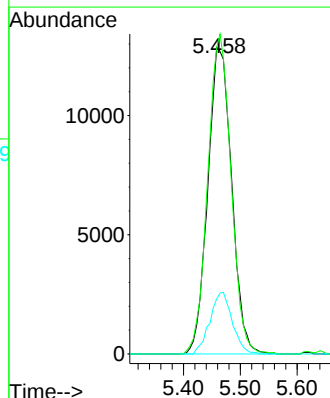
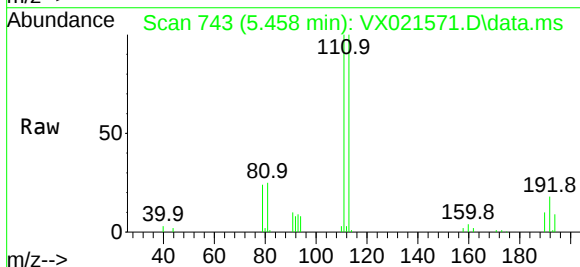


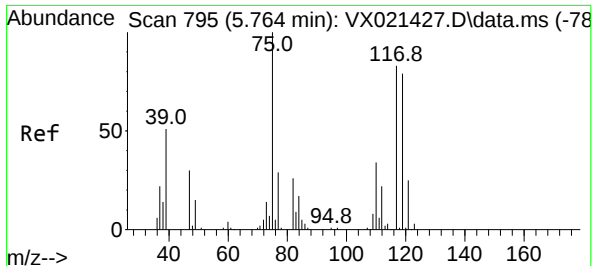

#36
1,1-Dichloropropene
Concen: 5.04 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.141 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 75 Resp: 5205
Ion Ratio Lower Upper
75 100
110 9.5 18.1 54.4#
77 0.0 25.3 37.9#

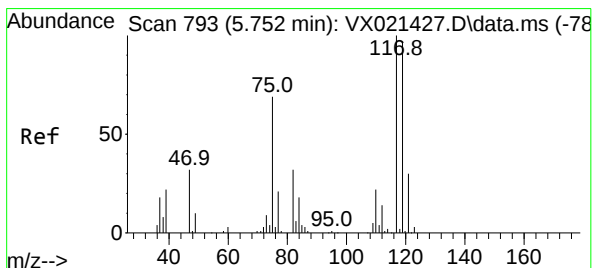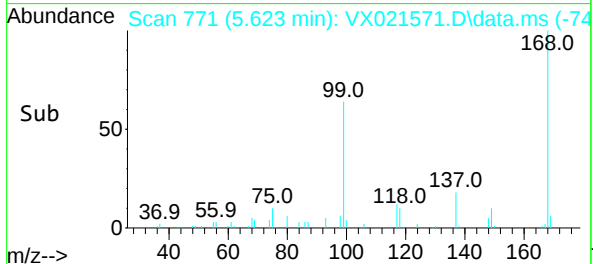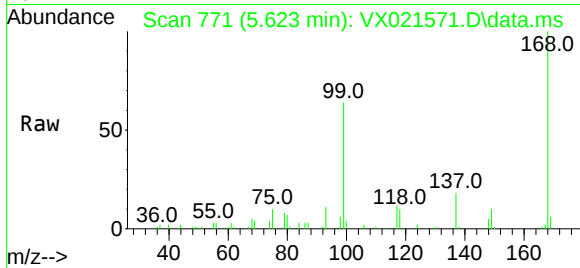

#38
Carbon Tetrachloride
Concen: 5.79 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.129 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 117 Resp: 6423
Ion Ratio Lower Upper
117 100
119 3.9 76.2 114.2#
121 0.0 24.8 37.2#

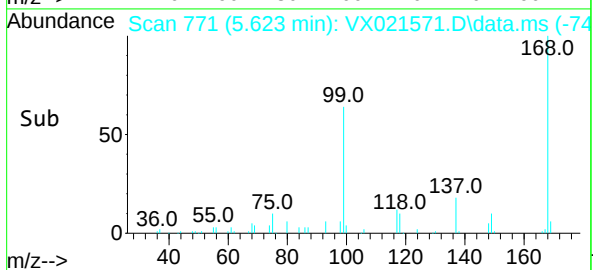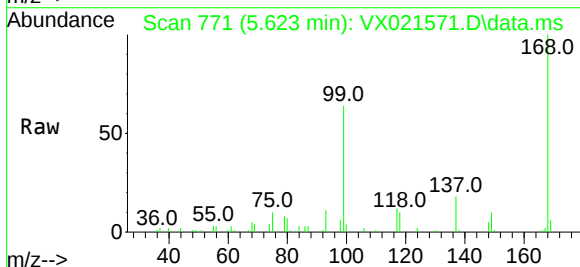

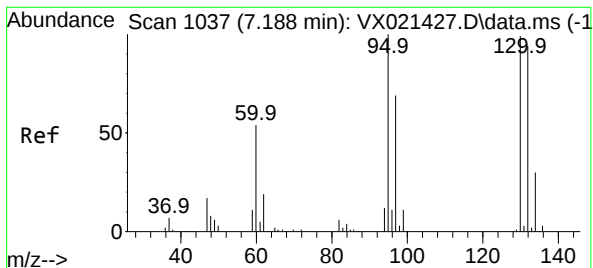

#44

Trichloroethene

Concen: 1.28 ug/l

RT: 7.188 min Scan# 1037

Delta R.T. 0.000 min





Lab File: VX021571.D

Acq: 29 Mar 2021 12:55

Tgt Ion:130 Resp: 993

Ion Ratio Lower Upper

130	100		
95	112.3	0.0	198.0

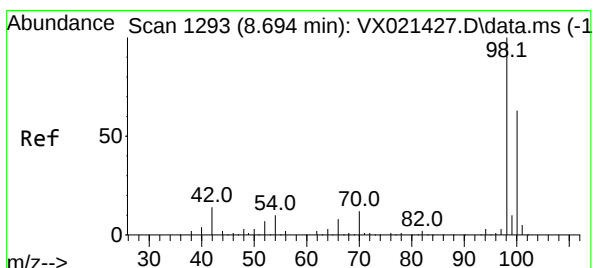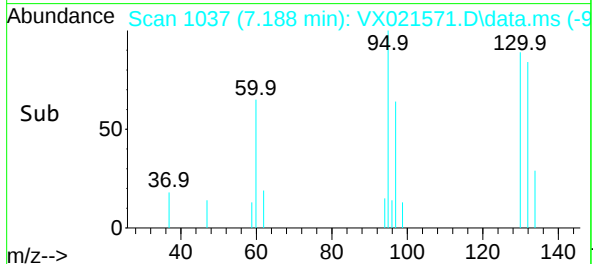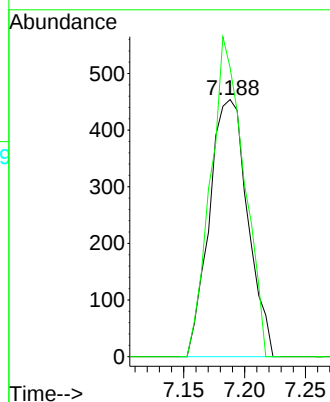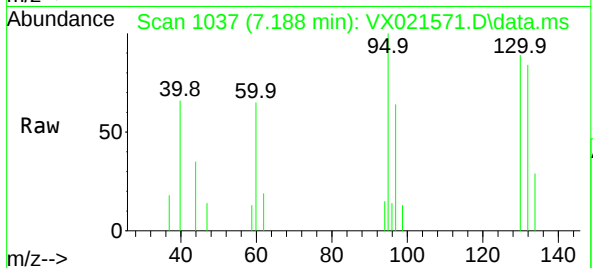

#50

Toluene-d8

Concen: 50.10 ug/l

RT: 8.694 min Scan# 1293

Delta R.T. 0.000 min




Lab File: VX021571.D


Acq: 29 Mar 2021 12:55

Tgt Ion: 98 Resp: 133624

Ion Ratio Lower Upper


98	100		
100	63.4	51.9	77.9

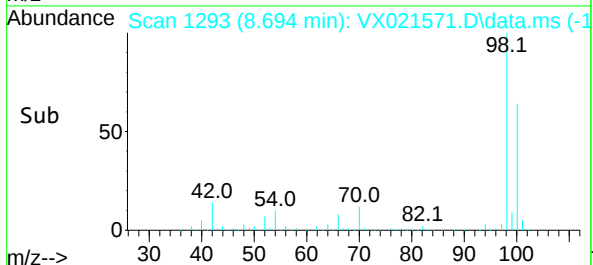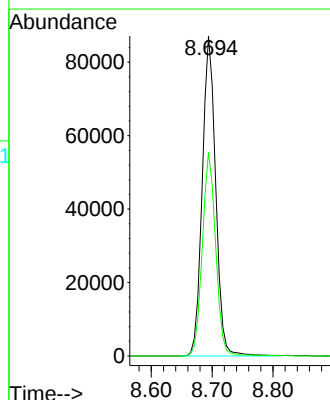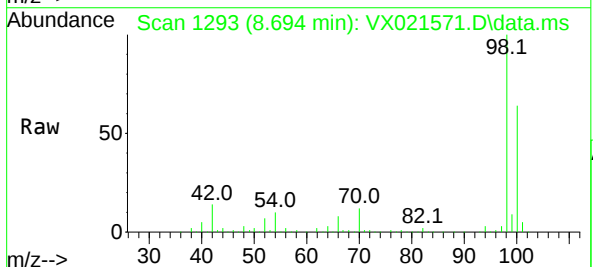






#55
1,1,2-Trichloroethane
Concen: 0.42 ug/l
RT: 9.141 min Scan# 1369
Delta R.T. -0.053 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Instrument :
MSVOA_X
ClientSampled :
MW-1







Tgt Ion:	97	Resp:	319
Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.3	103.9#
85	0.0	44.3	66.5#
99	0.0	50.3	75.5#

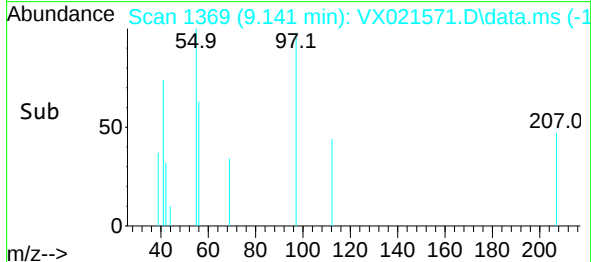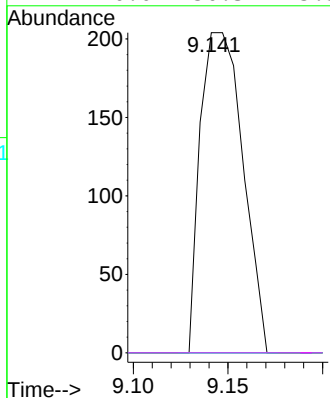

#56
Ethyl methacrylate
Concen: 2.17 ug/l
RT: 9.135 min Scan# 1368
Delta R.T. -0.024 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion:	69	Resp:	120
Ion	Ratio	Lower	Upper
69	100		
41	149.2	46.8	70.2#
39	147.5	24.7	37.1#


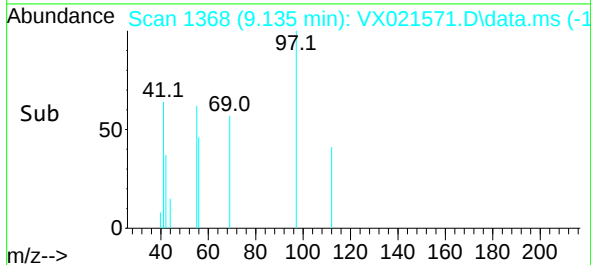
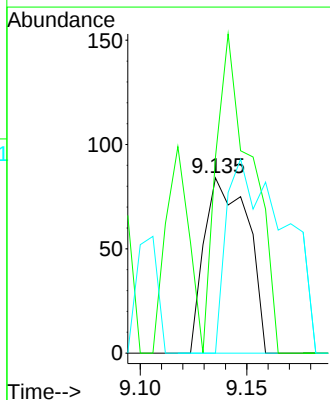
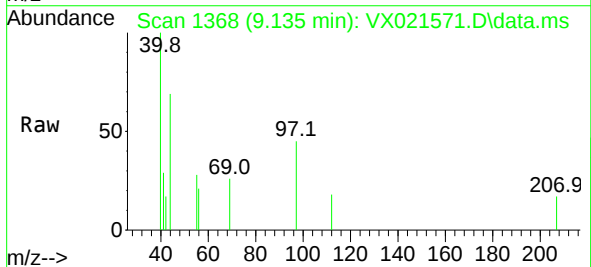




#62
4-Bromofluorobenzene
Concen: 52.41 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 95 Resp: 54349
Ion Ratio Lower Upper
95 100
174 77.1 0.0 154.6
176 74.5 0.0 155.8

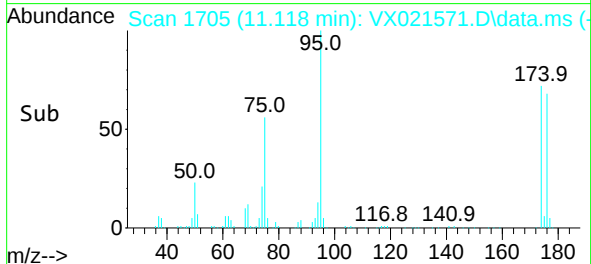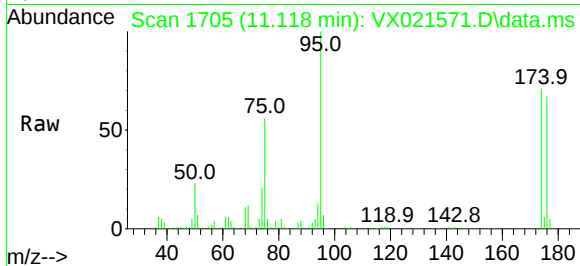

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 117 Resp: 106458
Ion Ratio Lower Upper
117 100
82 60.4 47.4 71.2
119 31.6 26.6 39.8


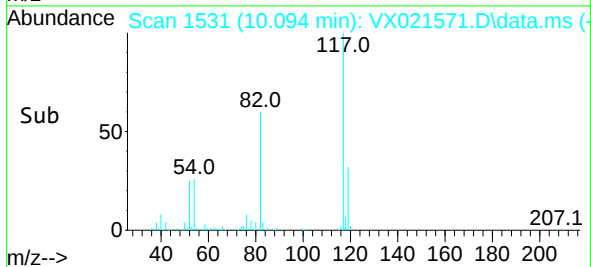

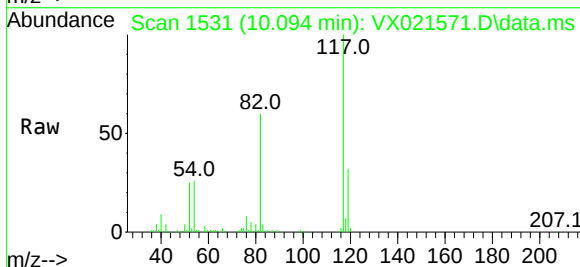




#67
Ethyl Benzene
Concen: 1.34 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 91 Resp: 5238
Ion Ratio Lower Upper
91 100
106 26.1 24.6 37.0

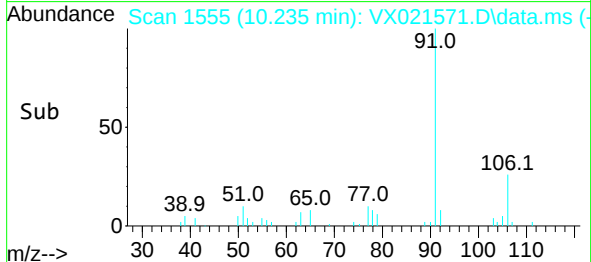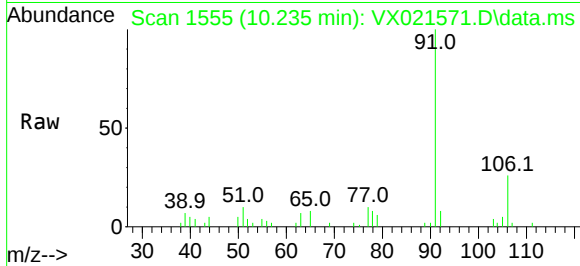

#68
m/p-Xylenes
Concen: 2.13 ug/l
RT: 10.341 min Scan# 1573
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 106 Resp: 2963
Ion Ratio Lower Upper
106 100
91 215.0 162.8 244.2


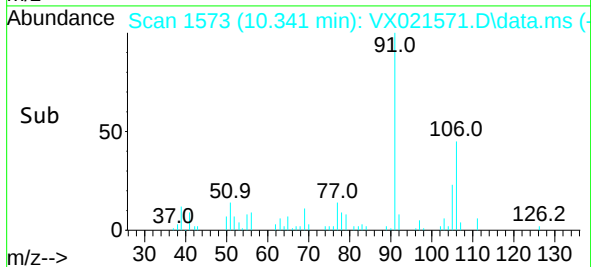

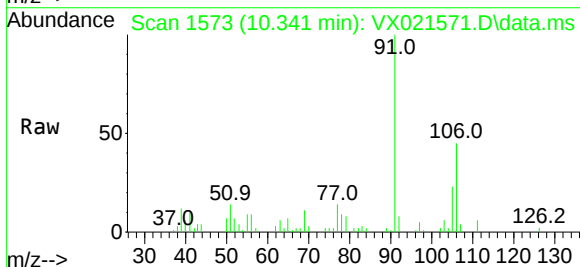


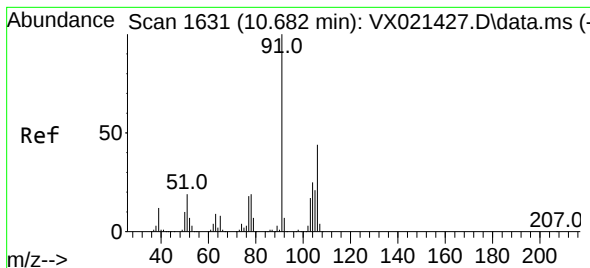

#69
o-Xylene
Concen: 0.22 ug/l
RT: 10.683 min Scan# 1631
Delta R.T. 0.001 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion:106 Resp: 301
Ion Ratio Lower Upper
106 100
91 203.0 108.1 324.2

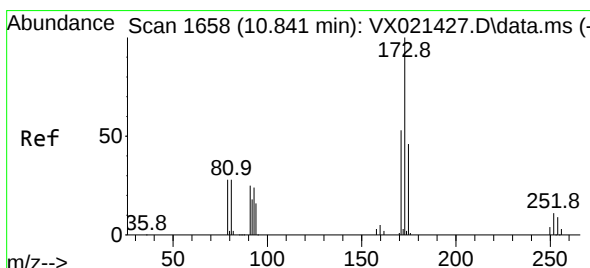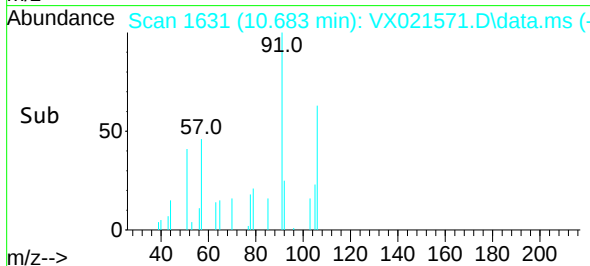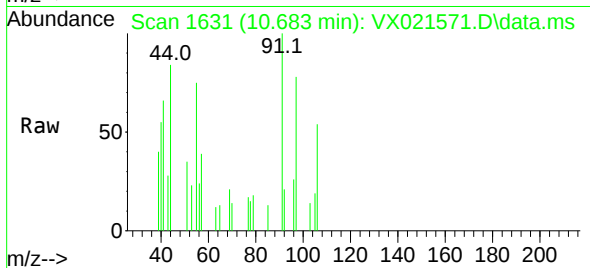

#71
Bromoform
Concen: 0.23 ug/l
RT: 11.112 min Scan# 1704
Delta R.T. 0.271 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion:173 Resp: 154
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.1 0.1#


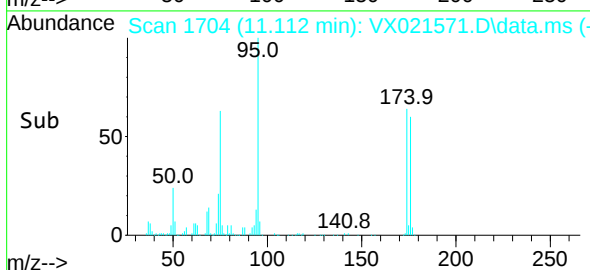

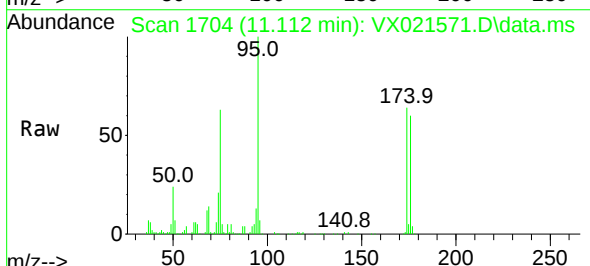




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion:152 Resp: 48214
Ion Ratio Lower Upper
152 100
115 63.5 41.1 123.3
150 158.5 0.0 349.0

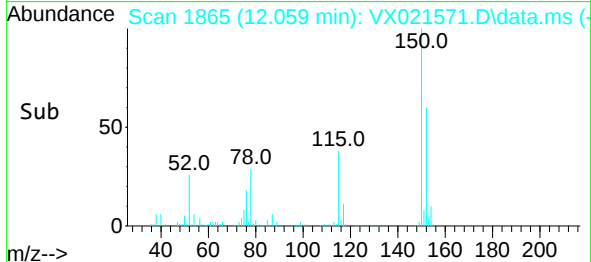

#73
Isopropylbenzene
Concen: 30.22 ug/l
RT: 11.000 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion:105 Resp: 102371
Ion Ratio Lower Upper
105 100
120 25.9 13.2 39.6


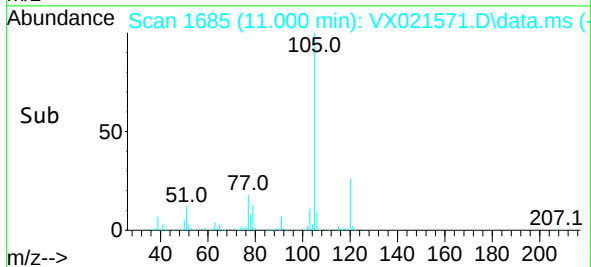

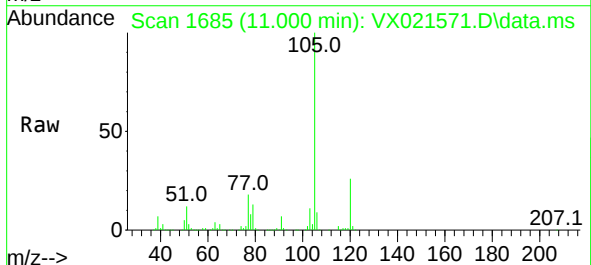




#74
N-amy1 acetate
Concen: 0.66 ug/l
RT: 10.894 min Scan# 1667
Delta R.T. 0.011 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion:	43	Resp:	1080
Ion	Ratio	Lower	Upper
43	100		
70	59.6	39.0	58.6#
55	362.2	21.5	32.3#
61	0.0	22.1	33.1#

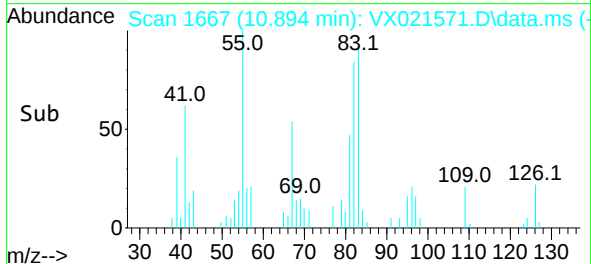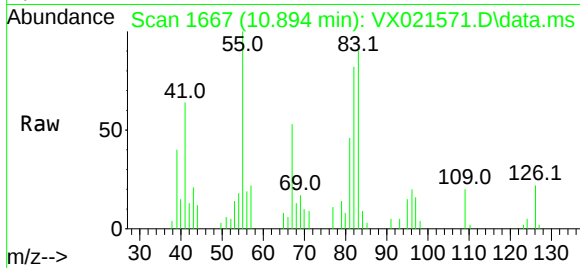

#75
1,1,2,2-Tetrachloroethane
Concen: 0.77 ug/l
RT: 11.259 min Scan# 1729
Delta R.T. 0.006 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion:	83	Resp:	919
Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.1	15.2#
85	6.0	31.8	95.4#


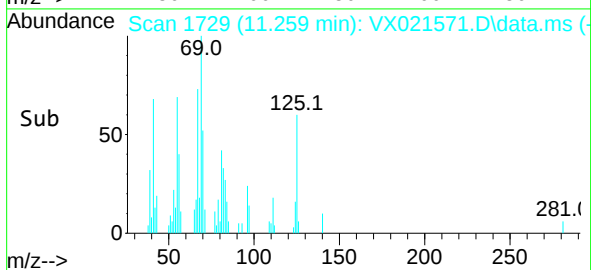

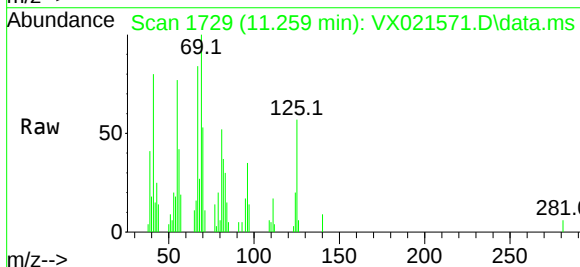




#76
1,2,3-Trichloropropane
Concen: 1.32 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. 0.064 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 75 Resp: 1484
Ion Ratio Lower Upper
75 100
77 609.2 19.1 57.5#



#78
n-propylbenzene
Concen: 50.00 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 91 Resp: 200026
Ion Ratio Lower Upper
91 100
120 21.4 11.5 34.5


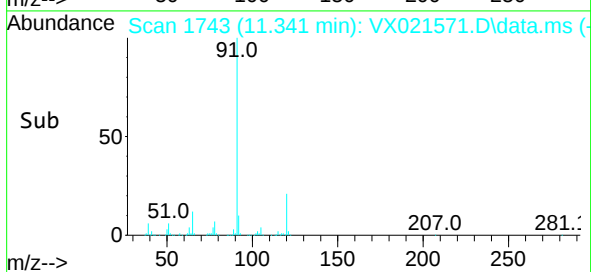






#79
2-Chlorotoluene
Concen: 82.42 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. -0.059 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 91 Resp: 200026
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

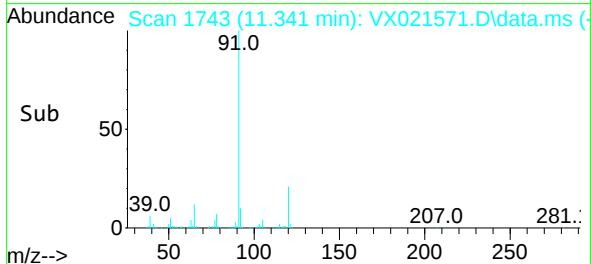

#80
1,3,5-Trimethylbenzene
Concen: 3.27 ug/l
RT: 11.436 min Scan# 1759
Delta R.T. -0.052 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 105 Resp: 9454
Ion Ratio Lower Upper
105 100
120 32.1 23.8 71.5


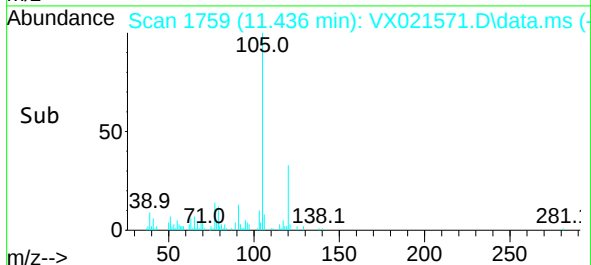

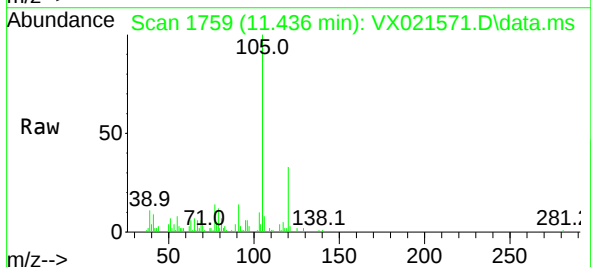




#81
trans-1,4-Dichloro-2-butene
Concen: 4.02 ug/l
RT: 11.000 min Scan# 1685
Delta R.T. -0.059 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampleId :
MW-1


Tgt Ion: 75 Resp: 1482
Ion Ratio Lower Upper
75 100
53 106.3 74.5 111.7
89 106.3 37.9 56.9#

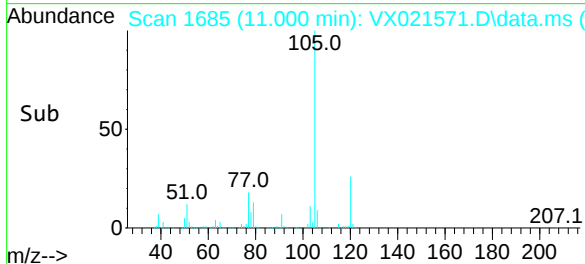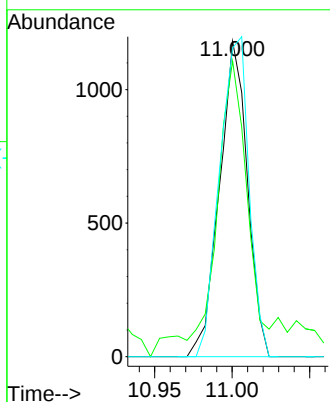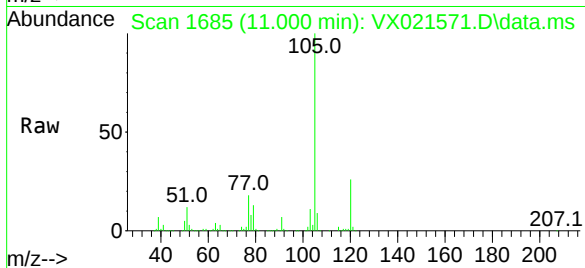

#82
4-Chlorotoluene
Concen: 69.42 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. -0.153 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 91 Resp: 200026
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


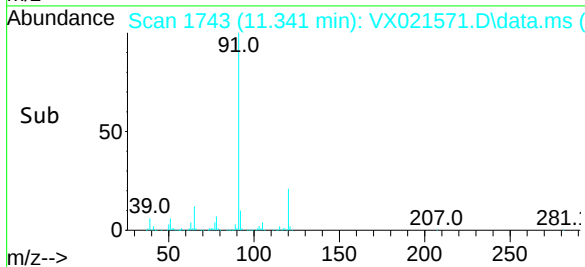
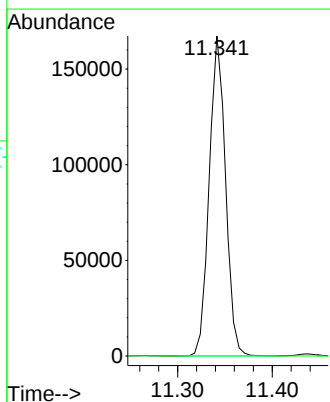
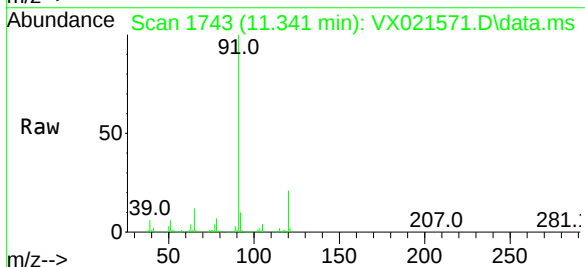




#83
tert-Butylbenzene
Concen: 3.65 ug/l
RT: 11.753 min Scan# 1813
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion:119 Resp: 10295
Ion Ratio Lower Upper
119 100
91 74.4 27.9 83.7
134 22.0 11.3 33.9

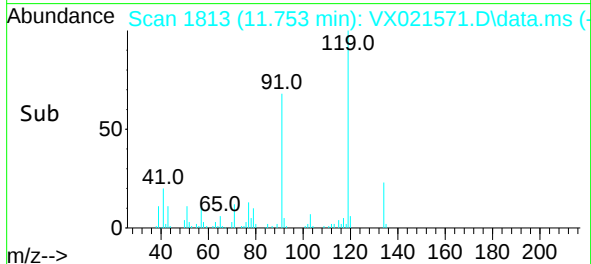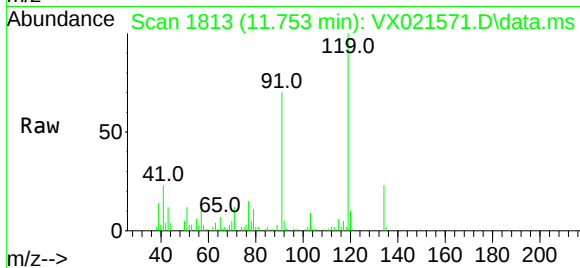

#84
1,2,4-Trimethylbenzene
Concen: 80.88 ug/l
RT: 11.789 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion:105 Resp: 235955
Ion Ratio Lower Upper
105 100
120 43.7 22.4 67.3


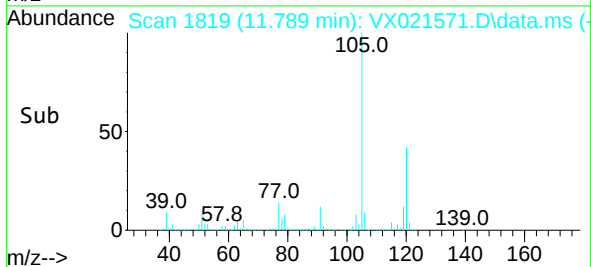

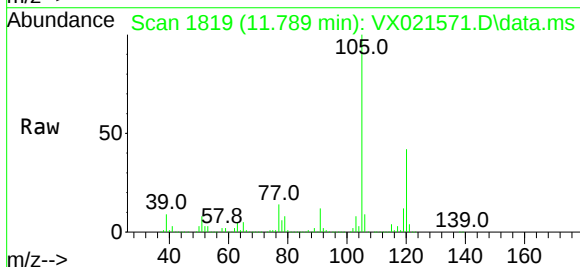




#85
 sec-Butylbenzene
 Concen: 13.29 ug/l
 RT: 11.930 min Scan# 1843
 Delta R.T. -0.000 min
 Lab File: VX021571.D
 Acq: 29 Mar 2021 12:55




Instrument :
 MSVOA_X
 ClientSampled :
 MW-1


Tgt Ion:105 Resp: 43181
 Ion Ratio Lower Upper
 105 100
 134 19.2 10.0 29.8

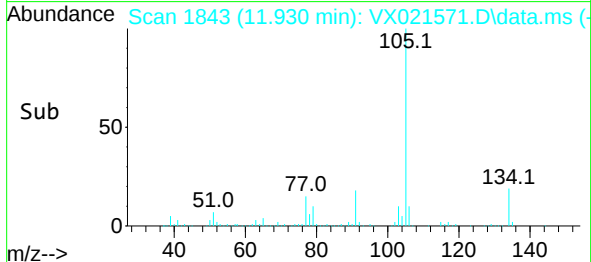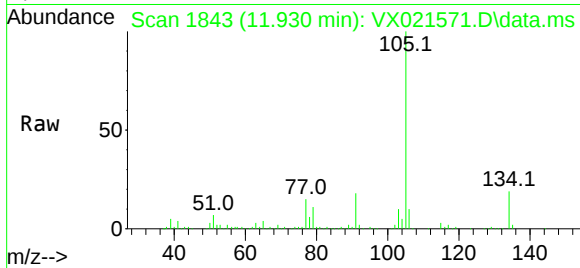

#86
 p-Isopropyltoluene
 Concen: 6.05 ug/l
 RT: 12.218 min Scan# 1892
 Delta R.T. 0.171 min
 Lab File: VX021571.D
 Acq: 29 Mar 2021 12:55

Tgt Ion:119 Resp: 17888
 Ion Ratio Lower Upper
 119 100
 134 29.5 12.9 38.7
 91 30.0 11.7 35.0


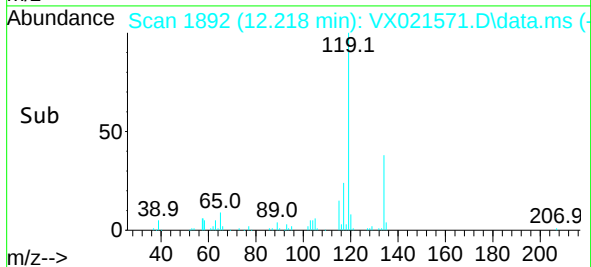

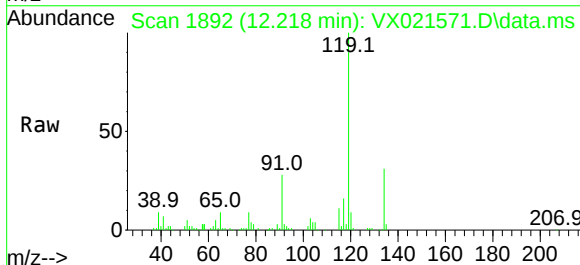


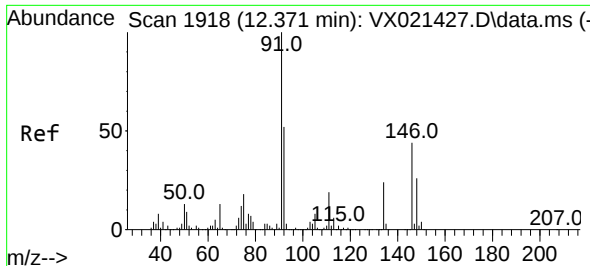

#89
n-Butylbenzene
Concen: 6.22 ug/l
RT: 12.371 min Scan# 1918
Delta R.T. 0.000 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55




Instrument :
MSVOA_X
ClientSampled :
MW-1


Tgt Ion: 91 Resp: 16860
Ion Ratio Lower Upper
91 100
92 45.3 27.4 82.0
134 42.1 13.2 39.5#

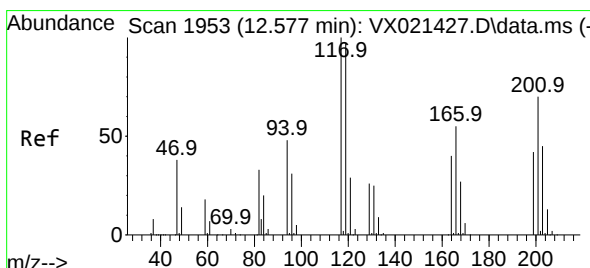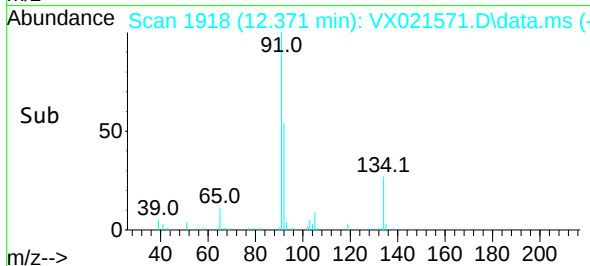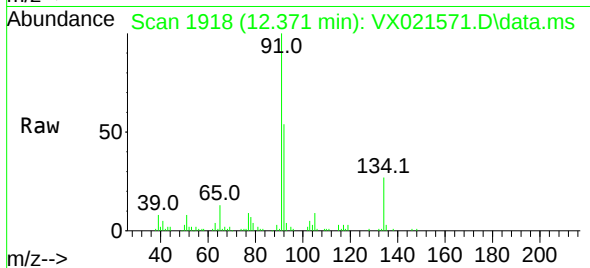

#90
Hexachloroethane
Concen: 12.70 ug/l
RT: 12.653 min Scan# 1966
Delta R.T. 0.076 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 117 Resp: 6780
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


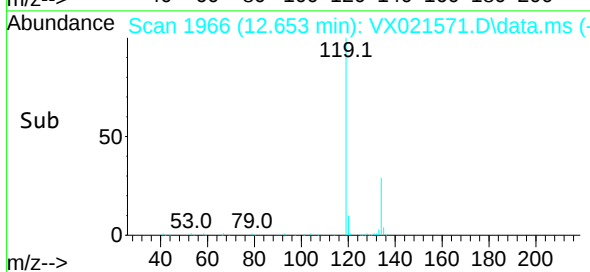

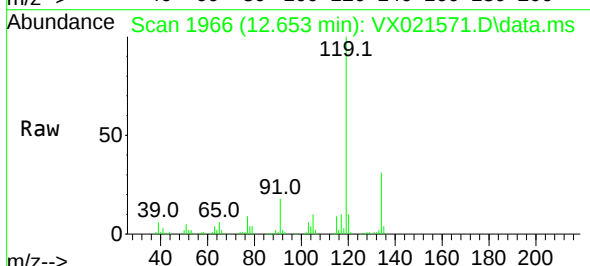


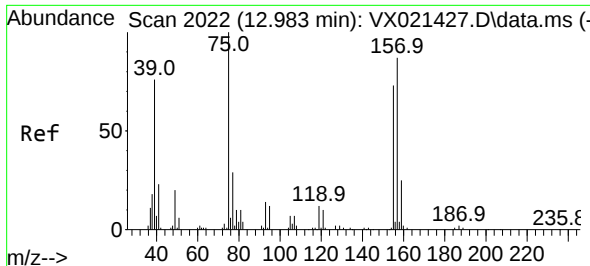

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.30 ug/l
RT: 13.001 min Scan# 2025
Delta R.T. 0.018 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Tgt Ion: 75 Resp: 105
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

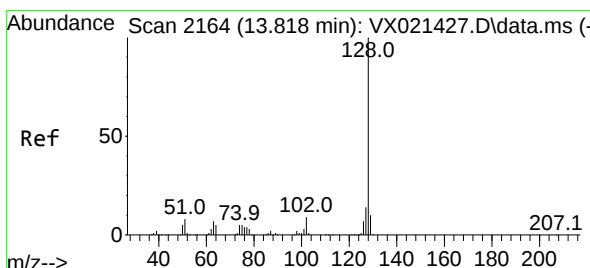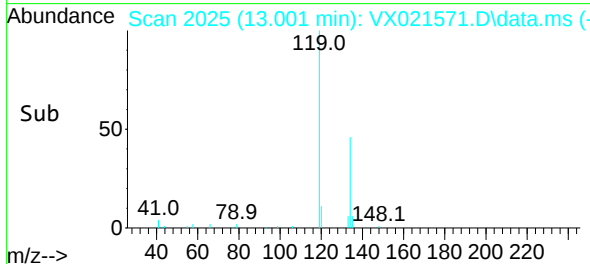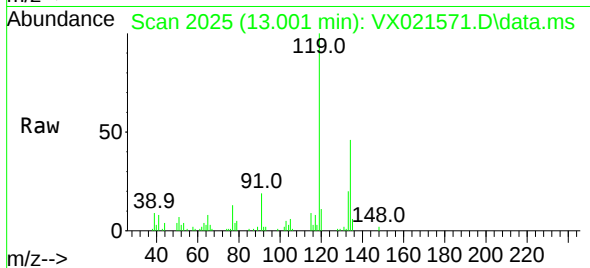

#95
Naphthalene
Concen: 3.43 ug/l
RT: 13.812 min Scan# 2163
Delta R.T. -0.006 min
Lab File: VX021571.D
Acq: 29 Mar 2021 12:55

Tgt Ion: 128 Resp: 10784
Ion Ratio Lower Upper
128 100
127 13.0 10.3 15.5
129 11.5 8.8 13.2

