

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021575.D
 Acq On : 29 Mar 2021 14:29
 Operator : JC/MD
 Sample : M1785-16 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-5R

Quant Time: Mar 30 03:27:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 24 12:25:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	62597	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	116607	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	118178	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	56913	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	54330	52.16	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 104.32%			
35) Dibromofluoromethane	5.458	113	41943	50.64	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.28%			
50) Toluene-d8	8.694	98	147630	50.02	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 100.04%			
62) 4-Bromofluorobenzene	11.118	95	62638	54.58	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 109.16%			
Target Compounds					Qvalue	
3) Chloromethane	1.317	50	1282	1.66	ug/l	100
10) Methyl Iodide	2.487	142	18	6.67	ug/l #	42
11) Tert butyl alcohol	3.023	59	206	1.20	ug/l #	73
13) Acrolein	2.246	56	18	4.50	ug/l #	24
16) Acetone	2.434	43	469	1.19	ug/l #	40
20) Methylene Chloride	2.834	84	221	0.29	ug/l #	88
29) Tetrahydrofuran	5.111	42	170	0.44	ug/l #	27
31) Cyclohexane	5.623	56	1754	1.53	ug/l #	30
36) 1,1-Dichloropropene	5.629	75	5804	5.08	ug/l #	50
38) Carbon Tetrachloride	5.629	117	7112	5.79	ug/l #	16
44) Trichloroethene	7.182	130	199	0.23	ug/l	97
51) 4-Methyl-2-Pentanone	8.694	43	840	0.64	ug/l #	1
55) 1,1,2-Trichloroethane	9.147	97	191	0.23	ug/l #	15
56) Ethyl methacrylate	9.023	69	56	2.12	ug/l #	1
67) Ethyl Benzene	10.235	91	3380	0.78	ug/l	98
68) m/p-Xylenes	10.335	106	6842	4.44	ug/l	89
69) o-Xylene	10.682	106	303	0.20	ug/l	74
73) Isopropylbenzene	11.000	105	28575	7.15	ug/l	98
74) N-amyl acetate	10.888	43	443	0.23	ug/l #	1
76) 1,2,3-Trichloropropane	11.118	75	34670	26.17	ug/l #	39
78) n-propylbenzene	11.341	91	64560	13.67	ug/l	98
79) 2-Chlorotoluene	11.418	91	3616	1.26	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.488	105	33639	9.85	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.118	75	34670	79.70	ug/l #	12
82) 4-Chlorotoluene	11.488	91	4221	1.24	ug/l #	45
83) tert-Butylbenzene	11.753	119	3851	1.16	ug/l	87
84) 1,2,4-Trimethylbenzene	11.788	105	151320	43.94	ug/l	99
85) sec-Butylbenzene	11.930	105	17160	4.47	ug/l	81
86) p-Isopropyltoluene	12.006	119	5974	1.71	ug/l	92
89) n-Butylbenzene	12.371	91	12720	3.98	ug/l #	69
90) Hexachloroethane	12.653	117	3612	5.73	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	13.006	75	101	2.24	ug/l #	1
95) Naphthalene	13.818	128	1052	0.28	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
MW-5R

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021575.D
Acq On : 29 Mar 2021 14:29
Operator : JC/MD
Sample : M1785-16 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5R

Quant Time: Mar 30 03:27:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration




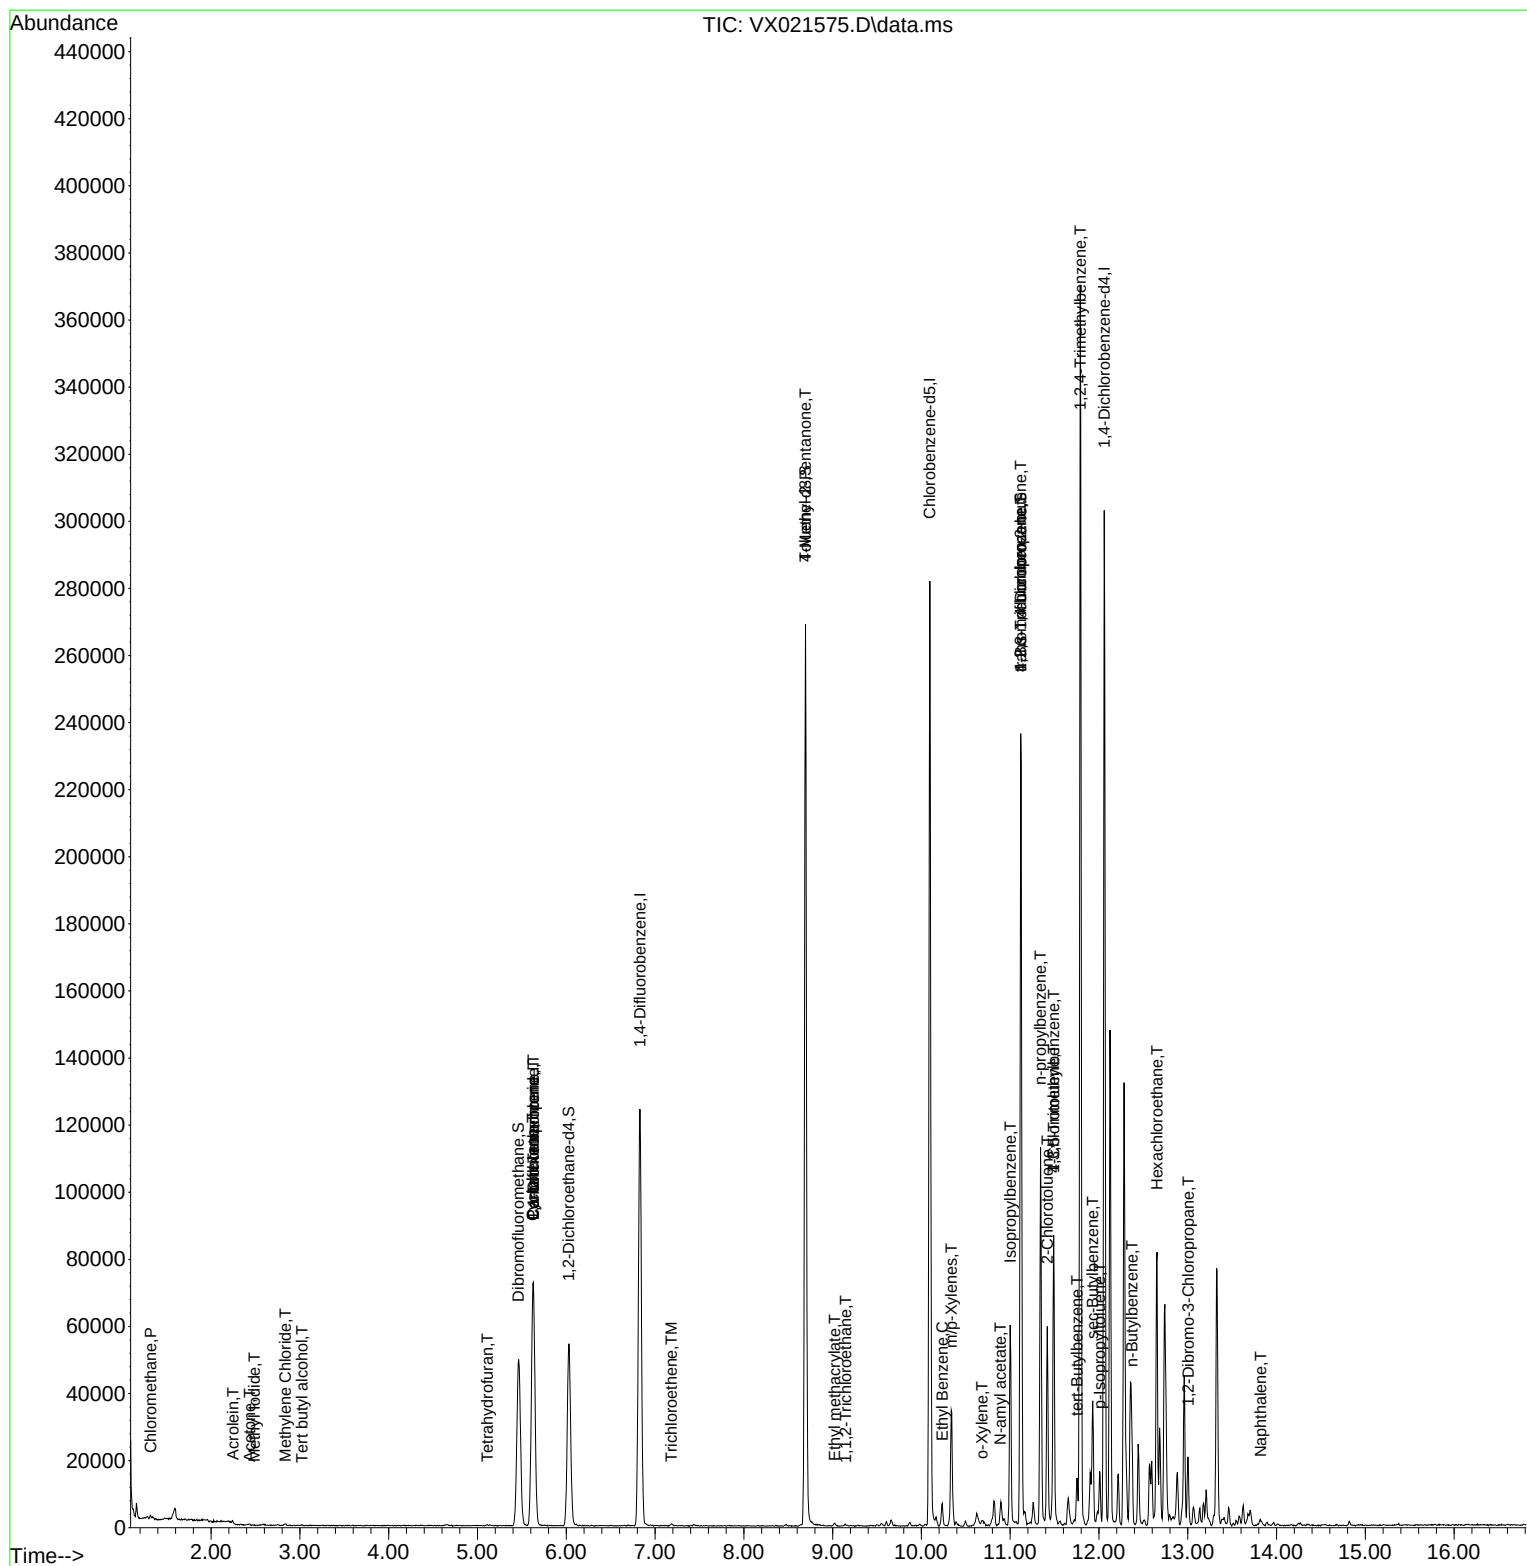


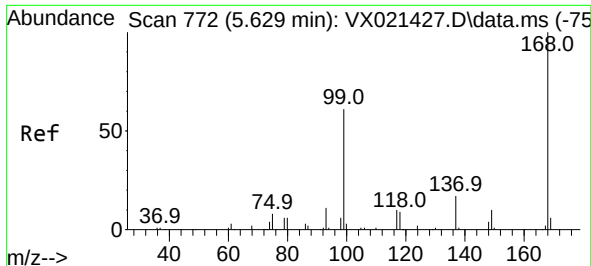

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:168 Resp: 62597
Ion Ratio Lower Upper
168 100
99 63.6 45.8 68.6

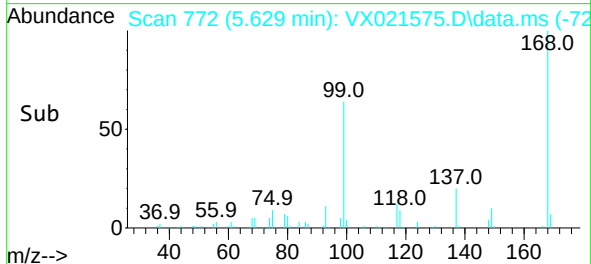

#3
Chloromethane
Concen: 1.66 ug/l
RT: 1.317 min Scan# 39
Delta R.T. 0.006 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 50 Resp: 1282
Ion Ratio Lower Upper
50 100
52 32.8 26.4 39.6

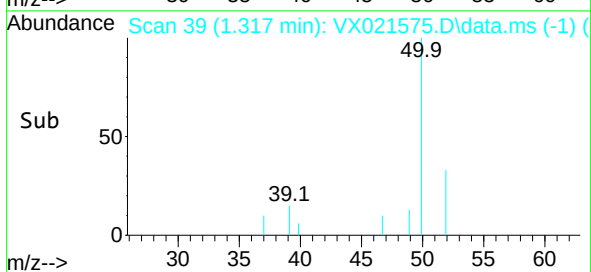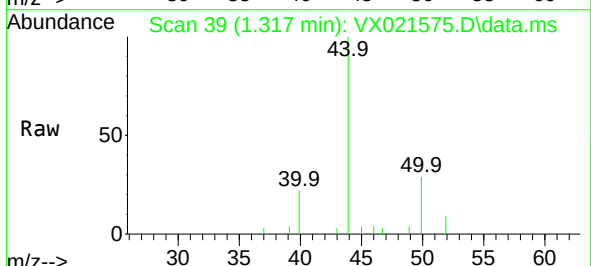



#10

Methyl Iodide

Concen: 6.67 ug/l

RT: 2.487 min Scan# 238

Delta R.T. 0.000 min

Lab File: VX021575.D

Acq: 29 Mar 2021 14:29





Instrument :

MSVOA_X

ClientSampleId :

MW-5R

Tgt Ion:	142	Resp:	18
Ion	Ratio	Lower	Upper
142	100		
127	0.0	33.3	49.9#
141	0.0	11.4	17.0#

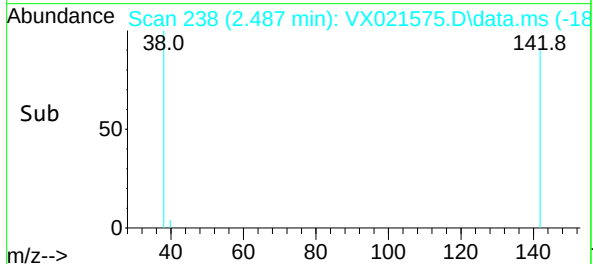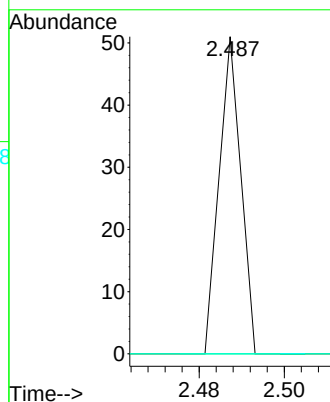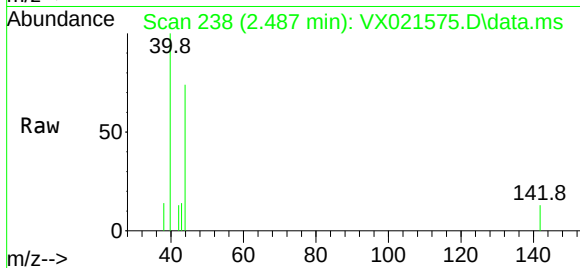

#11

Tert butyl alcohol

Concen: 1.20 ug/l




RT: 3.023 min Scan# 329


Delta R.T. -0.000 min

Lab File: VX021575.D

Acq: 29 Mar 2021 14:29

Tgt Ion:	59	Resp:	206
Ion	Ratio	Lower	Upper
59	100		
57	0.0	7.8	11.8#


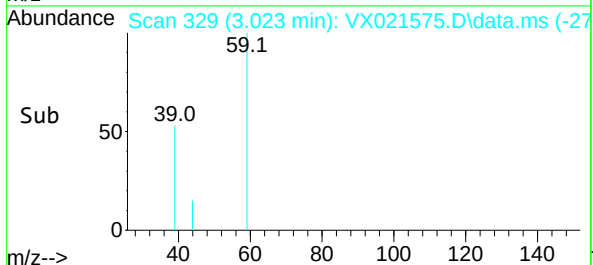
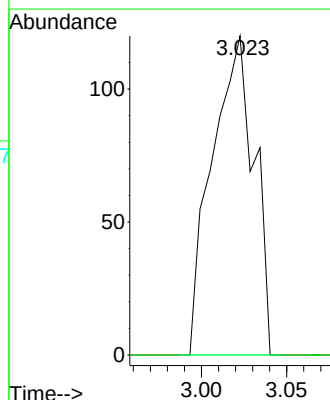
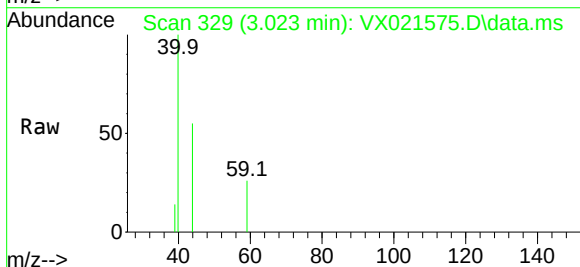




#13
Acrolein
Concen: 4.50 ug/l
RT: 2.246 min Scan# 197
Delta R.T. -0.030 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion: 56 Resp: 18
Ion Ratio Lower Upper
56 100
55 133.3 56.4 84.6#

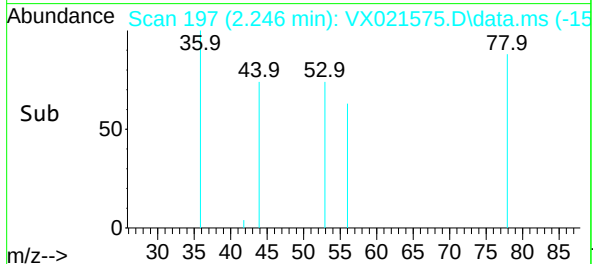

#16
Acetone
Concen: 1.19 ug/l
RT: 2.434 min Scan# 229
Delta R.T. 0.011 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 43 Resp: 469
Ion Ratio Lower Upper
43 100
58 0.0 27.8 41.8#

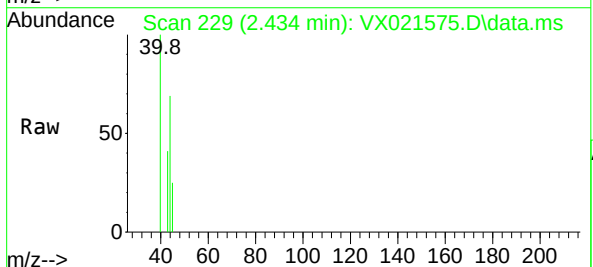



#20

Methylene Chloride

Concen: 0.29 ug/l

RT: 2.834 min Scan# 297

Delta R.T. 0.000 min

Lab File: VX021575.D

Acq: 29 Mar 2021 14:29

Tgt Ion: 84 Resp: 221





Ion Ratio Lower Upper

84 100

49 112.4 88.6 132.8

51 0.0 27.0 40.6#

86 60.0 50.3 75.5

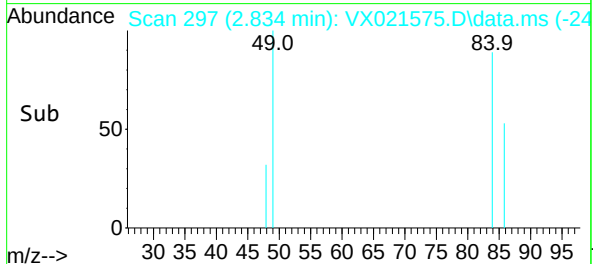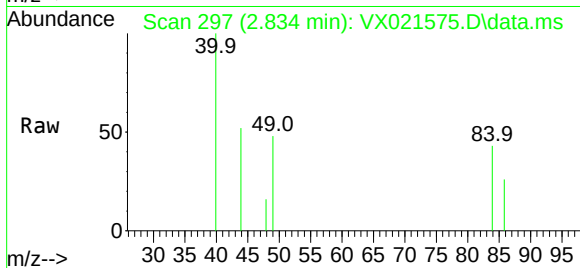

#29

Tetrahydrofuran

Concen: 0.44 ug/l

RT: 5.111 min Scan# 684

Delta R.T. 0.023 min

Lab File: VX021575.D

Acq: 29 Mar 2021 14:29




Tgt Ion: 42 Resp: 170


Ion Ratio Lower Upper

42 100

72 0.0 41.7 62.5#


71 0.0 38.4 57.6#

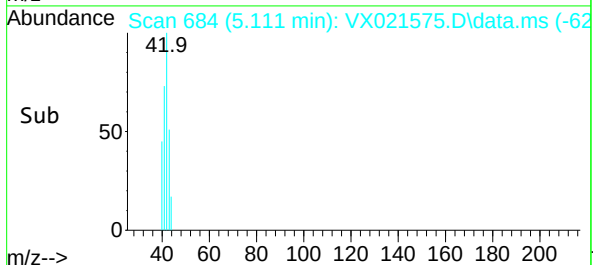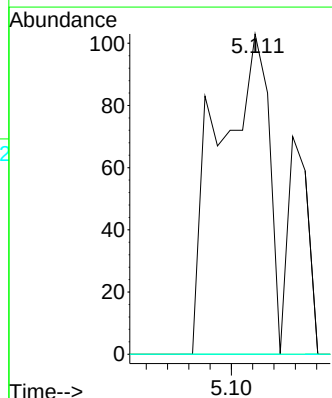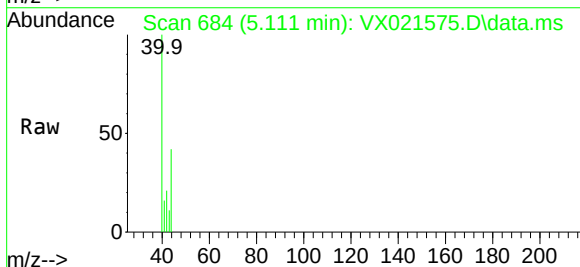






#31
Cyclohexane
Concen: 1.53 ug/l
RT: 5.623 min Scan# 771
Delta R.T. 0.076 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29


Instrument :
MSVOA_X
ClientSampled :
MW-5R





Tgt Ion: 56 Resp: 1754
Ion Ratio Lower Upper
56 100
69 177.7 25.3 37.9#
84 90.5 71.4 107.0




#33
1,2-Dichloroethane-d4
Concen: 52.16 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29



Tgt Ion: 65 Resp: 54330
Ion Ratio Lower Upper
65 100
67 49.7 0.0 105.4

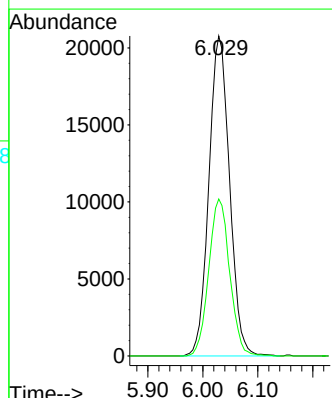



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.829 min Scan# 976

Delta R.T. -0.000 min

Lab File: VX021575.D

Acq: 29 Mar 2021 14:29





Tgt Ion:114 Resp: 116607

Ion Ratio Lower Upper

114 100

63 22.6 0.0 40.8

88 16.8 0.0 32.8

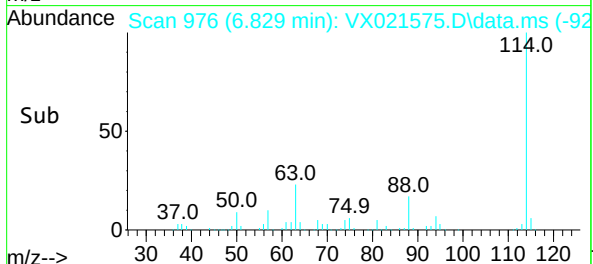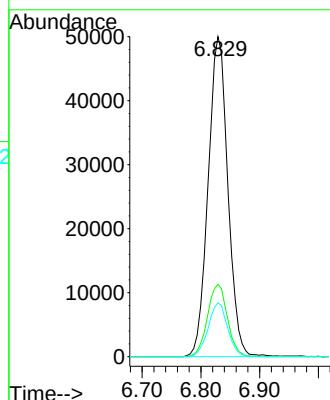

#35

Dibromofluoromethane

Concen: 50.64 ug/l

RT: 5.458 min Scan# 743

Delta R.T. -0.006 min

Lab File: VX021575.D

Acq: 29 Mar 2021 14:29




Tgt Ion:113 Resp: 41943


Ion Ratio Lower Upper

113 100

111 101.8 81.9 122.9

192 18.6 16.7 25.1


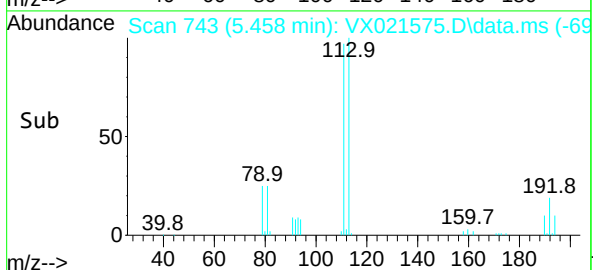
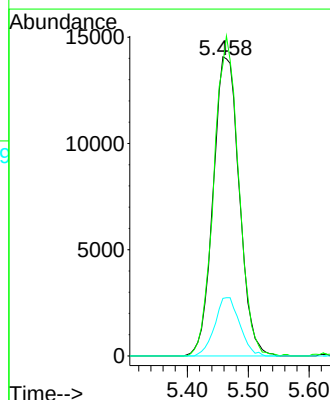





#36
1,1-Dichloropropene
Concen: 5.08 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.135 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampled :
MW-5R


Tgt Ion: 75 Resp: 5804
Ion Ratio Lower Upper
75 100
110 10.4 18.1 54.4#
77 0.0 25.3 37.9#

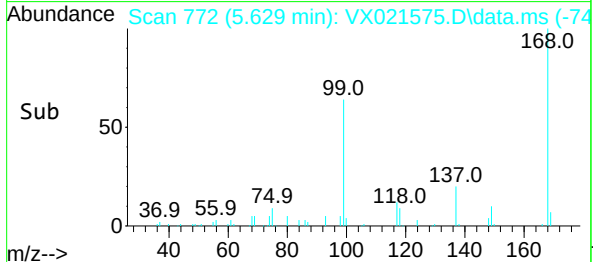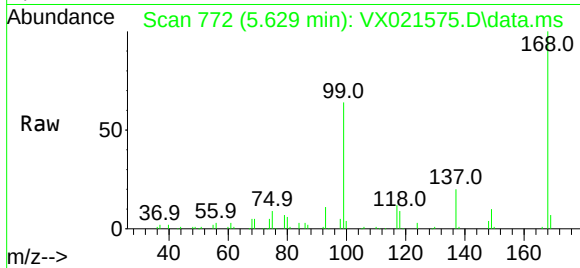

#38
Carbon Tetrachloride
Concen: 5.79 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.123 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 117 Resp: 7112
Ion Ratio Lower Upper
117 100
119 4.2 76.2 114.2#
121 0.0 24.8 37.2#


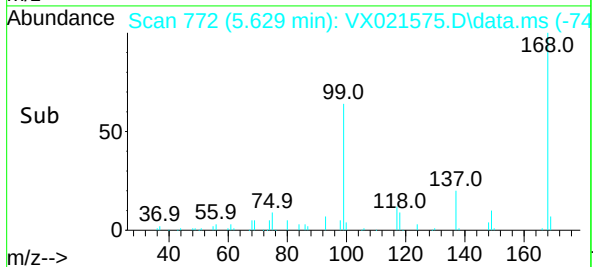

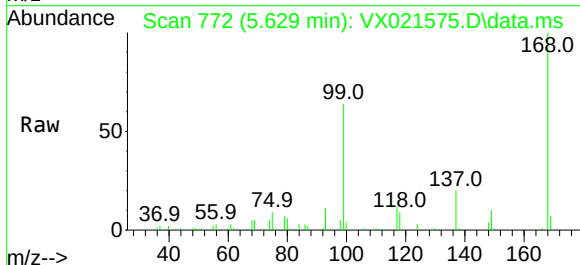




#44
Trichloroethene
Concen: 0.23 ug/l
RT: 7.182 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampled :
MW-5R


Tgt Ion:130 Resp: 199
Ion Ratio Lower Upper
130 100
95 102.5 0.0 198.0

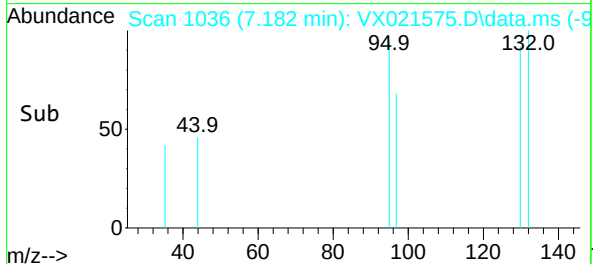

#50
Toluene-d8
Concen: 50.02 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 98 Resp: 147630
Ion Ratio Lower Upper
98 100
100 64.6 51.9 77.9


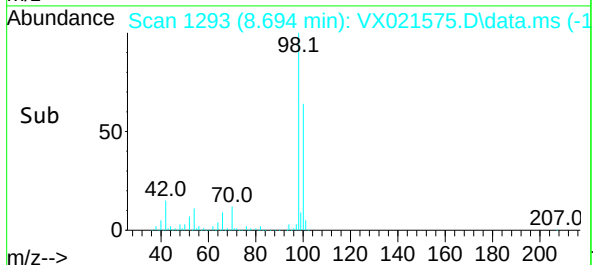

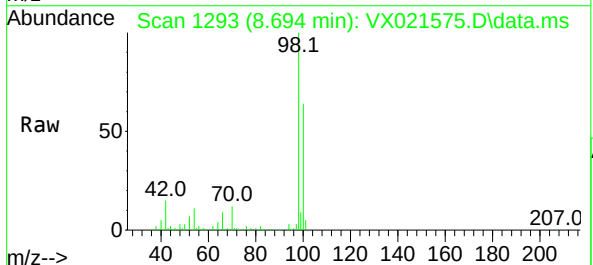


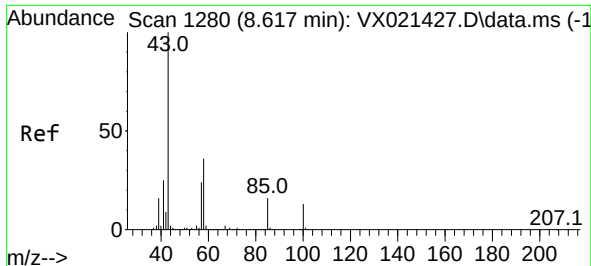

#51
4-Methyl-2-Pentanone
Concen: 0.64 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. 0.077 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampled :
MW-5R


Tgt Ion: 43 Resp: 840
Ion Ratio Lower Upper
43 100
58 169.5 35.4 53.0#

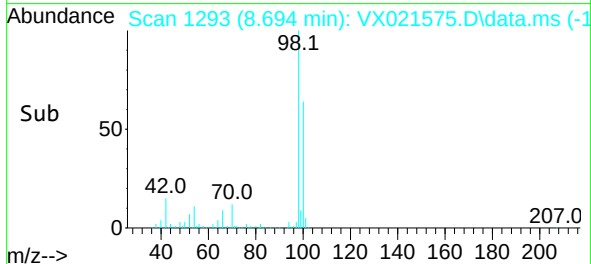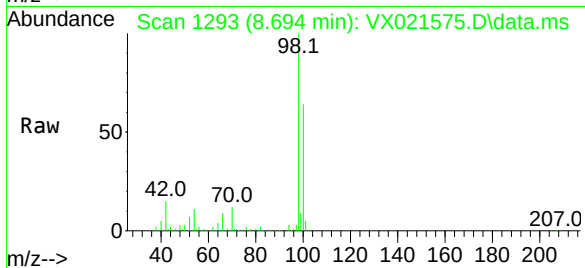

#55
1,1,2-Trichloroethane
Concen: 0.23 ug/l
RT: 9.147 min Scan# 1370
Delta R.T. -0.047 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 97 Resp: 191
Ion Ratio Lower Upper
97 100
83 0.0 69.3 103.9#
85 0.0 44.3 66.5#
99 0.0 50.3 75.5#




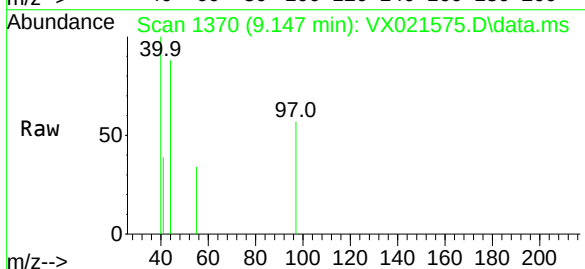


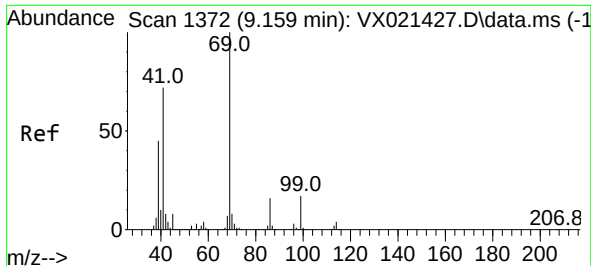

#56
Ethyl methacrylate
Concen: 2.12 ug/l
RT: 9.023 min Scan# 1349
Delta R.T. -0.136 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:	69	Resp:	56
Ion	Ratio	Lower	Upper
69	100		
41	153.6	46.8	70.2#
39	219.6	24.7	37.1#

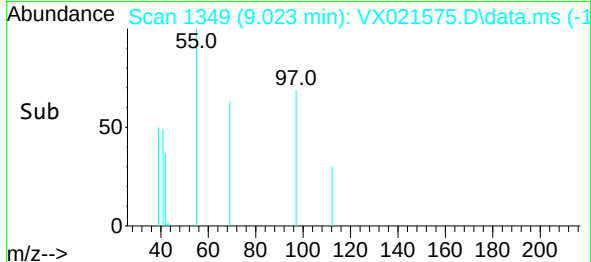

#62
4-Bromofluorobenzene
Concen: 54.58 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion:	95	Resp:	62638
Ion	Ratio	Lower	Upper
95	100		
174	73.0	0.0	154.6
176	68.5	0.0	155.8


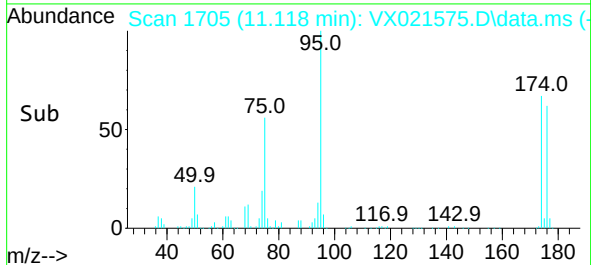

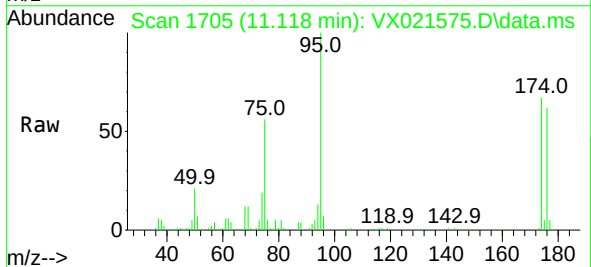


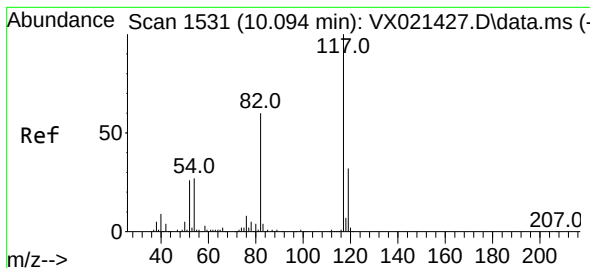

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:117 Resp: 118178
Ion Ratio Lower Upper
117 100
82 58.8 47.4 71.2
119 30.2 26.6 39.8

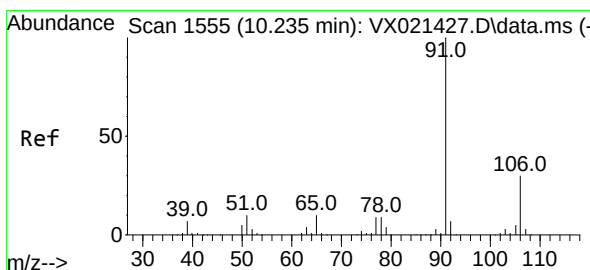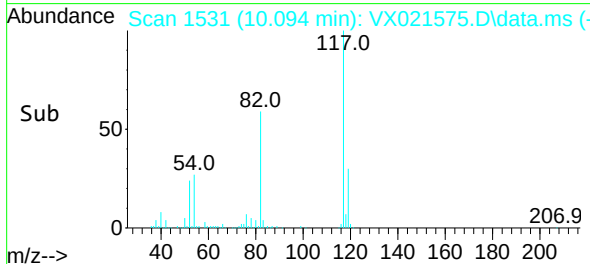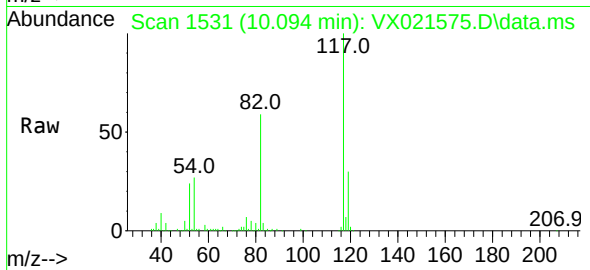

#67
Ethyl Benzene
Concen: 0.78 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 91 Resp: 3380
Ion Ratio Lower Upper
91 100
106 31.9 24.6 37.0


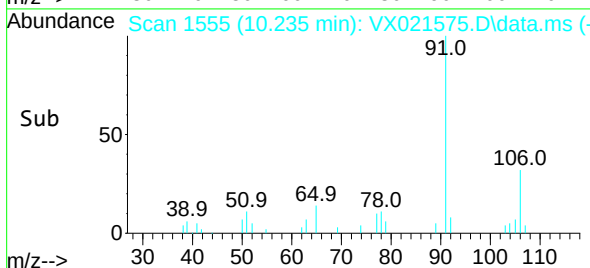

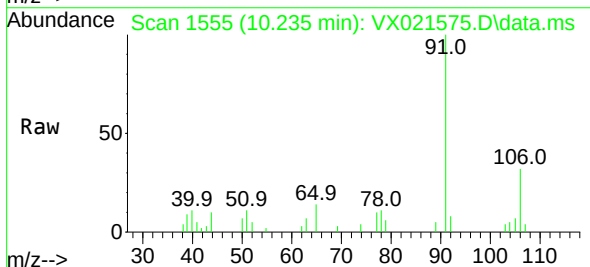




#68
m/p-Xylenes
Concen: 4.44 ug/l
RT: 10.335 min Scan# 1572
Delta R.T. -0.006 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:106 Resp: 6842
Ion Ratio Lower Upper
106 100
91 220.7 162.8 244.2

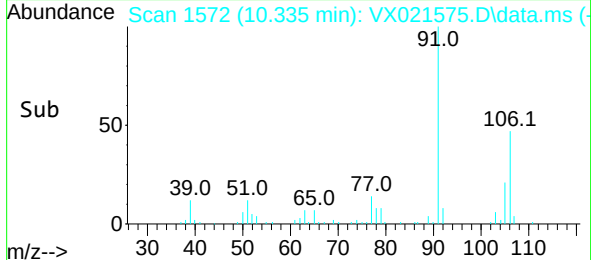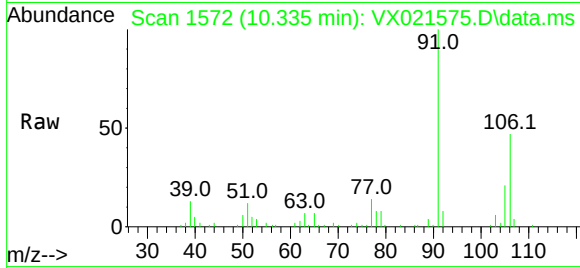

#69
o-Xylene
Concen: 0.20 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion:106 Resp: 303
Ion Ratio Lower Upper
106 100
91 258.1 108.1 324.2


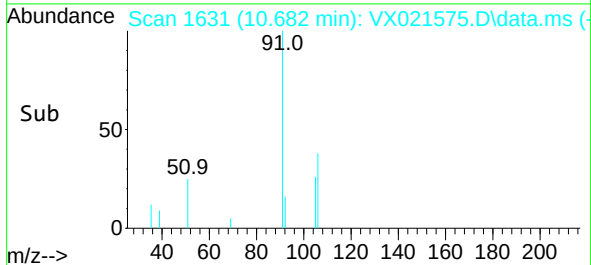

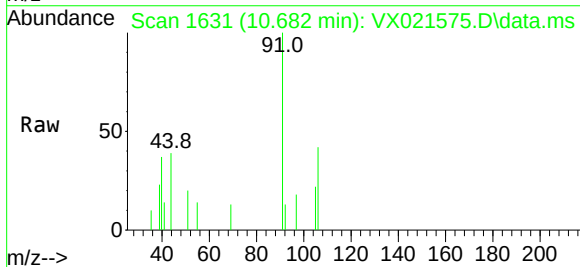


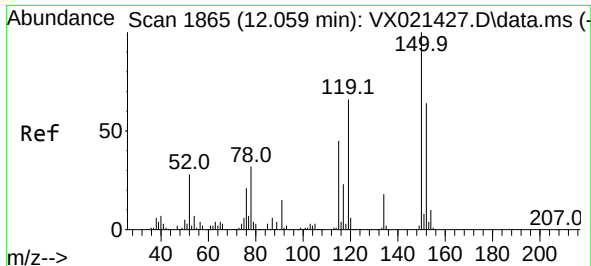

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:152 Resp: 56913
Ion Ratio Lower Upper
152 100
115 62.7 41.1 123.3
150 155.6 0.0 349.0

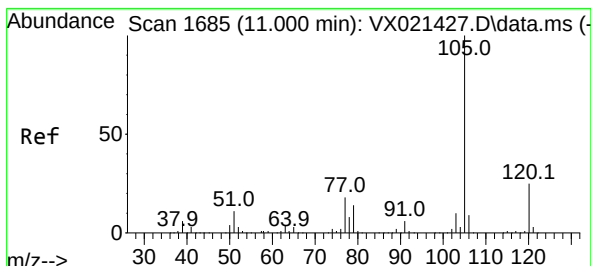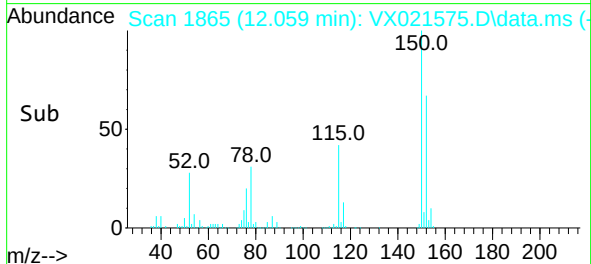

#73
Isopropylbenzene
Concen: 7.15 ug/l
RT: 11.000 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion:105 Resp: 28575
Ion Ratio Lower Upper
105 100
120 25.6 13.2 39.6


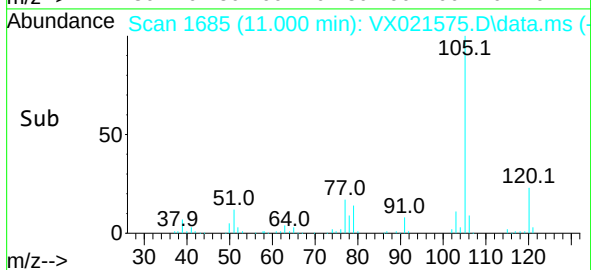

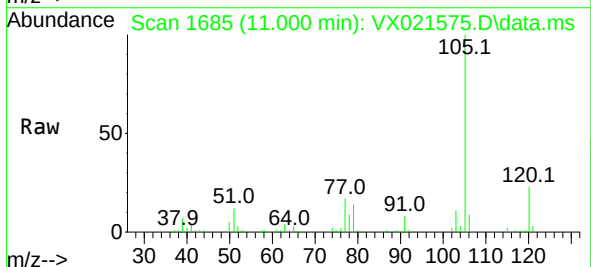




#74
N-amy1 acetate
Concen: 0.23 ug/l
RT: 10.888 min Scan# 1666
Delta R.T. 0.005 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampled :
MW-5R


Tgt Ion:	43	Resp:	443
Ion	Ratio	Lower	Upper
43	100		
70	78.8	39.0	58.6#
55	318.1	21.5	32.3#
61	0.0	22.1	33.1#

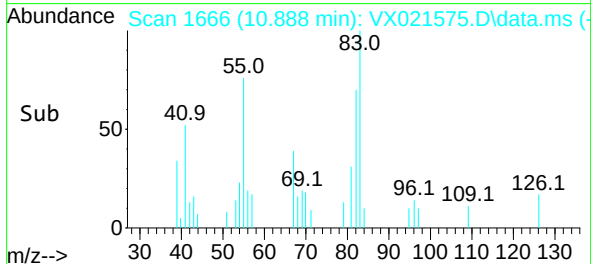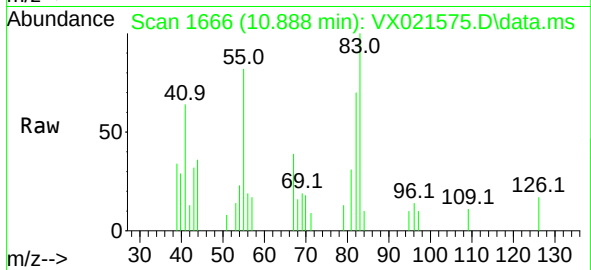

#76
1,2,3-Trichloropropane
Concen: 26.17 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion:	75	Resp:	34670
Ion	Ratio	Lower	Upper
75	100		
77	1.4	19.1	57.5#




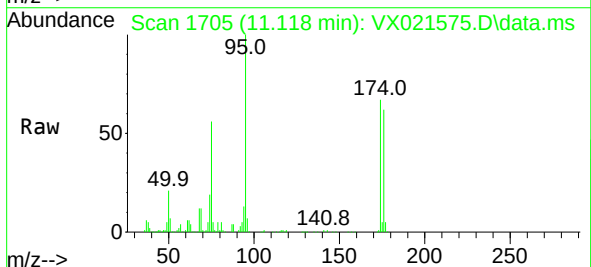


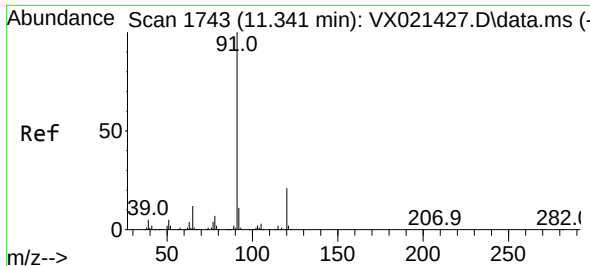

#78
n-propylbenzene
Concen: 13.67 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampled :
MW-5R


Tgt Ion: 91 Resp: 64560
Ion Ratio Lower Upper
91 100
120 21.9 11.5 34.5

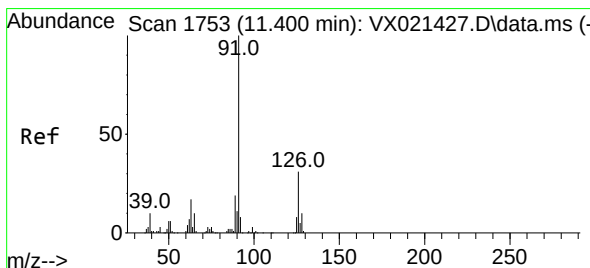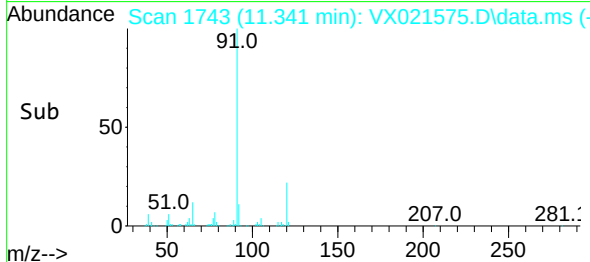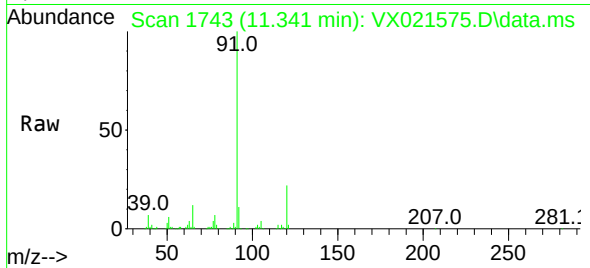

#79
2-Chlorotoluene
Concen: 1.26 ug/l
RT: 11.418 min Scan# 1756
Delta R.T. 0.018 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 91 Resp: 3616
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


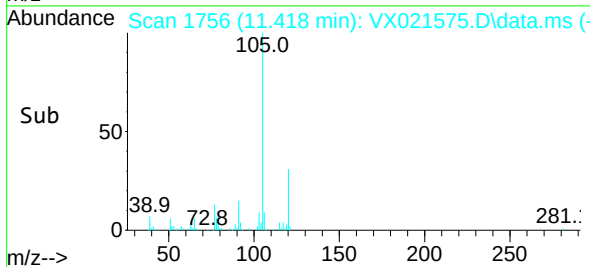

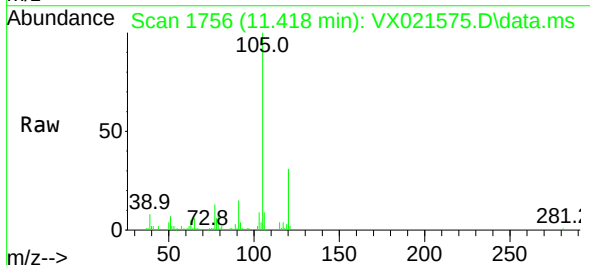


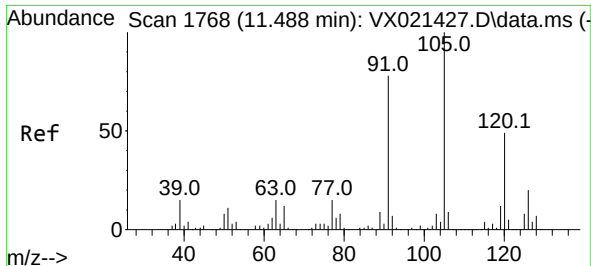

#80
1,3,5-Trimethylbenzene
Concen: 9.85 ug/l
RT: 11.488 min Scan# 1768
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampled :
MW-5R


Tgt Ion:105 Resp: 33639
Ion Ratio Lower Upper
105 100
120 48.8 23.8 71.5

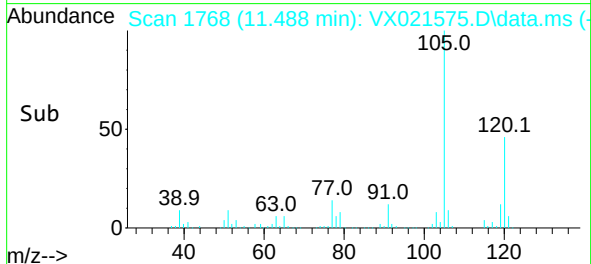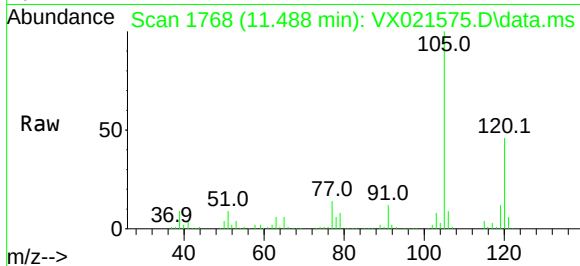

#81
trans-1,4-Dichloro-2-butene
Concen: 79.70 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 75 Resp: 34670
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#


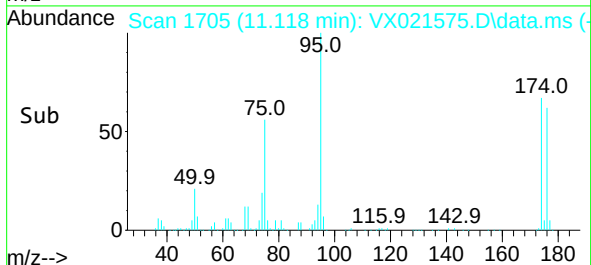

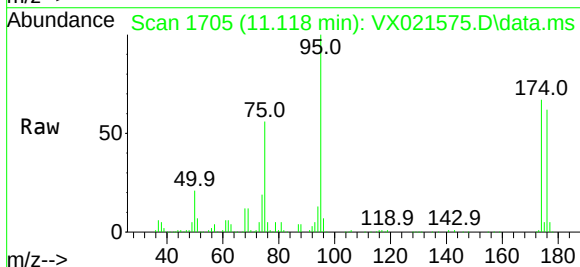




#82
4-Chlorotoluene
Concen: 1.24 ug/l
RT: 11.488 min Scan# 1768
Delta R.T. -0.006 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion: 91 Resp: 4221
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

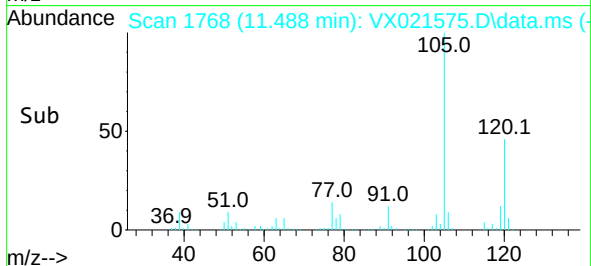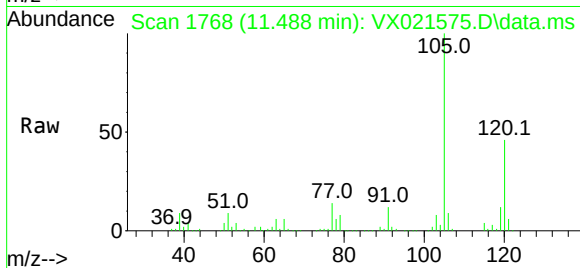

#83
tert-Butylbenzene
Concen: 1.16 ug/l
RT: 11.753 min Scan# 1813
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 119 Resp: 3851
Ion Ratio Lower Upper
119 100
91 68.4 27.9 83.7
134 23.9 11.3 33.9


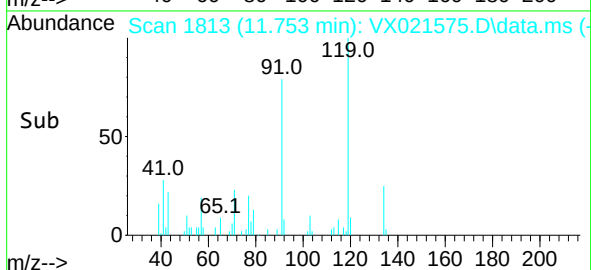

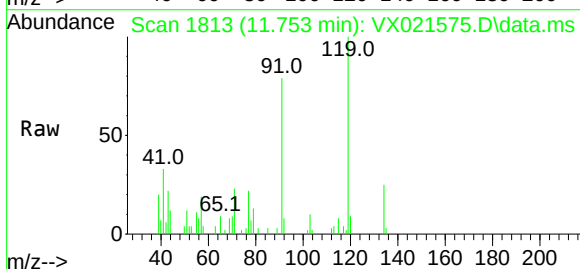




#84
1,2,4-Trimethylbenzene
Concen: 43.94 ug/l
RT: 11.788 min Scan# 1819
Delta R.T. -0.001 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:105 Resp: 151320
Ion Ratio Lower Upper
105 100
120 44.1 22.4 67.3

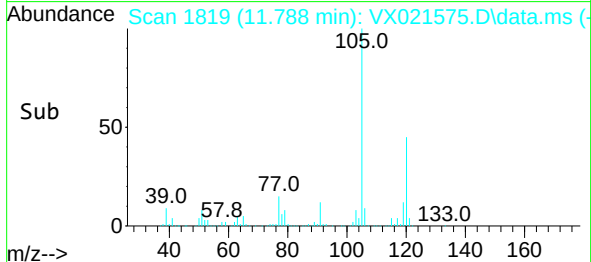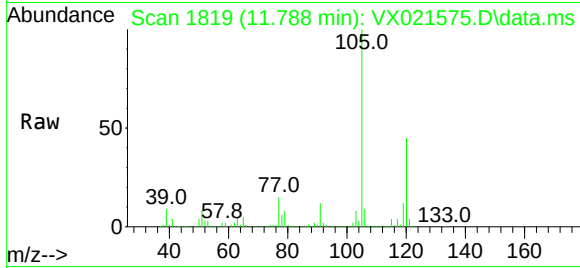

#85
sec-Butylbenzene
Concen: 4.47 ug/l
RT: 11.930 min Scan# 1843
Delta R.T. -0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion:105 Resp: 17160
Ion Ratio Lower Upper
105 100
134 28.5 10.0 29.8


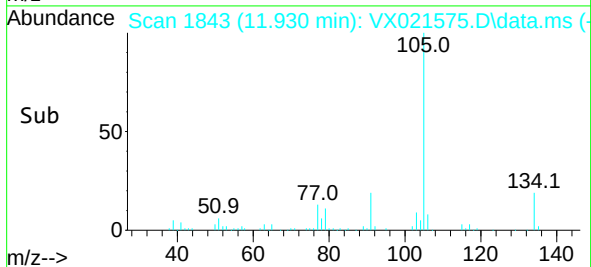

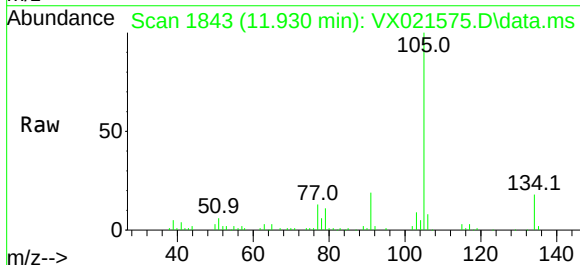


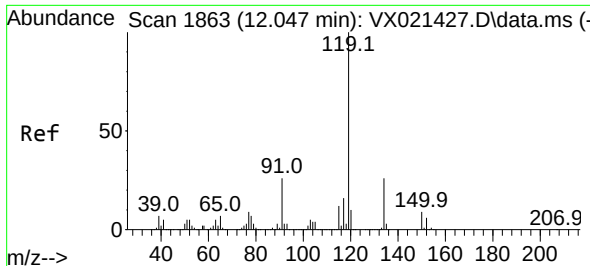

#86
p-Isopropyltoluene
Concen: 1.71 ug/l
RT: 12.006 min Scan# 1856
Delta R.T. -0.041 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:119 Resp: 5974
Ion Ratio Lower Upper
119 100
134 28.4 12.9 38.7
91 28.9 11.7 35.0

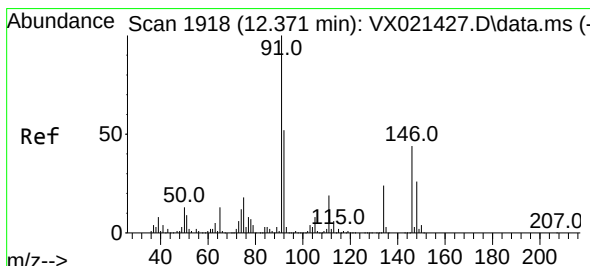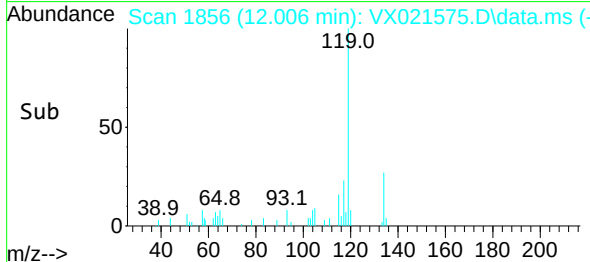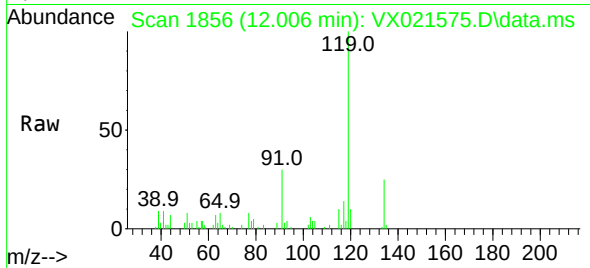

#89
n-Butylbenzene
Concen: 3.98 ug/l
RT: 12.371 min Scan# 1918
Delta R.T. -0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Tgt Ion: 91 Resp: 12720
Ion Ratio Lower Upper
91 100
92 39.1 27.4 82.0
134 52.0 13.2 39.5#


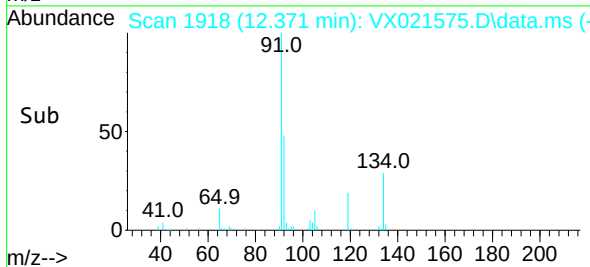

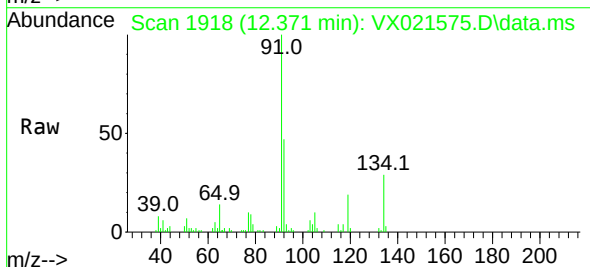




#90
Hexachloroethane
Concen: 5.73 ug/l
RT: 12.653 min Scan# 1966
Delta R.T. 0.076 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29




Instrument :
MSVOA_X
ClientSampleId :
MW-5R


Tgt Ion:117 Resp: 3612
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

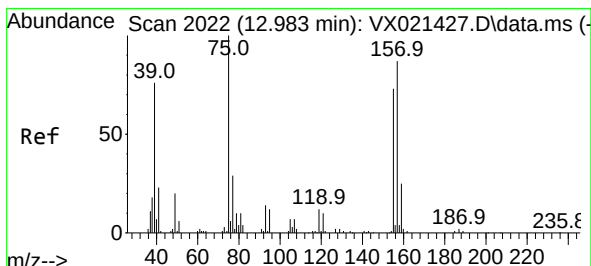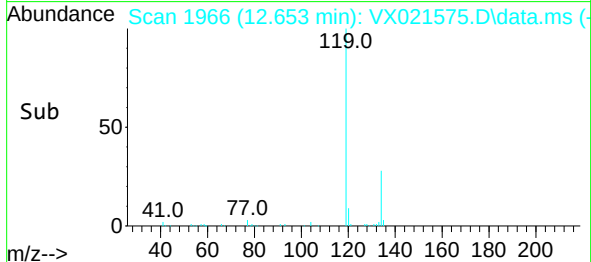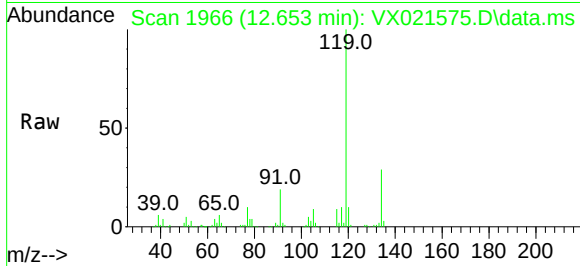

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.24 ug/l
RT: 13.006 min Scan# 2026
Delta R.T. 0.023 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29


Tgt Ion: 75 Resp: 101
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

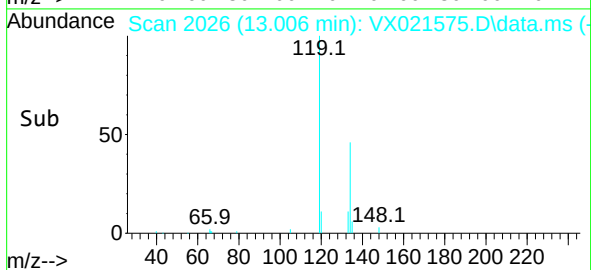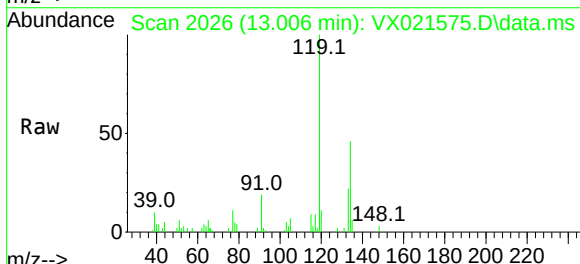

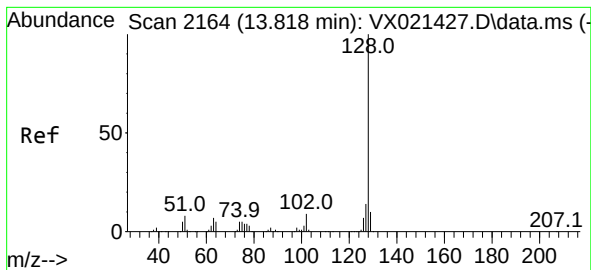

#95
Naphthalene
Concen: 0.28 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. 0.000 min
Lab File: VX021575.D
Acq: 29 Mar 2021 14:29

Instrument :
MSVOA_X
ClientSampleId :
MW-5R

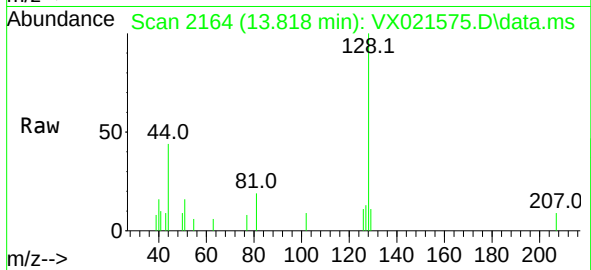

Tgt Ion:	128	Resp:	1052
Ion	Ratio	Lower	Upper
128	100		
127	12.1	10.3	15.5
129	9.5	8.8	13.2

