

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021583.D
 Acq On : 29 Mar 2021 17:36
 Operator : JC/MD
 Sample : M1860-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GWBR3-115-137-032621

Quant Time: Mar 30 03:30:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 24 12:25:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.635	168	60239	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.835	114	111811	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	114460	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.065	152	50262	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	52124	52.00	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	104.00%
35) Dibromofluoromethane	5.464	113	39865	50.19	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.38%
50) Toluene-d8	8.694	98	140473	49.63	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.26%
62) 4-Bromofluorobenzene	11.124	95	55973	50.87	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.74%


Target Compounds						Qvalue
3) Chloromethane	1.317	50	1617	2.16	ug/l	95
4) Vinyl Chloride	1.393	62	162	0.24	ug/l #	72
5) Bromomethane	1.640	94	130	0.48	ug/l	92
12) 1,1-Dichloroethene	2.352	96	13147	21.66	ug/l	93
13) Acrolein	2.270	56	18	4.51	ug/l #	1
16) Acetone	2.423	43	2352	6.21	ug/l #	88
18) Methyl Acetate	2.746	43	475	0.43	ug/l #	47
20) Methylene Chloride	2.840	84	684	0.92	ug/l #	84
21) trans-1,2-Dichloroethene	3.146	96	801	1.20	ug/l	91
24) 1,1-Dichloroethane	3.676	63	4165	3.23	ug/l	98
25) 2-Butanone	4.652	43	832	1.45	ug/l #	89
27) cis-1,2-Dichloroethene	4.558	96	12879	16.63	ug/l	97
30) Chloroform	5.170	83	10934	8.03	ug/l	94
31) Cyclohexane	5.623	56	1703	1.55	ug/l #	43
36) 1,1-Dichloropropene	5.623	75	5684	5.19	ug/l #	48
38) Carbon Tetrachloride	5.623	117	6645	5.64	ug/l #	16
39) Methylcyclohexane	7.188	83	934	0.77	ug/l #	1
42) 1,2-Dichloroethane	6.158	62	3180	2.36	ug/l	84
44) Trichloroethene	7.188	130	70899	86.36	ug/l	96
47) Bromodichloromethane	7.882	83	583	0.47	ug/l #	90
48) Methyl methacrylate	7.741	41	768	0.70	ug/l #	75
49) 1,4-Dioxane	7.723	88	185	9.42	ug/l #	48
51) 4-Methyl-2-Pentanone	8.623	43	409	0.32	ug/l #	69
52) Toluene	8.765	92	293400	152.69	ug/l	99
53) t-1,3-Dichloropropene	8.765	75	3804	3.01	ug/l #	1
59) 2-Hexanone	9.470	43	194	0.20	ug/l #	19
64) Tetrachloroethene	9.318	164	184	0.24	ug/l #	67
68) m/p-Xylenes	10.335	106	443	0.30	ug/l	94
76) 1,2,3-Trichloropropane	11.118	75	31627	27.03	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.118	75	31627	82.33	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.788	105	1303	0.43	ug/l	77
95) Naphthalene	13.818	128	1763	0.54	ug/l #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021583.D
Acq On : 29 Mar 2021 17:36
Operator : JC/MD
Sample : M1860-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621

Quant Time: Mar 30 03:30:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration



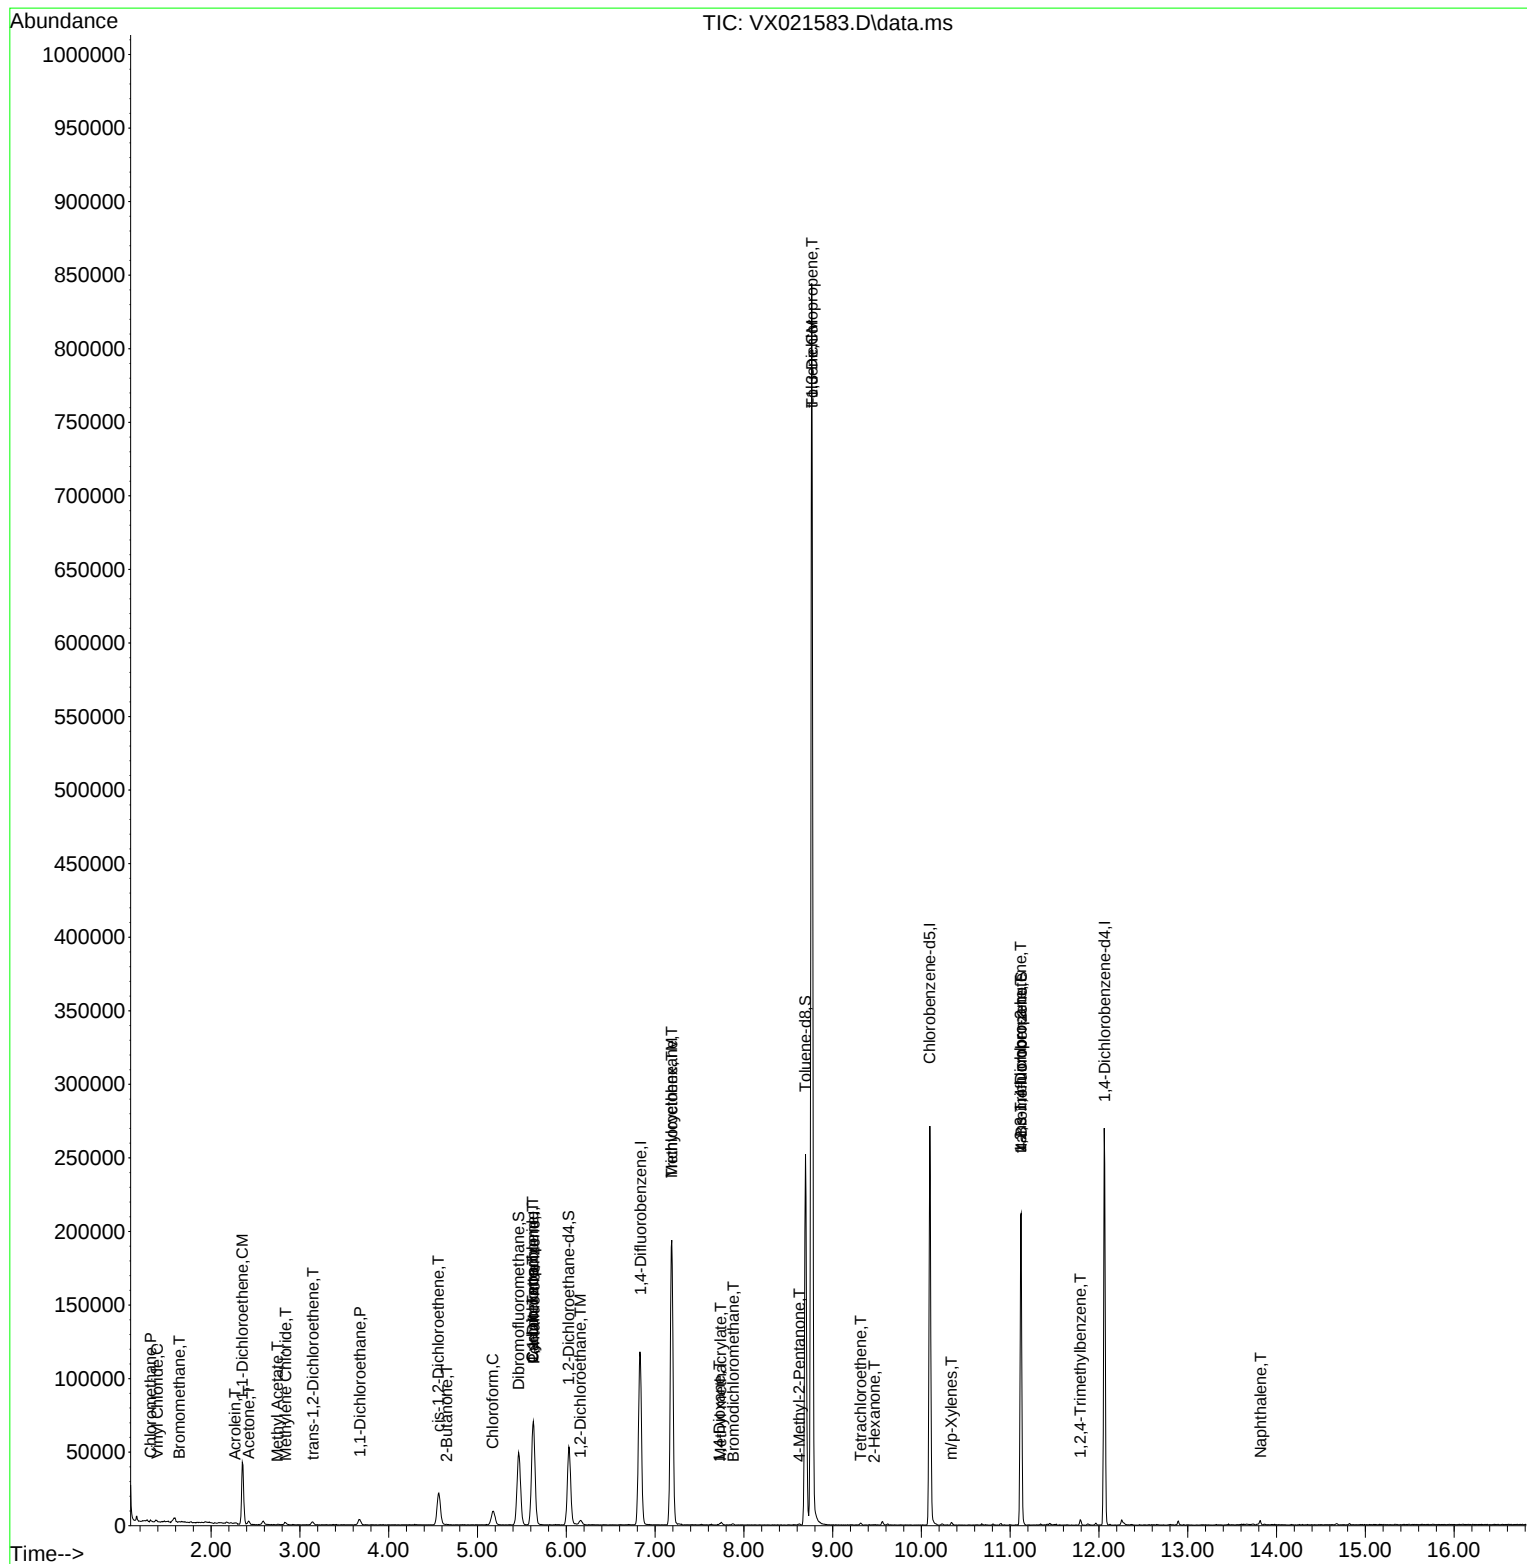




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.635 min Scan# 773
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion:168 Resp: 60239
Ion Ratio Lower Upper
168 100
99 59.6 45.8 68.6



#3
Chloromethane
Concen: 2.16 ug/l
RT: 1.317 min Scan# 39
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 50 Resp: 1617
Ion Ratio Lower Upper
50 100
52 30.3 26.4 39.6







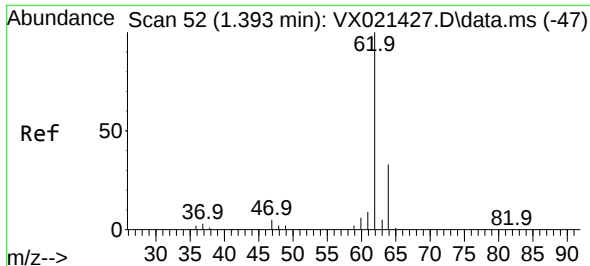

#4
 Vinyl Chloride
 Concen: 0.24 ug/l
 RT: 1.393 min Scan# 52
 Delta R.T. -0.000 min
 Lab File: VX021583.D
 Acq: 29 Mar 2021 17:36




Instrument :
 MSVOA_X
 ClientSampleId :
 GWBR3-115-137-032621


Tgt Ion: 62 Resp: 162
 Ion Ratio Lower Upper
 62 100
 64 47.9 25.7 38.5#

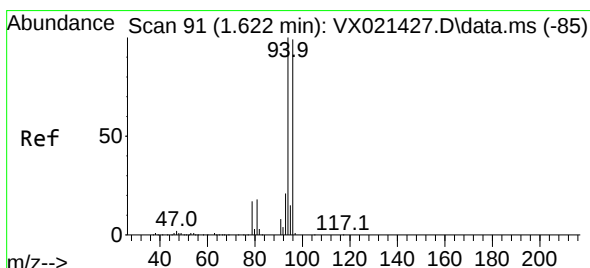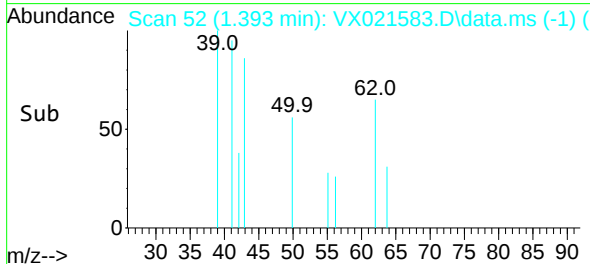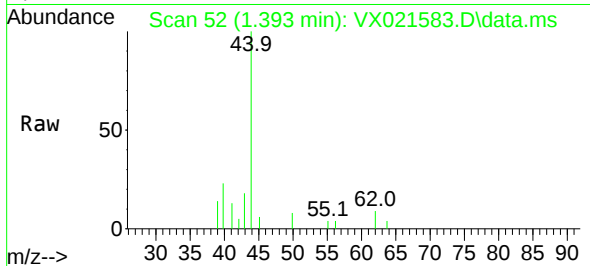

#5
 Bromomethane
 Concen: 0.48 ug/l
 RT: 1.640 min Scan# 94
 Delta R.T. 0.018 min
 Lab File: VX021583.D
 Acq: 29 Mar 2021 17:36

Tgt Ion: 94 Resp: 130
 Ion Ratio Lower Upper
 94 100
 96 103.5 76.4 114.6

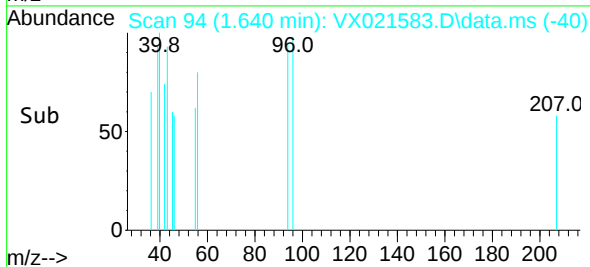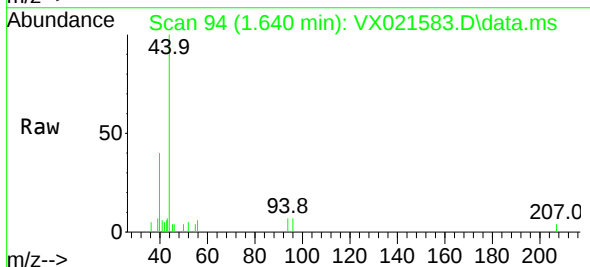



#12

1,1-Dichloroethene

Concen: 21.66 ug/l

RT: 2.352 min Scan# 215

Delta R.T. -0.000 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion: 96 Resp: 13147

Ion Ratio Lower Upper

96 100

61 167.8 124.6 187.0





98 61.7 50.6 76.0

Instrument :

MSVOA_X

ClientSampleId :

GWBR3-115-137-032621



#13

Acrolein

Concen: 4.51 ug/l

RT: 2.270 min Scan# 201

Delta R.T. -0.006 min

Lab File: VX021583.D




Acq: 29 Mar 2021 17:36

Tgt Ion: 56 Resp: 18

Ion Ratio Lower Upper

56 100

55 688.9 56.4 84.6#









#16
Acetone
Concen: 6.21 ug/l
RT: 2.423 min Scan# 227
Delta R.T. -0.000 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621

Tgt Ion: 43 Resp: 2352
Ion Ratio Lower Upper
43 100
58 27.7 27.8 41.8#



#18
Methyl Acetate
Concen: 0.43 ug/l
RT: 2.746 min Scan# 282
Delta R.T. -0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 43 Resp: 475
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#









#20
Methylene Chloride
Concen: 0.92 ug/l
RT: 2.840 min Scan# 298
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621

Tgt Ion: 84 Resp: 684




Ion	Ratio	Lower	Upper
84	100		
49	94.8	88.6	132.8
51	30.4	27.0	40.6
86	45.9	50.3	75.5#

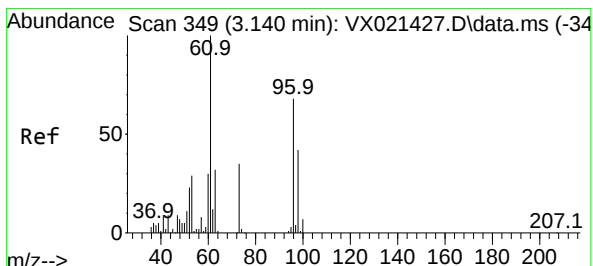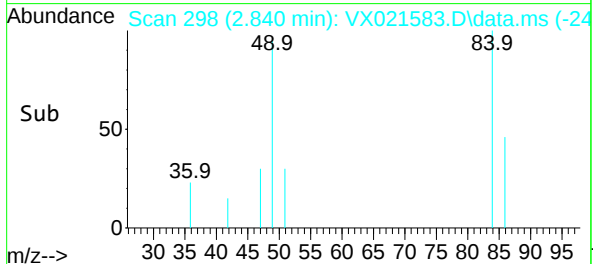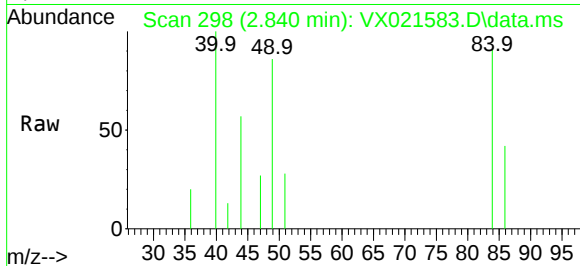


#21
trans-1,2-Dichloroethene
Concen: 1.20 ug/l
RT: 3.146 min Scan# 350
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 96 Resp: 801

Ion	Ratio	Lower	Upper
96	100		
61	149.1	107.7	161.5
98	63.8	50.4	75.6


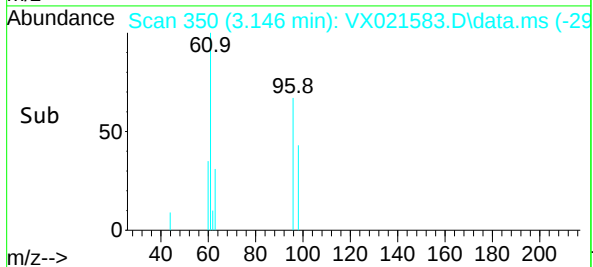

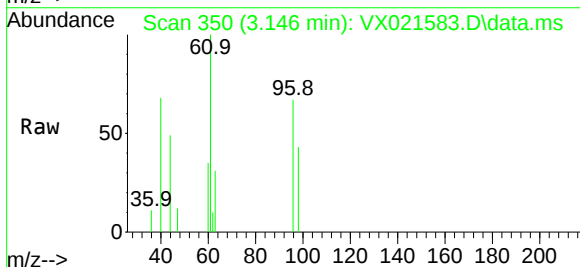


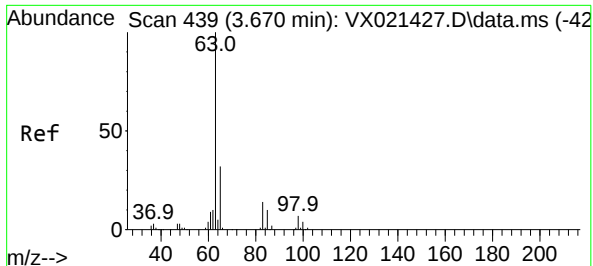

#24
1,1-Dichloroethane
Concen: 3.23 ug/l
RT: 3.676 min Scan# 440
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion: 63	Resp: 4165
Ion Ratio	Lower Upper
63 100	
98 8.0	3.8 11.2
100 4.3	2.5 7.5

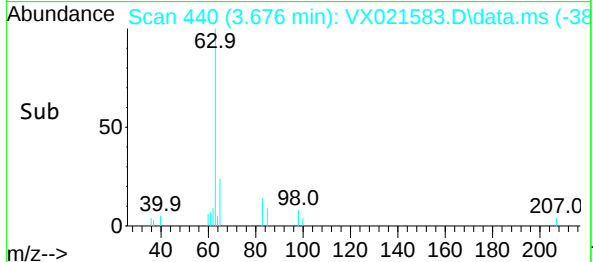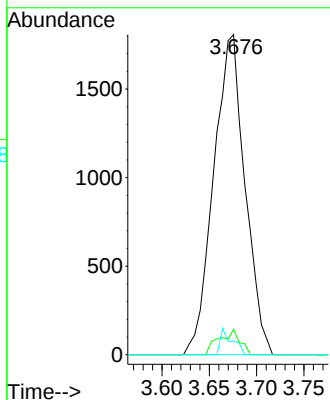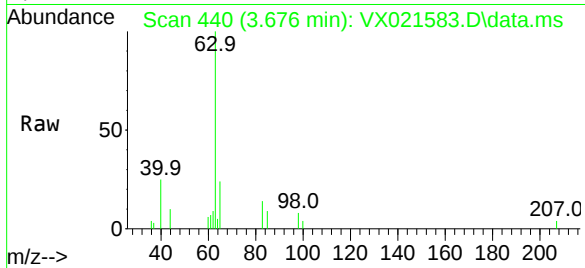

#25
2-Butanone
Concen: 1.45 ug/l
RT: 4.652 min Scan# 606
Delta R.T. 0.017 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 43	Resp: 832
Ion Ratio	Lower Upper
43 100	
72 23.5	23.7 35.5#

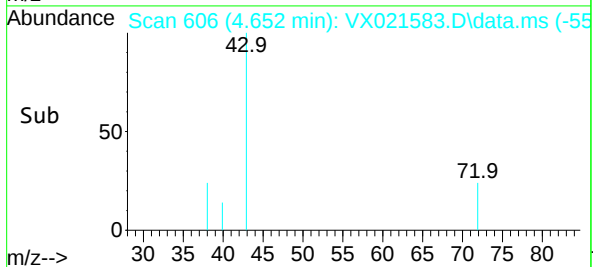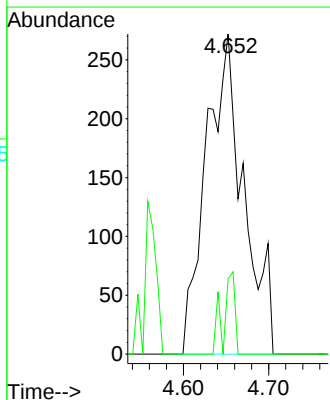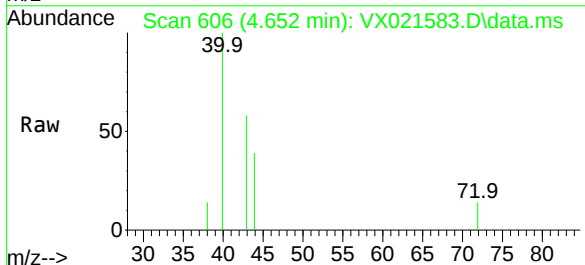



#27

cis-1,2-Dichloroethene

Concen: 16.63 ug/l

RT: 4.558 min Scan# 590

Delta R.T. 0.000 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion: 96 Resp: 12879





Ion	Ratio	Lower	Upper
96	100		
61	137.1	0.0	285.6
98	64.4	0.0	129.6

Instrument :

MSVOA_X

ClientSampleId :

GWBR3-115-137-032621

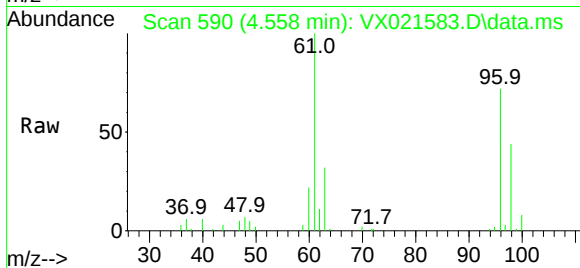

#30

Chloroform

Concen: 8.03 ug/l

RT: 5.170 min Scan# 694




Delta R.T. -0.006 min


Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion: 83 Resp: 10934


Ion	Ratio	Lower	Upper
83	100		
85	60.4	52.0	78.0

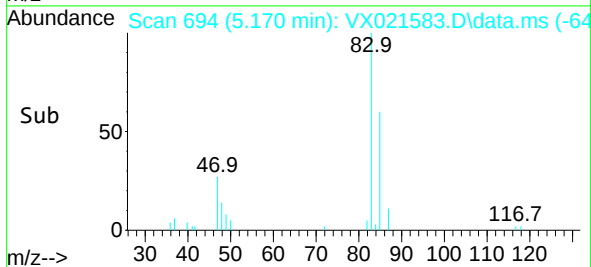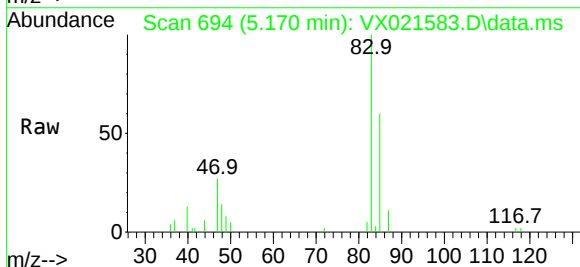






#31
Cyclohexane
Concen: 1.55 ug/l
RT: 5.623 min Scan# 771
Delta R.T. 0.076 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621







Tgt Ion: 56 Resp: 1703
Ion Ratio Lower Upper
56 100
69 148.8 25.3 37.9#
84 91.3 71.4 107.0



#33
1,2-Dichloroethane-d4
Concen: 52.00 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 65 Resp: 52124
Ion Ratio Lower Upper
65 100
67 50.0 0.0 105.4

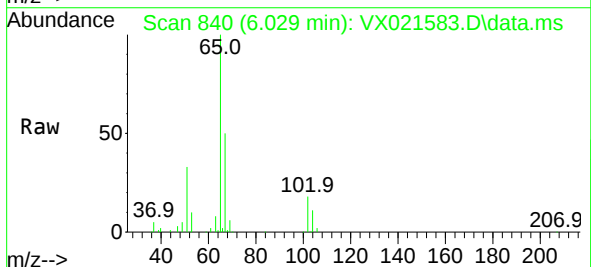

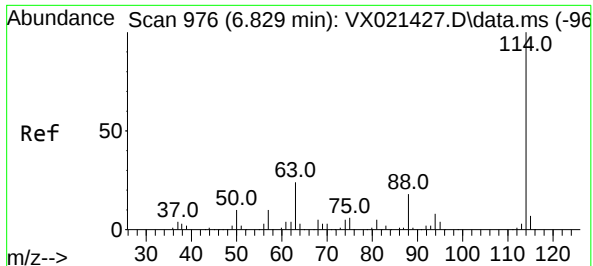

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.835 min Scan# 977

Delta R.T. 0.006 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36





Tgt Ion:114 Resp: 111811

Ion Ratio Lower Upper

114 100

63 22.5 0.0 40.8

88 16.3 0.0 32.8

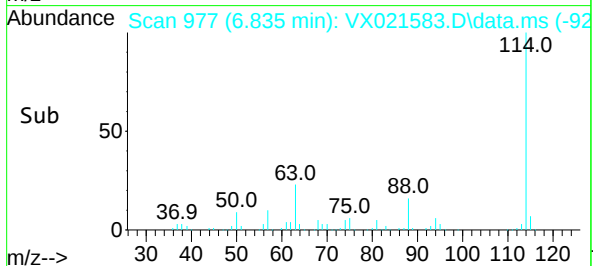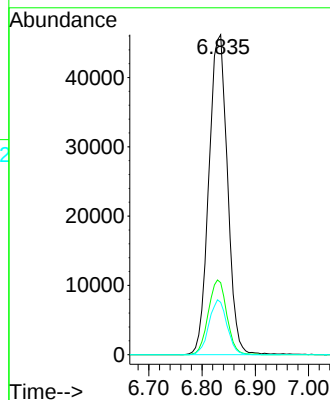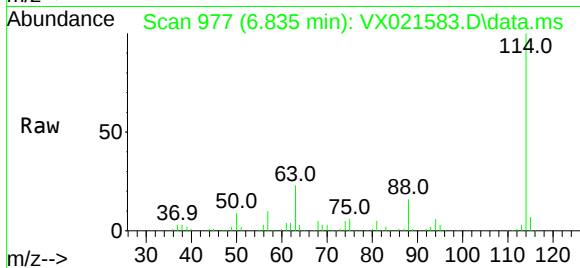

#35

Dibromofluoromethane

Concen: 50.19 ug/l

RT: 5.464 min Scan# 744

Delta R.T. 0.000 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36




Tgt Ion:113 Resp: 39865


Ion Ratio Lower Upper

113 100

111 103.7 81.9 122.9

192 19.4 16.7 25.1

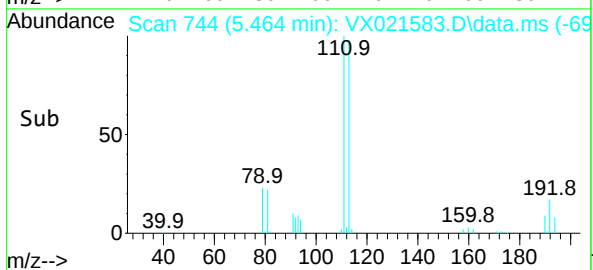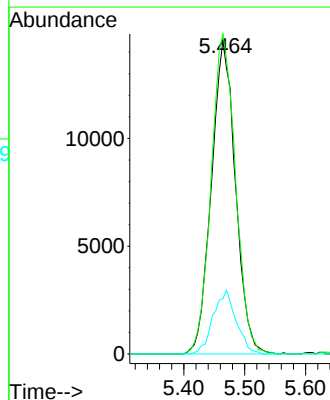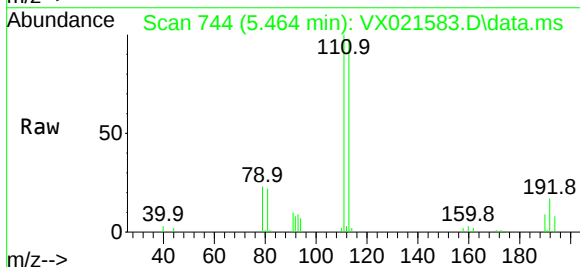

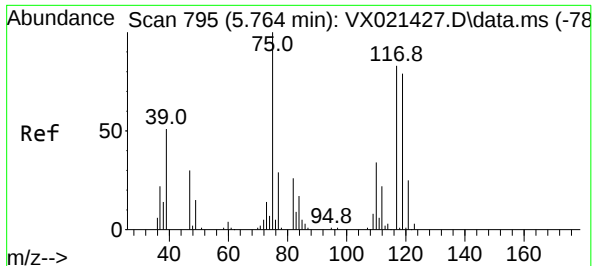

#36

1,1-Dichloropropene

Concen: 5.19 ug/l

RT: 5.623 min Scan# 771

Delta R.T. -0.141 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36





Tgt Ion:	75	Resp:	5684
Ion	Ratio	Lower	Upper
75	100		
110	8.4	18.1	54.4#
77	0.0	25.3	37.9#

Instrument :

MSVOA_X

ClientSampleId :

GWBR3-115-137-032621

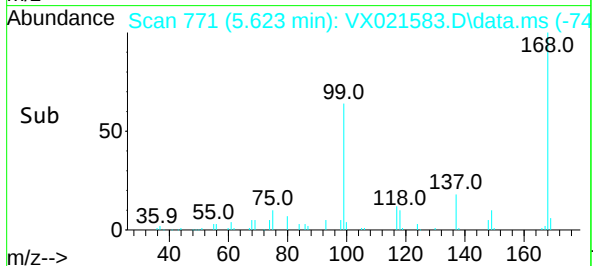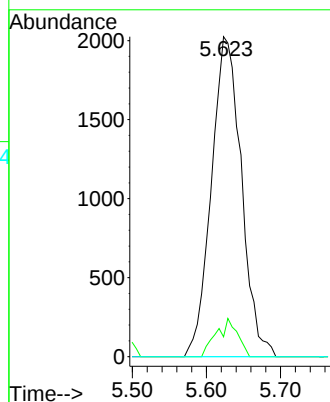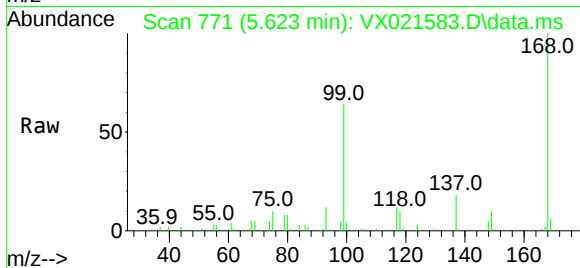

#38

Carbon Tetrachloride

Concen: 5.64 ug/l




RT: 5.623 min Scan# 771


Delta R.T. -0.129 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion:	117	Resp:	6645
Ion	Ratio	Lower	Upper
117	100		
119	5.0	76.2	114.2#
121	0.0	24.8	37.2#

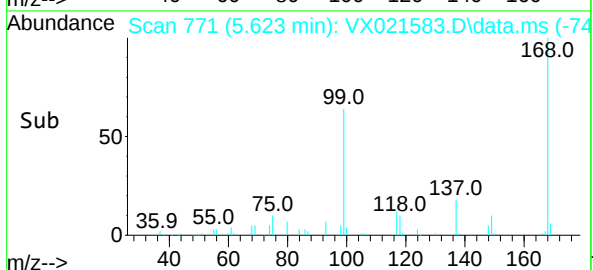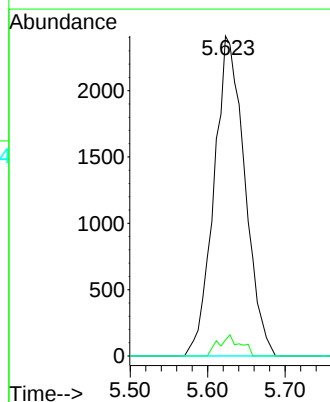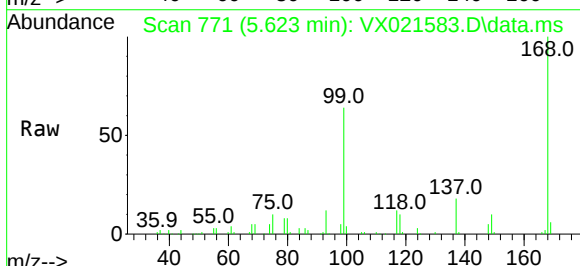



#39

Methylcyclohexane

Concen: 0.77 ug/l

RT: 7.188 min Scan# 1037

Delta R.T. -0.247 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36





Instrument :

MSVOA_X

ClientSampleId :

GWBR3-115-137-032621

Tgt Ion:	83	Resp:	934
Ion	Ratio	Lower	Upper
83	100		
55	0.0	58.9	88.3#
98	195.8	38.1	57.1#



#42

1,2-Dichloroethane

Concen: 2.36 ug/l




RT: 6.158 min Scan# 862


Delta R.T. 0.000 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion:	62	Resp:	3180
Ion	Ratio	Lower	Upper
62	100		
98	4.0	0.0	20.2





#44

Trichloroethene

Concen: 86.36 ug/l

RT: 7.188 min Scan# 1037

Delta R.T. -0.000 min





Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion:130 Resp: 70899

Ion Ratio Lower Upper

130	100		
95	103.2	0.0	198.0

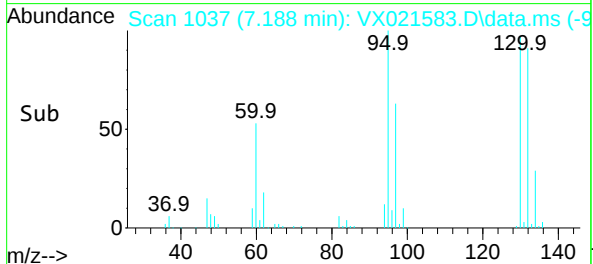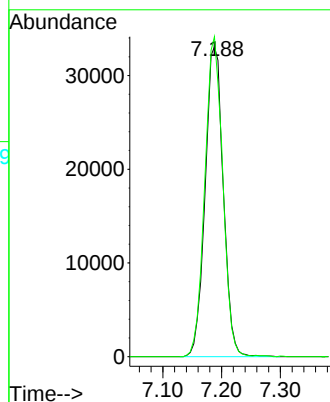

#47

Bromodichloromethane

Concen: 0.47 ug/l

RT: 7.882 min Scan# 1155

Delta R.T. 0.006 min




Lab File: VX021583.D


Acq: 29 Mar 2021 17:36

Tgt Ion: 83 Resp: 583

Ion Ratio Lower Upper

83	100		
85	57.9	51.4	77.0
127	0.0	6.8	10.2

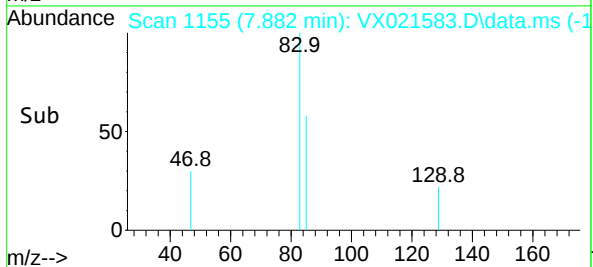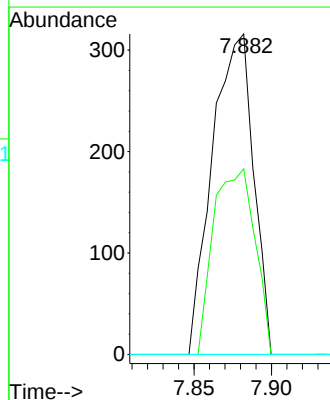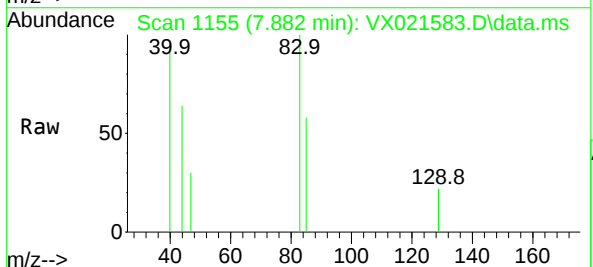

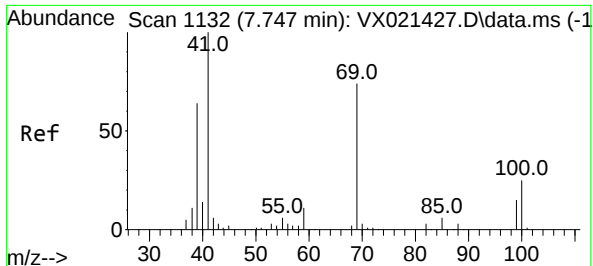

#48

Methyl methacrylate

Concen: 0.70 ug/l

RT: 7.741 min Scan# 1131

Delta R.T. -0.006 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion: 41 Resp: 768

Ion Ratio Lower Upper

41 100

69 76.6 76.0 114.0





39 82.3 44.6 67.0#

Instrument :

MSVOA_X

ClientSampleId :

GWBR3-115-137-032621

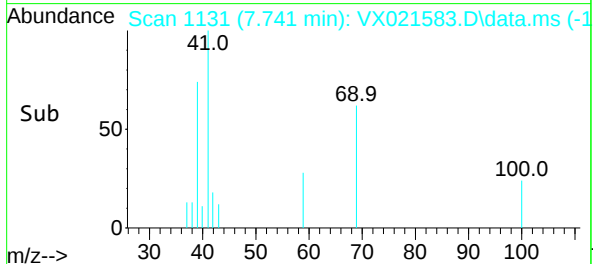

#49

1,4-Dioxane

Concen: 9.42 ug/l

RT: 7.723 min Scan# 1128

Delta R.T. 0.011 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36




Tgt Ion: 88 Resp: 185


Ion Ratio Lower Upper

88 100

43 105.9 23.2 34.8#

58 57.8 55.0 82.4


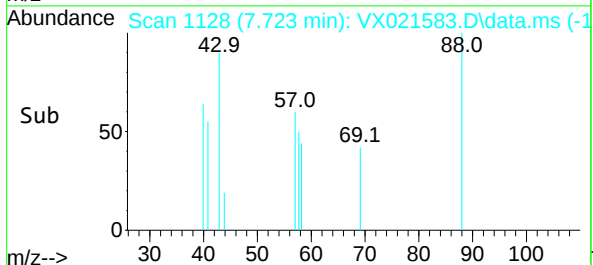

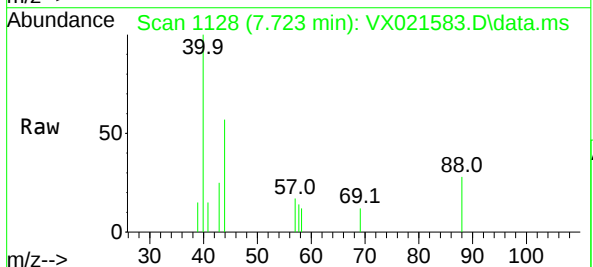


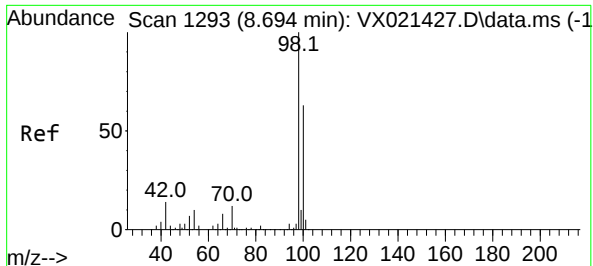

#50
Toluene-d8
Concen: 49.63 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion: 98 Resp: 140473
Ion Ratio Lower Upper
98 100
100 64.8 51.9 77.9

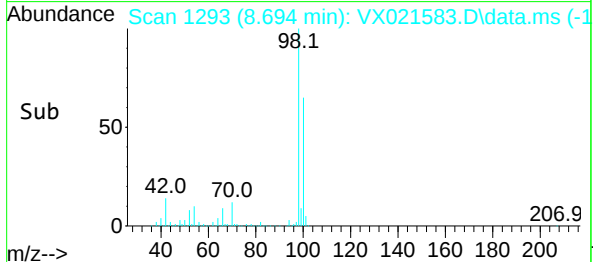

#51
4-Methyl-2-Pentanone
Concen: 0.32 ug/l
RT: 8.623 min Scan# 1281
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 43 Resp: 409
Ion Ratio Lower Upper
43 100
58 24.0 35.4 53.0#


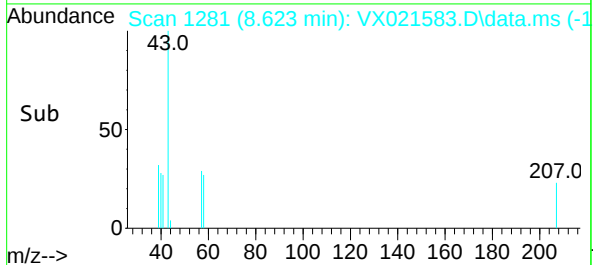

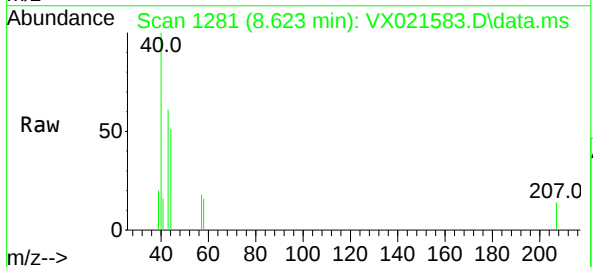




#52
Toluene
Concen: 152.69 ug/l
RT: 8.765 min Scan# 1305
Delta R.T. -0.000 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion: 92 Resp: 293400
Ion Ratio Lower Upper
92 100
91 173.3 137.1 205.7



#53
t-1,3-Dichloropropene
Concen: 3.01 ug/l
RT: 8.765 min Scan# 1305
Delta R.T. -0.258 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 75 Resp: 3804
Ion Ratio Lower Upper
75 100
77 168.8 24.9 37.3#







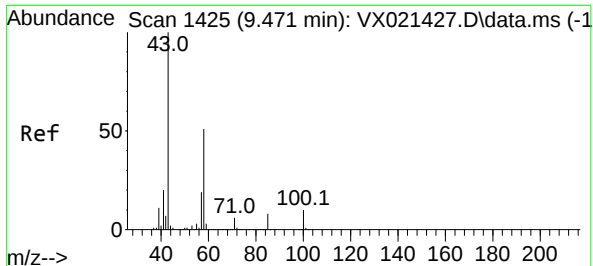

#59
2-Hexanone
Concen: 0.20 ug/l
RT: 9.470 min Scan# 1425
Delta R.T. -0.001 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion: 43 Resp: 194
Ion Ratio Lower Upper
43 100
58 0.0 30.9 92.8#

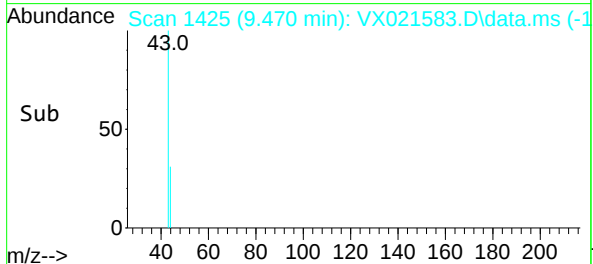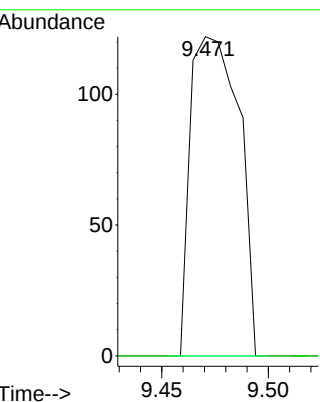

#62
4-Bromofluorobenzene
Concen: 50.87 ug/l
RT: 11.124 min Scan# 1706
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 95 Resp: 55973
Ion Ratio Lower Upper
95 100
174 73.7 0.0 154.6
176 71.5 0.0 155.8


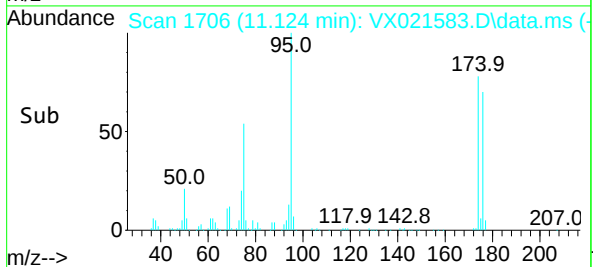
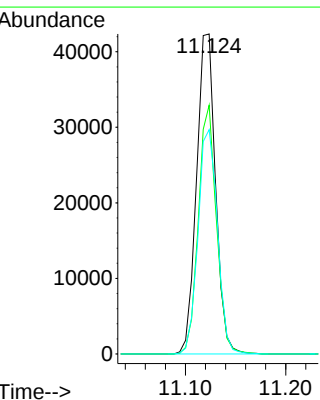
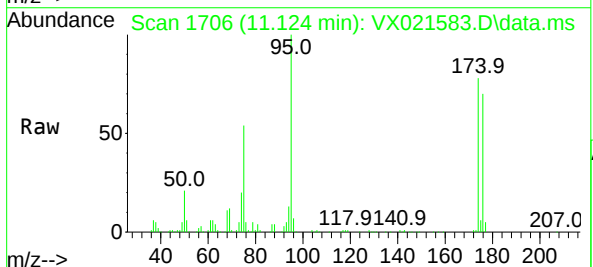




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion:117 Resp: 114460
Ion Ratio Lower Upper
117 100
82 60.3 47.4 71.2
119 31.7 26.6 39.8



#64
Tetrachloroethene
Concen: 0.24 ug/l
RT: 9.318 min Scan# 1399
Delta R.T. -0.000 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion:164 Resp: 184
Ion Ratio Lower Upper
164 100
166 174.6 103.4 155.2#
129 117.6 70.8 106.2#
131 114.1 72.5 108.7#




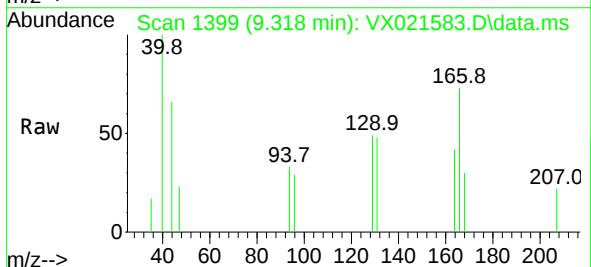




#68
m/p-Xylenes
Concen: 0.30 ug/l
RT: 10.335 min Scan# 1572
Delta R.T. -0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion:106 Resp: 443
Ion Ratio Lower Upper
106 100
91 194.4 162.8 244.2

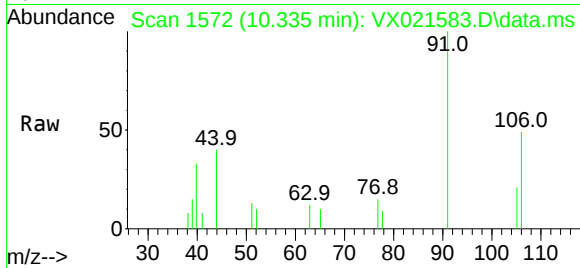

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.065 min Scan# 1866
Delta R.T. 0.006 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion:152 Resp: 50262
Ion Ratio Lower Upper
152 100
115 63.8 41.1 123.3
150 156.5 0.0 349.0




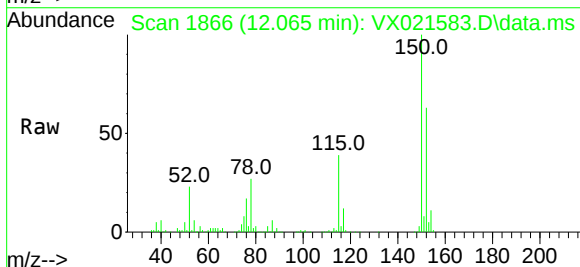




#76
1,2,3-Trichloropropane
Concen: 27.03 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36




Instrument :
MSVOA_X
ClientSampleId :
GWBR3-115-137-032621


Tgt Ion: 75 Resp: 31627
Ion Ratio Lower Upper
75 100
77 1.0 19.1 57.5#

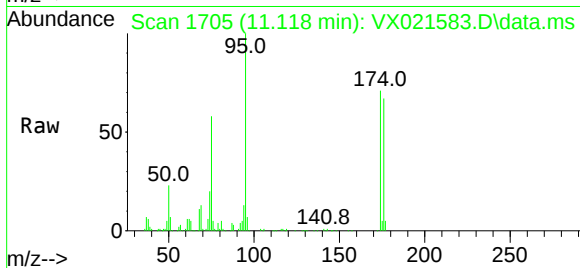

#81
trans-1,4-Dichloro-2-butene
Concen: 82.33 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021583.D
Acq: 29 Mar 2021 17:36

Tgt Ion: 75 Resp: 31627
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

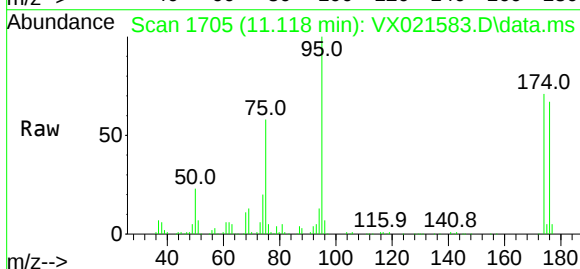



#84

1,2,4-Trimethylbenzene

Concen: 0.43 ug/l

RT: 11.788 min Scan# 1819

Delta R.T. -0.001 min

Lab File: VX021583.D





Acq: 29 Mar 2021 17:36

Tgt Ion:105 Resp: 1303

Ion Ratio Lower Upper

105 100

120 29.9 22.4 67.3

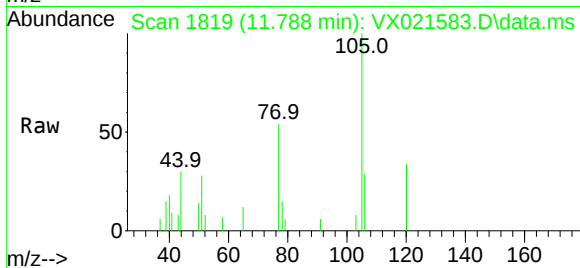

#95

Naphthalene

Concen: 0.54 ug/l

RT: 13.818 min Scan# 2164

Delta R.T. 0.000 min

Lab File: VX021583.D

Acq: 29 Mar 2021 17:36

Tgt Ion:128 Resp: 1763

Ion Ratio Lower Upper

128 100

127 14.1 10.3 15.5

129 8.2 8.8 13.2#

