

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021570.D
 Acq On : 29 Mar 2021 12:32
 Operator : JC/MD
 Sample : M1787-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP03-20210319

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	209	217	232	rVB	156556	299123	30.38%	8.589%
2	5.464	733	744	758	rBV	47082	135790	13.79%	3.899%
3	5.629	760	772	785	rVB	69419	191046	19.40%	5.485%
4	6.029	829	840	853	rBV	52363	136919	13.91%	3.931%
5	6.829	964	976	989	rBV	115451	278548	28.29%	7.998%
6	7.188	1027	1037	1054	rBV	463734	984672	100.00%	28.272%
7	8.694	1285	1293	1308	rBV	244809	390485	39.66%	11.212%
8	9.318	1393	1399	1405	rBV	31518	45986	4.67%	1.320%
9	10.094	1525	1531	1546	rVB	274129	375385	38.12%	10.778%
10	11.118	1700	1705	1714	rBV	228608	293685	29.83%	8.432%
11	12.059	1860	1865	1872	rBV	281333	351162	35.66%	10.083%




Sum of corrected areas: 3482801

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021570.D
Acq On : 29 Mar 2021 12:32
Operator : JC/MD
Sample : M1787-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

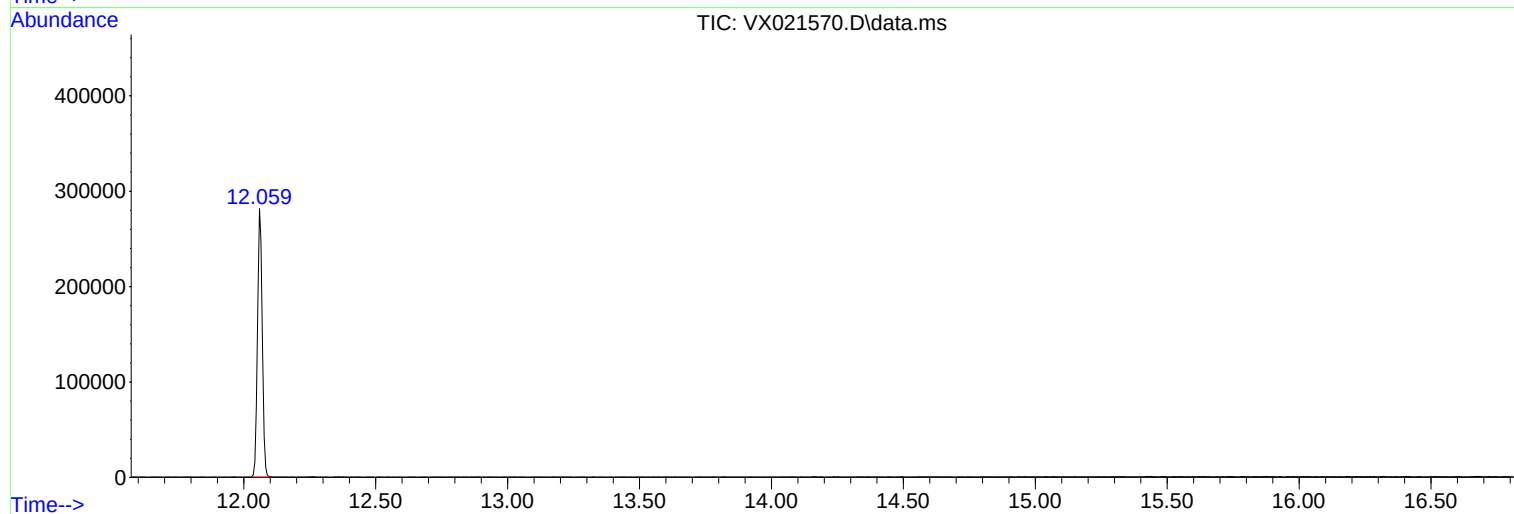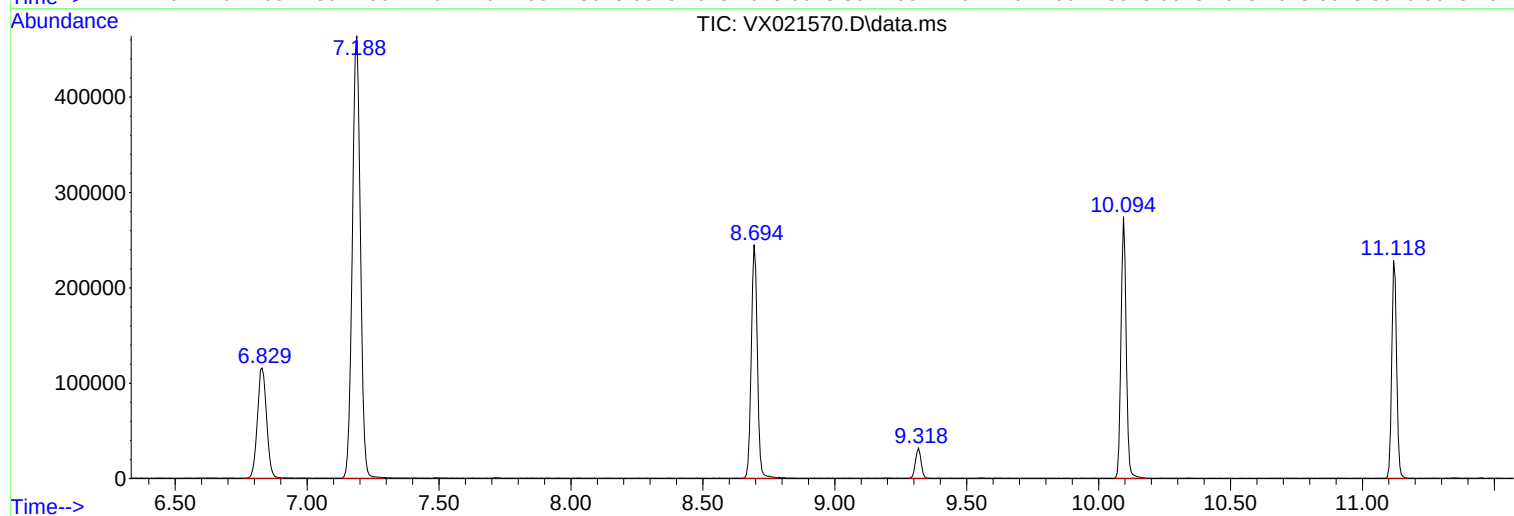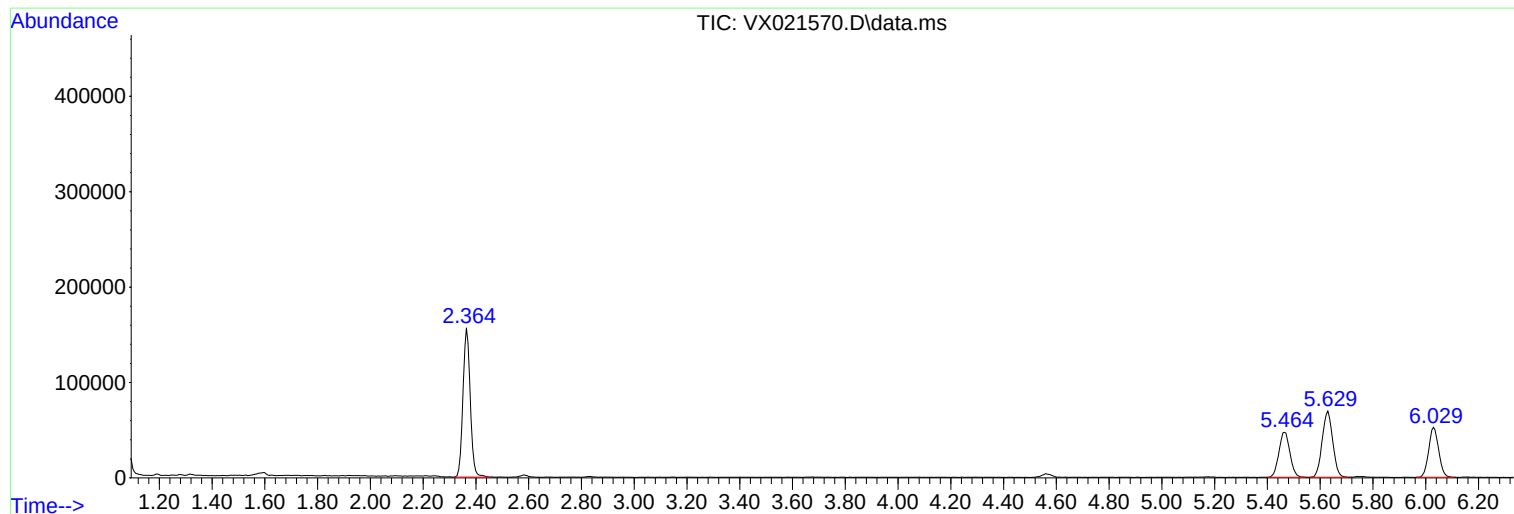

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021570.D
Acq On : 29 Mar 2021 12:32
Operator : JC/MD
Sample : M1787-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021570.D
Acq On : 29 Mar 2021 12:32
Operator : JC/MD
Sample : M1787-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20210319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
