

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021598.D
 Acq On : 30 Mar 2021 00:17
 Operator : JC/MD
 Sample : M1843-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW178I-20210324

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	77	87	90	rVB4	3169	6779	1.79%	0.332%
2	3.164	346	353	360	rBV3	2343	5282	1.39%	0.259%
3	5.464	732	744	756	rBV	48580	135600	35.80%	6.649%
4	5.629	760	772	785	rVV	68093	189149	49.94%	9.275%
5	6.029	829	840	855	rVB2	51453	134865	35.61%	6.613%
6	6.829	966	976	989	rBV	116943	274304	72.43%	13.451%
7	7.188	1031	1037	1046	rVB3	2518	5188	1.37%	0.254%
8	8.694	1286	1293	1308	rBV	241546	378741	100.00%	18.572%
9	10.094	1525	1531	1547	rVB	256703	351525	92.81%	17.238%
10	11.118	1699	1705	1715	rBV	206336	263901	69.68%	12.941%
11	12.059	1860	1865	1872	rVB	235538	293963	77.62%	14.415%




Sum of corrected areas: 2039297

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021598.D
Acq On : 30 Mar 2021 00:17
Operator : JC/MD
Sample : M1843-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

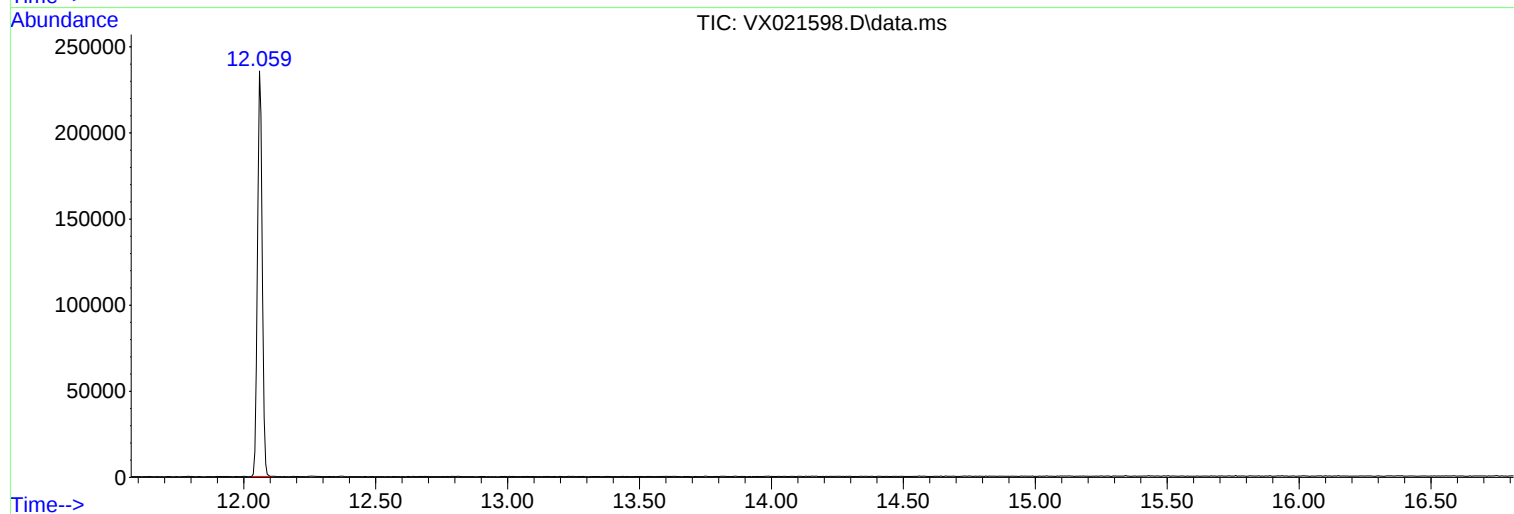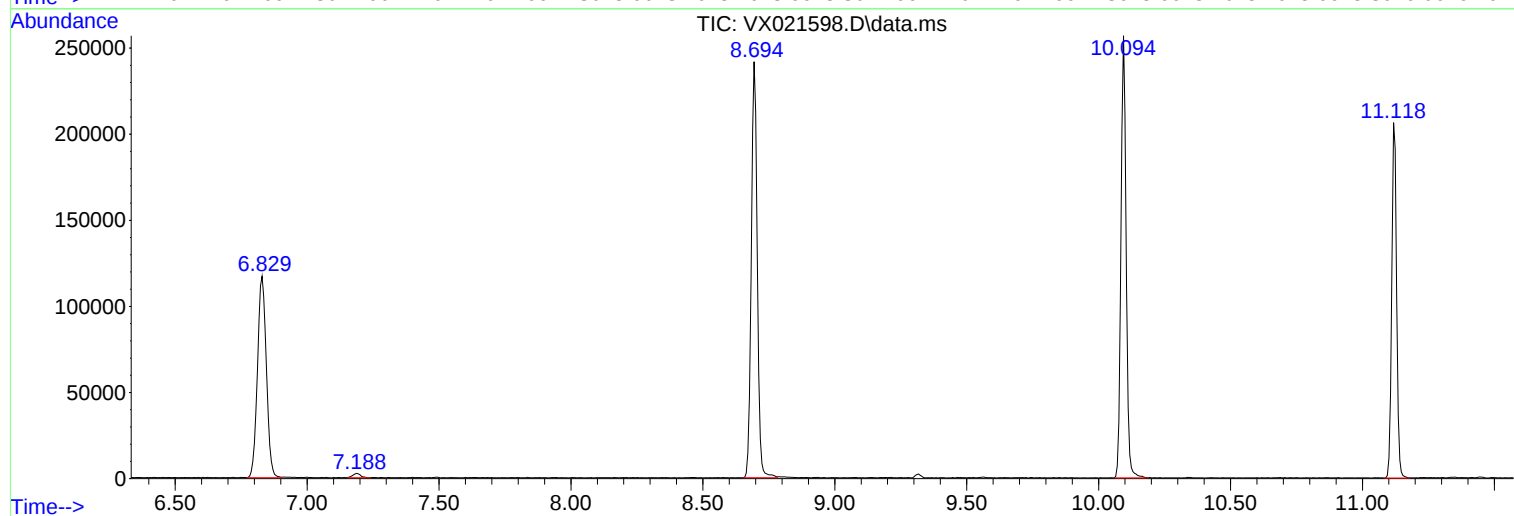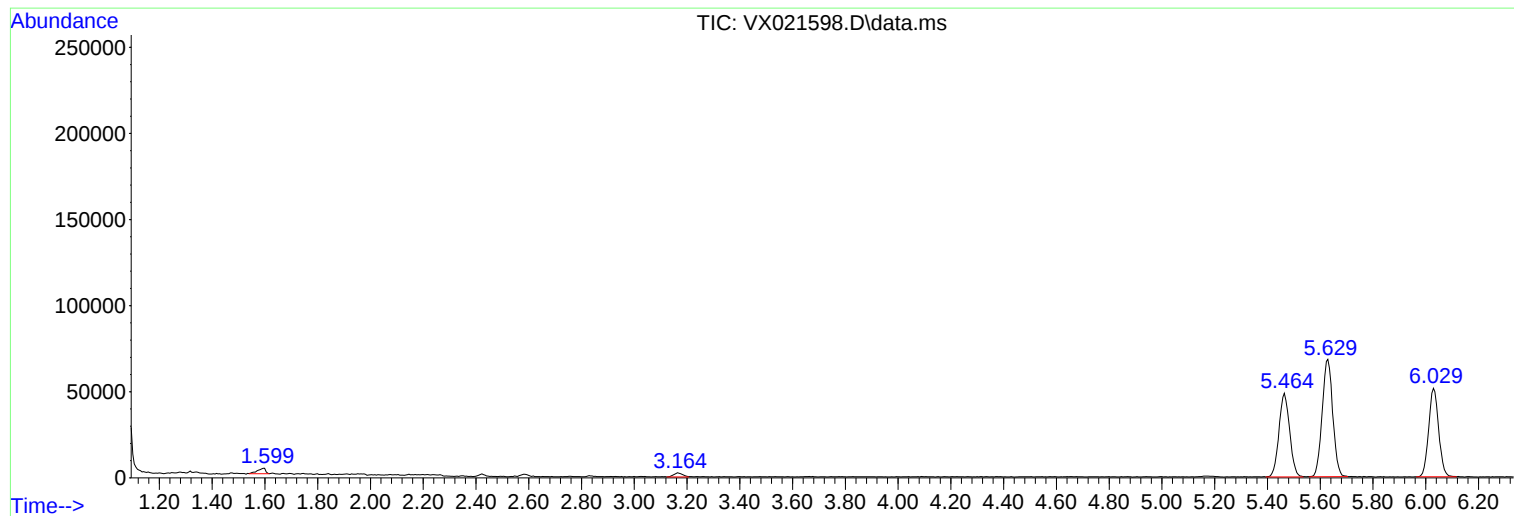

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021598.D
Acq On : 30 Mar 2021 00:17
Operator : JC/MD
Sample : M1843-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021598.D
Acq On : 30 Mar 2021 00:17
Operator : JC/MD
Sample : M1843-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
