

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021604.D
 Acq On : 30 Mar 2021 02:37
 Operator : JC/MD
 Sample : M1843-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP07-20210324

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.358	210	216	223	rBV2	15690	28625	3.49%	0.983%
2	2.581	247	254	263	rBV	4626	9209	1.12%	0.316%
3	5.464	732	744	760	rBV	46418	130310	15.90%	4.473%
4	5.629	760	772	786	rBV	65405	181448	22.15%	6.228%
5	6.029	826	840	855	rBV	50474	132135	16.13%	4.535%
6	6.829	965	976	991	rBV	111439	262441	32.03%	9.008%
7	7.188	1026	1037	1049	rBV	386218	819356	100.00%	28.124%
8	8.694	1286	1293	1306	rBV	241794	371554	45.35%	12.753%
9	10.094	1525	1531	1548	rVB	264623	360880	44.04%	12.387%
10	11.118	1699	1705	1716	rBV	223198	279887	34.16%	9.607%
11	12.059	1859	1865	1873	rBV	280711	337563	41.20%	11.587%




Sum of corrected areas: 2913408

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021604.D
Acq On : 30 Mar 2021 02:37
Operator : JC/MD
Sample : M1843-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP07-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

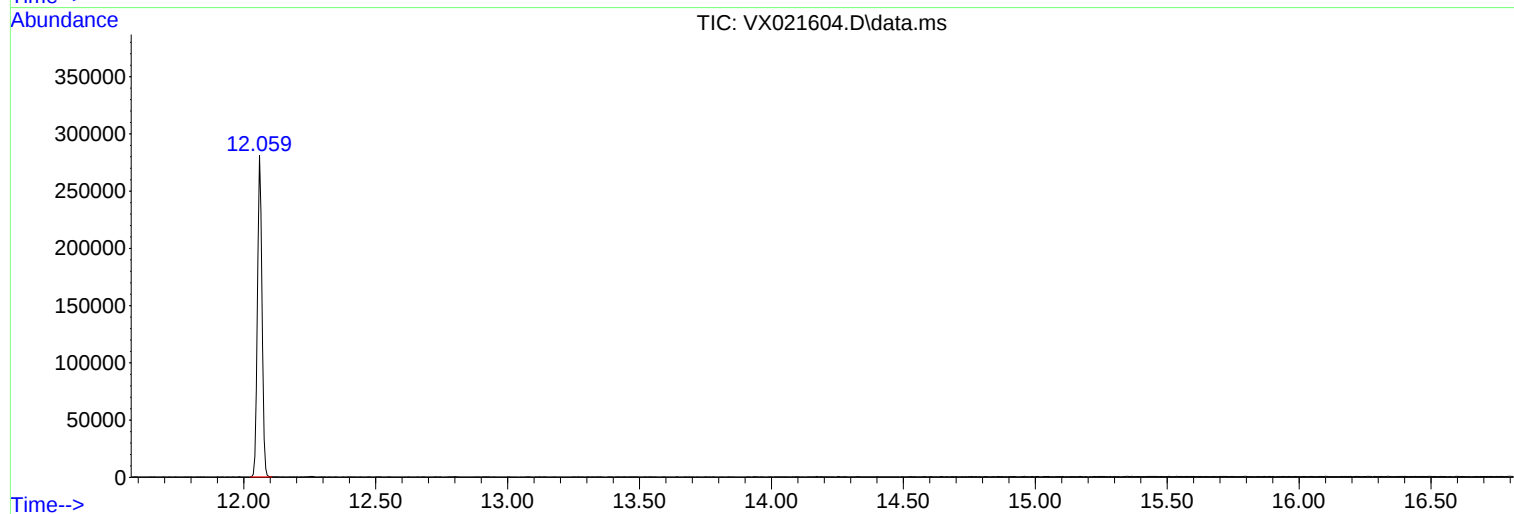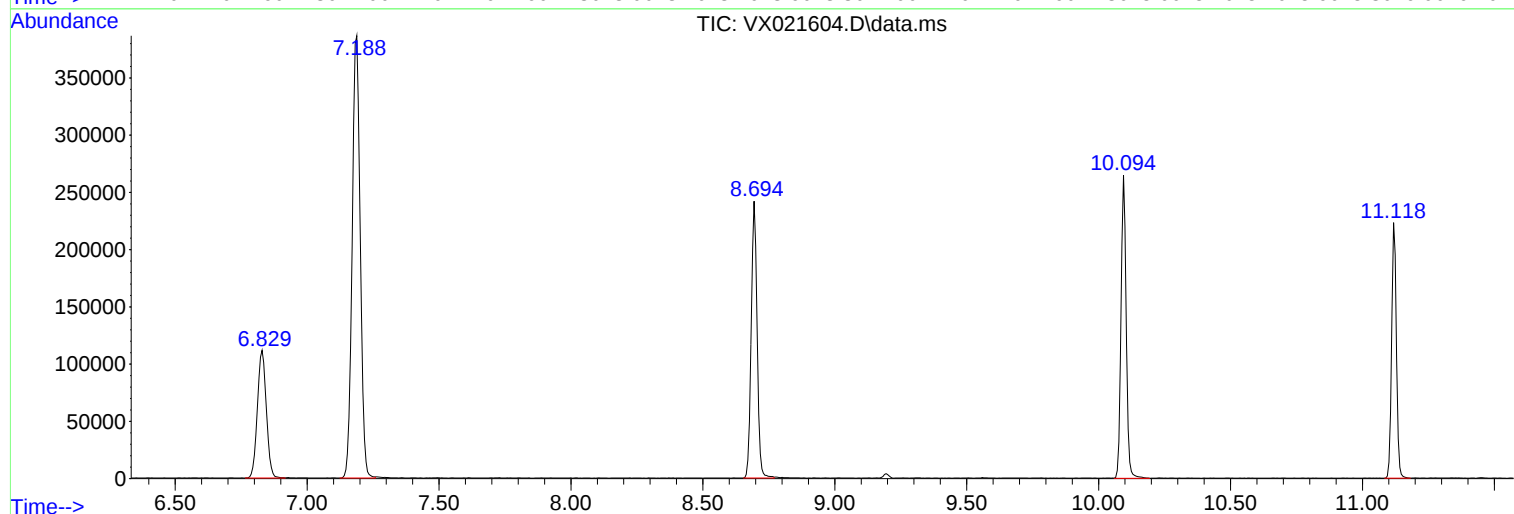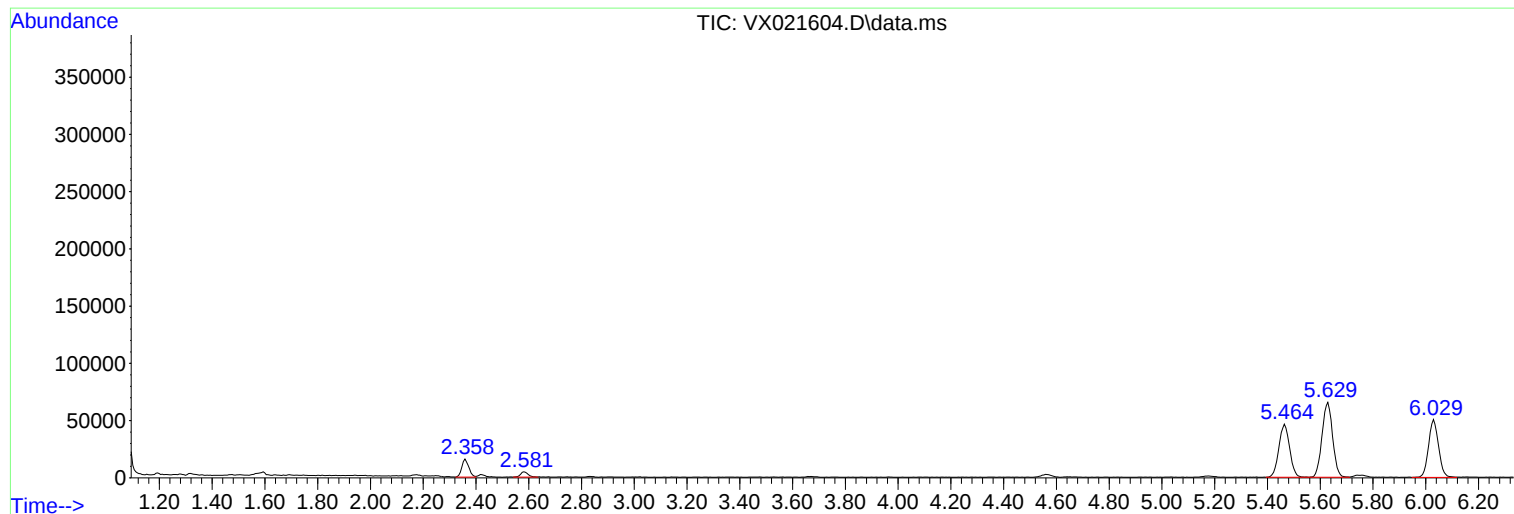

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021604.D
Acq On : 30 Mar 2021 02:37
Operator : JC/MD
Sample : M1843-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP07-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021604.D
Acq On : 30 Mar 2021 02:37
Operator : JC/MD
Sample : M1843-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP07-20210324

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
