

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021605.D
 Acq On : 30 Mar 2021 03:01
 Operator : JC/MD
 Sample : M1843-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE117D2-20210325

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	77	86	89	rBV5	2622	5540	1.44%	0.265%
2	2.582	242	254	262	rVB	3323	6615	1.72%	0.317%
3	5.464	731	744	759	rBV2	48925	137747	35.82%	6.601%
4	5.629	761	772	785	rVV3	67938	192578	50.07%	9.229%
5	6.029	830	840	855	rBV2	52177	137263	35.69%	6.578%
6	6.829	966	976	989	rBV	118282	278621	72.45%	13.352%
7	7.188	1031	1037	1047	rBV4	2656	5415	1.41%	0.259%
8	8.694	1286	1293	1309	rBV	247681	384586	100.00%	18.430%
9	10.094	1525	1531	1548	rVB	267777	360486	93.73%	17.275%
10	11.118	1699	1705	1717	rBV	214404	271044	70.48%	12.989%
11	12.059	1859	1865	1875	rVB	262568	306872	79.79%	14.706%




Sum of corrected areas: 2086767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021605.D
Acq On : 30 Mar 2021 03:01
Operator : JC/MD
Sample : M1843-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

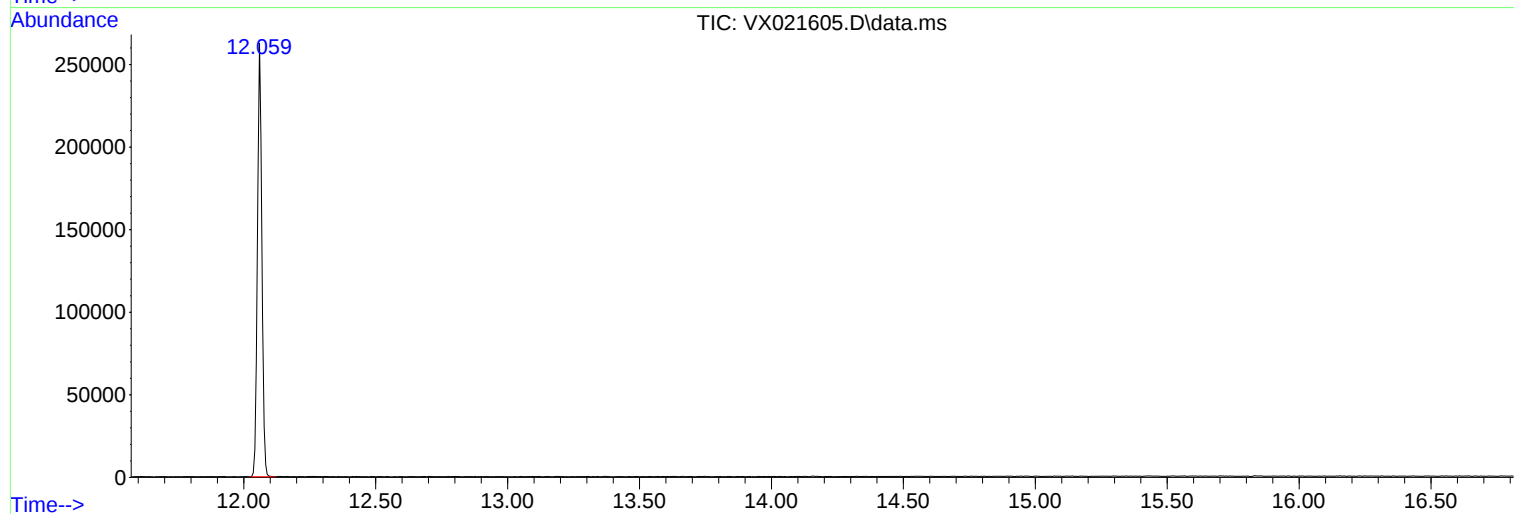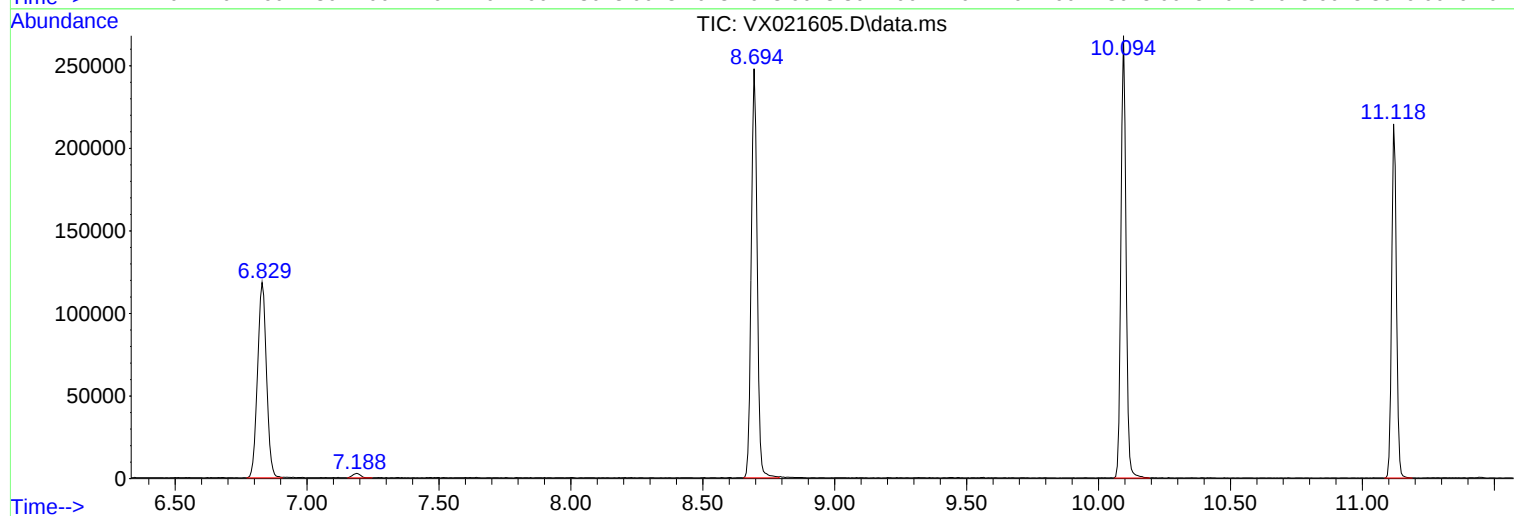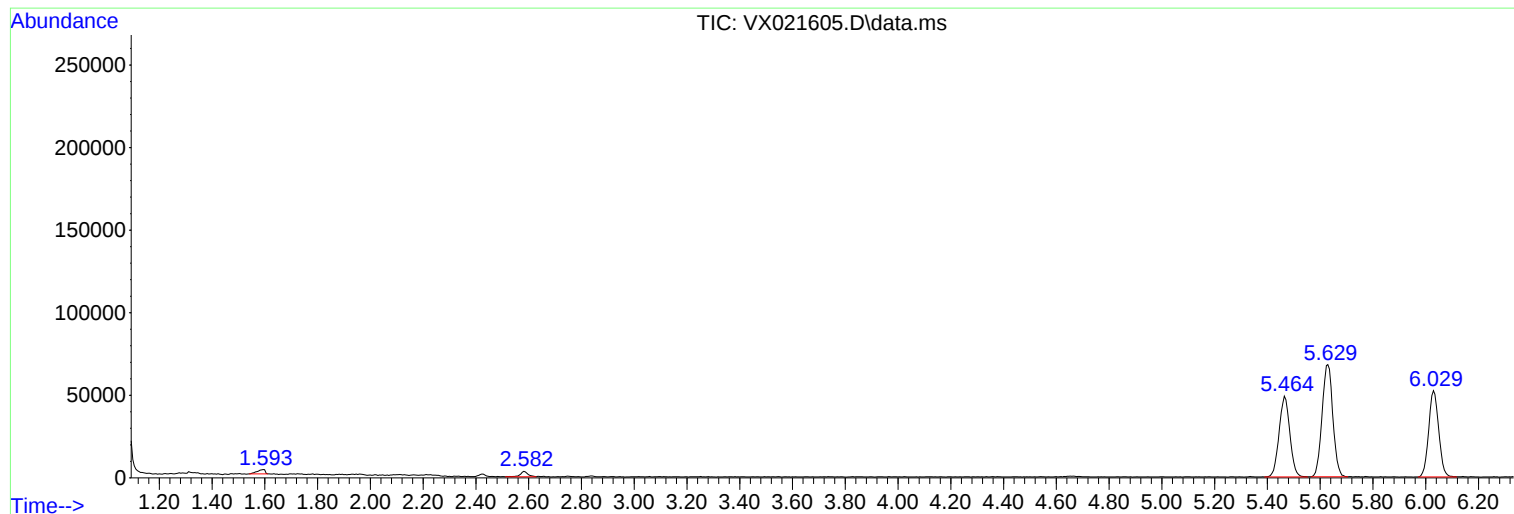

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021605.D
Acq On : 30 Mar 2021 03:01
Operator : JC/MD
Sample : M1843-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021605.D
Acq On : 30 Mar 2021 03:01
Operator : JC/MD
Sample : M1843-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
