


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021592.D
 Acq On : 29 Mar 2021 21:08
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260
 Last Update : Wed Mar 24 12:25:26 2021

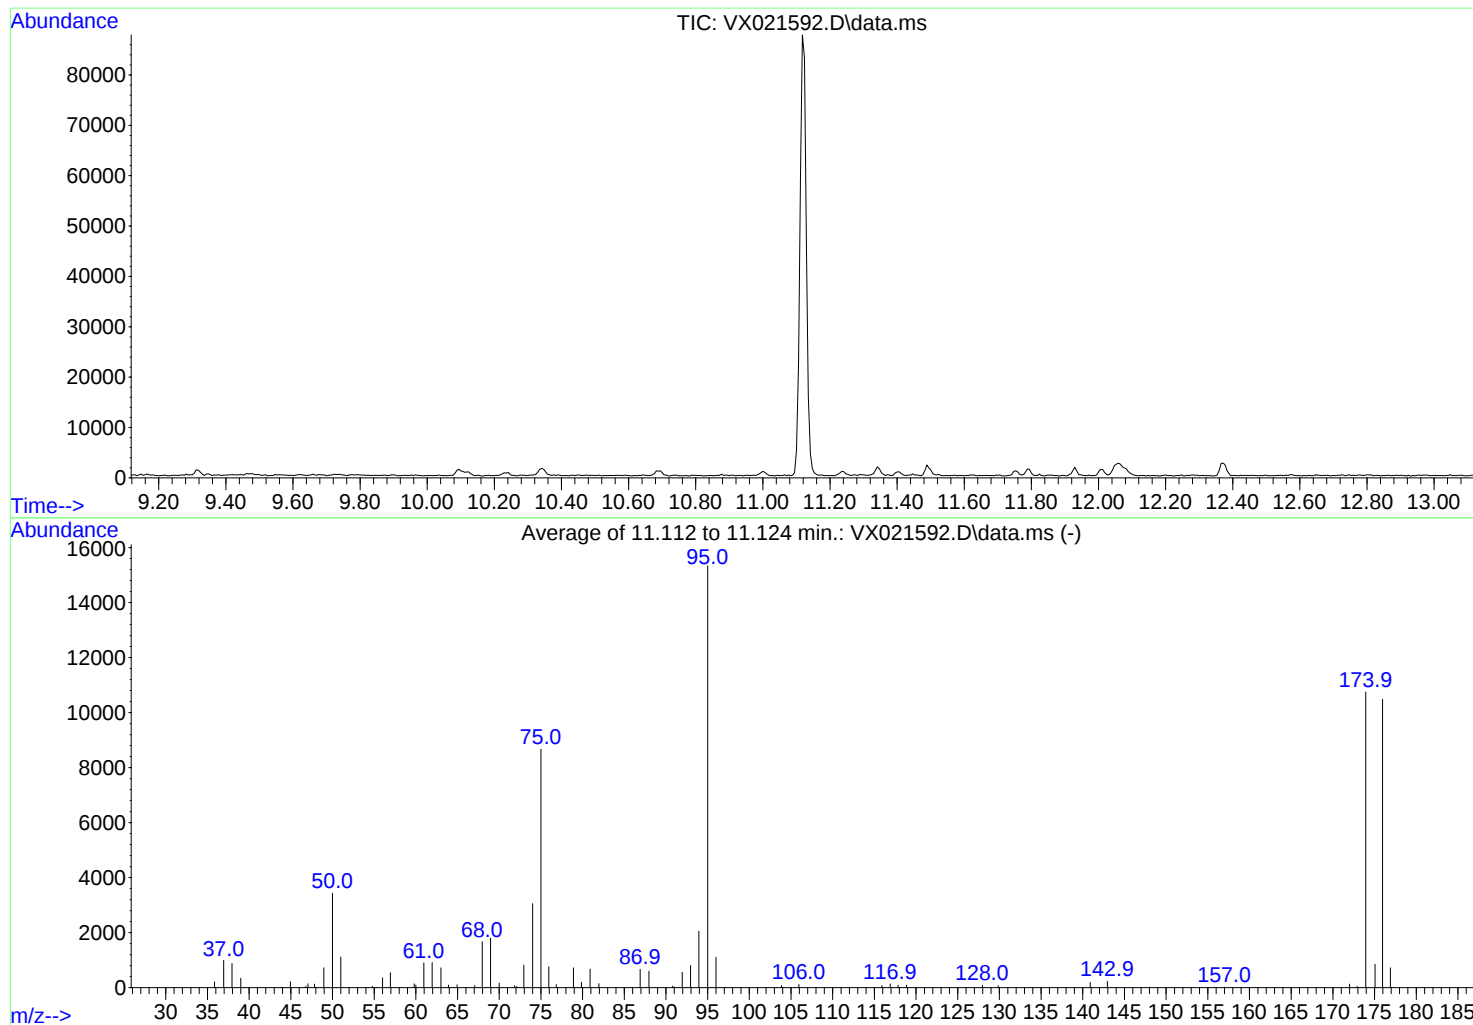

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	3432	PASS
75	95	30	60	56.5	8669	PASS
95	95	100	100	100.0	15335	PASS
96	95	5	9	7.2	1099	PASS
173	174	0.00	2	0.4	47	PASS
174	95	50	100	70.1	10749	PASS
175	174	5	9	7.9	850	PASS
176	174	95	101	97.5	10480	PASS
177	176	5	9	6.9	723	PASS