


Bromoform

Response Ratio

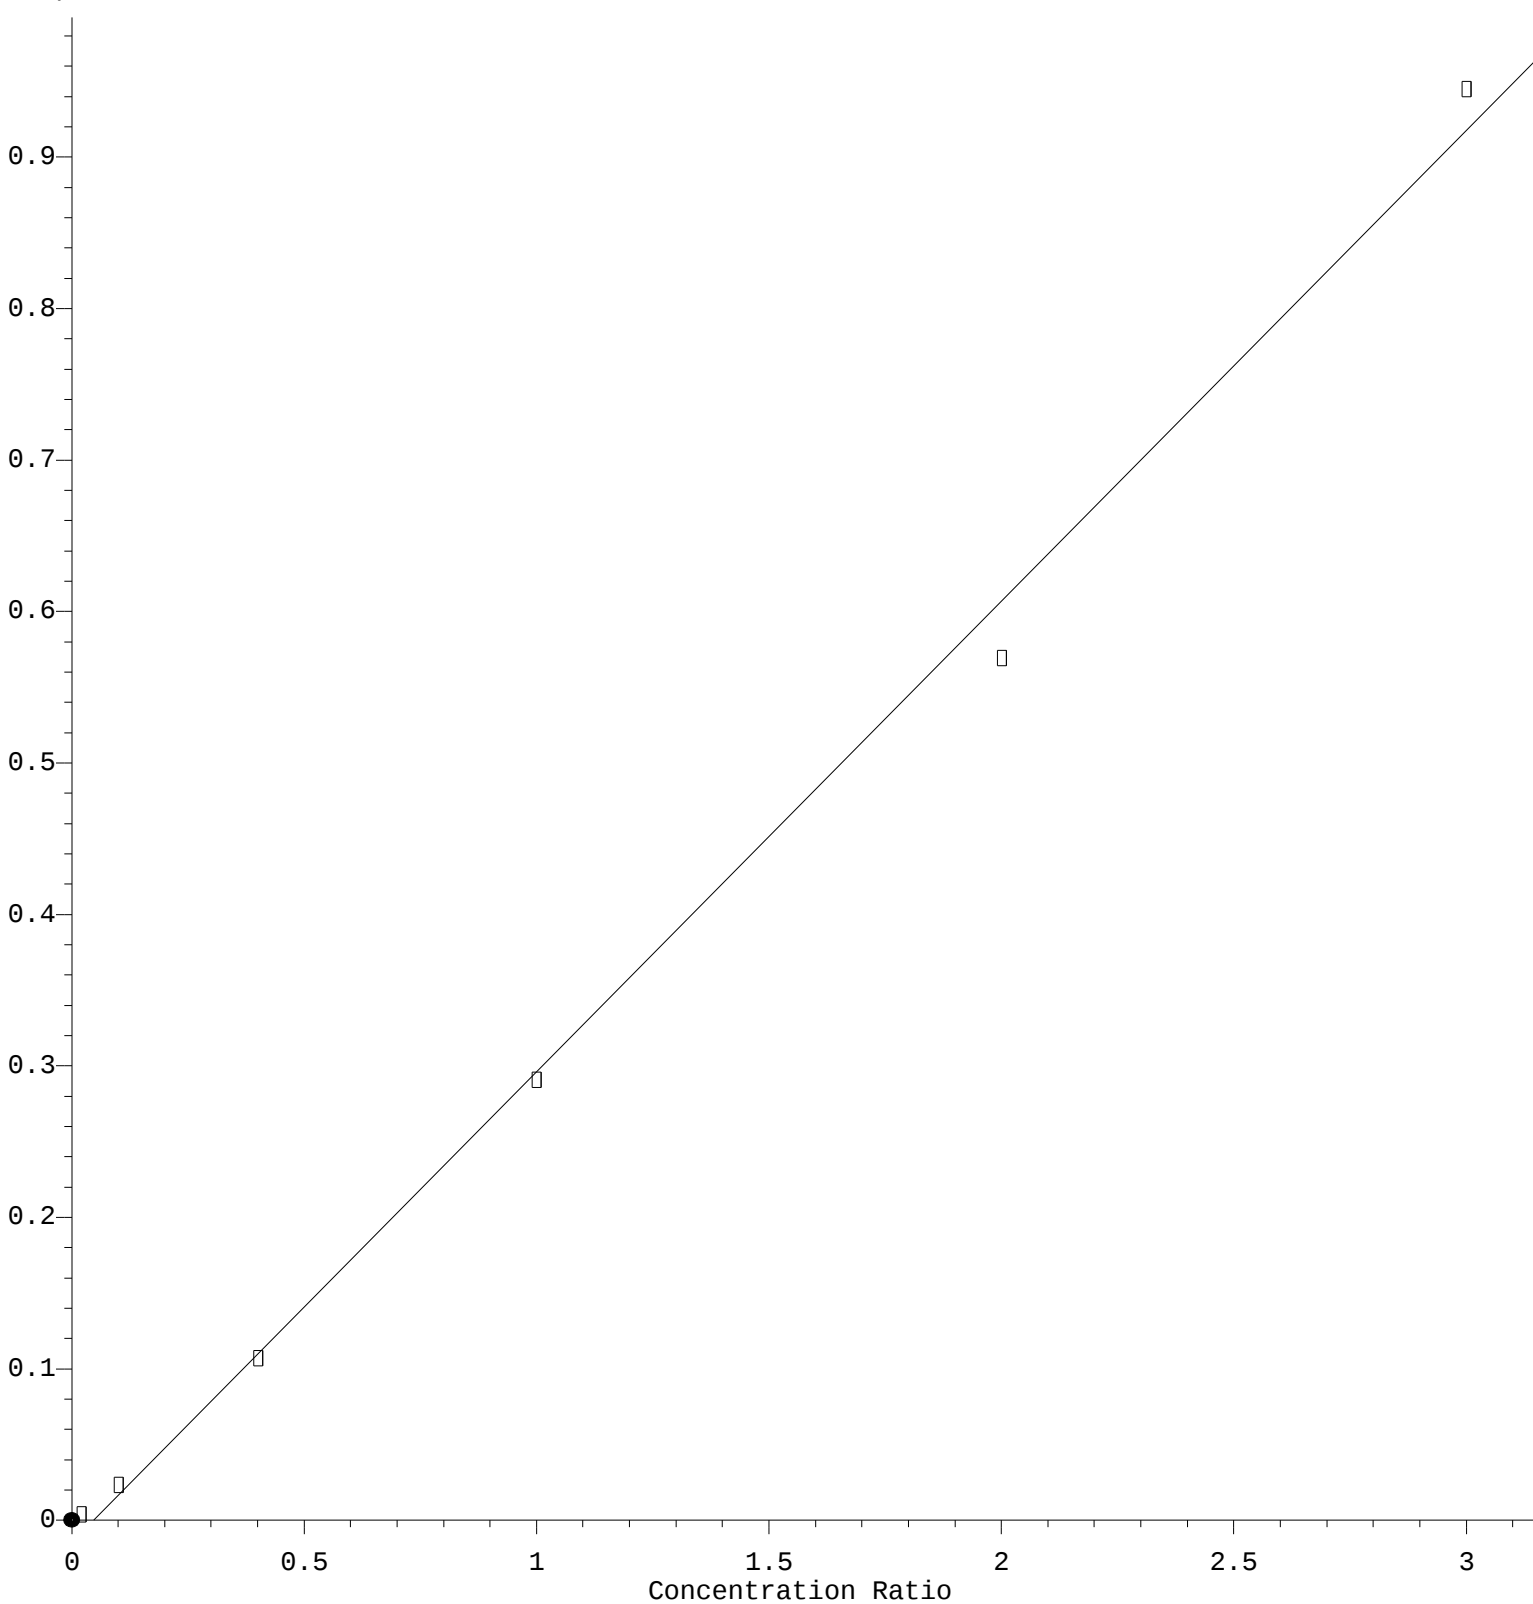

$$\text{Response} = 3.107\text{e-}001 * \text{Amt} - 1.463\text{e-}002$$


Coef of Det (r^2) = 0.996483 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Calibration Table Last Updated: Wed Mar 30 04:39:27 2022

trans-1,4-Dichloro-2-butene

Response Ratio

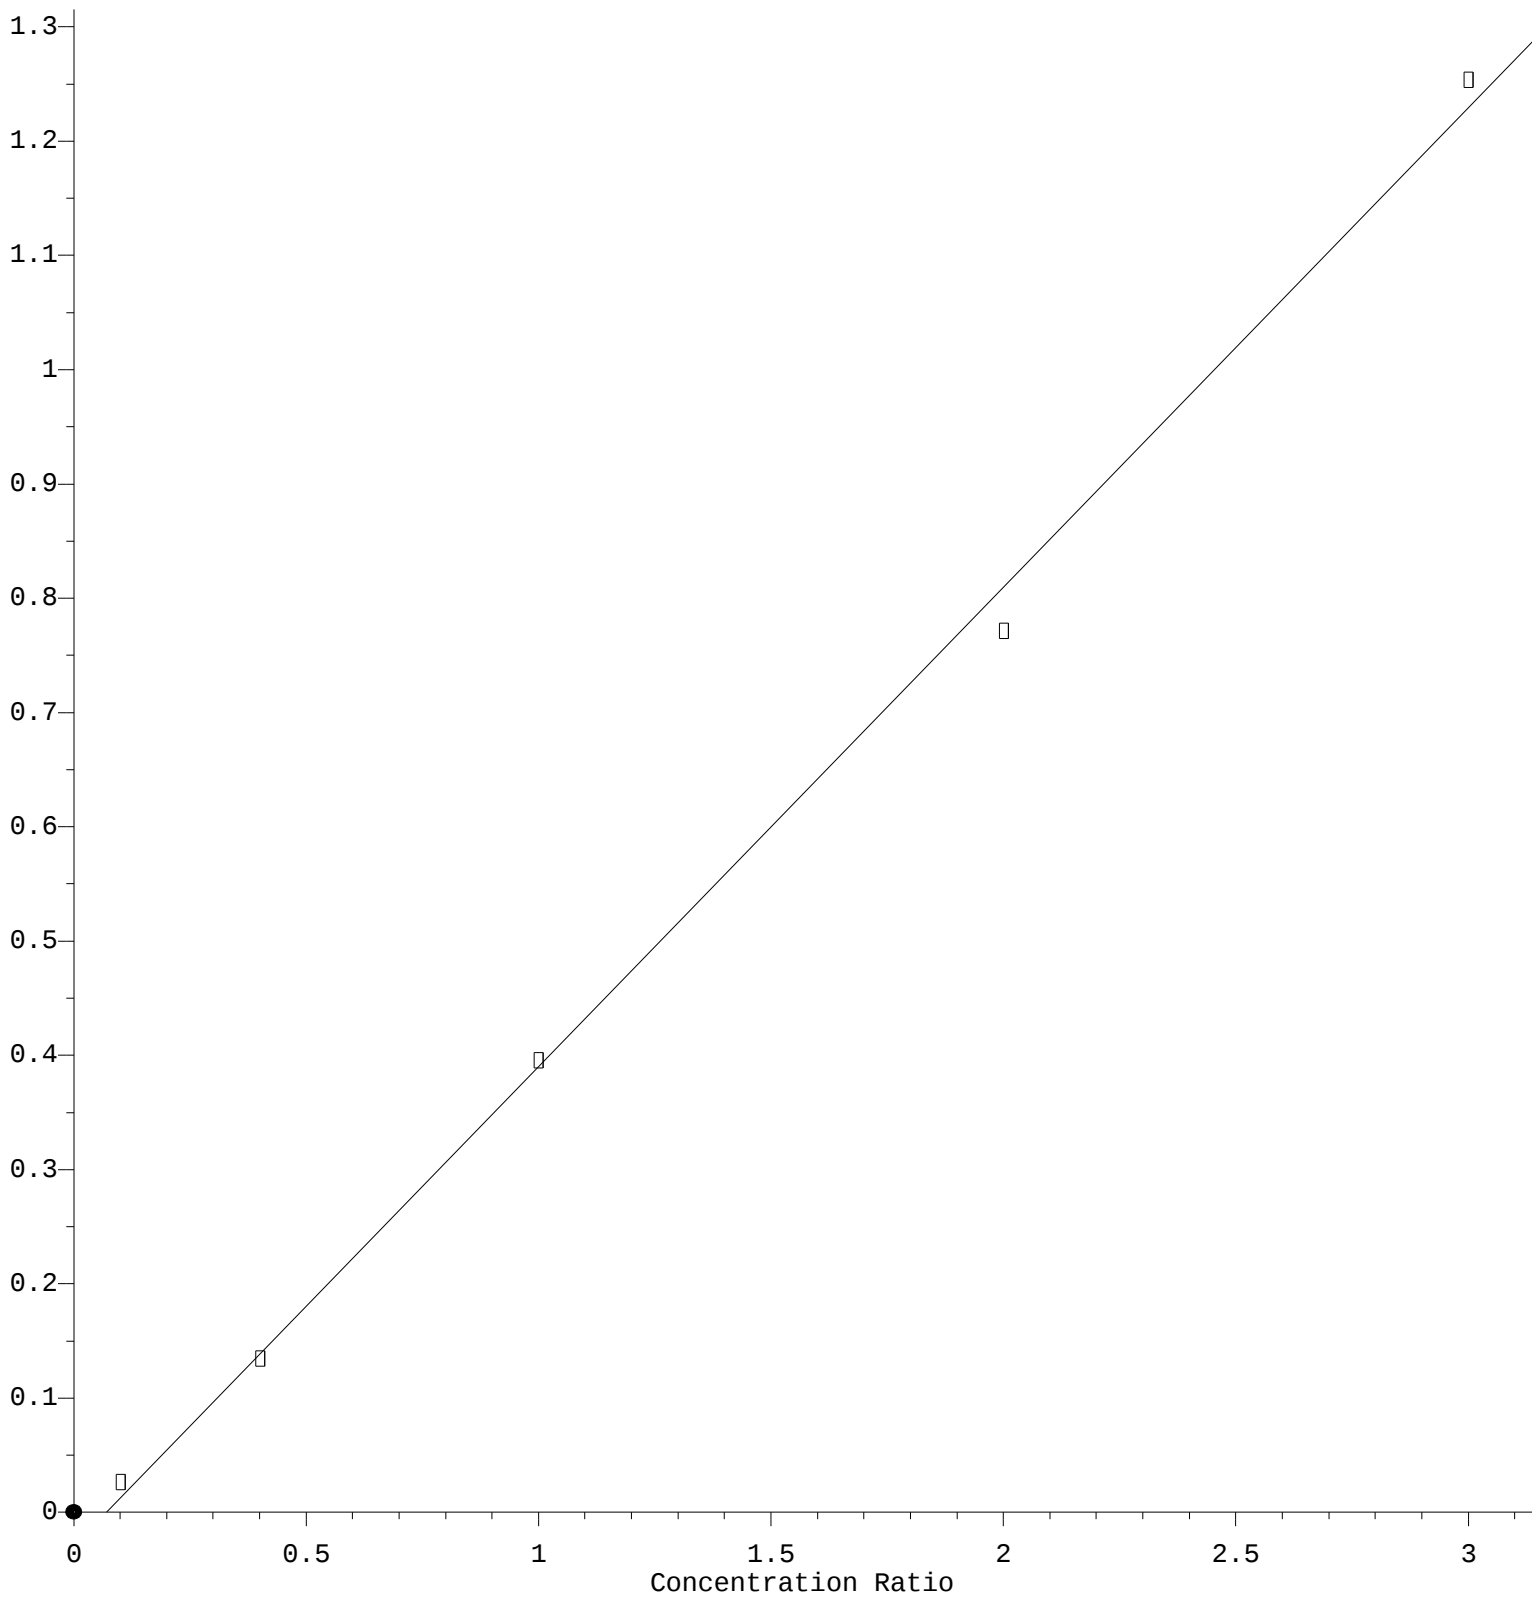

$$\text{Response} = 4.195\text{e-}001 * \text{Amt} - 2.933\text{e-}002$$


Coef of Det (r^2) = 0.997722 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Calibration Table Last Updated: Wed Mar 30 04:39:27 2022

Hexachlorobutadiene

Response Ratio

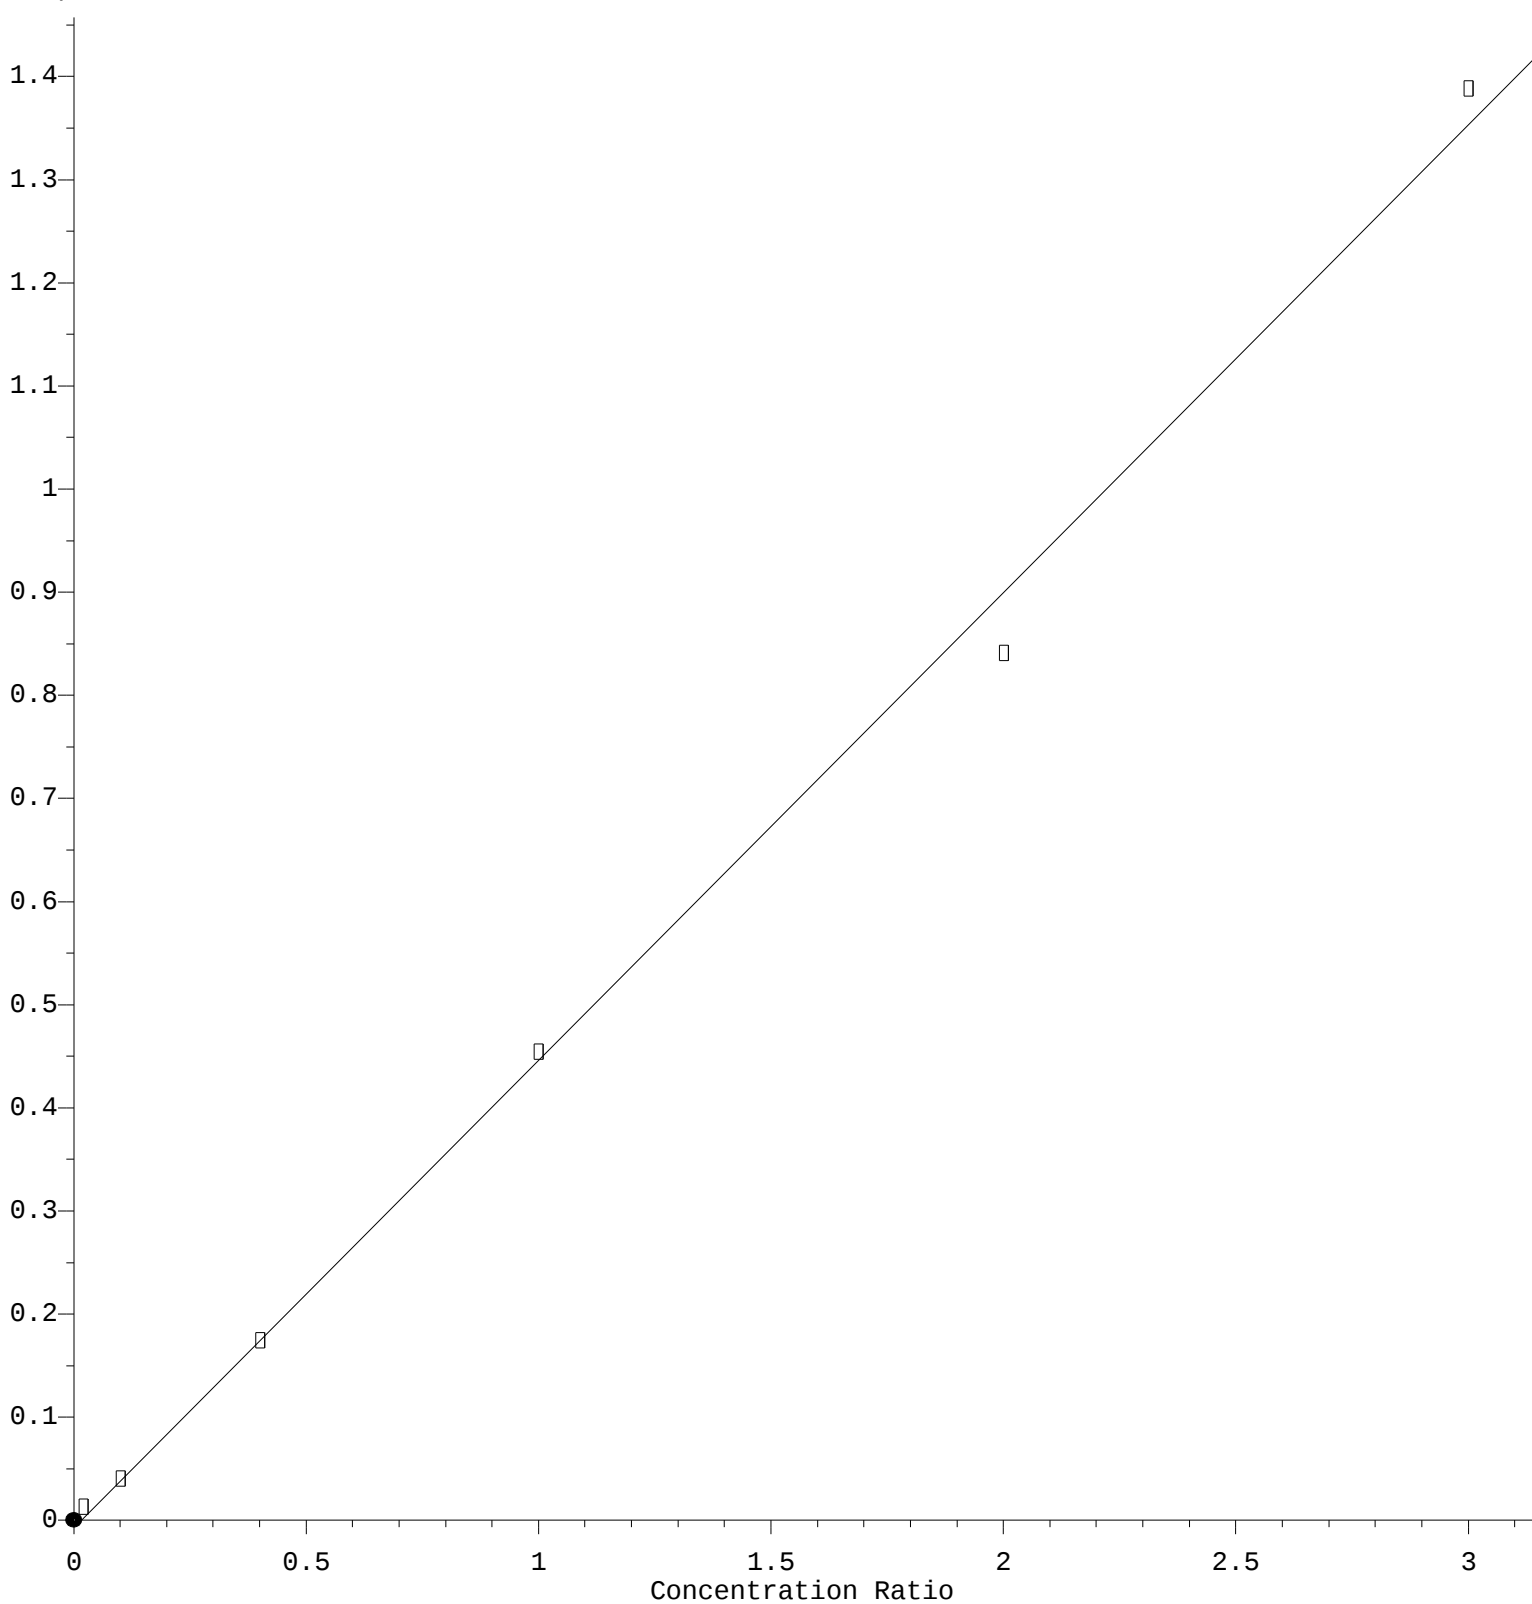

$$\text{Response} = 4.533\text{e-}001 * \text{Amt} - 7.373\text{e-}003$$

Coef of Det (r^2) = 0.996666 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M

Calibration Table Last Updated: Wed Mar 30 04:39:27 2022