
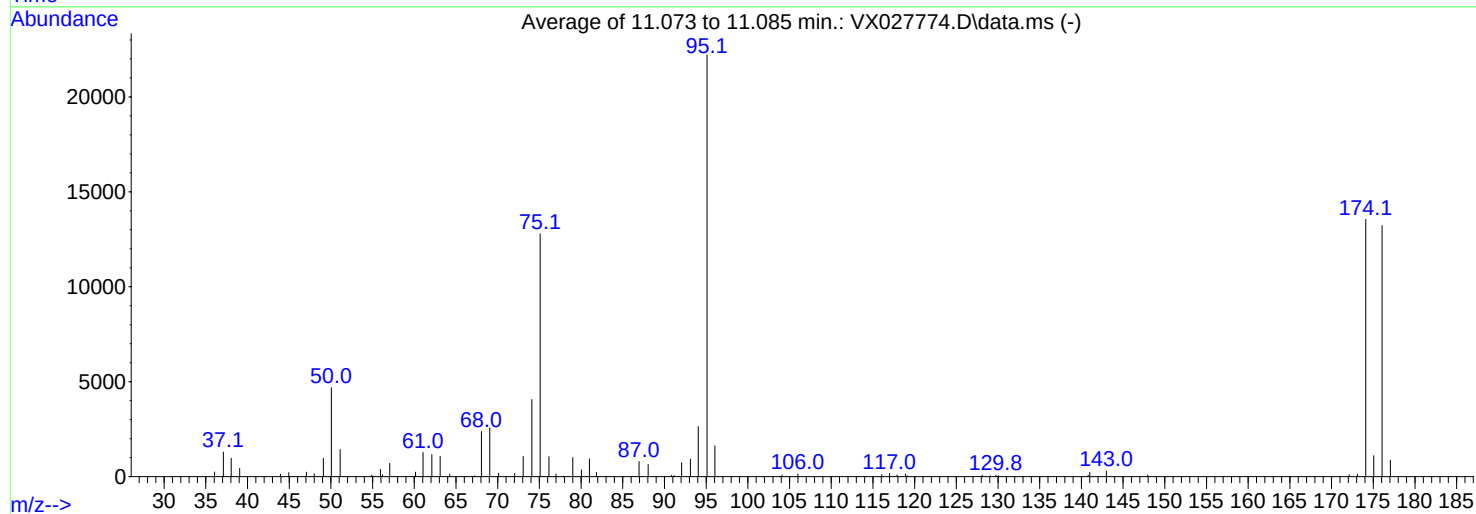


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032922\
Data File : VX027774.D
Acq On : 29 Mar 2022 12:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Title : SW846 8260
Last Update : Wed Mar 30 04:39:27 2022

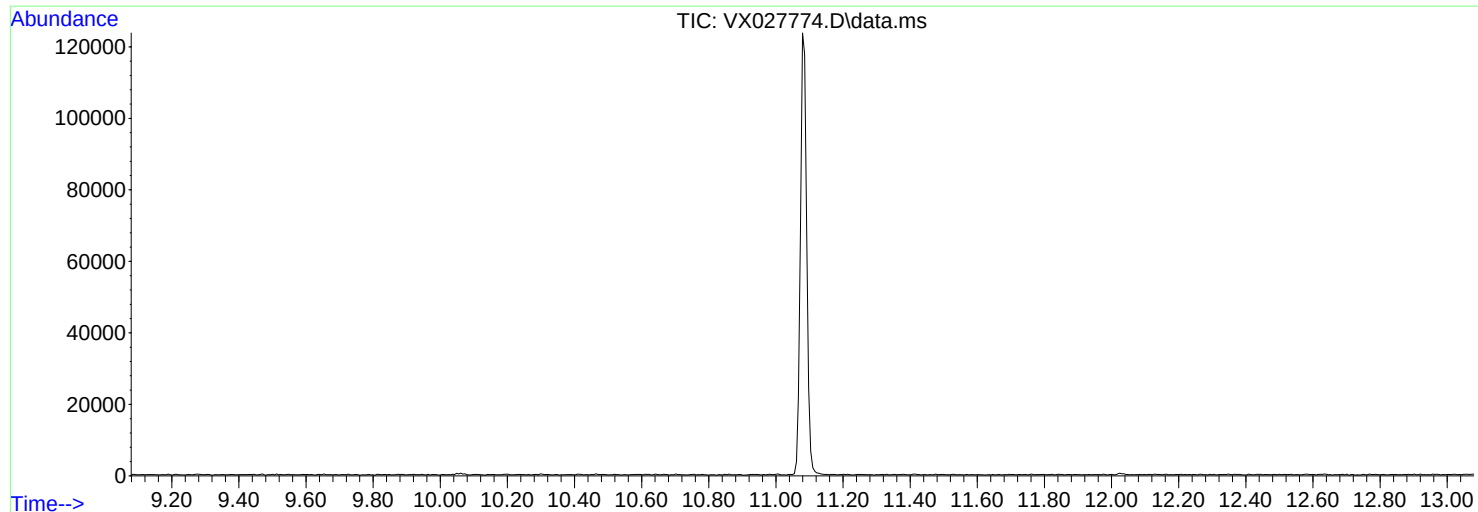

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	4684	PASS
75	95	30	60	57.5	12783	PASS
95	95	100	100	100.0	22216	PASS
96	95	5	9	7.3	1625	PASS
173	174	0.00	2	1.0	129	PASS
174	95	50	100	61.0	13548	PASS
175	174	5	9	8.1	1104	PASS
176	174	95	101	97.6	13219	PASS
177	176	5	9	6.5	863	PASS