
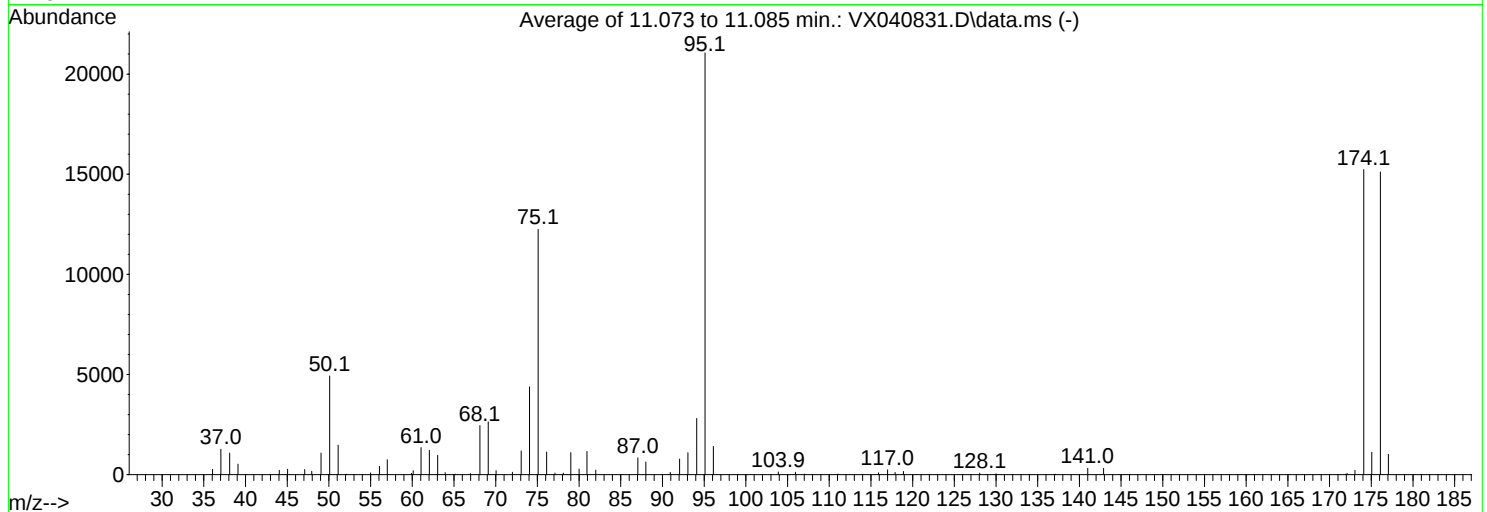


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032924\
Data File : VX040831.D
Acq On : 29 Mar 2024 08:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X032824W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Mar 29 05:24:11 2024

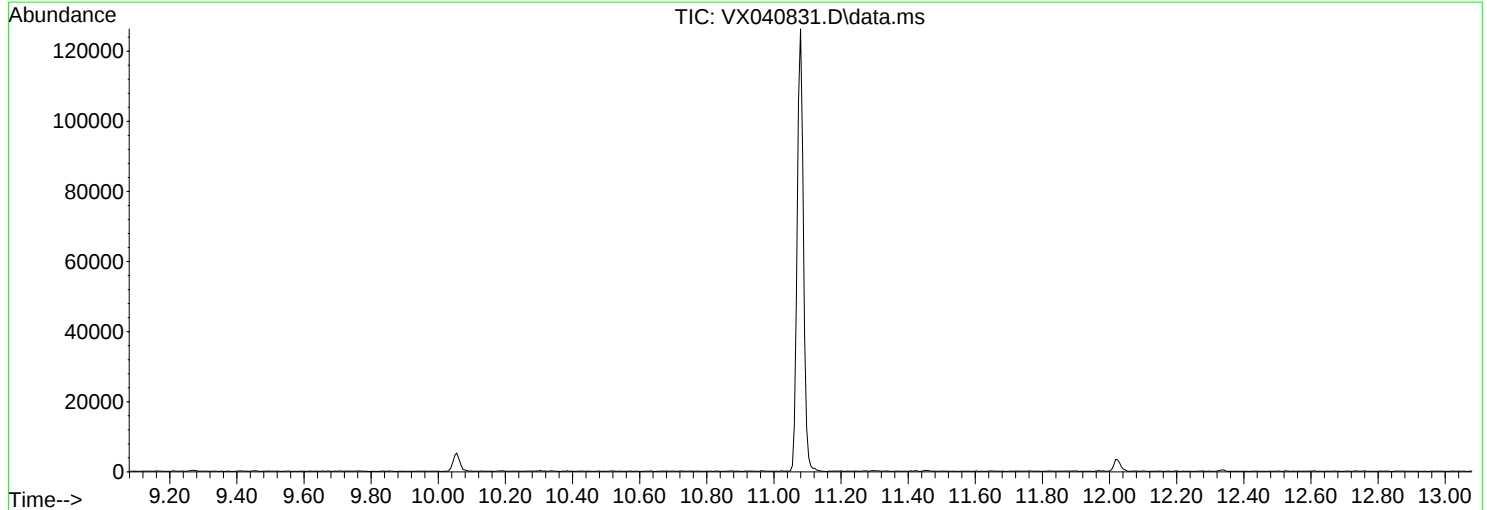

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	4931	PASS
75	95	30	60	58.2	12249	PASS
95	95	100	100	100.0	21061	PASS
96	95	5	9	6.7	1413	PASS
173	174	0.00	2	1.4	212	PASS
174	95	50	100	72.3	15235	PASS
175	174	5	9	7.3	1118	PASS
176	174	95	101	99.2	15119	PASS
177	176	5	9	6.7	1011	PASS