

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
 Data File : VX021638.D
 Acq On : 30 Mar 2021 18:26
 Operator : JC/MD
 Sample : M1843-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE117D2-20210325

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M

Title : SW846 8260

Signal : TIC: VX021638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	78	87	90	rBV7	3398	6500	1.69%	0.303%
2	2.581	246	254	262	rBV	13238	24542	6.39%	1.145%
3	4.658	595	607	617	rBV2	3102	10285	2.68%	0.480%
4	5.464	733	744	758	rBV2	46542	135708	35.35%	6.329%
5	5.629	761	772	786	rBV2	66032	188563	49.12%	8.795%
6	6.029	828	840	851	rBV	51866	135674	35.34%	6.328%
7	6.829	964	976	987	rBV	115983	274251	71.44%	12.791%
8	8.694	1286	1293	1302	rBV	242178	383884	100.00%	17.904%
9	10.094	1525	1531	1549	rVB	278357	370642	96.55%	17.287%
10	11.118	1698	1705	1713	rBV	224310	284076	74.00%	13.249%
11	12.059	1859	1865	1873	rVB	273125	329942	85.95%	15.389%




Sum of corrected areas: 2144067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021638.D
Acq On : 30 Mar 2021 18:26
Operator : JC/MD
Sample : M1843-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

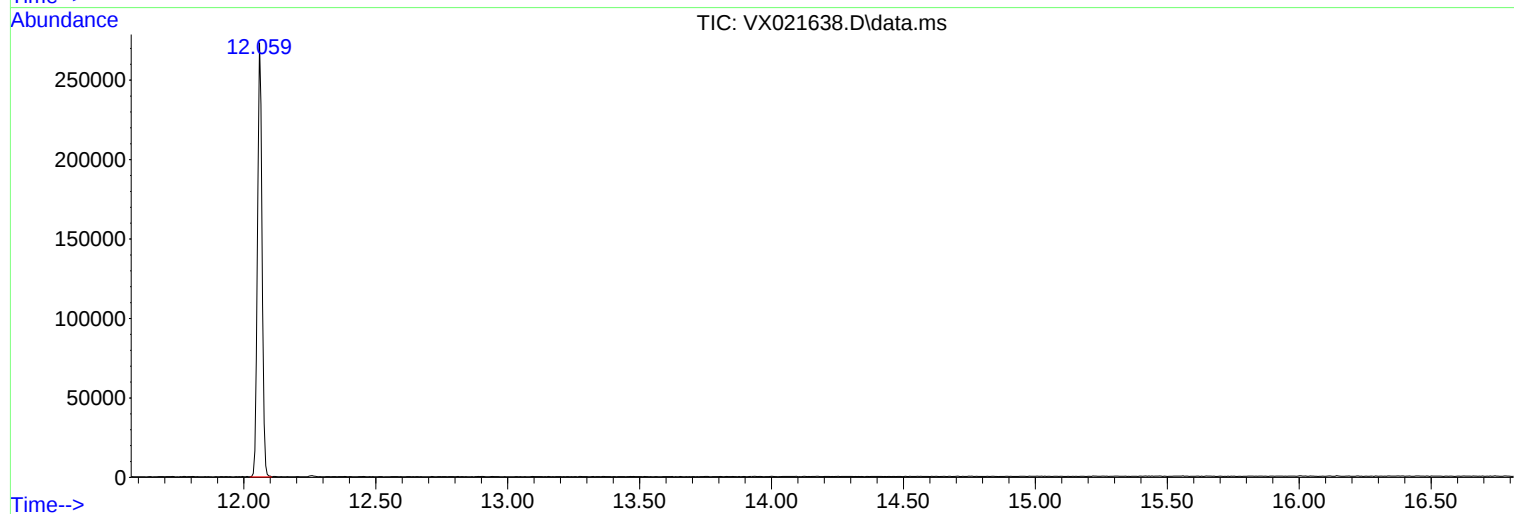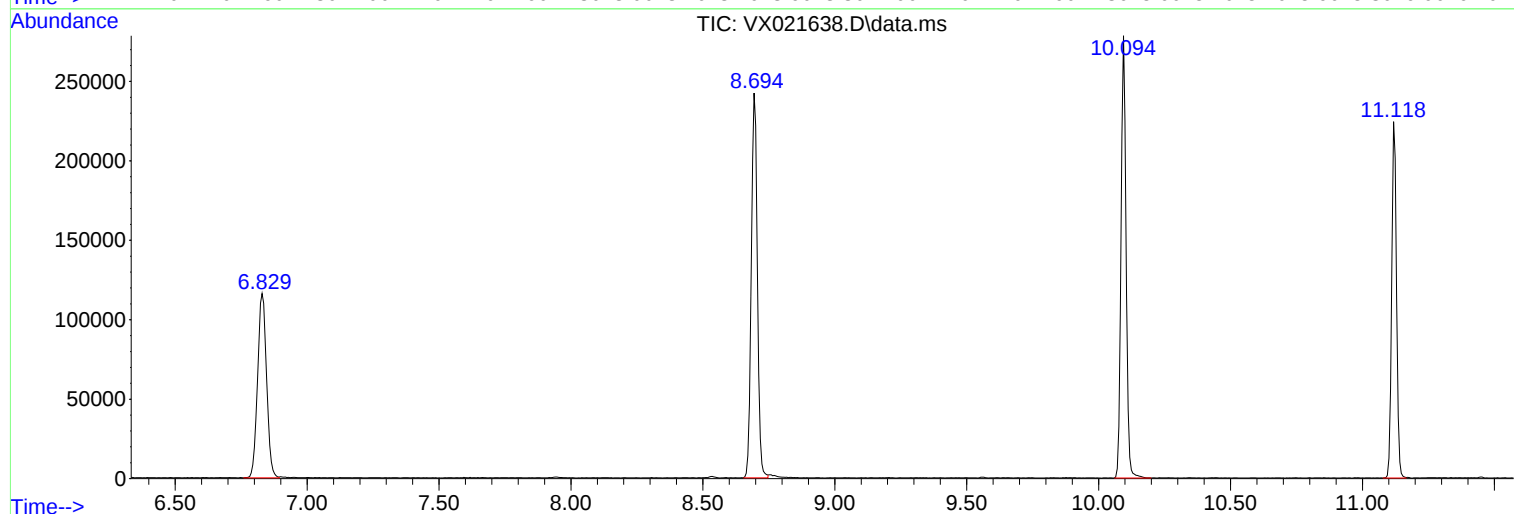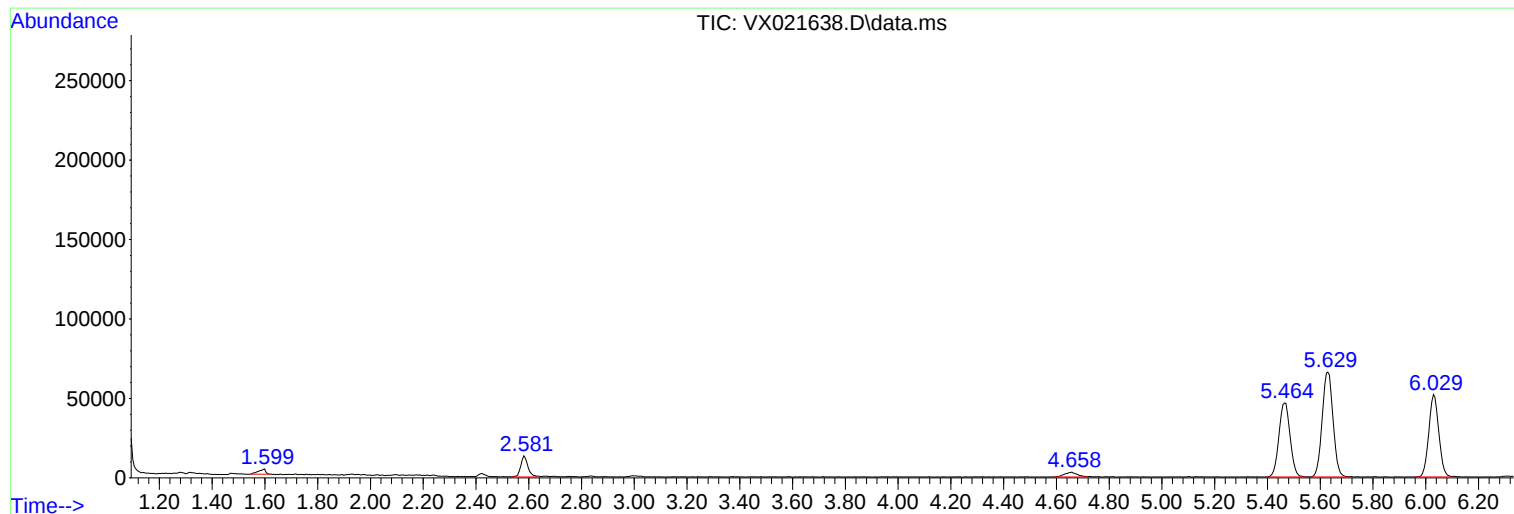

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021638.D
Acq On : 30 Mar 2021 18:26
Operator : JC/MD
Sample : M1843-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021638.D
Acq On : 30 Mar 2021 18:26
Operator : JC/MD
Sample : M1843-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D2-20210325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
