

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
 Data File : VX021639.D
 Acq On : 30 Mar 2021 18:49
 Operator : JC/MD
 Sample : M1861-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 021-OUTFALL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Title : SW846 8260

Signal : TIC: VX021639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	62	66	72	rBV	4003	5177	1.26%	0.218%
2	1.593	79	86	91	rVB5	3138	6725	1.64%	0.284%
3	2.422	217	227	235	rBV	12199	21074	5.14%	0.889%
4	2.581	246	254	262	rBV	2726	6098	1.49%	0.257%
5	3.111	337	344	351	rBV	2024	4438	1.08%	0.187%
6	4.076	500	508	516	rVB5	2372	5632	1.37%	0.238%
7	4.635	593	603	613	rBV	2391	7402	1.81%	0.312%
8	5.464	732	744	758	rBV	50361	141924	34.64%	5.988%
9	5.629	760	772	787	rVB	73165	200434	48.92%	8.457%
10	6.029	829	840	853	rBV	54016	143562	35.04%	6.057%
11	6.829	966	976	989	rBV	120646	286548	69.94%	12.090%
12	7.329	1054	1061	1068	rBV7	1776	4112	1.00%	0.173%
13	8.617	1273	1280	1286	rBV	6136	10352	2.53%	0.437%
14	8.694	1286	1293	1315	rVV	263306	409693	100.00%	17.286%
15	9.559	1435	1440	1447	rBV4	3065	4566	1.11%	0.193%
16	10.094	1525	1531	1547	rVB	295483	396020	96.66%	16.709%
17	10.694	1629	1633	1639	rBV	6247	7752	1.89%	0.327%
18	11.118	1699	1705	1713	rBV	250003	317643	77.53%	13.402%
19	12.059	1860	1865	1874	rBV	322807	385649	94.13%	16.271%
20	12.253	1893	1898	1906	rBV2	2820	5342	1.30%	0.225%




Sum of corrected areas: 2370143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021639.D
Acq On : 30 Mar 2021 18:49
Operator : JC/MD
Sample : M1861-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
021-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

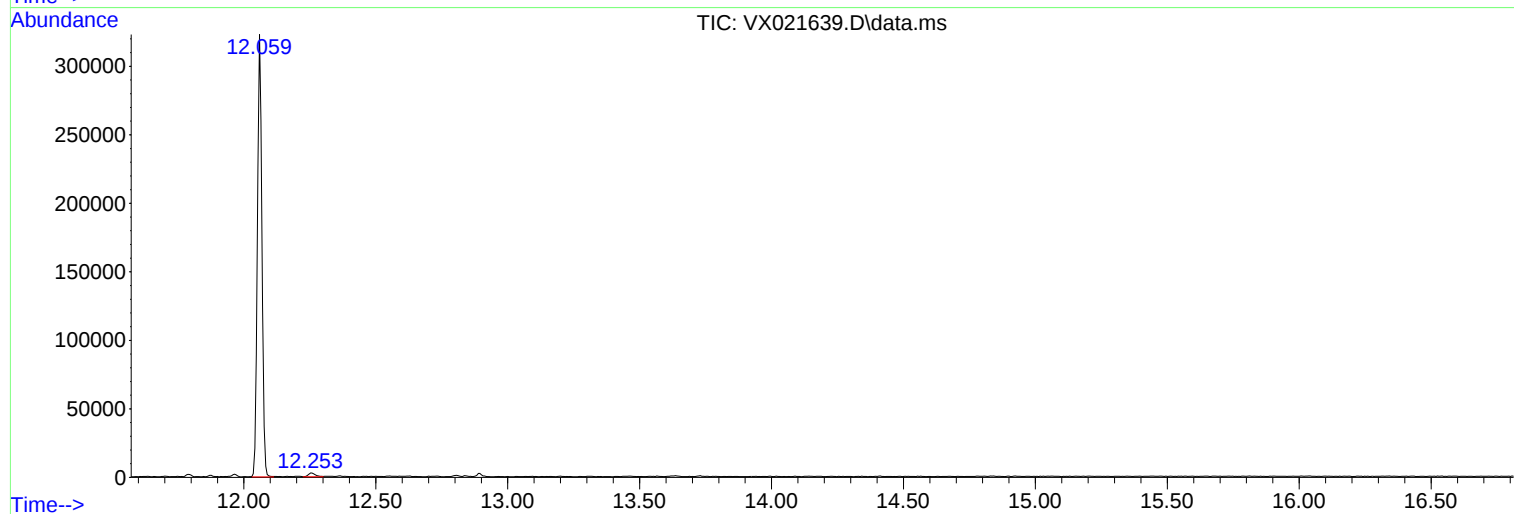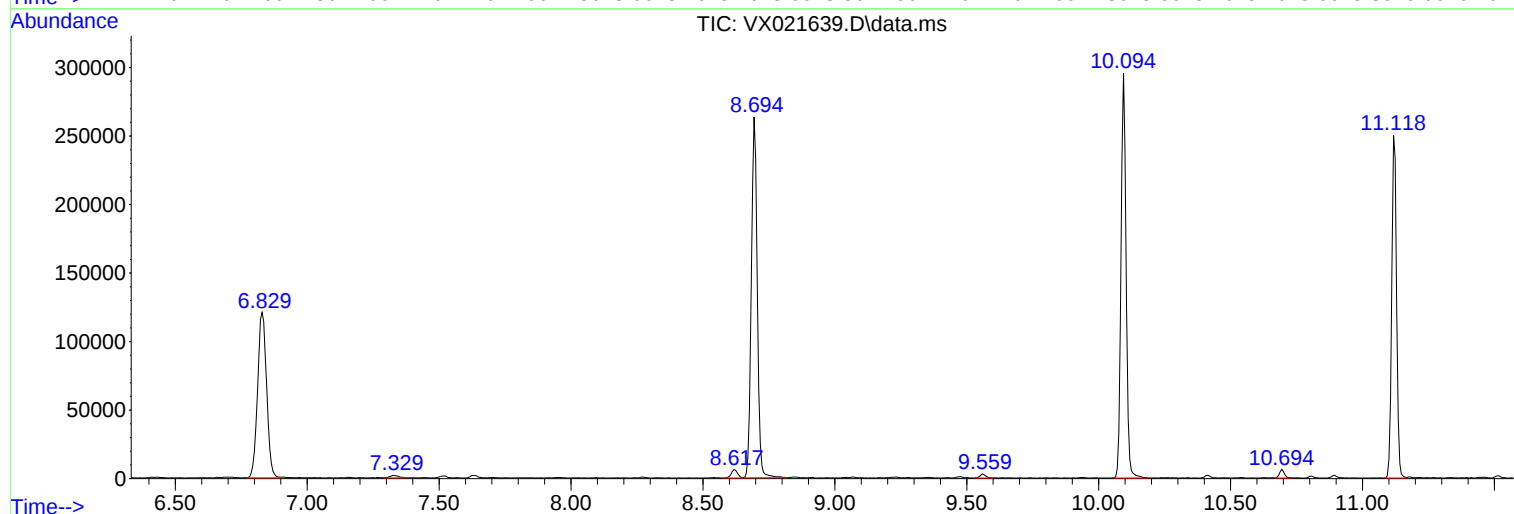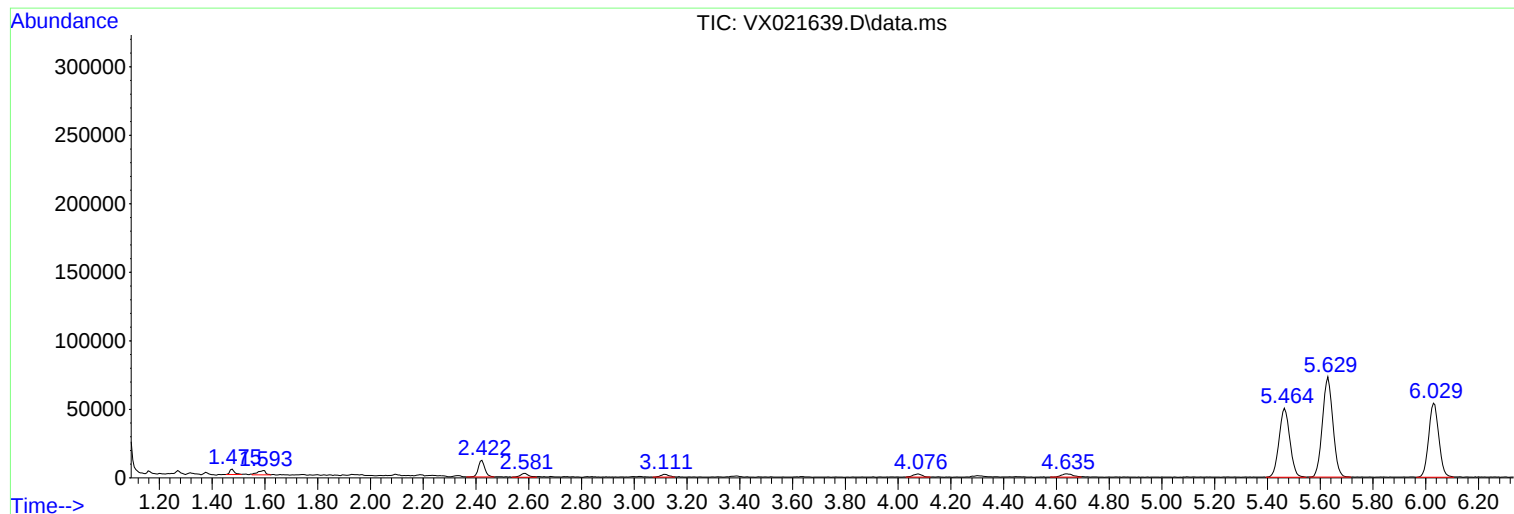

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021639.D
Acq On : 30 Mar 2021 18:49
Operator : JC/MD
Sample : M1861-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
021-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX033021\
Data File : VX021639.D
Acq On : 30 Mar 2021 18:49
Operator : JC/MD
Sample : M1861-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
021-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------